

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\WX050819\
 Data File : VX009405.D
 Acq On : 08 May 2019 17:54
 Operator : JC/SP
 Sample : K2643-02
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 OR-03-050719-A

Quant Time: May 09 06:32:17 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X042919W.M
 Quant Title : SW846 8260
 QLast Update : Wed May 08 03:31:13 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.67	168	176505	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.86	114	285332	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.11	117	247426	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.08	152	97138	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	6.06	65	117466	48.75	ug/l	0.00
Spiked Amount			Recovery	=	97.50%	
35) Dibromofluoromethane	5.50	113	86979	48.49	ug/l	0.00
Spiked Amount			Recovery	=	96.98%	
50) Toluene-d8	8.71	98	359121	49.59	ug/l	0.00
Spiked Amount			Recovery	=	99.18%	
62) 4-Bromofluorobenzene	11.13	95	115137	43.76	ug/l	0.00
Spiked Amount			Recovery	=	87.52%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
5) Bromomethane	1.64	94	274	0.211	ug/l	95
10) Methyl Iodide	2.51	142	48	4.617	ug/l #	42
11) Tert butyl alcohol	3.05	59	1565	2.806	ug/l #	73
13) Acrolein	2.29	56	458	0.907	ug/l #	72
16) Acetone	2.45	43	13863	10.715	ug/l	92
18) Methyl Acetate	2.78	43	4820	1.566	ug/l	92
20) Methylene Chloride	2.85	84	8264	3.945	ug/l	93
25) 2-Butanone	4.69	43	2896	1.440	ug/l #	86
28) Bromochloromethane	5.02	49	110	Below Cal	#	20
29) Tetrahydrofuran	5.15	42	2205	1.704	ug/l #	66
31) Cyclohexane	5.65	56	3895	1.093	ug/l #	1
36) 1,1-Dichloropropene	5.67	75	13943	5.258	ug/l #	51
38) Carbon Tetrachloride	5.66	117	16767	6.960	ug/l #	16
43) Isopropyl Acetate	6.45	43	12364	2.092	ug/l	99
48) Methyl methacrylate	7.68	41	8153	2.781	ug/l #	19
49) 1,4-Dioxane	7.73	88	23	0.387	ug/l #	1
51) 4-Methyl-2-Pentanone	8.62	43	88178	22.829	ug/l #	50
54) cis-1,3-Dichloropropene	8.62	75	38242	11.369	ug/l #	58
57) 1,3-Dichloropropane	9.54	76	8614	2.405	ug/l #	43
59) 2-Hexanone	9.44	43	12411	4.091	ug/l #	26
74) N-amyl acetate	10.69	43	13562	3.293	ug/l #	57
76) 1,2,3-Trichloropropane	11.13	75	57084	25.334	ug/l #	34
80) 1,3,5-Trimethylbenzene	11.51	105	2546	0.428	ug/l	96
81) trans-1,4-Dichloro-2-buten	11.13	75	57084	64.821	ug/l #	10
84) 1,2,4-Trimethylbenzene	11.80	105	3014	0.505	ug/l	92
95) Naphthalene	13.83	128	14047	1.983	ug/l	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX050819\
Data File : VX009405.D
Acq On : 08 May 2019 17:54
Operator : JC/SP
Sample : K2643-02
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
OR-03-050719-A

Quant Time: May 09 06:32:17 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X042919W.M
Quant Title : SW846 8260
QLast Update : Wed May 08 03:31:13 2019
Response via : Initial Calibration

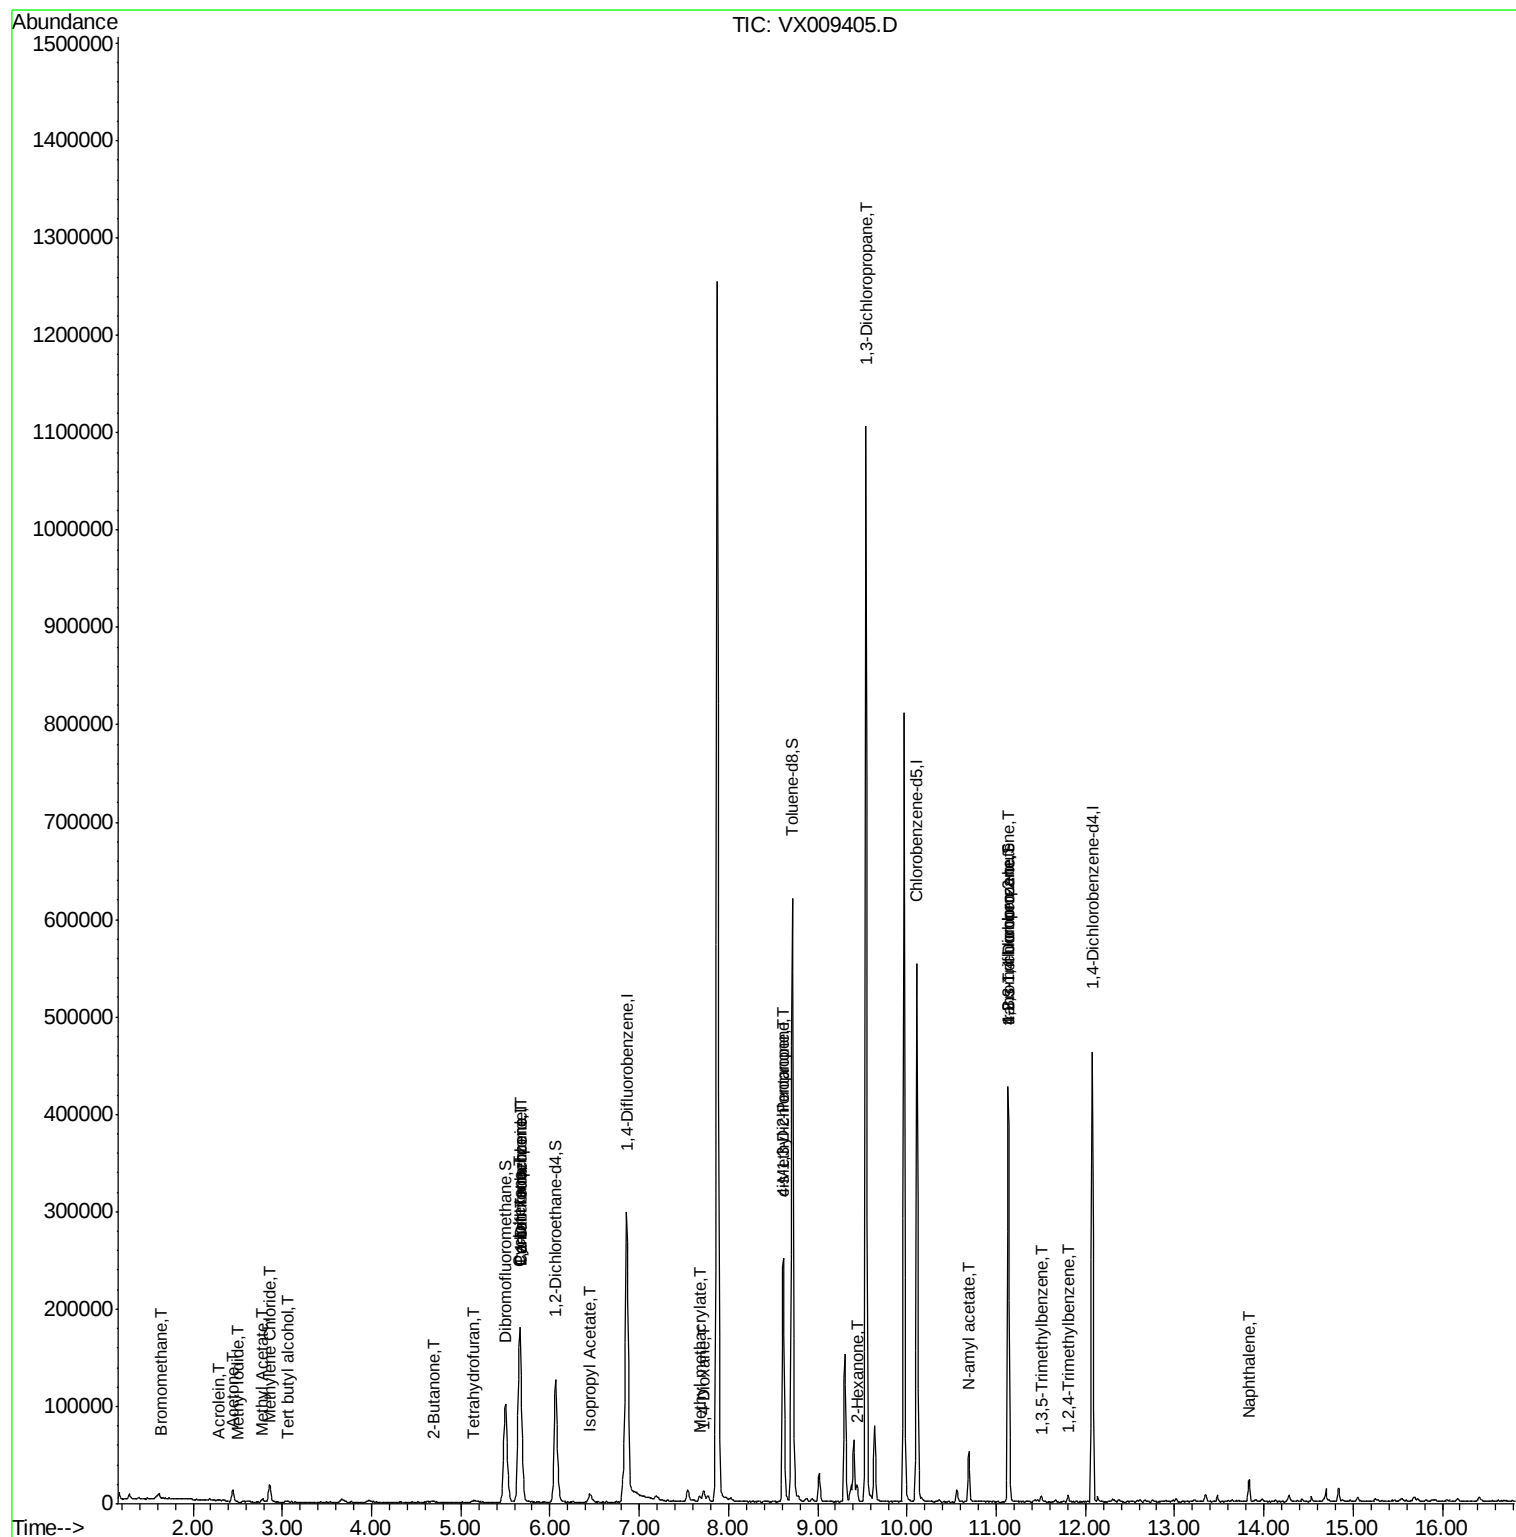

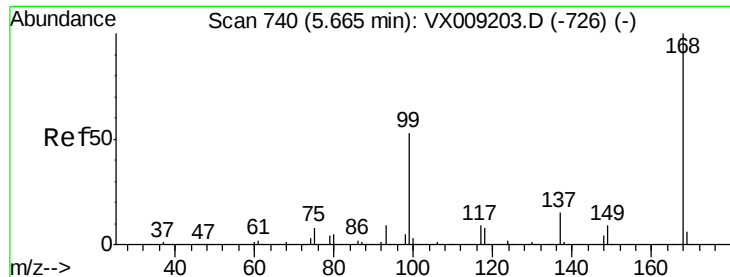

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.67 min Scan# 740

Delta R.T. 0.00 min

Lab File: VX009405.D

Acq: 08 May 2019 17:54

Instrument :

MSVOA_X

ClientSampleId :


OR-03-050719-A

Tot Ion:168 Resp: 176505

Ion Ratio Lower Upper




168 100

99 54.7 42.3 63.5

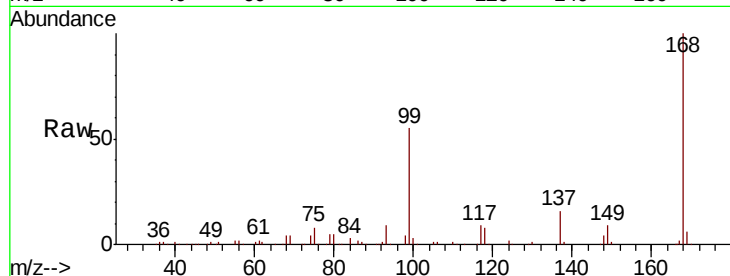

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

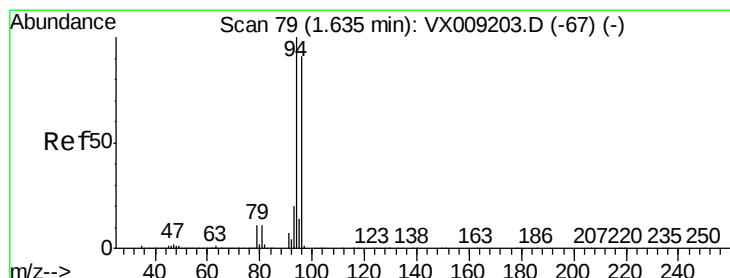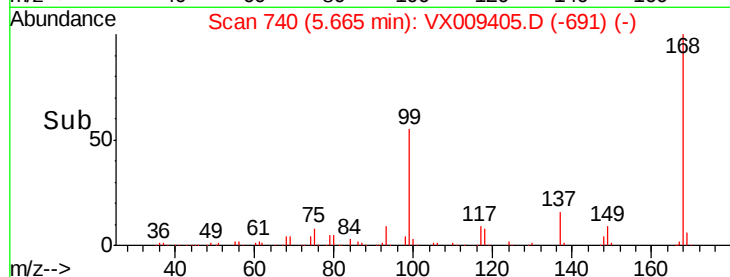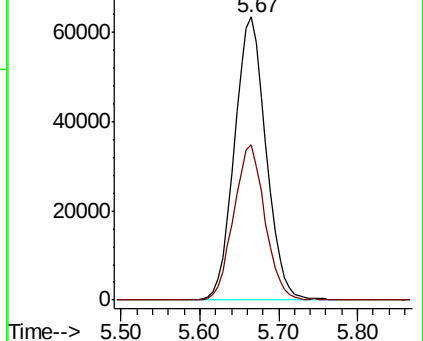

#5

Bromomethane

Concen: 0.211 ug/l

RT: 1.64 min Scan# 80

Delta R.T. 0.01 min

Lab File: VX009405.D


Acq: 08 May 2019 17:54

Tgt Ion: 94 Resp: 274

Ion Ratio Lower Upper



94 100


96 96.0 73.0 109.6

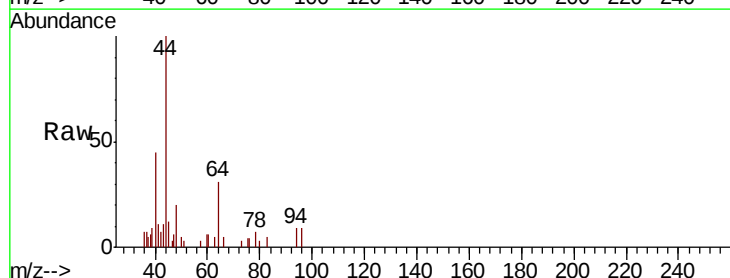

Abundance Ion 93.90 (93.60 to 94.60): VX0

Ion 95.90 (95.60 to 96.60): VX0



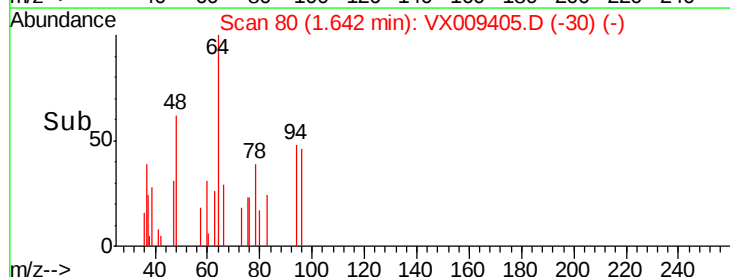
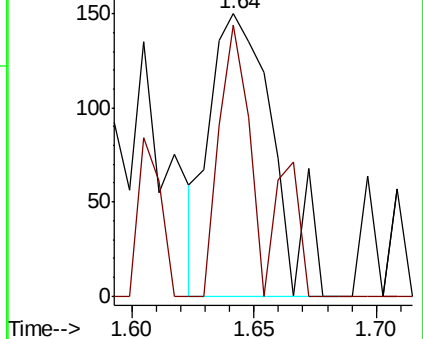




#10
Methvl Iodide
Concen: 4.617 ug/l
RT: 2.51 min Scan# 222
Delta R.T. 0.00 min
Lab File: VX009405.D
Acq: 08 May 2019 17:54




Instrument :
MSVOA_X
ClientSampleId :
OR-03-050719-A


Tot Ion:142 Resp: 48
Ion Ratio Lower Upper
142 100
127 0.0 32.7 49.1#
141 0.0 11.5 17.3#

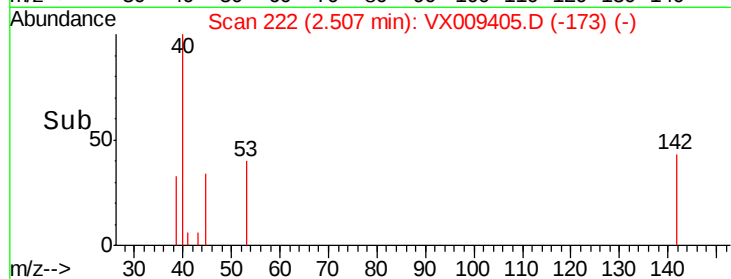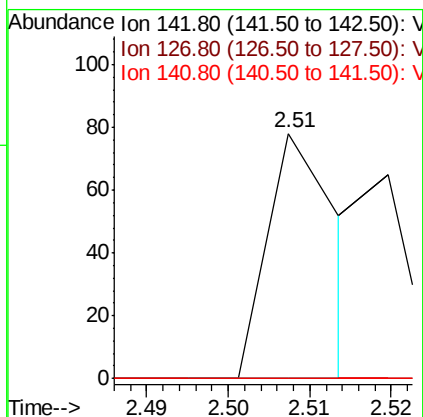

#11
Tert butyl alcohol
Concen: 2.806 ug/l
RT: 3.05 min Scan# 311
Delta R.T. 0.00 min
Lab File: VX009405.D
Acq: 08 May 2019 17:54

Tgt Ion: 59 Resp: 1565
Ion Ratio Lower Upper
59 100
57 20.1 8.2 12.2#

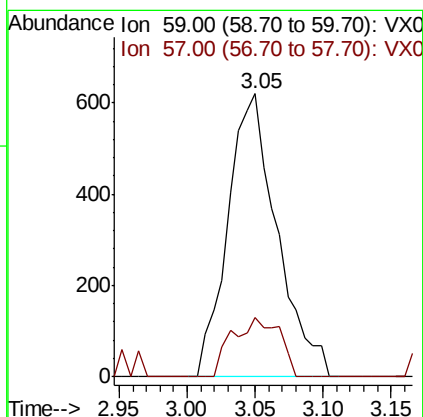



#13

Acrolein

Concen: 0.907 ug/l

RT: 2.29 min Scan# 186

Delta R.T. -0.01 min

Lab File: VX009405.D

Acq: 08 May 2019 17:54

Instrument :

MSVOA_X

ClientSampleId :





OR-03-050719-A

Tot Ion: 56 Resp: 458

Ion Ratio Lower Upper

56 100

55 47.6 56.6 85.0#

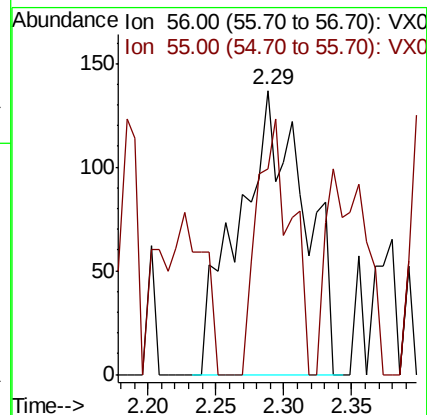

#16

Acetone

Concen: 10.715 ug/l

RT: 2.45 min Scan# 212

Delta R.T. 0.00 min

Lab File: VX009405.D




Acq: 08 May 2019 17:54


Tgt Ion: 43 Resp: 13863

Ion Ratio Lower Upper

43 100

58 26.6 24.9 37.3


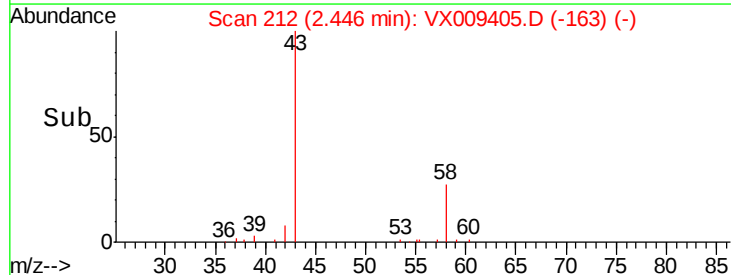
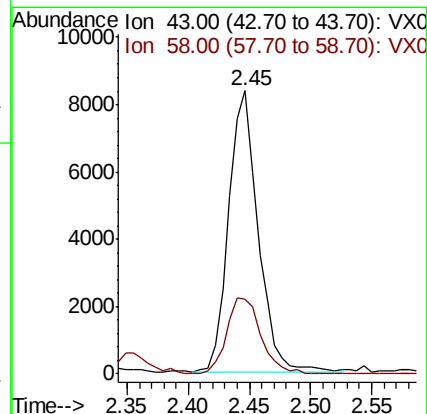



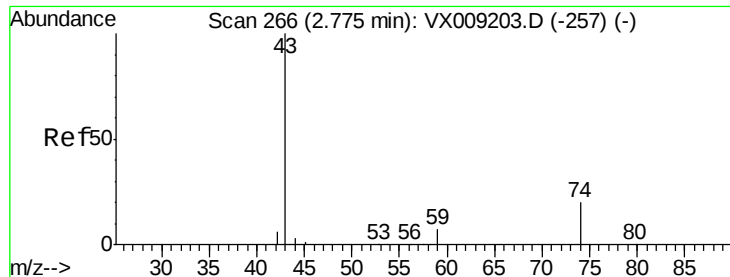

#18
Methvl Acetate
Concen: 1.566 ug/l
RT: 2.78 min Scan# 266
Delta R.T. 0.00 min
Lab File: VX009405.D
Acq: 08 May 2019 17:54




Instrument :
MSVOA_X
ClientSampleId :
OR-03-050719-A


Tot Ion: 43 Resp: 4820
Ion Ratio Lower Upper
43 100
74 23.9 16.2 24.4

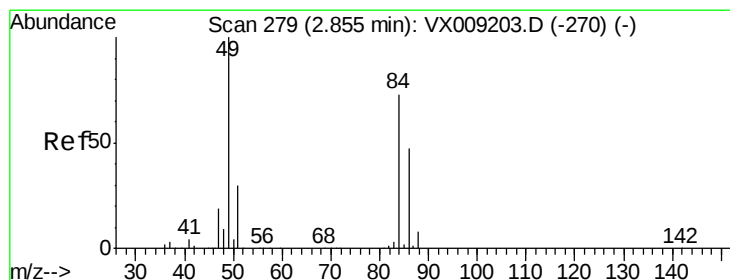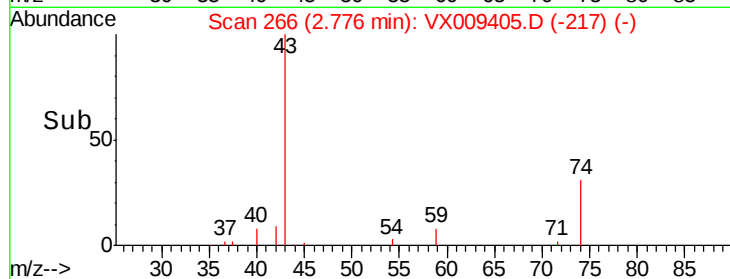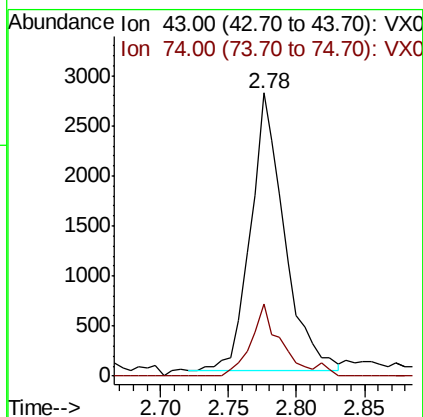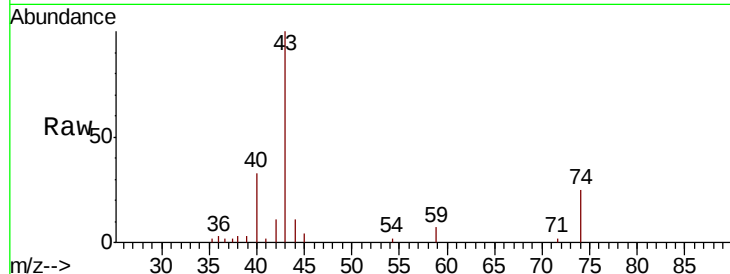

#20
Methylene Chloride
Concen: 3.945 ug/l
RT: 2.85 min Scan# 279
Delta R.T. 0.00 min
Lab File: VX009405.D
Acq: 08 May 2019 17:54

Tgt Ion: 84 Resp: 8264
Ion Ratio Lower Upper
84 100
49 122.9 109.9 164.9
51 41.8 32.7 49.1
86 65.6 52.0 78.0

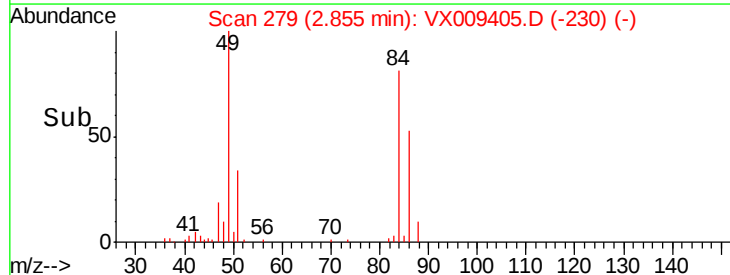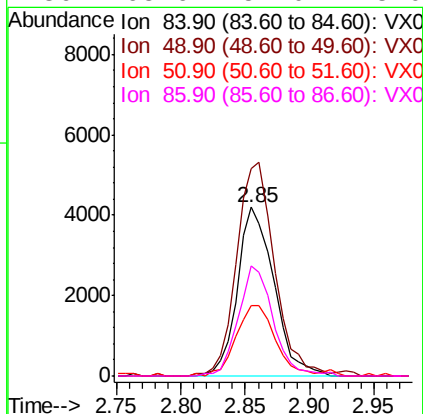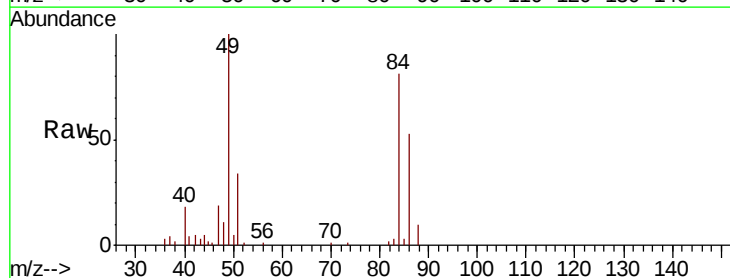

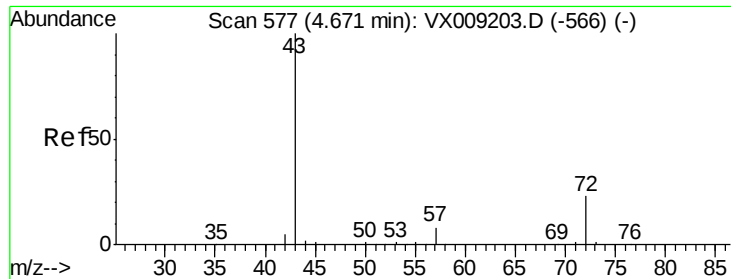

#25

2-Butanone

Concen: 1.440 ug/l

RT: 4.69 min Scan# 580

Delta R.T. 0.02 min

Lab File: VX009405.D

Acq: 08 May 2019 17:54

Instrument :

MSVOA_X

ClientSampleId :


OR-03-050719-A

Tot Ion: 43 Resp: 2896

Ion Ratio Lower Upper


43 100

72 15.9 18.2 27.2#





Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 72.00 (71.70 to 72.70): VX0

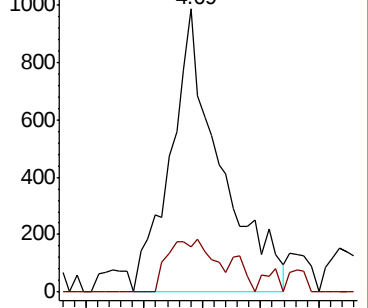

Time-->



#28

Bromochloromethane

Concen: Below Cal

RT: 5.02 min Scan# 634

Delta R.T. 0.01 min

Lab File: VX009405.D

Acq: 08 May 2019 17:54


Tgt Ion: 49 Resp: 110

Ion Ratio Lower Upper

49 100

129 0.0 0.0 3.8


130 0.0 51.2 76.8#




Abundance Ion 48.90 (48.60 to 49.60): VX0


Ion 128.80 (128.50 to 129.50): V

Ion 129.80 (129.50 to 130.50): V

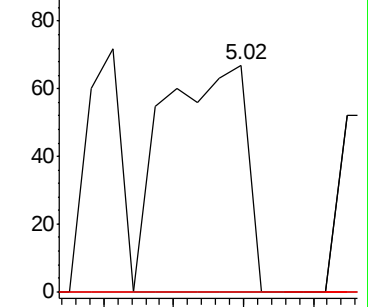

Time-->









#29
Tetrahydrofuran
Concen: 1.704 ug/l
RT: 5.15 min Scan# 655
Delta R.T. 0.02 min
Lab File: VX009405.D
Acq: 08 May 2019 17:54




Instrument :
MSVOA_X
ClientSampleId :
OR-03-050719-A


Tot Ion	Ratio	Lower	Upper
42	100		
72	0.0	30.4	45.6#
71	33.9	28.6	43.0

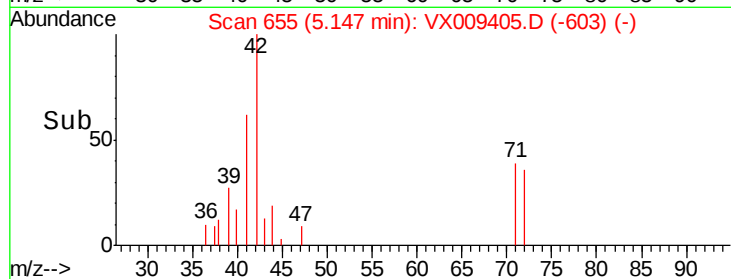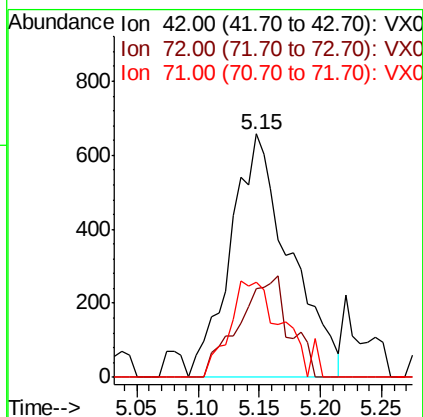

#31
Cyclohexane
Concen: 1.093 ug/l
RT: 5.65 min Scan# 738
Delta R.T. 0.07 min
Lab File: VX009405.D
Acq: 08 May 2019 17:54

Tgt Ion	Ratio	Lower	Upper
56	100		
69	161.1	23.4	35.0#
84	148.1	61.9	92.9#



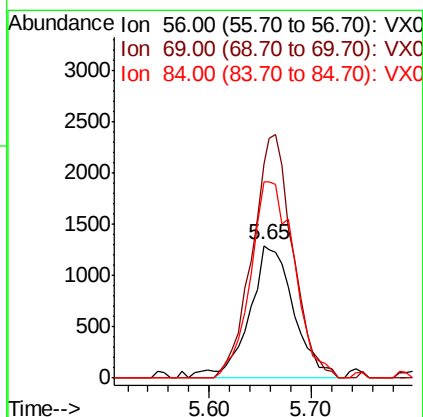



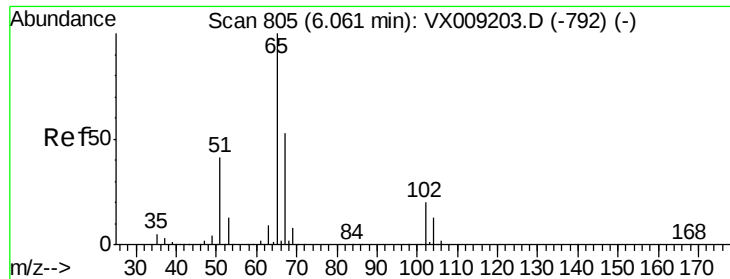

#33
 1,2-Dichloroethane-d4
 Concen: 48.751 ug/l
 RT: 6.06 min Scan# 805
 Delta R.T. 0.00 min
 Lab File: VX009405.D
 Acq: 08 May 2019 17:54




Instrument :
 MSVOA_X
 ClientSampleId :
 OR-03-050719-A


Tot Ion: 65 Resp: 117466
 Ion Ratio Lower Upper
 65 100
 67 53.3 0.0 106.6

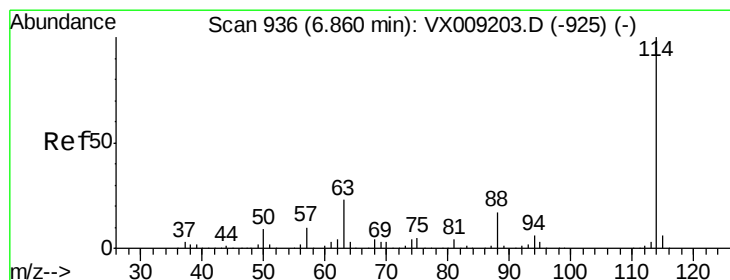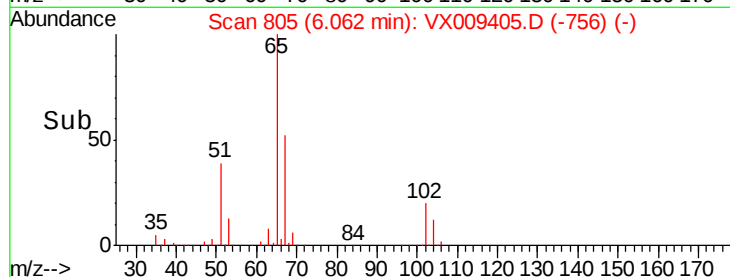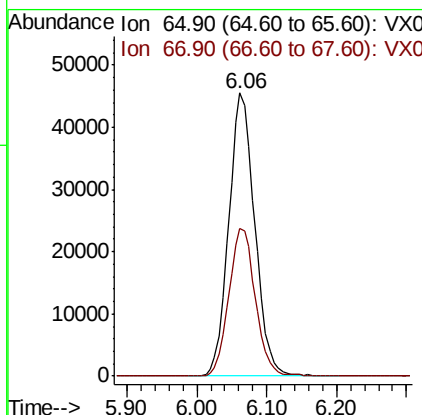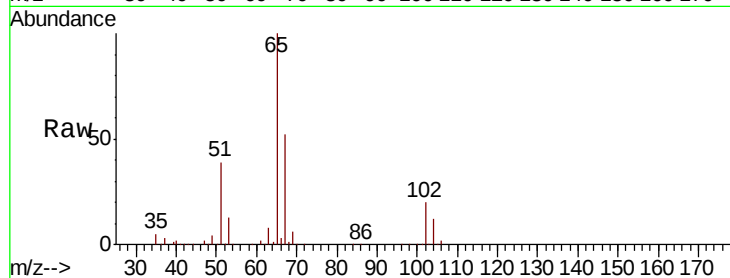

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 6.86 min Scan# 936
 Delta R.T. 0.00 min
 Lab File: VX009405.D
 Acq: 08 May 2019 17:54

Tgt Ion: 114 Resp: 285332
 Ion Ratio Lower Upper
 114 100
 63 22.8 0.0 45.6
 88 16.4 0.0 33.2


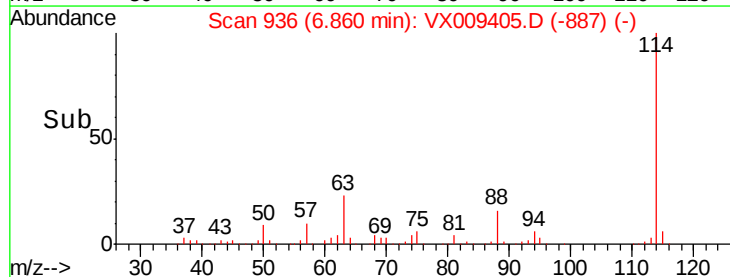
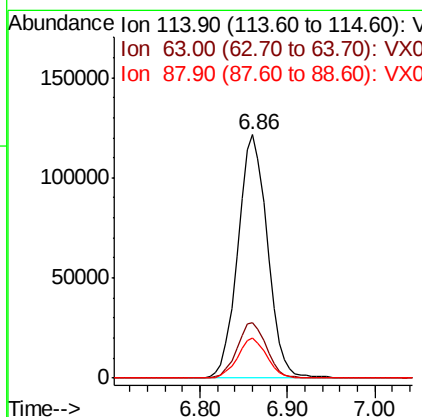
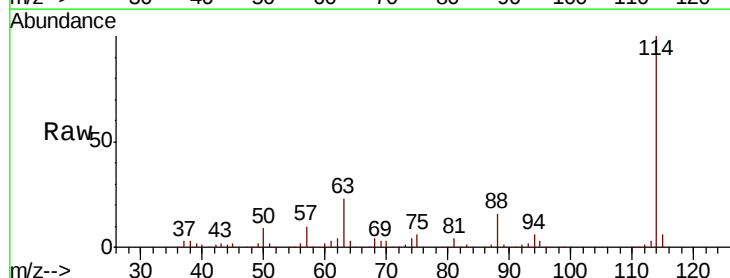


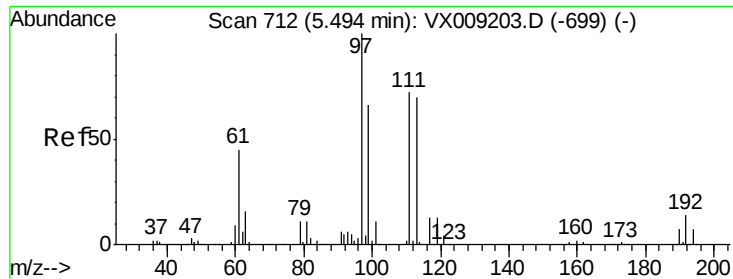

#35
 Dibromofluoromethane
 Concen: 48.491 ug/l
 RT: 5.50 min Scan# 713
 Delta R.T. 0.01 min
 Lab File: VX009405.D
 Acq: 08 May 2019 17:54




Instrument :
 MSVOA_X
 ClientSampleId :
 OR-03-050719-A


Tot Ion:113 Resp: 86979
 Ion Ratio Lower Upper
 113 100
 111 102.2 82.8 124.2
 192 21.6 17.0 25.6

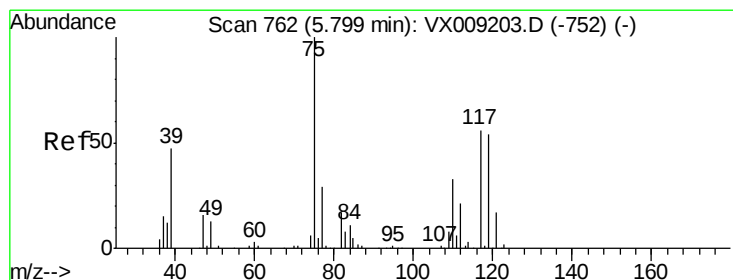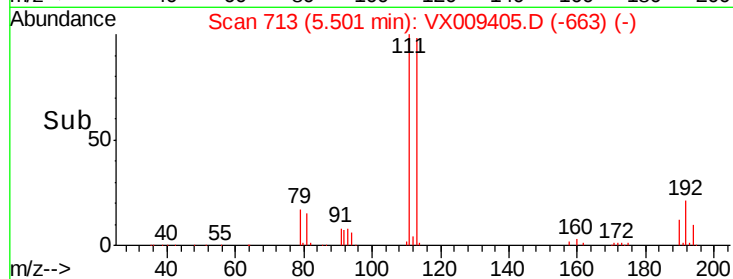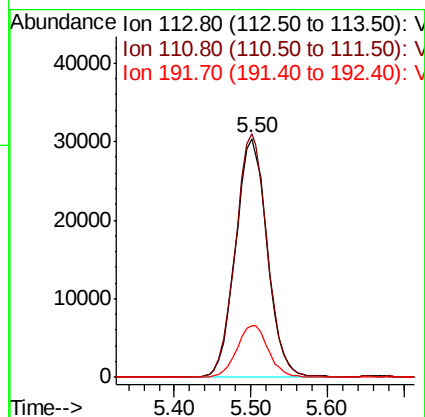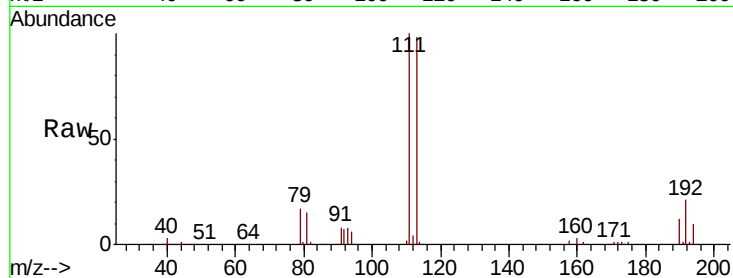

#36
 1,1-Dichloropropene
 Concen: 5.258 ug/l
 RT: 5.67 min Scan# 740
 Delta R.T. -0.13 min
 Lab File: VX009405.D
 Acq: 08 May 2019 17:54

Tgt Ion: 75 Resp: 13943
 Ion Ratio Lower Upper
 75 100
 110 8.7 16.9 50.6#
 77 0.5 24.8 37.2#

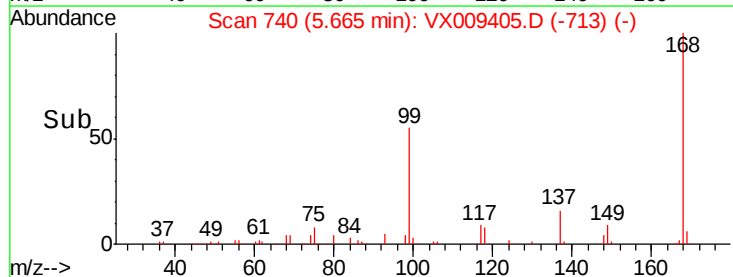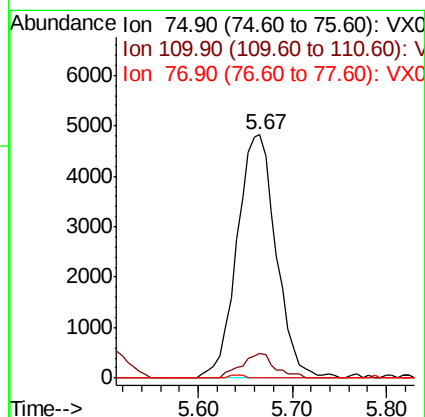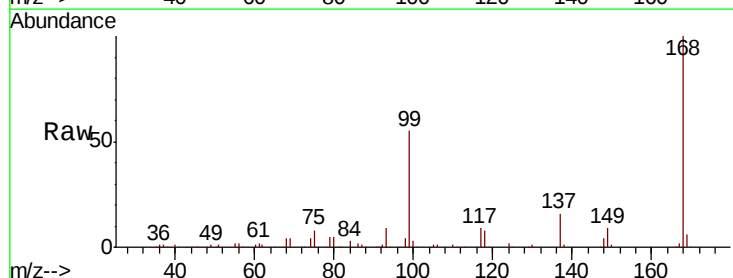


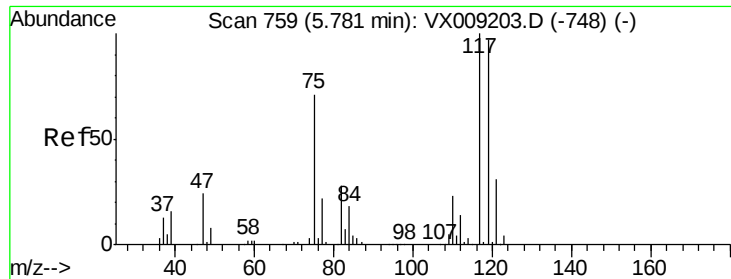




#38
Carbon Tetrachloride
Concen: 6.960 ug/l
RT: 5.66 min Scan# 739
Delta R.T. -0.12 min
Lab File: VX009405.D
Acq: 08 May 2019 17:54

Instrument :
MSVOA_X
ClientSampleId :
OR-03-050719-A

Tot Ion:117 Resp: 16767
Ion Ratio Lower Upper
117 100
119 5.1 77.5 116.3#
121 0.0 24.7 37.1#




Abundance Ion 116.80 (116.50 to 117.50): V
Ion 118.80 (118.50 to 119.50): V
Ion 120.80 (120.50 to 121.50): V


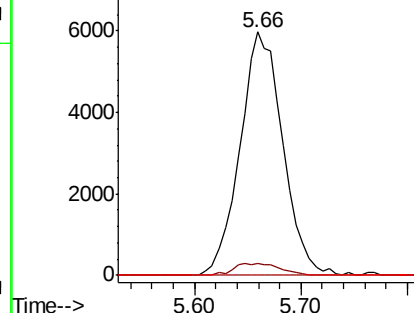



#43
Isopropyl Acetate
Concen: 2.092 ug/l
RT: 6.45 min Scan# 868
Delta R.T. 0.00 min
Lab File: VX009405.D
Acq: 08 May 2019 17:54

Tgt Ion: 43 Resp: 12364
Ion Ratio Lower Upper
43 100
61 19.6 15.1 22.7
87 11.8 9.0 13.6



Abundance Ion 43.00 (42.70 to 43.70): VX0
Ion 61.00 (60.70 to 61.70): VX0
Ion 87.00 (86.70 to 87.70): VX0




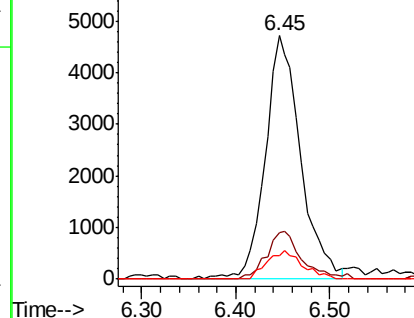


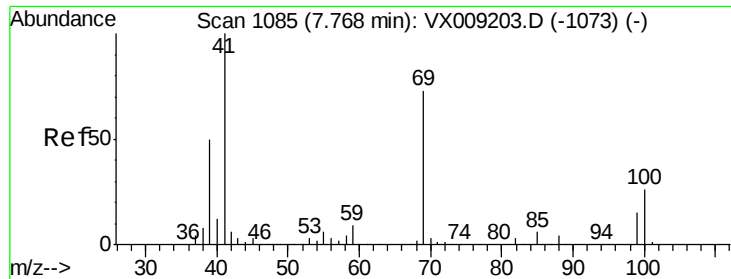

#48
Methvl methacrylate
Concen: 2.781 ug/l
RT: 7.68 min Scan# 1070
Delta R.T. -0.09 min
Lab File: VX009405.D
Acq: 08 May 2019 17:54




Instrument :
MSVOA_X
ClientSampleId :
OR-03-050719-A


Tot Ion: 41 Resp: 8153
Ion Ratio Lower Upper
41 100
69 0.2 59.1 88.7#
39 0.0 40.4 60.6#

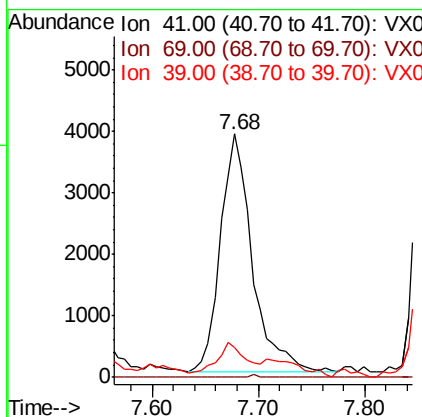

#49
1,4-Dioxane
Concen: 0.387 ug/l
RT: 7.73 min Scan# 1079
Delta R.T. -0.01 min
Lab File: VX009405.D
Acq: 08 May 2019 17:54

Tgt Ion: 88 Resp: 23
Ion Ratio Lower Upper
88 100
43 0.0 28.6 42.8#
58 2021.7 61.7 92.5#

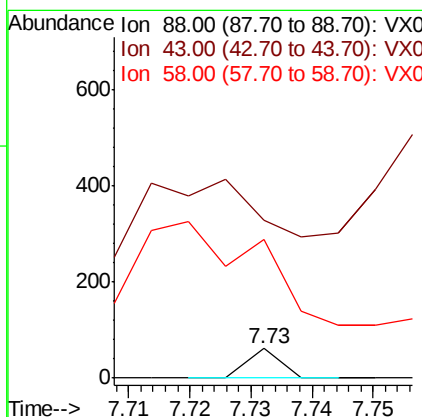

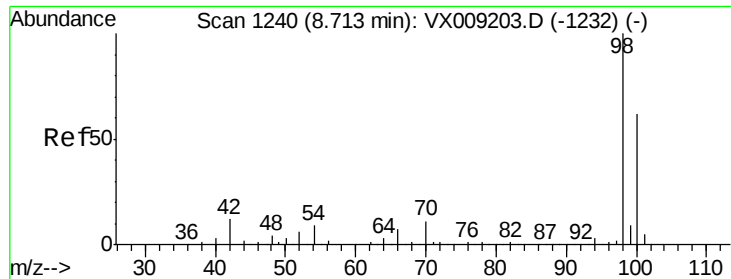

#50

Toluene-d8

Concen: 49.591 ug/l

RT: 8.71 min Scan# 1240

Delta R.T. 0.00 min

Lab File: VX009405.D

Acq: 08 May 2019 17:54

Instrument :

MSVOA_X

ClientSampleId :


OR-03-050719-A

Tot Ion: 98 Resp: 359121

Ion Ratio Lower Upper

98 100

100 63.8 51.2 76.8



Abundance Ion 98.00 (97.70 to 98.70): VX0

Ion 100.00 (99.70 to 100.70): VX

8.71

250000

200000



150000

100000

50000

0

Time--> 8.60 8.70 8.80



#51

4-Methyl-2-Pentanone

Concen: 22.829 ug/l

RT: 8.62 min Scan# 1224

Delta R.T. -0.02 min

Lab File: VX009405.D


Acq: 08 May 2019 17:54

Tgt Ion: 43 Resp: 88178

Ion Ratio Lower Upper

43 100

58 7.4 29.5 44.3#



Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0

8.62

60000

50000

40000


30000


20000

10000

0

Time--> 8.50 8.55 8.60 8.65 8.70





#54

cis-1,3-Dichloropropene

Concen: 11.369 ug/l

RT: 8.62 min Scan# 1224

Delta R.T. 0.18 min

Lab File: VX009405.D

Acq: 08 May 2019 17:54

Instrument :

MSVOA_X

ClientSampleId :

OR-03-050719-A


Tot Ion: 75 Resp: 38242

Ion Ratio Lower Upper

75 100

77 0.5 24.6 36.8#




39 26.5 40.6 60.8#



Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 76.90 (76.60 to 77.60): VX0

Ion 39.00 (38.70 to 39.70): VX0

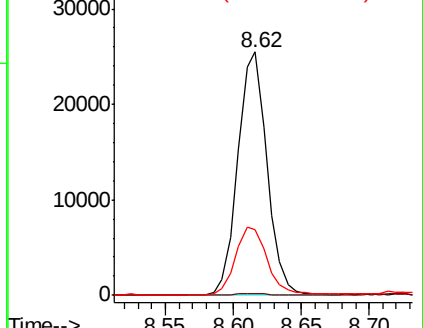

#57

1,3-Dichloropropane

Concen: 2.405 ug/l

RT: 9.54 min Scan# 1376

Delta R.T. 0.17 min

Lab File: VX009405.D


Acq: 08 May 2019 17:54

Tgt Ion: 76 Resp: 8614

Ion Ratio Lower Upper



76 100


78 0.3 25.5 38.3#



Abundance Ion 75.90 (75.60 to 76.60): VX0

Ion 77.90 (77.60 to 78.60): VX0




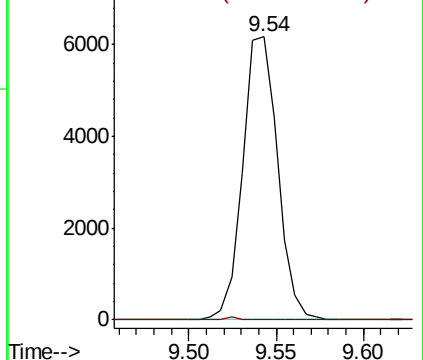




#59
2-Hexanone
Concen: 4.091 ug/l
RT: 9.44 min Scan# 1359
Delta R.T. -0.05 min
Lab File: VX009405.D
Acq: 08 May 2019 17:54




Instrument :
MSVOA_X
ClientSampleId :
OR-03-050719-A


Tot Ion: 43 Resp: 12411
Ion Ratio Lower Upper
43 100
58 0.0 25.9 77.7#

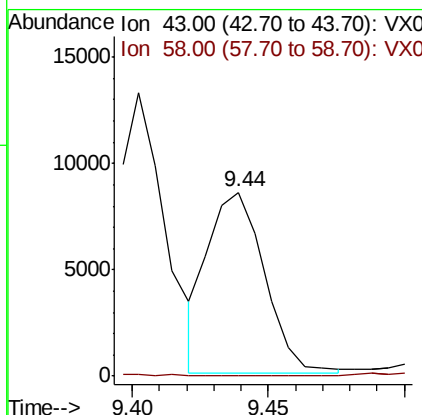

#62
4-Bromofluorobenzene
Concen: 43.756 ug/l
RT: 11.13 min Scan# 1637
Delta R.T. 0.00 min
Lab File: VX009405.D
Acq: 08 May 2019 17:54

Tgt Ion: 95 Resp: 115137
Ion Ratio Lower Upper
95 100
174 81.9 0.0 161.6
176 78.7 0.0 159.2

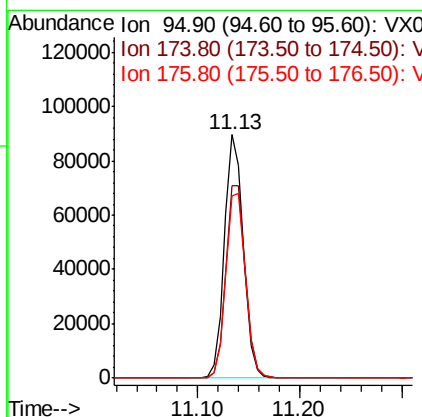


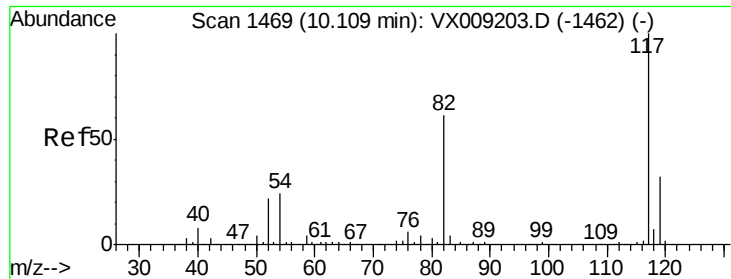




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.11 min Scan# 1469
Delta R.T. 0.00 min
Lab File: VX009405.D
Acq: 08 May 2019 17:54

Instrument :
MSVOA_X
ClientSampleId :
OR-03-050719-A

Tot Ion:117 Resp: 247426
Ion Ratio Lower Upper
117 100
82 59.8 48.8 73.2
119 31.8 25.8 38.6




Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): VX0
Ion 118.90 (118.60 to 119.60): V


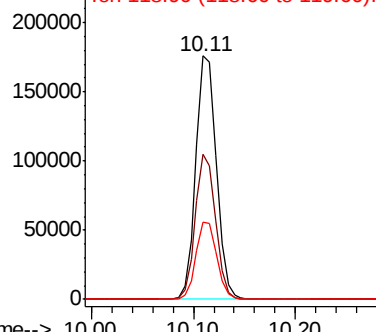



#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.08 min Scan# 1792
Delta R.T. 0.00 min
Lab File: VX009405.D
Acq: 08 May 2019 17:54

Tgt Ion:152 Resp: 97138
Ion Ratio Lower Upper
152 100
115 58.2 41.2 123.6
150 159.4 0.0 346.4



Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

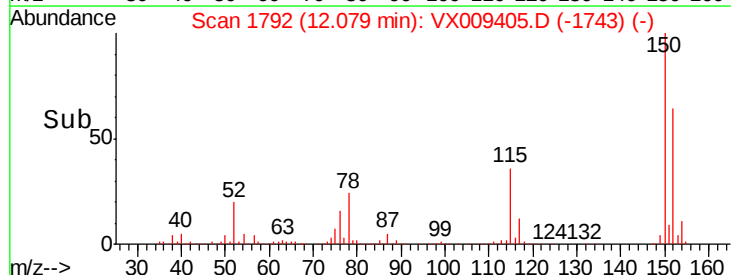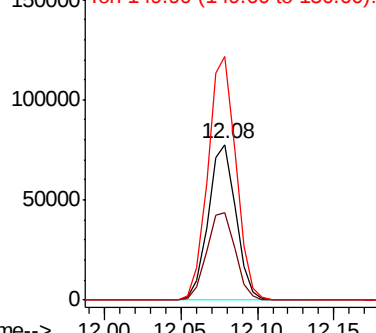

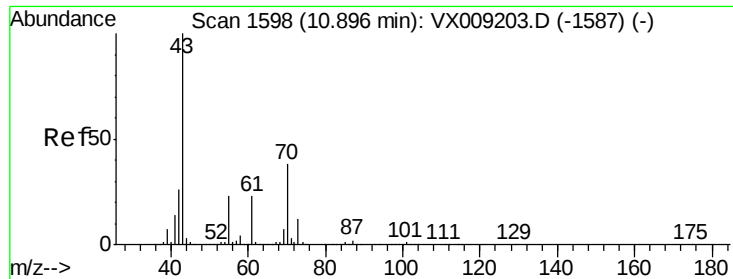

#74

N-amvl acetate

Concen: 3.293 ug/l

RT: 10.69 min Scan# 1565

Delta R.T. -0.20 min

Lab File: VX009405.D

Acq: 08 May 2019 17:54

Instrument :

MSVOA_X

ClientSampleId :

OR-03-050719-A

Tot Ion: 43 Resp: 13562


Ion Ratio Lower Upper

43 100

70 2.5 30.0 45.0#

55 5.1 17.9 26.9#

61 10.3 18.4 27.6#



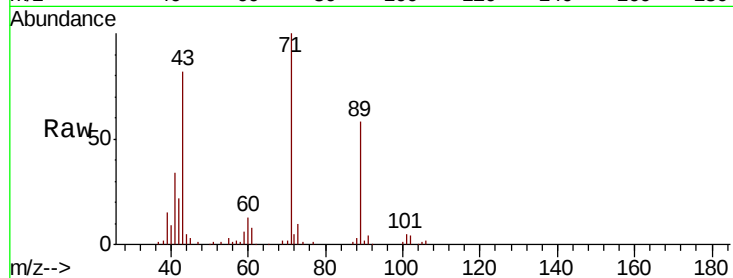


Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 70.00 (69.70 to 70.70): VX0

Ion 55.00 (54.70 to 55.70): VX0

Ion 61.00 (60.70 to 61.70): VX0

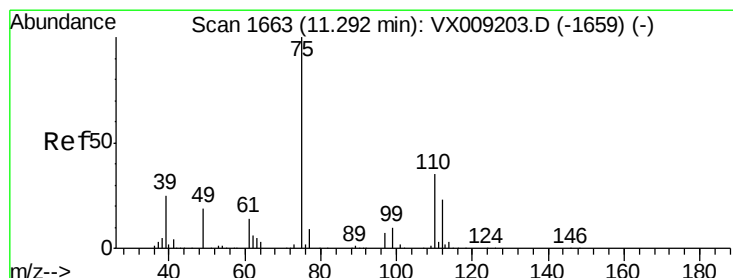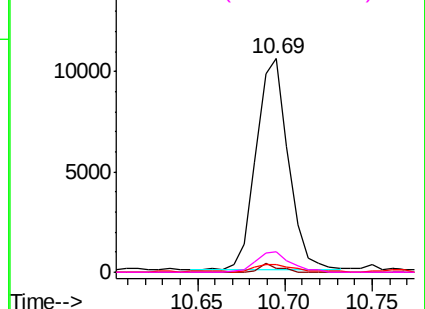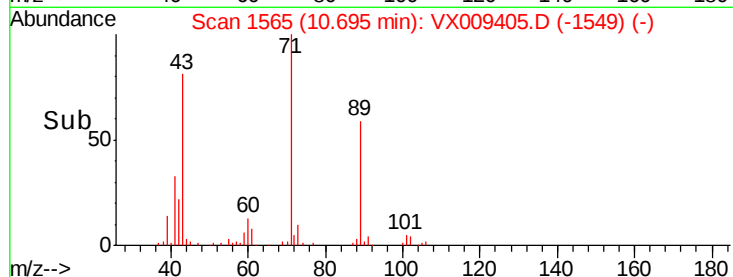

#76

1,2,3-Trichloropropane

Concen: 25.334 ug/l

RT: 11.13 min Scan# 1637

Delta R.T. -0.16 min

Lab File: VX009405.D


Acq: 08 May 2019 17:54

Tgt Ion: 75 Resp: 57084

Ion Ratio Lower Upper



75 100


77 1.3 22.1 66.1#

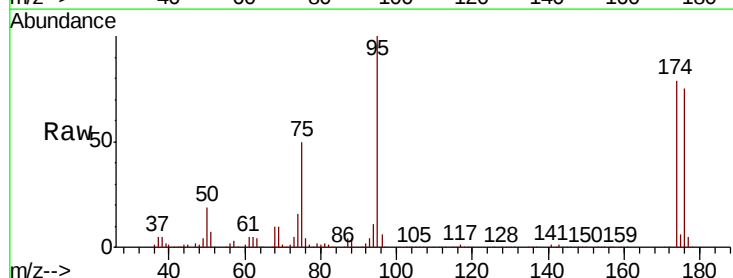

Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 77.00 (76.70 to 77.70): VX0



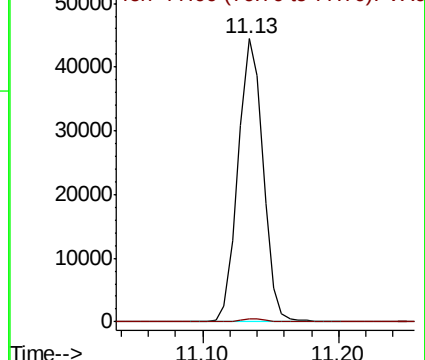
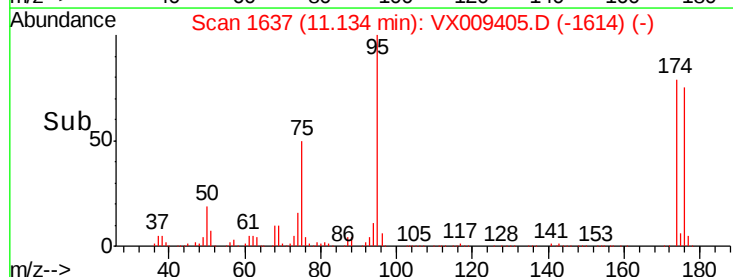




#80
 1,3,5-Trimethylbenzene
 Concen: 0.428 ug/l
 RT: 11.51 min Scan# 1698
 Delta R.T. 0.00 min
 Lab File: VX009405.D
 Acq: 08 May 2019 17:54




Instrument :
 MSVOA_X
 ClientSampleId :
 OR-03-050719-A


Tot Ion:105 Resp: 2546
 Ion Ratio Lower Upper
 105 100
 120 51.2 24.3 72.9

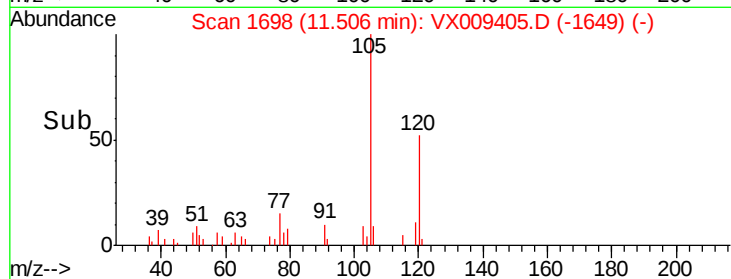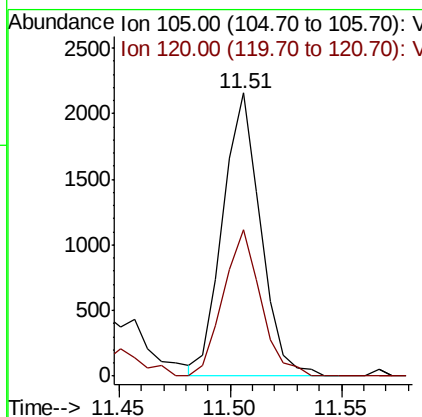

#81
 trans-1,4-Dichloro-2-butene
 Concen: 64.821 ug/l
 RT: 11.13 min Scan# 1637
 Delta R.T. 0.06 min
 Lab File: VX009405.D
 Acq: 08 May 2019 17:54

Tgt Ion: 75 Resp: 57084
 Ion Ratio Lower Upper
 75 100
 53 0.0 79.0 118.6#
 89 0.0 34.7 52.1#


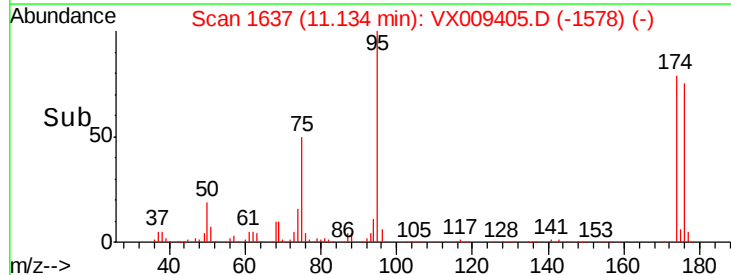
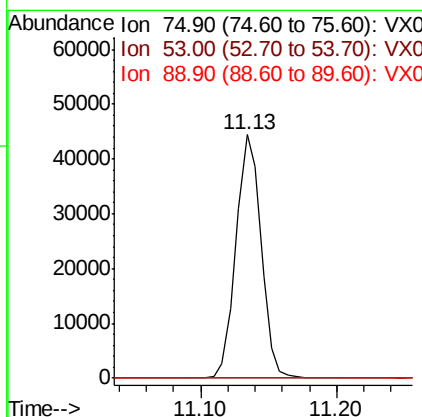



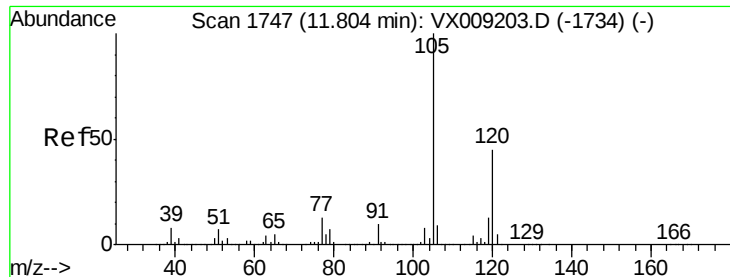

#84
 1,2,4-Trimethylbenzene
 Concen: 0.505 ug/l
 RT: 11.80 min Scan# 1747
 Delta R.T. 0.00 min
 Lab File: VX009405.D
 Acq: 08 May 2019 17:54

Instrument :
 MSVOA_X
 ClientSampleId :
 OR-03-050719-A

Tot Ion:105 Resp: 3014
 Ion Ratio Lower Upper
 105 100
 120 39.1 22.0 66.0

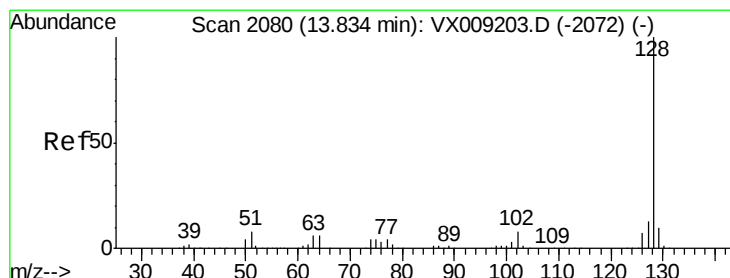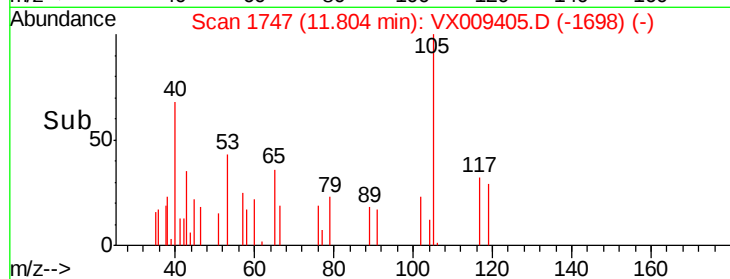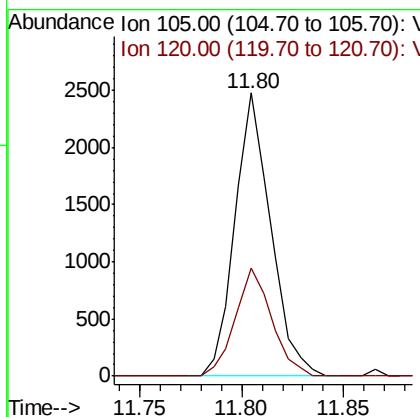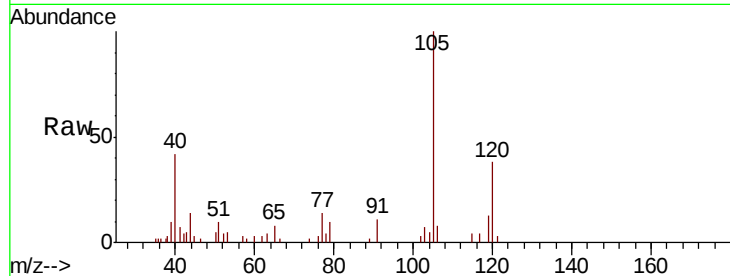

#95
 Naphthalene
 Concen: 1.983 ug/l
 RT: 13.83 min Scan# 2080
 Delta R.T. 0.00 min
 Lab File: VX009405.D
 Acq: 08 May 2019 17:54

Tgt Ion:128 Resp: 14047
 Ion Ratio Lower Upper
 128 100
 127 12.7 10.4 15.6
 129 11.8 8.6 13.0

