

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX050823\
 Data File : VX035552.D
 Acq On : 08 May 2023 12:03
 Operator : JC/MD
 Sample : VX0508MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0508MBL01

Quant Time: May 09 03:40:23 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X042523W.M
 Quant Title : SW846 8260
 QLast Update : Tue Apr 25 16:31:40 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	262933	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	428600	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	395090	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	184751	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	155229	48.935	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery =	97.880%		
35) Dibromofluoromethane	5.385	113	134426	51.100	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	102.200%		
50) Toluene-d8	8.647	98	504019	50.790	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery =	101.580%		
62) 4-Bromofluorobenzene	11.079	95	193978	51.962	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	103.920%		
Target Compounds						
					Qvalue	
13) Acrolein	2.239	56	348	0.613	ug/l #	63
15) Acrylonitrile	3.075	53	453	0.314	ug/l #	20
16) Acetone	2.398	43	911	0.661	ug/l	92
17) Carbon Disulfide	2.514	76	3811	0.623	ug/l	96
20) Methylene Chloride	2.794	84	1864	0.590	ug/l	88
21) trans-1,2-Dichloroethene	3.099	96	586	0.211	ug/l #	66
29) Tetrahydrofuran	5.044	42	265	0.206	ug/l #	34
31) Cyclohexane	5.550	56	4943	1.098	ug/l #	1
36) 1,1-Dichloropropene	5.556	75	19296	4.698	ug/l #	51
38) Carbon Tetrachloride	5.544	117	25216	6.467	ug/l #	16
68) m/p-Xylenes	10.299	106	1552	0.274	ug/l	97
76) 1,2,3-Trichloropropane	11.079	75	93583	25.393	ug/l #	35
78) n-propylbenzene	11.305	91	4315	0.278	ug/l	95
79) 2-Chlorotoluene	11.366	91	2507	0.259	ug/l	95
80) 1,3,5-Trimethylbenzene	11.451	105	2924	0.257	ug/l	88
81) trans-1,4-Dichloro-2-b...	11.079	75	93583	82.244	ug/l #	8
82) 4-Chlorotoluene	11.457	91	3105	0.285	ug/l	99
83) tert-Butylbenzene	11.713	119	3031	0.265	ug/l	93
84) 1,2,4-Trimethylbenzene	11.756	105	3288	0.287	ug/l	96
85) sec-Butylbenzene	11.890	105	4201	0.300	ug/l	96
86) p-Isopropyltoluene	12.012	119	3752	0.315	ug/l	82
87) 1,3-Dichlorobenzene	11.969	146	2402	0.377	ug/l	94
88) 1,4-Dichlorobenzene	11.969	146	2402	0.359	ug/l	93
89) n-Butylbenzene	12.335	91	4308	0.428	ug/l	94
90) Hexachloroethane	12.536	117	561	0.307	ug/l	96
91) 1,2-Dichlorobenzene	12.341	146	2235	0.350	ug/l	93
93) 1,2,4-Trichlorobenzene	13.591	180	3404	0.849	ug/l	97
94) Hexachlorobutadiene	13.725	225	3362	1.910	ug/l	93
95) Naphthalene	13.780	128	9720	0.787	ug/l	99
96) 1,2,3-Trichlorobenzene	13.963	180	4068	1.008	ug/l	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: May 09 03:40:23 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X042523W.M
Quant Title : SW846 8260
QLast Update : Tue Apr 25 16:31:40 2023
Response via : Initial Calibration









#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. 0.001 min
Lab File: VX035552.D
Acq: 08 May 2023 12:03




Instrument :
MSVOA_X
ClientSampleId :
VX0508MBL01


Tgt Ion:168 Resp: 262933
Ion Ratio Lower Upper
168 100
99 56.2 45.7 68.5

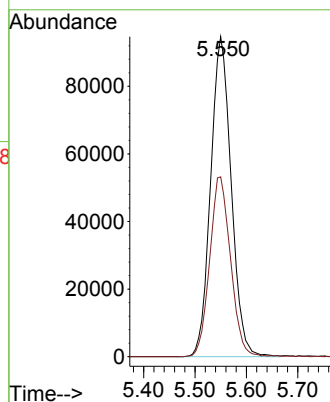

#13
Acrolein
Concen: 0.613 ug/l
RT: 2.239 min Scan# 189
Delta R.T. 0.000 min
Lab File: VX035552.D
Acq: 08 May 2023 12:03


Tgt Ion: 56 Resp: 348
Ion Ratio Lower Upper
56 100
55 101.4 56.6 85.0#

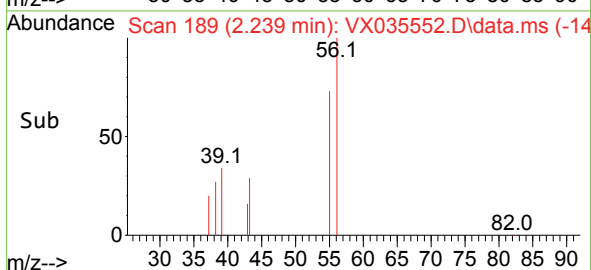






#15
Acrylonitrile
Concen: 0.314 ug/l
RT: 3.075 min Scan# 31
Delta R.T. 0.007 min
Lab File: VX035552.D
Acq: 08 May 2023 12:03


Instrument :
MSVOA_X
ClientSampleId :
VX0508MBL01





Tgt Ion: 53 Resp: 453
Ion Ratio Lower Upper
53 100
52 169.8 66.2 99.2#
51 59.8 28.3 42.5#

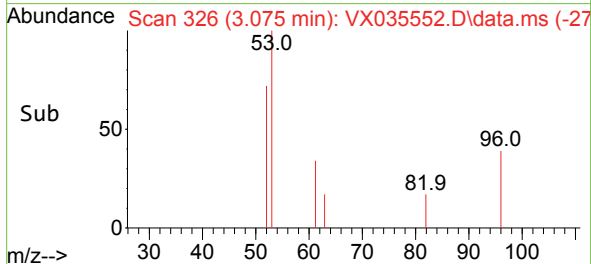


#16
Acetone
Concen: 0.661 ug/l
RT: 2.398 min Scan# 215
Delta R.T. -0.000 min
Lab File: VX035552.D
Acq: 08 May 2023 12:03

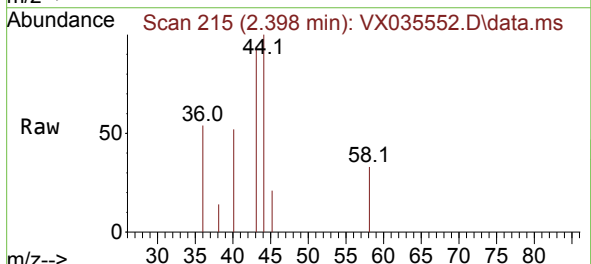

Tgt Ion: 43 Resp: 911
Ion Ratio Lower Upper
43 100
58 35.3 24.7 37.1



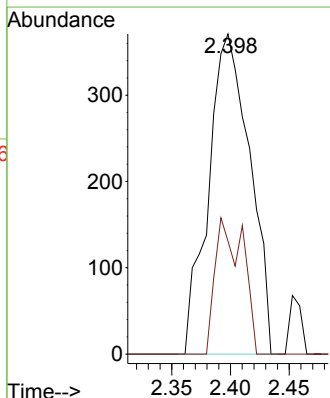





#17
Carbon Disulfide
Concen: 0.623 ug/l
RT: 2.514 min Scan# 21
Delta R.T. 0.001 min
Lab File: VX035552.D
Acq: 08 May 2023 12:03




Instrument :
MSVOA_X
ClientSampleId :
VX0508MBL01


Tgt Ion: 76 Resp: 3811
Ion Ratio Lower Upper
76 100
78 10.3 7.2 10.8

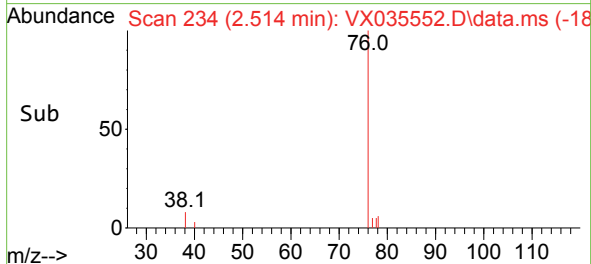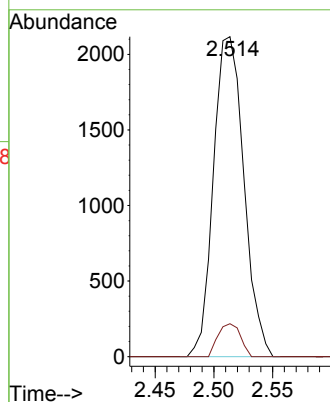

#20
Methylene Chloride
Concen: 0.590 ug/l
RT: 2.794 min Scan# 280
Delta R.T. 0.006 min
Lab File: VX035552.D
Acq: 08 May 2023 12:03

Tgt Ion: 84 Resp: 1864
Ion Ratio Lower Upper
84 100
49 111.9 103.8 155.8
51 33.3 31.8 47.8
86 60.6 51.4 77.2


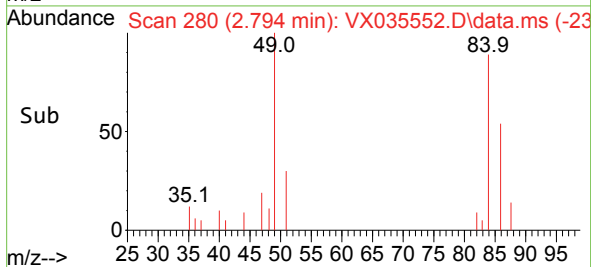

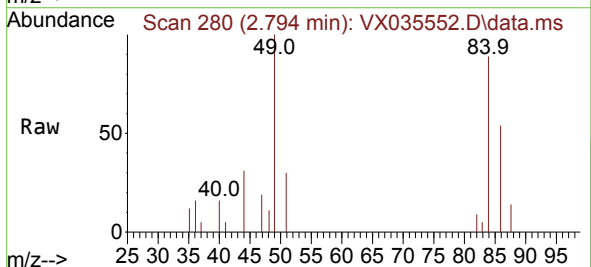


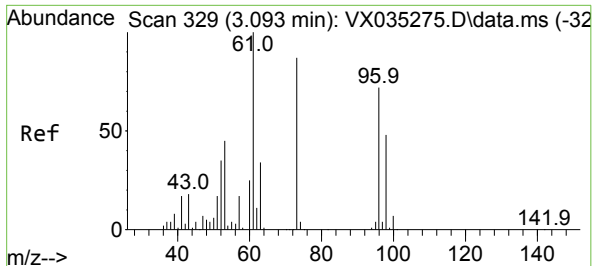

#21
trans-1,2-Dichloroethene
Concen: 0.211 ug/l
RT: 3.099 min Scan# 311
Delta R.T. 0.006 min
Lab File: VX035552.D
Acq: 08 May 2023 12:03




Instrument :
MSVOA_X
ClientSampleId :
VX0508MBL01


Tgt Ion: 96 Resp: 586
Ion Ratio Lower Upper
96 100
61 91.4 113.0 169.6#
98 49.2 52.1 78.1#

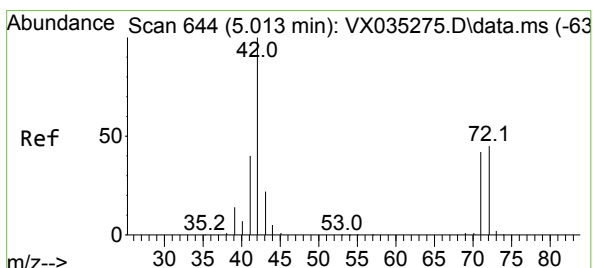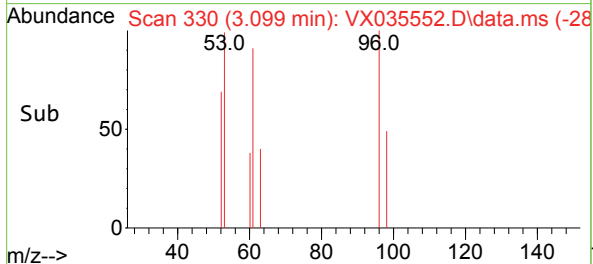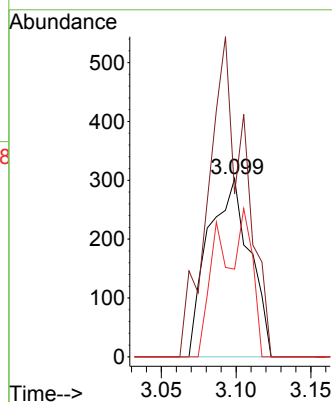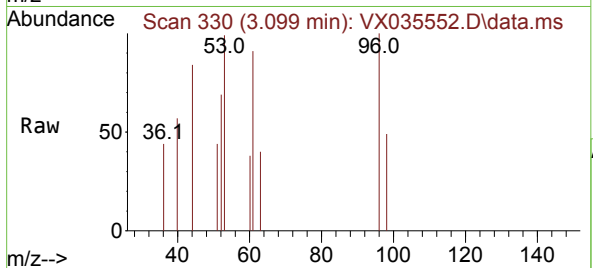

#29
Tetrahydrofuran
Concen: 0.206 ug/l
RT: 5.044 min Scan# 649
Delta R.T. 0.031 min
Lab File: VX035552.D
Acq: 08 May 2023 12:03

Tgt Ion: 42 Resp: 265
Ion Ratio Lower Upper
42 100
72 0.0 34.5 51.7#
71 0.0 32.1 48.1#


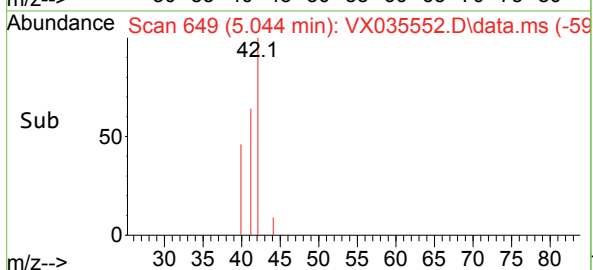
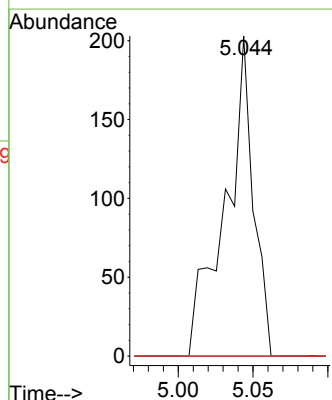
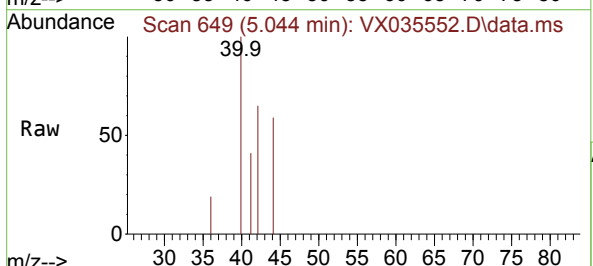


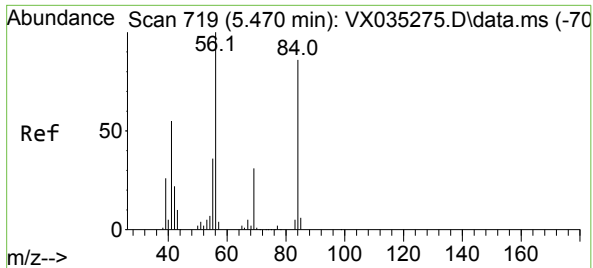

#31
Cyclohexane
Concen: 1.098 ug/l
RT: 5.550 min Scan# 719
Delta R.T. 0.080 min
Lab File: VX035552.D
Acq: 08 May 2023 12:03




Instrument :
MSVOA_X
ClientSampleId :
VX0508MBL01


Tgt Ion: 56 Resp: 4943
Ion Ratio Lower Upper
56 100
69 215.6 23.7 35.5#
84 170.1 68.5 102.7#

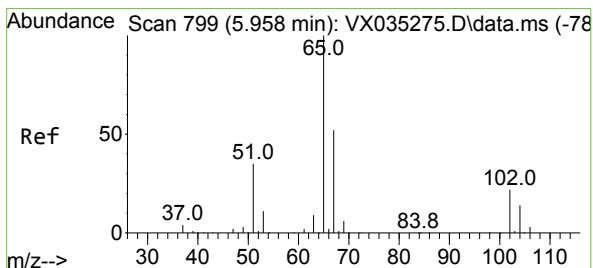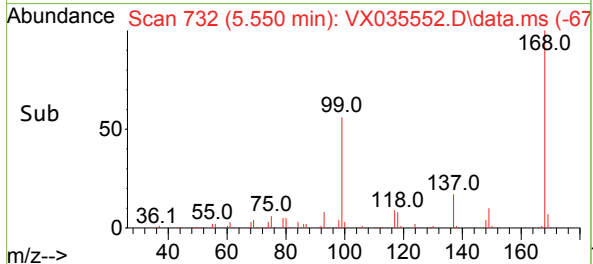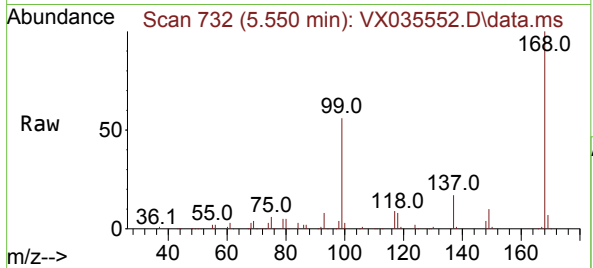

#33
1,2-Dichloroethane-d4
Concen: 48.935 ug/l
RT: 5.952 min Scan# 798
Delta R.T. -0.006 min
Lab File: VX035552.D
Acq: 08 May 2023 12:03

Tgt Ion: 65 Resp: 155229
Ion Ratio Lower Upper
65 100
67 52.3 0.0 104.0


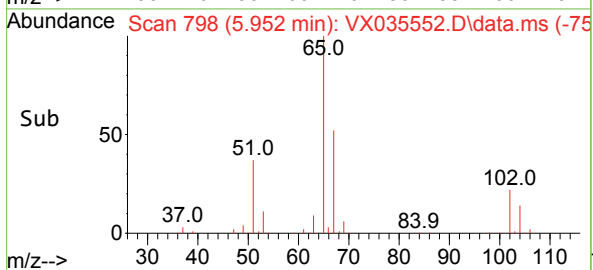

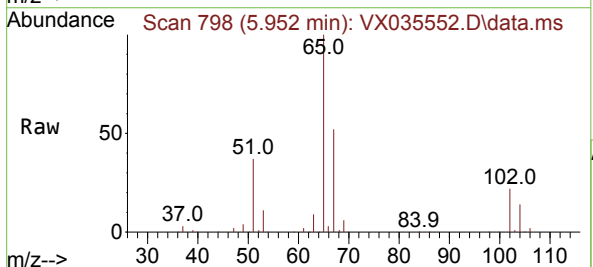




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.757 min Scan# 91
Delta R.T. -0.006 min
Lab File: VX035552.D
Acq: 08 May 2023 12:03




Instrument :
MSVOA_X
ClientSampleId :
VX0508MBL01


Tgt Ion:114 Resp: 428600
Ion Ratio Lower Upper
114 100
63 19.0 0.0 42.2
88 16.6 0.0 33.2

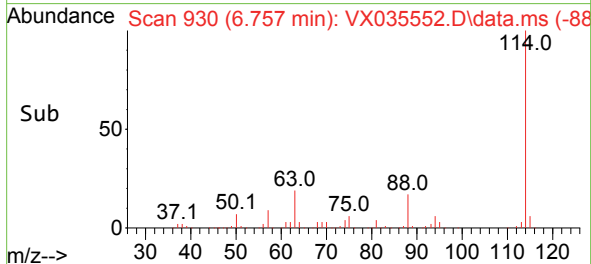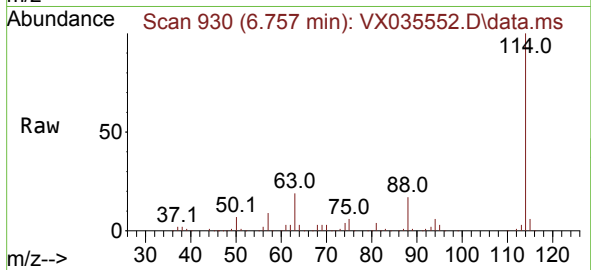

#35
Dibromofluoromethane
Concen: 51.100 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.000 min
Lab File: VX035552.D
Acq: 08 May 2023 12:03

Tgt Ion:113 Resp: 134426
Ion Ratio Lower Upper
113 100
111 102.2 83.7 125.5
192 20.9 15.4 23.2


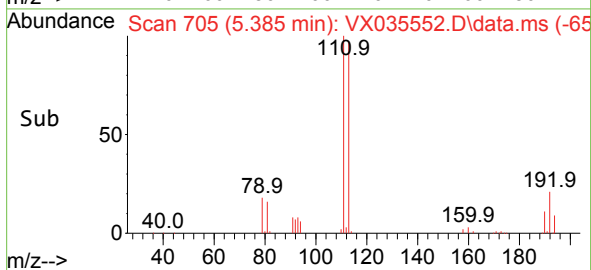

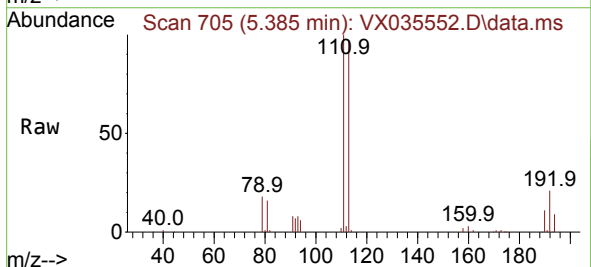




#36
1,1-Dichloropropene
Concen: 4.698 ug/l
RT: 5.556 min Scan# 711
Delta R.T. -0.134 min
Lab File: VX035552.D
Acq: 08 May 2023 12:03




Instrument :
MSVOA_X
ClientSampleId :
VX0508MBL01


Tgt Ion: 75 Resp: 19296
Ion Ratio Lower Upper
75 100
110 9.5 17.5 52.5#
77 0.0 24.3 36.5#

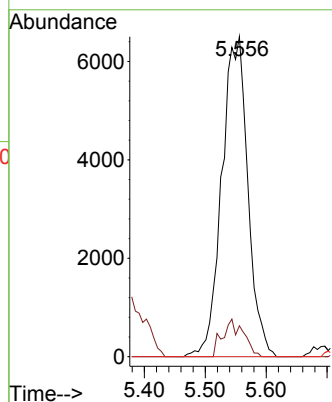

#38
Carbon Tetrachloride
Concen: 6.467 ug/l
RT: 5.544 min Scan# 731
Delta R.T. -0.133 min
Lab File: VX035552.D
Acq: 08 May 2023 12:03

Tgt Ion: 117 Resp: 25216
Ion Ratio Lower Upper
117 100
119 4.6 76.6 114.8#
121 0.0 23.8 35.6#


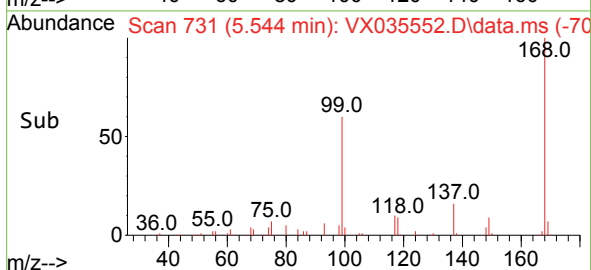
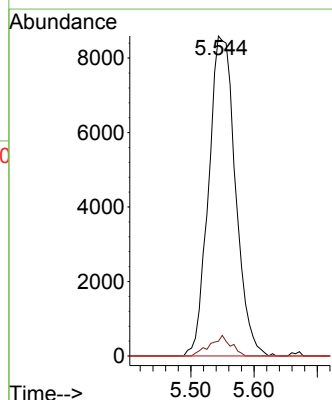





#50
Toluene-d8
Concen: 50.790 ug/l
RT: 8.647 min Scan# 1240
Delta R.T. 0.001 min
Lab File: VX035552.D
Acq: 08 May 2023 12:03




Instrument :
MSVOA_X
ClientSampleId :
VX0508MBL01


Tgt Ion: 98 Resp: 504019
Ion Ratio Lower Upper
98 100
100 66.9 52.5 78.7

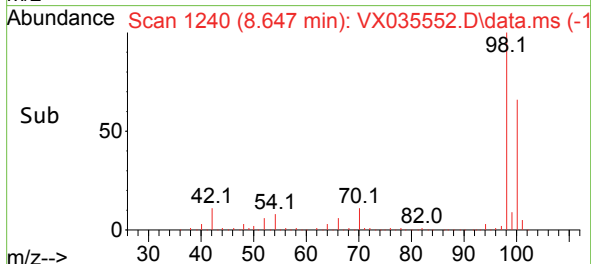

#62
4-Bromofluorobenzene
Concen: 51.962 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX035552.D
Acq: 08 May 2023 12:03

Tgt Ion: 95 Resp: 193978
Ion Ratio Lower Upper
95 100
174 78.4 0.0 147.4
176 77.4 0.0 140.6


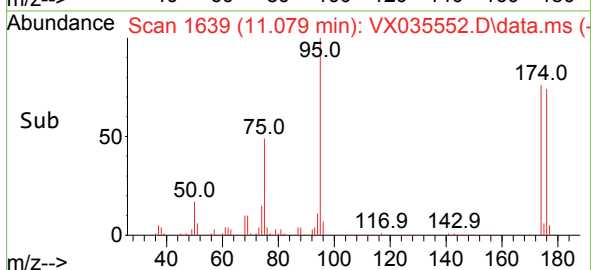






#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX035552.D
Acq: 08 May 2023 12:03




Instrument :
MSVOA_X
ClientSampleId :
VX0508MBL01


Tgt Ion:117 Resp: 395090
Ion Ratio Lower Upper
117 100
82 54.7 45.0 67.4
119 32.6 26.0 39.0

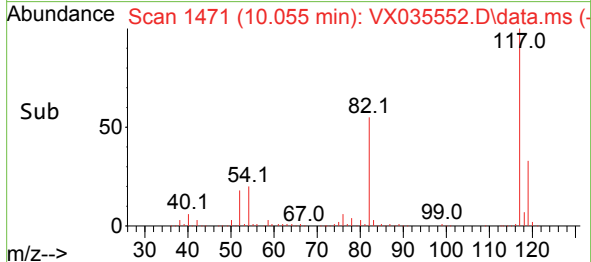

#68
m/p-Xylenes
Concen: 0.274 ug/l
RT: 10.299 min Scan# 1511
Delta R.T. -0.000 min
Lab File: VX035552.D
Acq: 08 May 2023 12:03

Tgt Ion:106 Resp: 1552
Ion Ratio Lower Upper
106 100
91 200.1 164.0 246.0

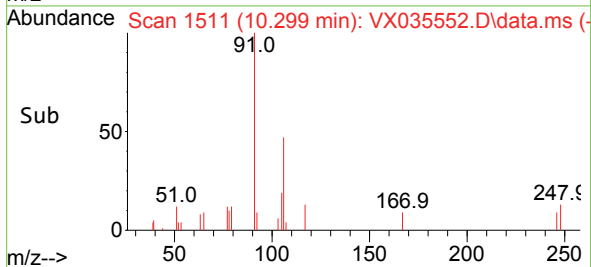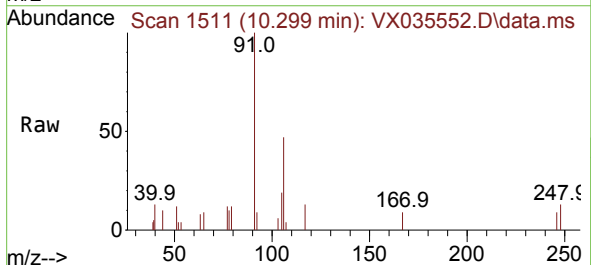



#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.024 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX035552.D

Acq: 08 May 2023 12:03

Instrument :

MSVOA_X

ClientSampleId :

VX0508MBL01





Tgt Ion:152 Resp: 184751

Ion Ratio Lower Upper

152 100

115 60.1 45.0 135.0

150 157.7 0.0 352.4

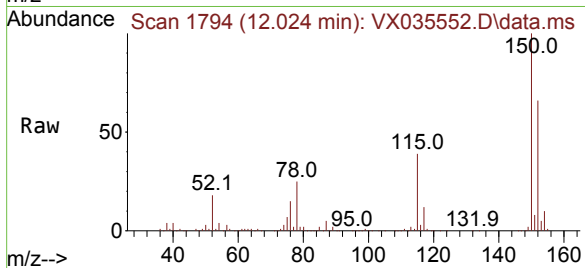

#76

1,2,3-Trichloropropane

Concen: 25.393 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. -0.158 min

Lab File: VX035552.D




Acq: 08 May 2023 12:03


Tgt Ion: 75 Resp: 93583

Ion Ratio Lower Upper

75 100

77 1.2 21.6 64.8#


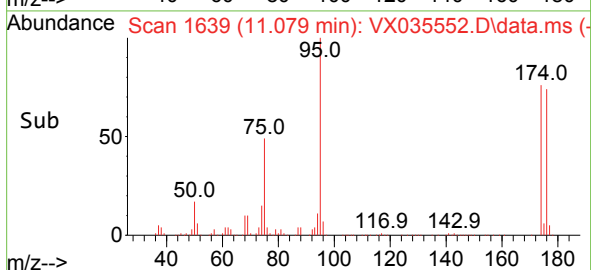

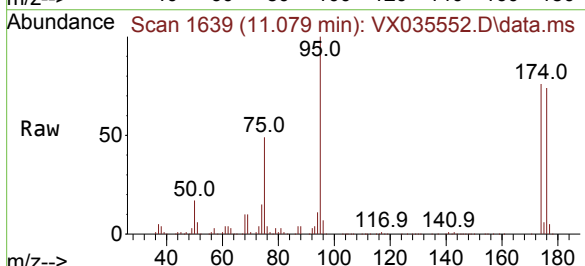




#78
n-propylbenzene
Concen: 0.278 ug/l
RT: 11.305 min Scan# 1676
Delta R.T. 0.001 min
Lab File: VX035552.D
Acq: 08 May 2023 12:03




Instrument :
MSVOA_X
ClientSampleId :
VX0508MBL01


Tgt Ion: 91 Resp: 4315
Ion Ratio Lower Upper
91 100
120 20.4 11.5 34.5

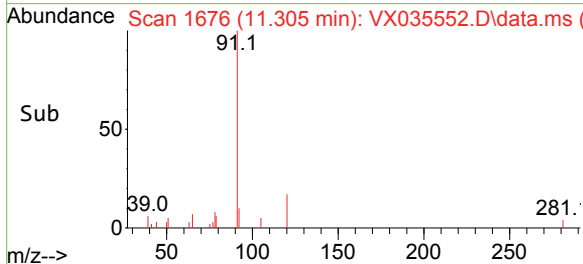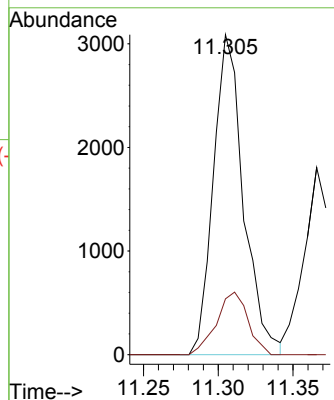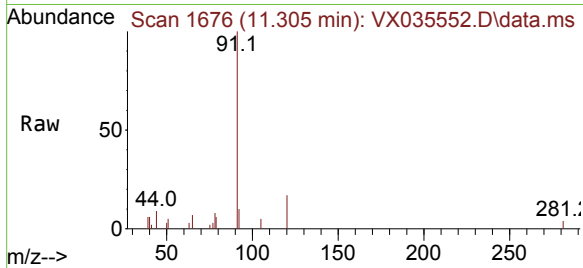

#79
2-Chlorotoluene
Concen: 0.259 ug/l
RT: 11.366 min Scan# 1686
Delta R.T. 0.001 min
Lab File: VX035552.D
Acq: 08 May 2023 12:03

Tgt Ion: 91 Resp: 2507
Ion Ratio Lower Upper
91 100
126 29.8 16.3 48.9

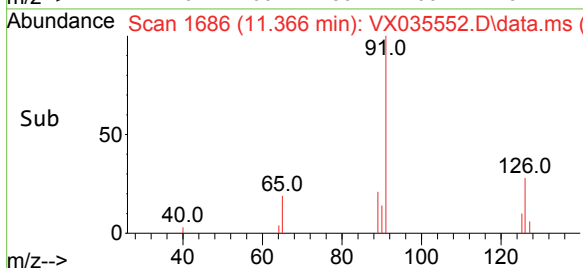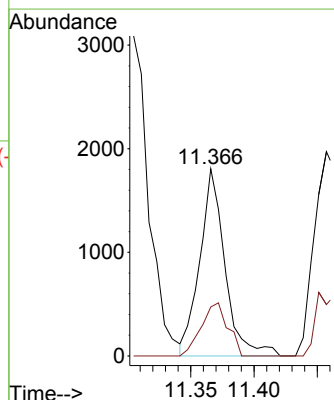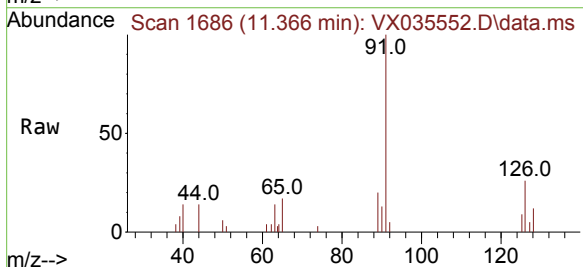



#80

1,3,5-Trimethylbenzene

Concen: 0.257 ug/l

RT: 11.451 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX035552.D

Acq: 08 May 2023 12:03

Instrument :

MSVOA_X

ClientSampleId :





VX0508MBL01

Tgt Ion:105 Resp: 2924

Ion Ratio Lower Upper

105 100

120 55.5 23.7 71.1

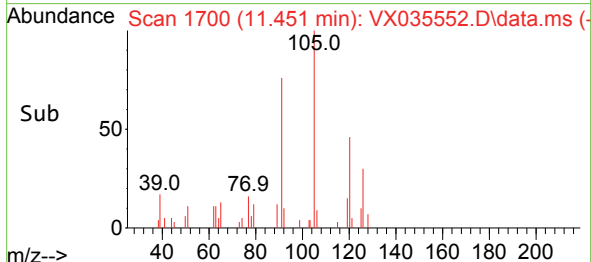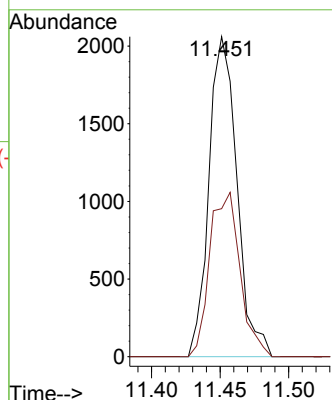

#81

trans-1,4-Dichloro-2-butene

Concen: 82.244 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. 0.061 min

Lab File: VX035552.D

Acq: 08 May 2023 12:03




Tgt Ion: 75 Resp: 93583


Ion Ratio Lower Upper

75 100

53 0.0 82.6 124.0#

89 0.0 36.9 55.3#

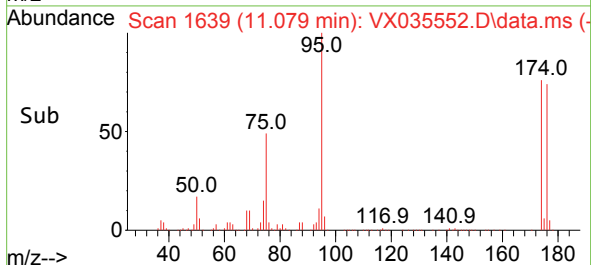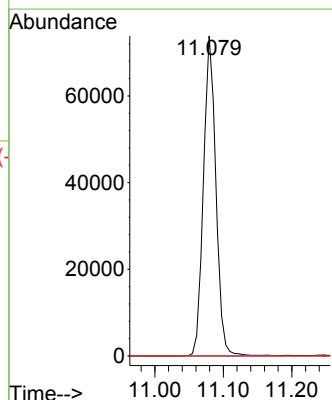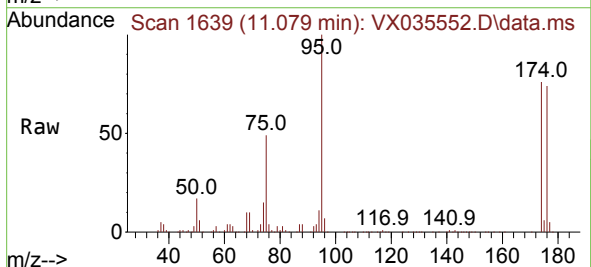



#82

4-Chlorotoluene

Concen: 0.285 ug/l

RT: 11.457 min Scan# 1701

Delta R.T. 0.006 min

Lab File: VX035552.D

Acq: 08 May 2023 12:03

Instrument :

MSVOA_X

ClientSampleId :





VX0508MBL01

Tgt Ion: 91 Resp: 3105

Ion Ratio Lower Upper

91 100

126 29.0 14.2 42.6

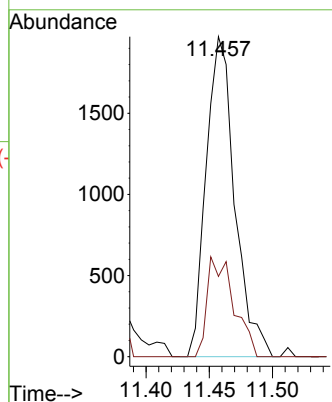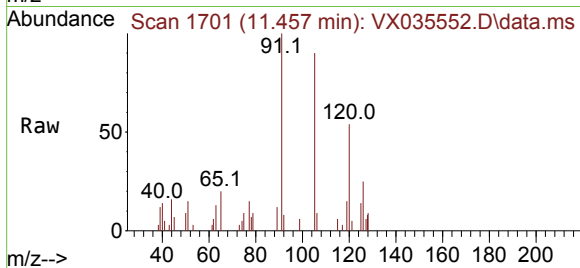

#83

tert-Butylbenzene

Concen: 0.265 ug/l

RT: 11.713 min Scan# 1743

Delta R.T. 0.000 min

Lab File: VX035552.D

Acq: 08 May 2023 12:03




Tgt Ion: 119 Resp: 3031


Ion Ratio Lower Upper

119 100

91 67.0 30.6 92.0

134 25.8 11.8 35.4


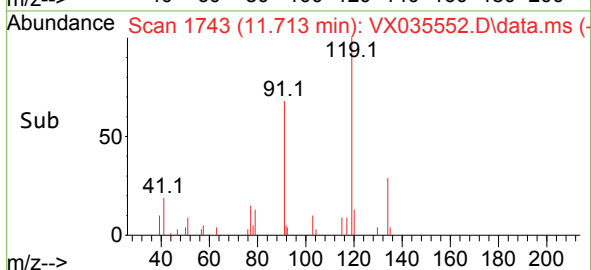
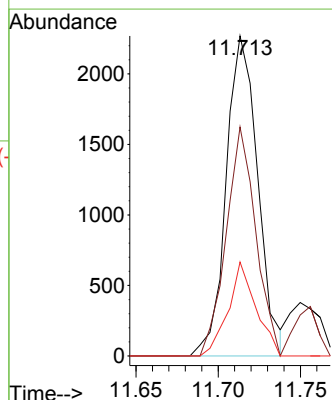
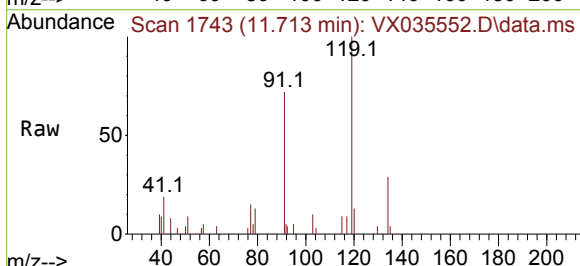




#84
1,2,4-Trimethylbenzene
Concen: 0.287 ug/l
RT: 11.756 min Scan# 11750
Delta R.T. 0.007 min
Lab File: VX035552.D
Acq: 08 May 2023 12:03




Instrument :
MSVOA_X
ClientSampleId :
VX0508MBL01


Tgt Ion:105 Resp: 3288
Ion Ratio Lower Upper
105 100
120 42.3 22.4 67.0

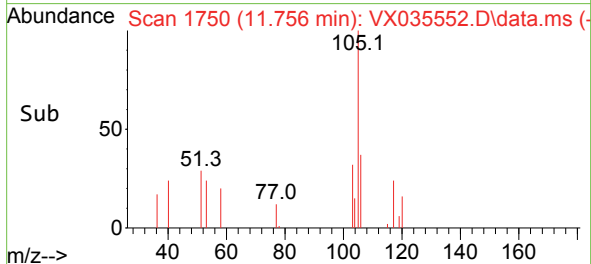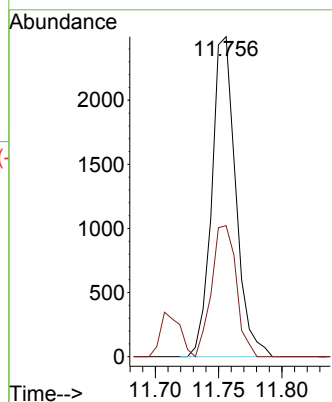

#85
sec-Butylbenzene
Concen: 0.300 ug/l
RT: 11.890 min Scan# 1772
Delta R.T. 0.000 min
Lab File: VX035552.D
Acq: 08 May 2023 12:03

Tgt Ion:105 Resp: 4201
Ion Ratio Lower Upper
105 100
134 22.1 10.2 30.4

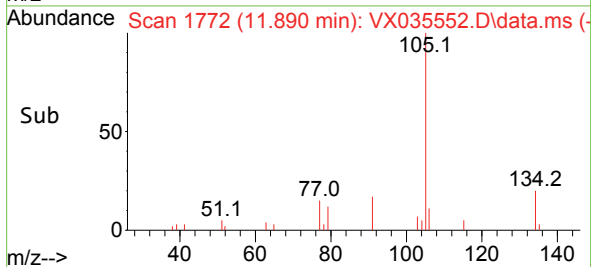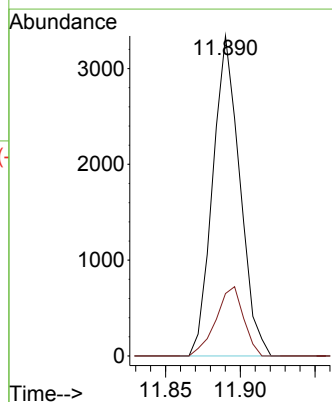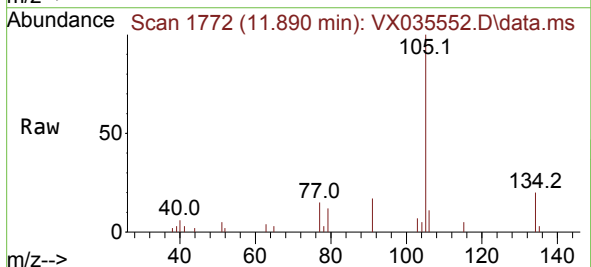



#86

p-Isopropyltoluene

Concen: 0.315 ug/l

RT: 12.012 min Scan# 1

Delta R.T. 0.006 min

Lab File: VX035552.D

Acq: 08 May 2023 12:03

Instrument :

MSVOA_X

ClientSampleId :

VX0508MBL01





Tgt Ion:119 Resp: 3752

Ion Ratio Lower Upper

119 100

134 32.8 13.2 39.5

91 37.4 12.9 38.7

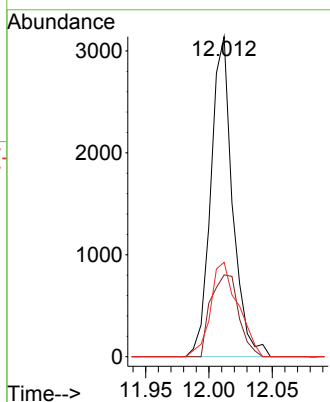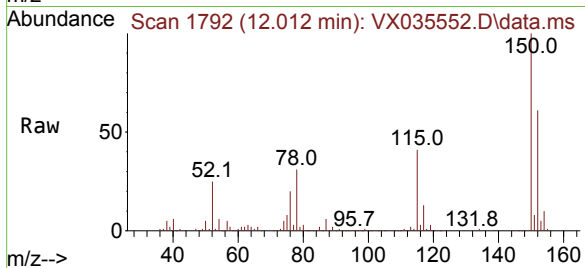

#87

1,3-Dichlorobenzene

Concen: 0.377 ug/l

RT: 11.969 min Scan# 1785

Delta R.T. 0.000 min

Lab File: VX035552.D

Acq: 08 May 2023 12:03




Tgt Ion:146 Resp: 2402


Ion Ratio Lower Upper

146 100

111 41.9 20.9 62.8

148 71.6 31.6 95.0


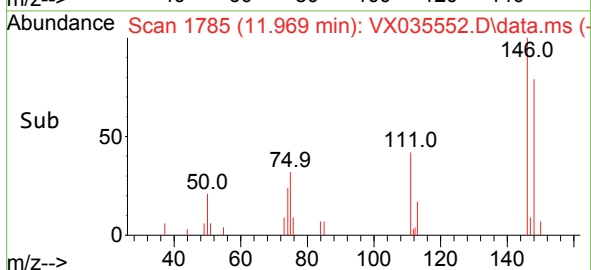

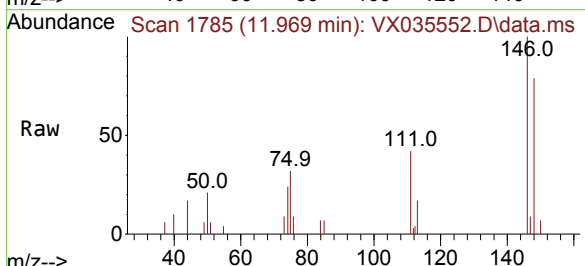




#88
1,4-Dichlorobenzene
Concen: 0.359 ug/l
RT: 11.969 min Scan# 1785
Delta R.T. -0.073 min
Lab File: VX035552.D
Acq: 08 May 2023 12:03




Instrument :
MSVOA_X
ClientSampleId :
VX0508MBL01


Tgt Ion:146 Resp: 2402
Ion Ratio Lower Upper
146 100
111 41.9 20.6 61.9
148 71.6 31.8 95.4

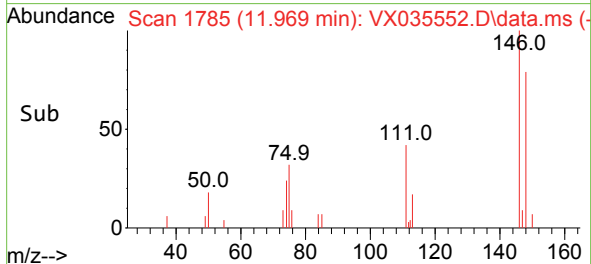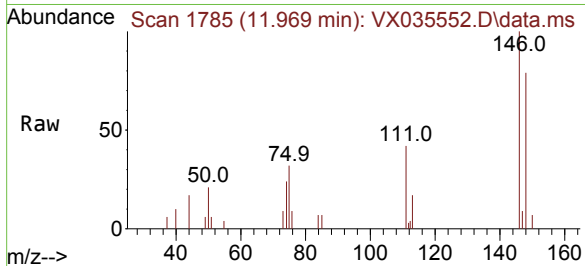

#89
n-Butylbenzene
Concen: 0.428 ug/l
RT: 12.335 min Scan# 1845
Delta R.T. 0.000 min
Lab File: VX035552.D
Acq: 08 May 2023 12:03

Tgt Ion: 91 Resp: 4308
Ion Ratio Lower Upper
91 100
92 59.1 27.7 83.0
134 30.4 13.0 38.9


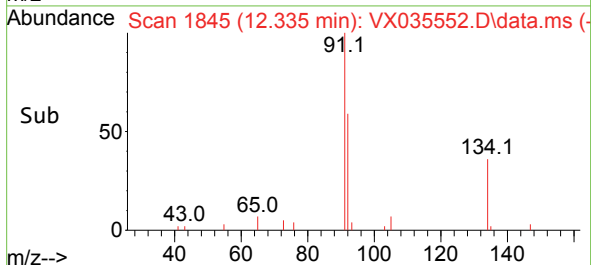
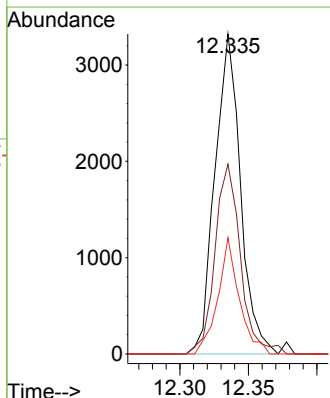
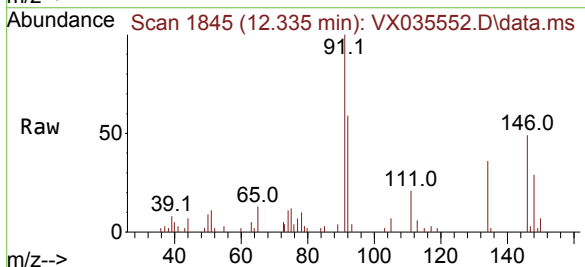




#90
Hexachloroethane
Concen: 0.307 ug/l
RT: 12.536 min Scan# 117
Delta R.T. 0.000 min
Lab File: VX035552.D
Acq: 08 May 2023 12:03




Instrument :
MSVOA_X
ClientSampleId :
VX0508MBL01


Tgt Ion:117 Resp: 561
Ion Ratio Lower Upper
117 100
201 72.2 34.4 103.1

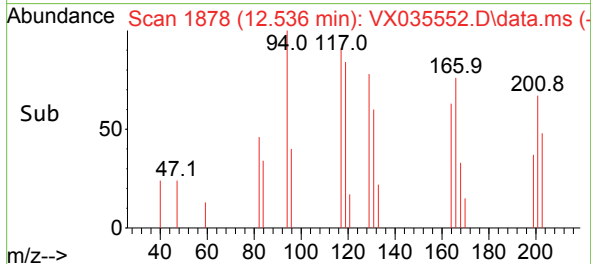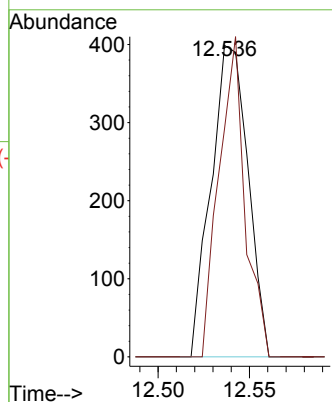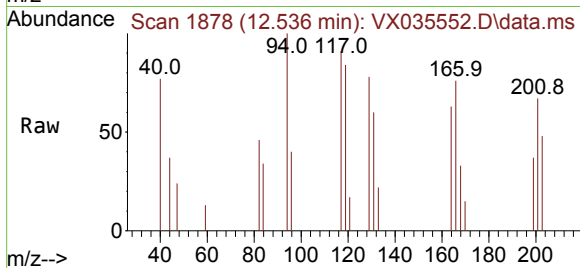

#91
1,2-Dichlorobenzene
Concen: 0.350 ug/l
RT: 12.341 min Scan# 1846
Delta R.T. 0.006 min
Lab File: VX035552.D
Acq: 08 May 2023 12:03

Tgt Ion:146 Resp: 2235
Ion Ratio Lower Upper
146 100
111 49.5 22.0 66.0
148 60.0 32.0 96.0


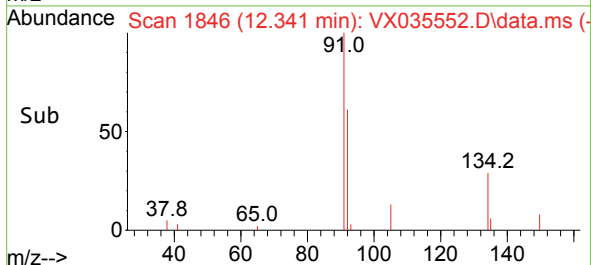
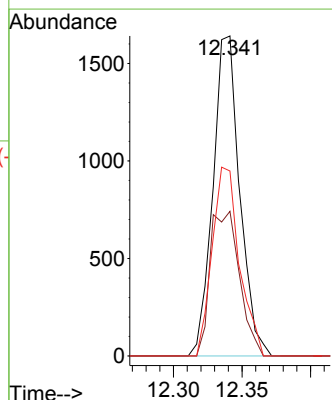
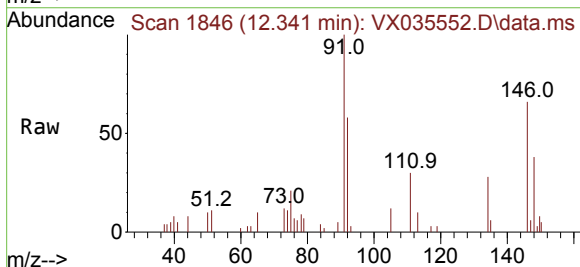




#93
1,2,4-Trichlorobenzene
Concen: 0.849 ug/l
RT: 13.591 min Scan# 2051
Delta R.T. 0.006 min
Lab File: VX035552.D
Acq: 08 May 2023 12:03




Instrument :
MSVOA_X
ClientSampleId :
VX0508MBL01


Tgt Ion:180 Resp: 3404
Ion Ratio Lower Upper
180 100
182 96.3 47.0 141.0
145 34.9 15.9 47.7

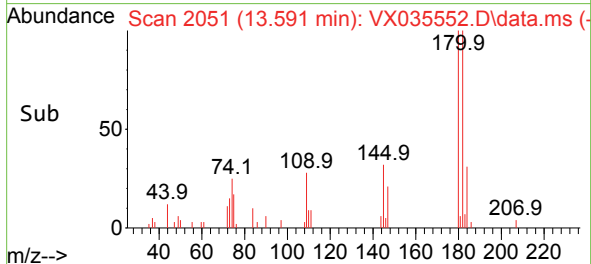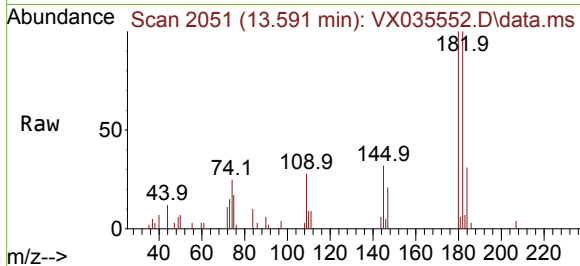

#94
Hexachlorobutadiene
Concen: 1.910 ug/l
RT: 13.725 min Scan# 2073
Delta R.T. 0.000 min
Lab File: VX035552.D
Acq: 08 May 2023 12:03

Tgt Ion:225 Resp: 3362
Ion Ratio Lower Upper
225 100
223 61.8 32.1 96.5
227 55.9 31.8 95.4



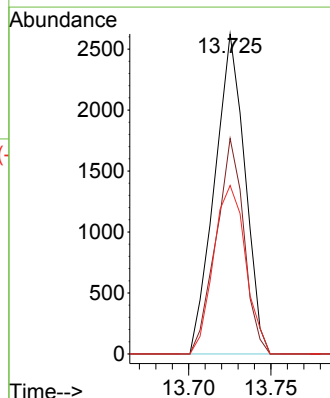
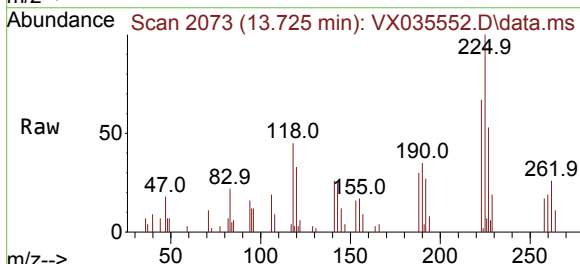




#95
Naphthalene
Concen: 0.787 ug/l
RT: 13.780 min Scan# 2081
Delta R.T. 0.006 min
Lab File: VX035552.D
Acq: 08 May 2023 12:03

Instrument :
MSVOA_X
ClientSampleId :
VX0508MBL01

Tgt Ion:128 Resp: 9720
Ion Ratio Lower Upper
128 100
127 13.4 10.2 15.4
129 11.0 8.6 13.0

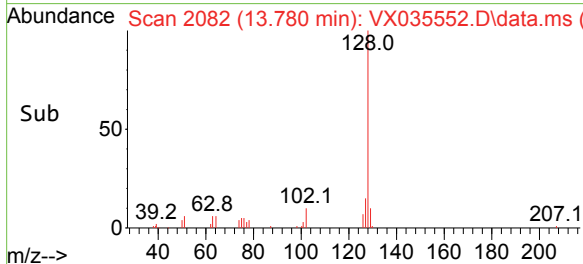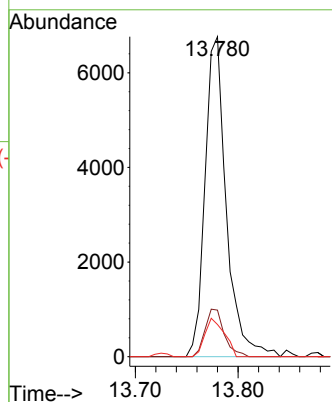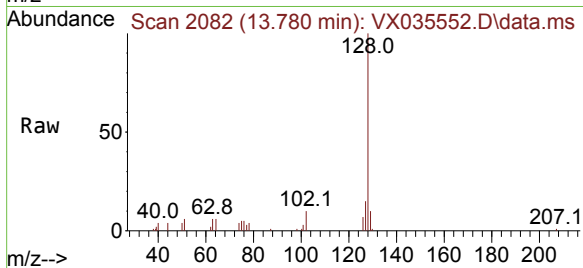

#96
1,2,3-Trichlorobenzene
Concen: 1.008 ug/l
RT: 13.963 min Scan# 2112
Delta R.T. -0.000 min
Lab File: VX035552.D
Acq: 08 May 2023 12:03

Tgt Ion:180 Resp: 4068
Ion Ratio Lower Upper
180 100
182 89.3 48.0 144.2
145 34.5 17.7 53.1

