

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX050823\
 Data File : VX035553.D
 Acq On : 08 May 2023 12:26
 Operator : JC/MD
 Sample : VX0508WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0508WBL01

Quant Time: May 09 03:40:50 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X042523W.M
 Quant Title : SW846 8260
 QLast Update : Tue Apr 25 16:31:40 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.549	168	266155	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	440786	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	403085	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	190678	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	156507	48.741	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	97.480%
35) Dibromofluoromethane	5.385	113	134671	49.778	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	99.560%
50) Toluene-d8	8.646	98	512110	50.179	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	100.360%
62) 4-Bromofluorobenzene	11.079	95	197707	51.497	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	103.000%


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX050823\
Data File : VX035553.D
Acq On : 08 May 2023 12:26
Operator : JC/MD
Sample : VX0508WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0508WBL01

Quant Time: May 09 03:40:50 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X042523W.M
Quant Title : SW846 8260
QLast Update : Tue Apr 25 16:31:40 2023
Response via : Initial Calibration




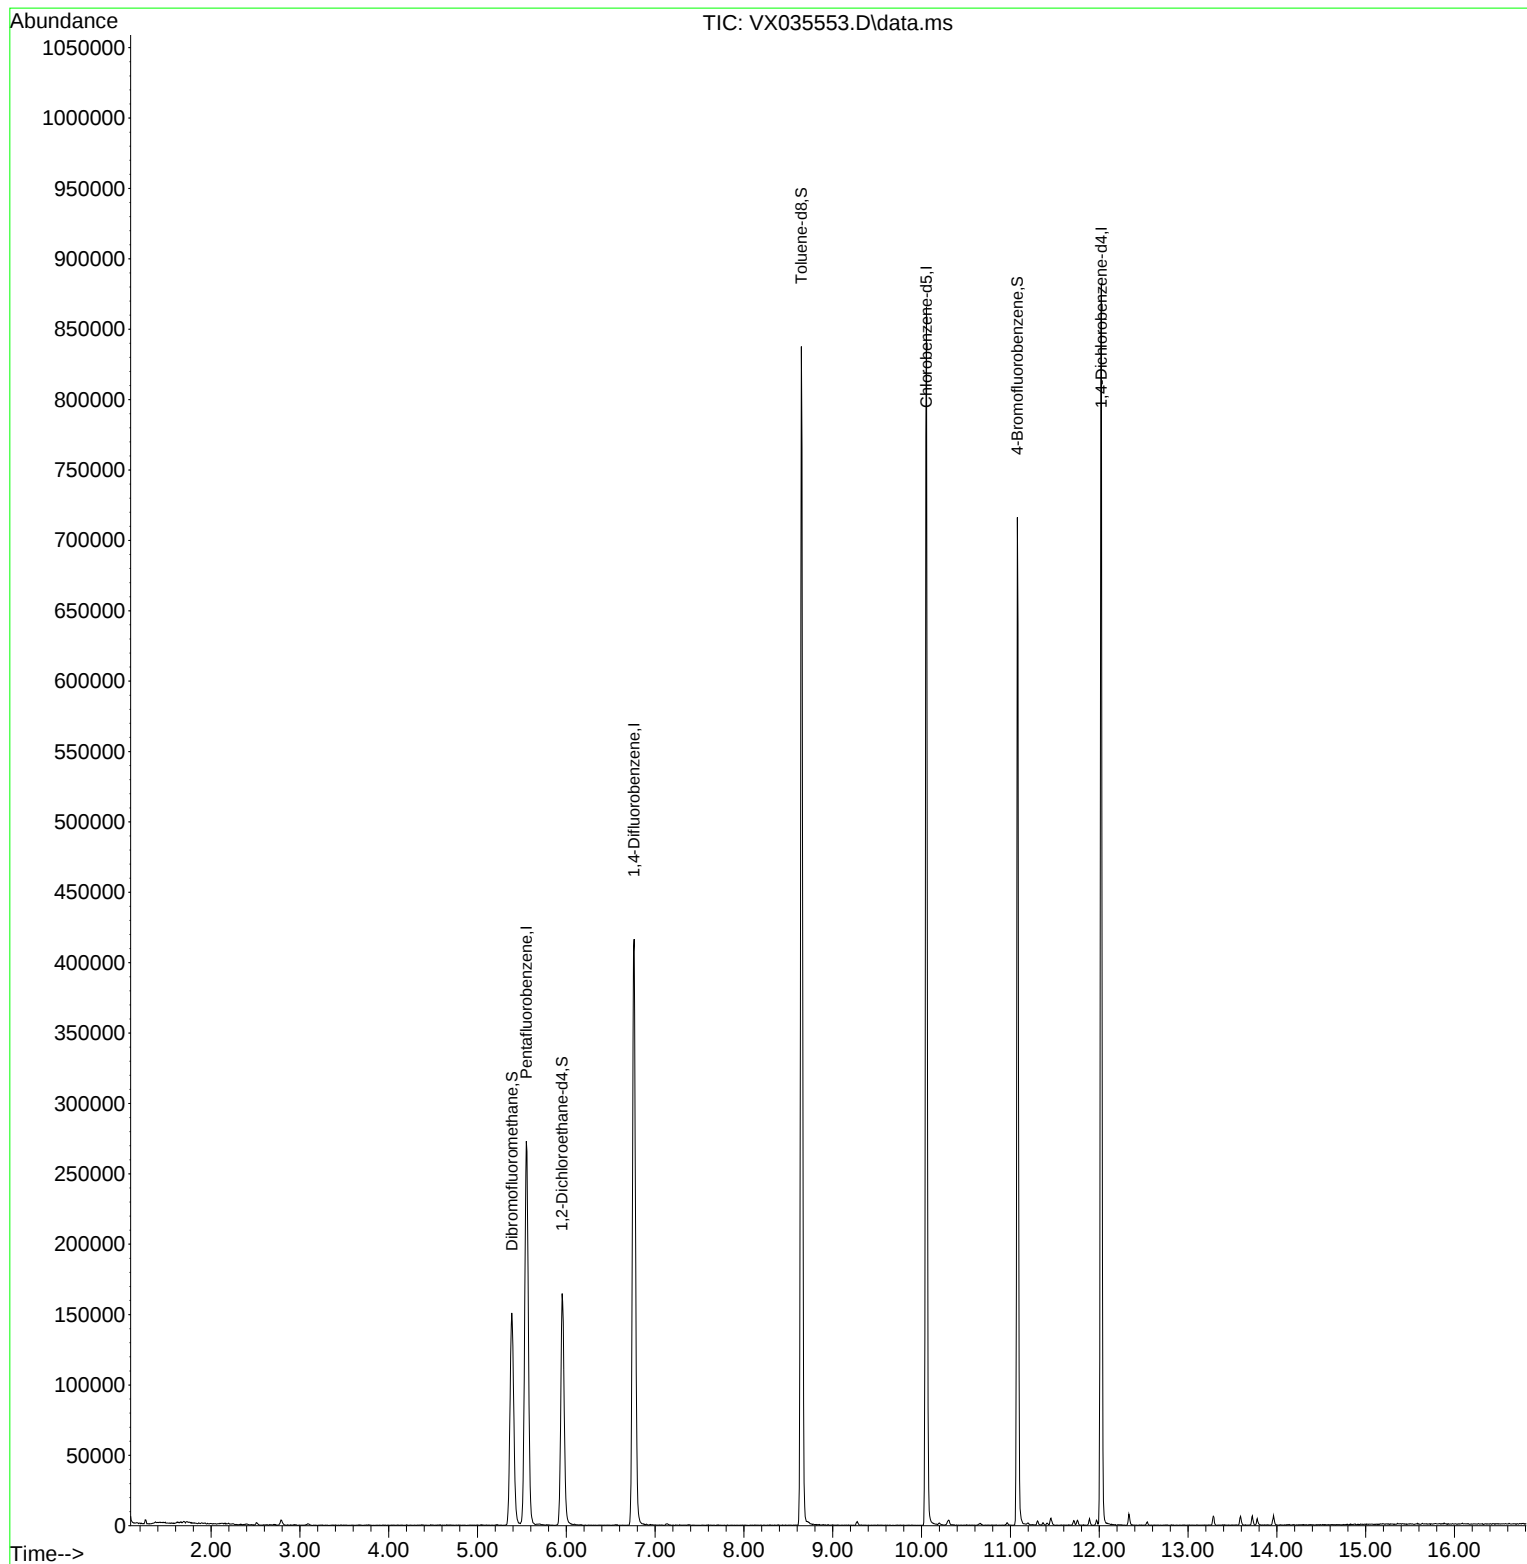




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.549 min Scan# 71
Delta R.T. 0.000 min
Lab File: VX035553.D
Acq: 08 May 2023 12:26




Instrument :
MSVOA_X
ClientSampleId :
VX0508WBL01

Tgt Ion:168 Resp: 266155
Ion Ratio Lower Upper
168 100
99 56.9 45.7 68.5

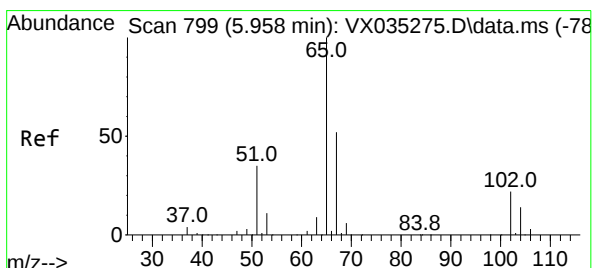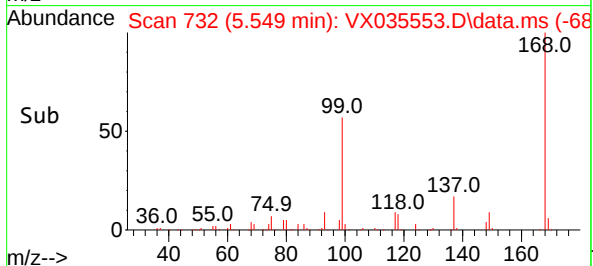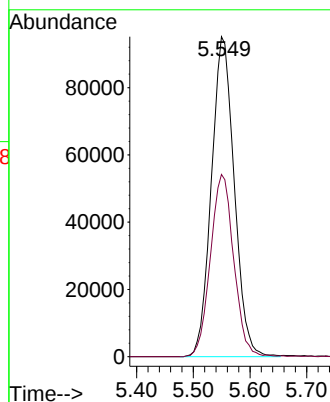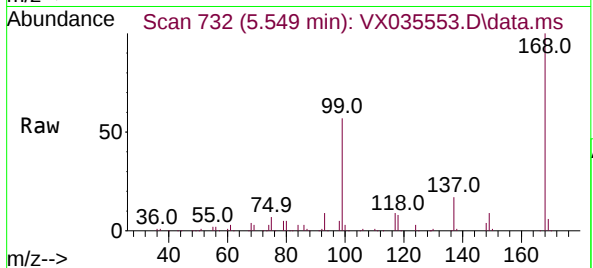

#33
1,2-Dichloroethane-d4
Concen: 48.741 ug/l
RT: 5.952 min Scan# 798
Delta R.T. -0.006 min
Lab File: VX035553.D
Acq: 08 May 2023 12:26

Tgt Ion: 65 Resp: 156507
Ion Ratio Lower Upper
65 100
67 52.0 0.0 104.0


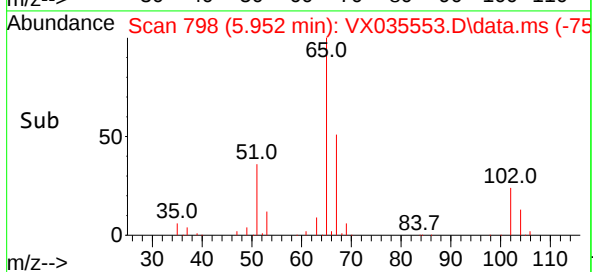
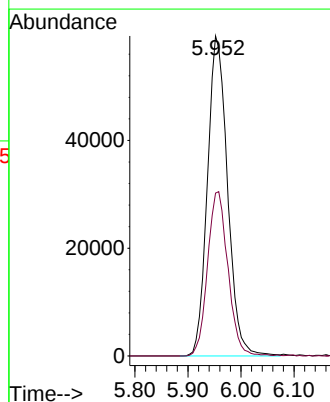
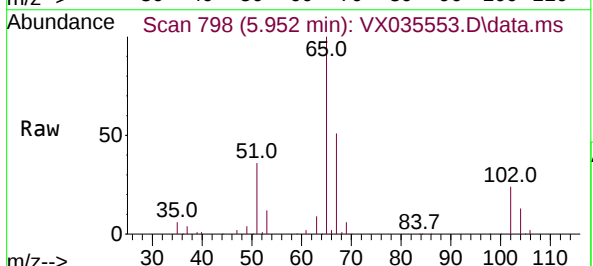




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. -0.000 min
Lab File: VX035553.D
Acq: 08 May 2023 12:26




Instrument :
MSVOA_X
ClientSampleId :
VX0508WBL01


Tgt Ion:114 Resp: 440786
Ion Ratio Lower Upper
114 100
63 19.5 0.0 42.2
88 16.2 0.0 33.2

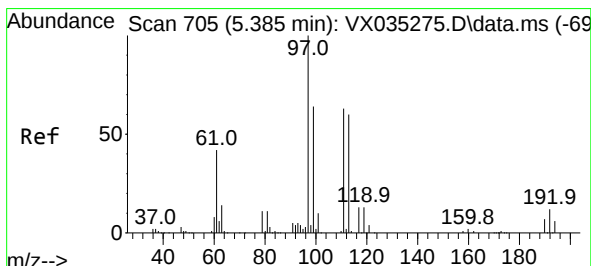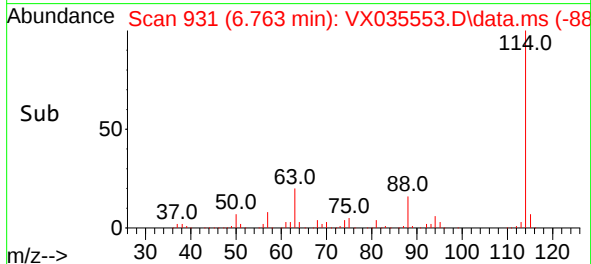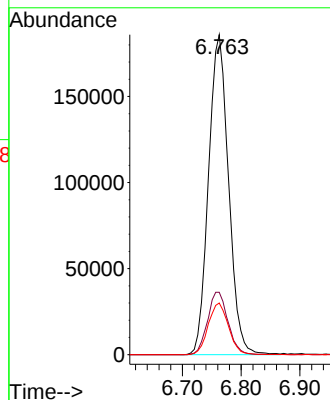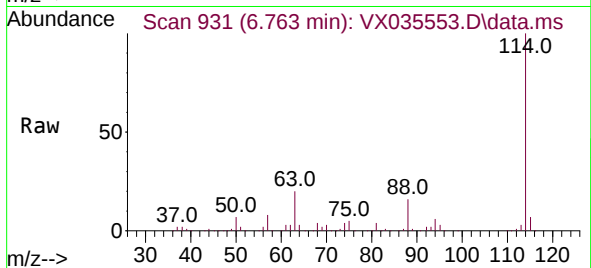

#35
Dibromofluoromethane
Concen: 49.778 ug/l
RT: 5.385 min Scan# 705
Delta R.T. -0.000 min
Lab File: VX035553.D
Acq: 08 May 2023 12:26

Tgt Ion:113 Resp: 134671
Ion Ratio Lower Upper
113 100
111 103.6 83.7 125.5
192 20.8 15.4 23.2


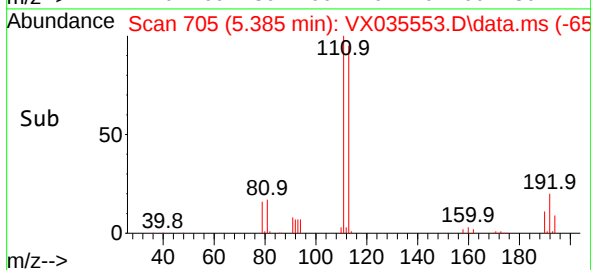
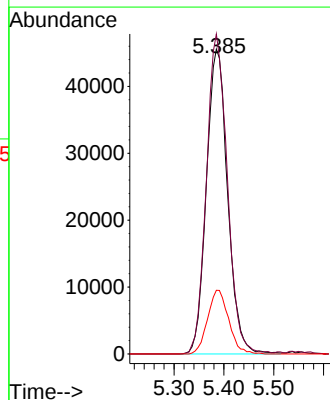
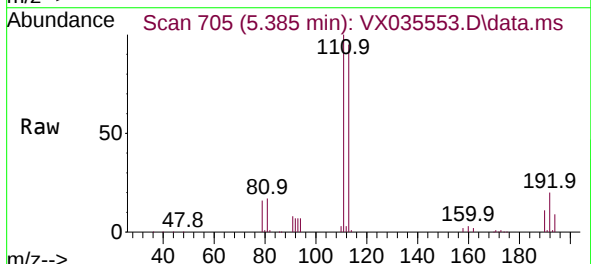


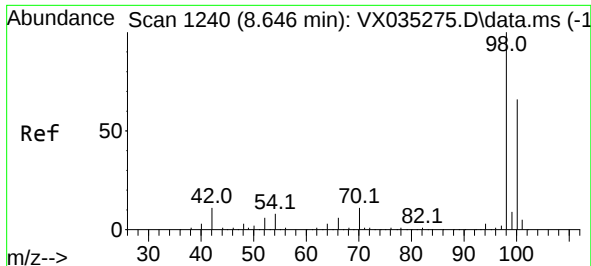

#50
Toluene-d8
Concen: 50.179 ug/l
RT: 8.646 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX035553.D
Acq: 08 May 2023 12:26




Instrument :
MSVOA_X
ClientSampleId :
VX0508WBL01


Tgt Ion: 98 Resp: 512110
Ion Ratio Lower Upper
98 100
100 66.3 52.5 78.7

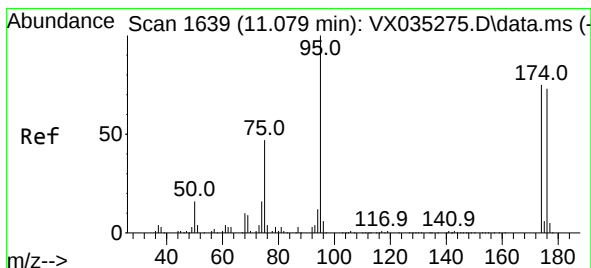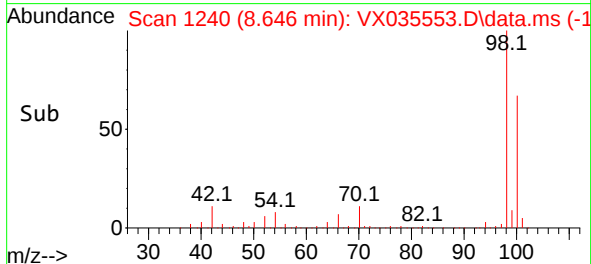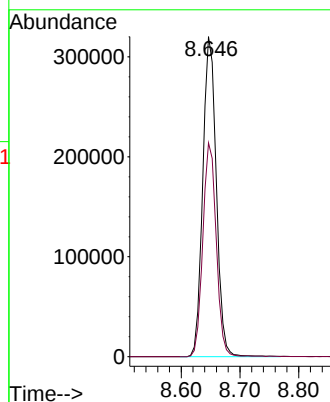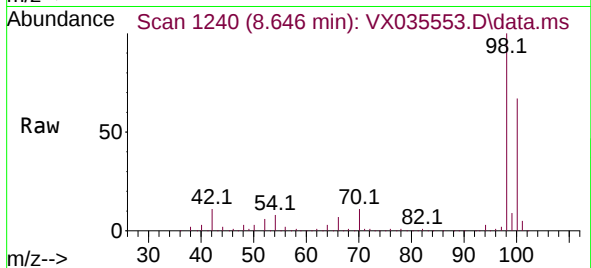

#62
4-Bromofluorobenzene
Concen: 51.497 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.000 min
Lab File: VX035553.D
Acq: 08 May 2023 12:26

Tgt Ion: 95 Resp: 197707
Ion Ratio Lower Upper
95 100
174 78.9 0.0 147.4
176 76.0 0.0 140.6


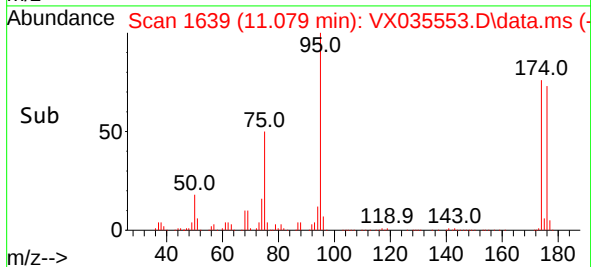
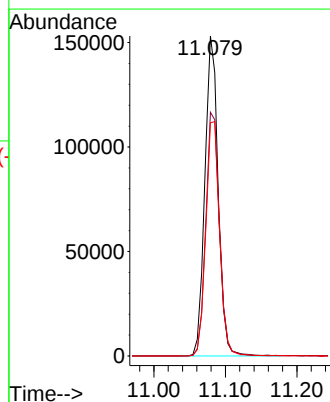
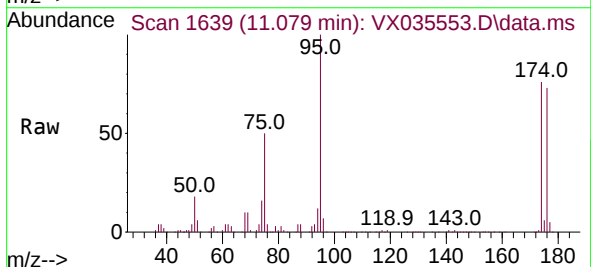


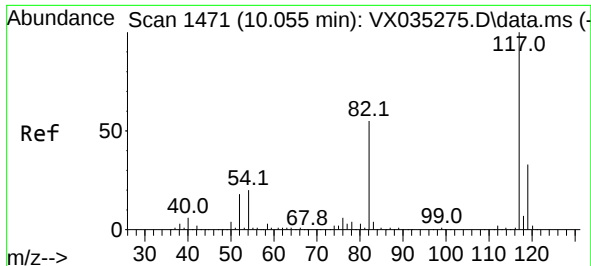

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX035553.D
Acq: 08 May 2023 12:26

Instrument :
MSVOA_X
ClientSampleId :
VX0508WBL01

Tgt Ion:117 Resp: 403085
Ion Ratio Lower Upper
117 100
82 55.2 45.0 67.4
119 32.4 26.0 39.0

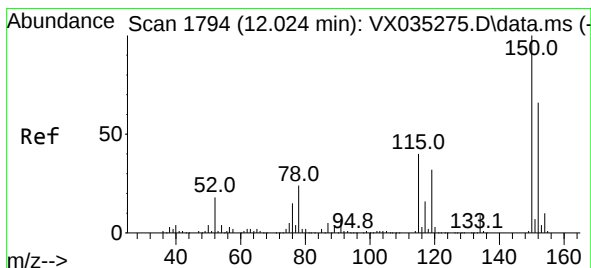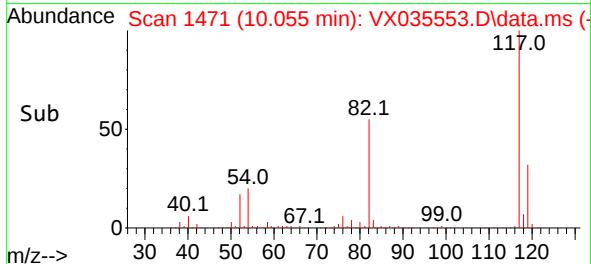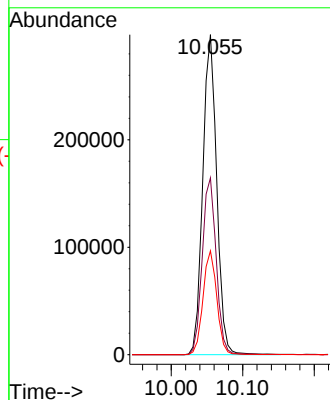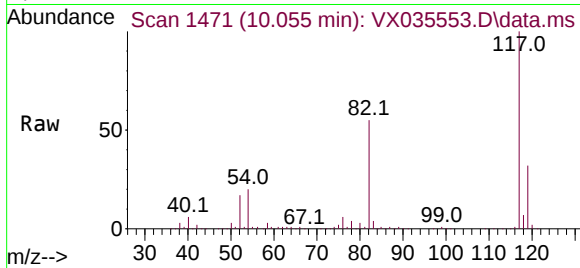

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. -0.000 min
Lab File: VX035553.D
Acq: 08 May 2023 12:26

Tgt Ion:152 Resp: 190678
Ion Ratio Lower Upper
152 100
115 59.8 45.0 135.0
150 154.4 0.0 352.4

