

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX050823\
Data File : VX035566.D
Acq On : 08 May 2023 17:34
Operator : JC/MD
Sample : 02660-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
WATER-SAMPLE-API-3-6

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X042523W.M

Title : SW846 8260

Signal : TIC: VX035566.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.385	692	705	721	rBV	133638	397393	33.35%	6.121%
2	5.550	721	732	747	rVB2	242309	689618	57.87%	10.621%
3	5.958	787	799	817	rBV	144848	388705	32.62%	5.987%
4	6.763	921	931	948	rBV	371884	891685	74.83%	13.733%
5	8.647	1234	1240	1259	rBV	761918	1191664	100.00%	18.354%
6	10.055	1465	1471	1487	rBV	768256	1053104	88.37%	16.220%
7	11.079	1634	1639	1654	rBV	648799	819014	68.73%	12.614%
8	12.024	1788	1794	1808	rBV	781566	1010190	84.77%	15.559%
9	15.207	2312	2316	2320	rVB2	10781	14867	1.25%	0.229%
10	15.981	2439	2443	2451	rVB4	10256	18851	1.58%	0.290%
11	16.164	2468	2473	2482	rVB5	7442	17708	1.49%	0.273%




Sum of corrected areas: 6492799

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX050823\
Data File : VX035566.D
Acq On : 08 May 2023 17:34
Operator : JC/MD
Sample : 02660-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
WATER-SAMPLE-API-3-6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X042523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

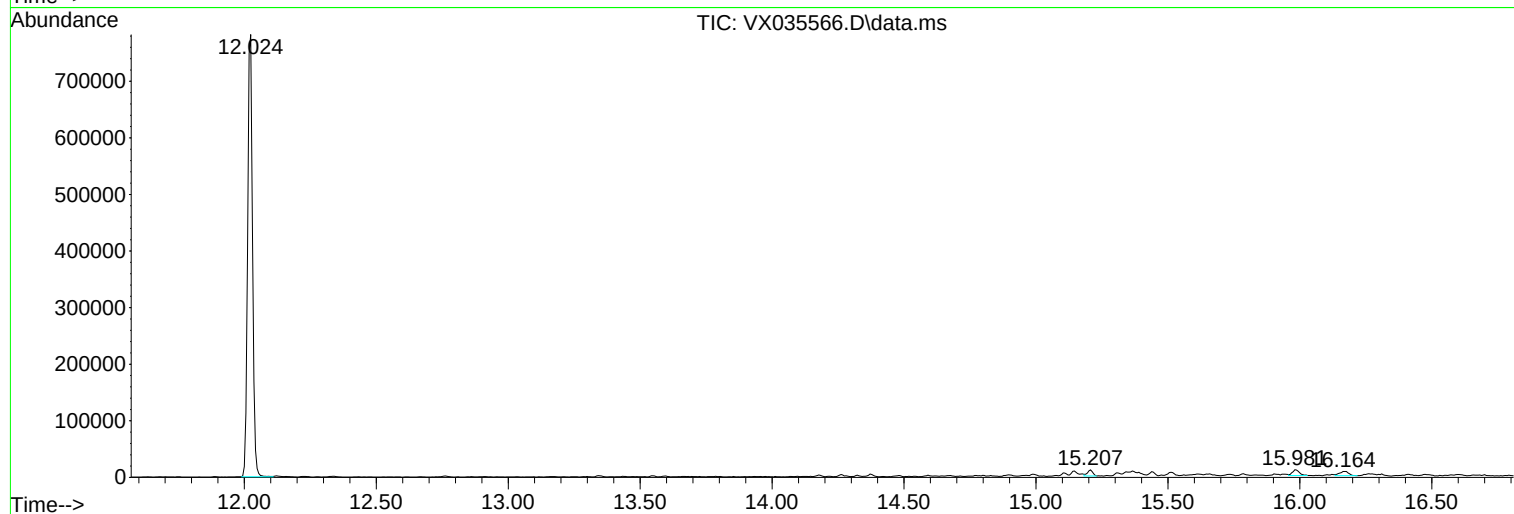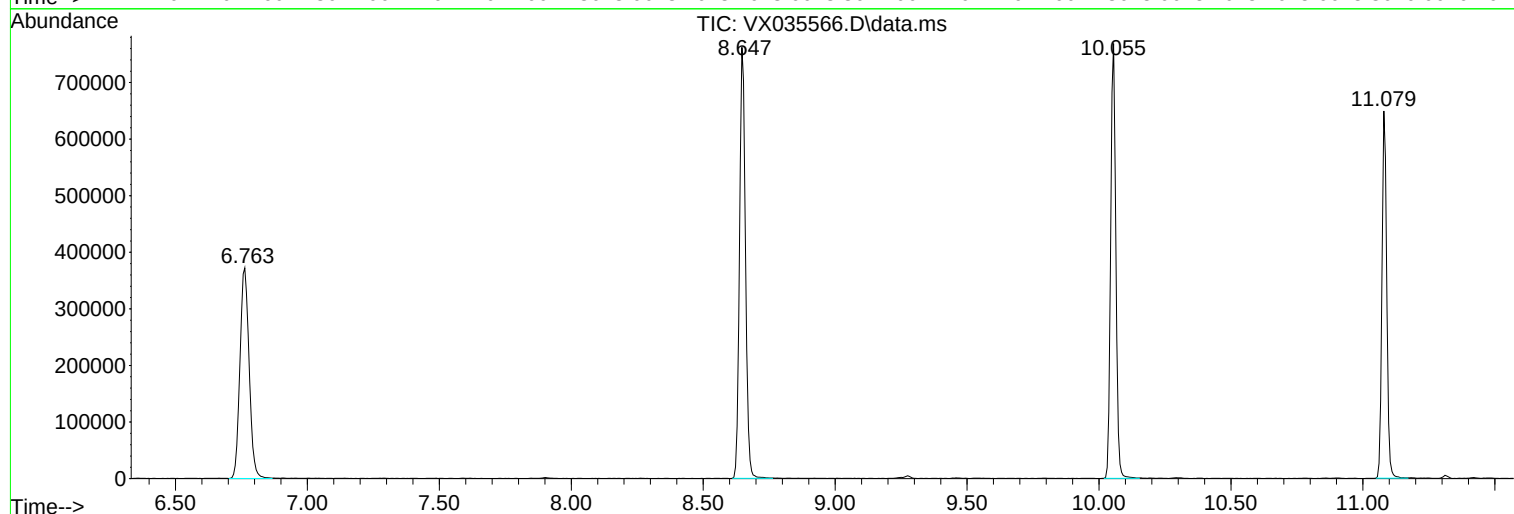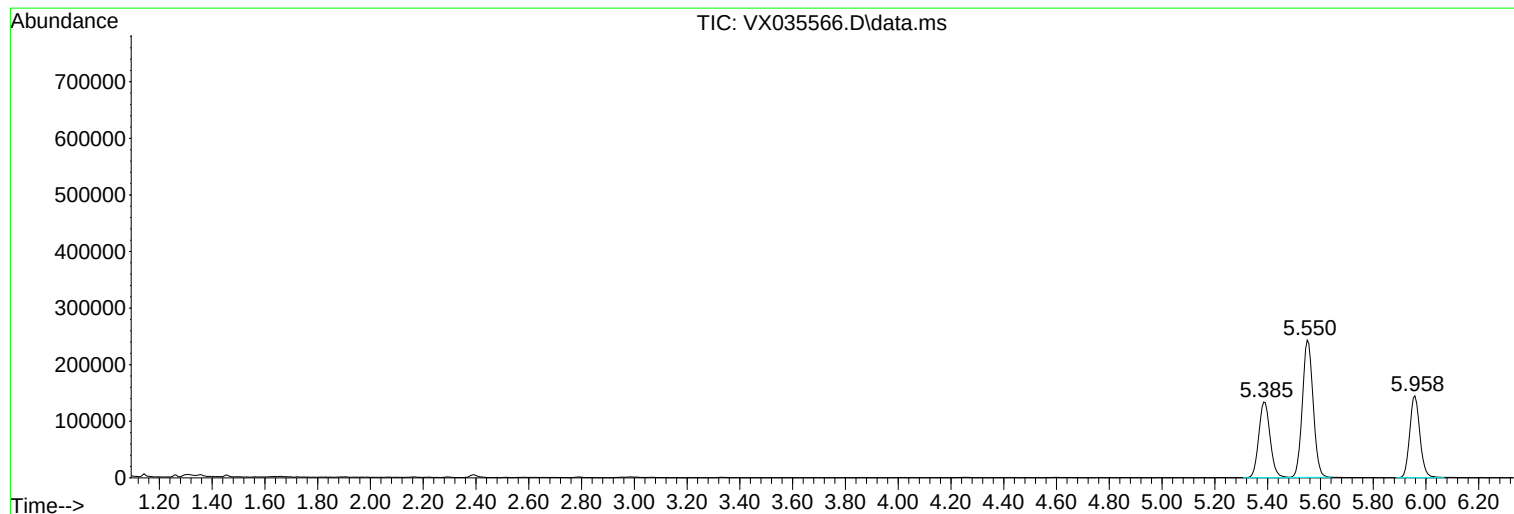

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX050823\
Data File : VX035566.D
Acq On : 08 May 2023 17:34
Operator : JC/MD
Sample : 02660-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
WATER-SAMPLE-API-3-6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X042523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX050823\
Data File : VX035566.D
Acq On : 08 May 2023 17:34
Operator : JC/MD
Sample : 02660-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
WATER-SAMPLE-API-3-6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X042523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------