

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX050924\
 Data File : VX041431.D
 Acq On : 09 May 2024 12:42
 Operator : JC/MD
 Sample : VX0509WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK675

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML050924WMA.M
 Title : VOC Analysis

Signal : TIC: VX041431.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.258	24	28	32	rBV3	2879	3875	0.38%	0.047%
2	1.374	43	47	57	rBV	88941	134379	13.11%	1.641%
3	1.648	88	92	105	rVB	72923	117197	11.43%	1.431%
4	2.294	192	198	209	rBV	245188	378546	36.92%	4.622%
5	2.392	211	214	219	rVB	2150	2953	0.29%	0.036%
6	2.502	229	232	238	rVB	3304	4653	0.45%	0.057%
7	2.648	255	256	258	rBV	137	141	0.01%	0.002%
8	2.788	274	279	286	rBV2	2889	5349	0.52%	0.065%
9	2.941	297	304	316	rVB	6579	15768	1.54%	0.193%
10	3.087	323	328	340	rBV4	2069	5753	0.56%	0.070%
11	3.203	345	347	348	rBV2	225	168	0.02%	0.002%
12	3.349	370	371	378	rBV3	169	241	0.02%	0.003%
13	3.605	409	413	420	rBV3	550	1112	0.11%	0.014%
14	3.697	425	428	431	rBV3	162	200	0.02%	0.002%
15	3.782	439	442	443	rBV2	143	174	0.02%	0.002%
16	3.873	455	457	459	rBV	124	147	0.01%	0.002%
17	3.910	461	463	465	rBV2	168	127	0.01%	0.002%
18	3.977	472	474	477	rBV	142	162	0.02%	0.002%
19	4.172	505	506	509	rBV2	192	187	0.02%	0.002%
20	4.465	546	554	570	rBV	70581	226242	22.07%	2.763%
21	4.910	622	627	634	rVB5	553	1318	0.13%	0.016%
22	5.050	638	650	670	rBV	137338	427677	41.71%	5.222%
23	5.361	699	701	702	rBV	715	560	0.05%	0.007%
24	5.556	727	733	740	rBV4	1128	2429	0.24%	0.030%
25	5.629	743	745	747	rBV	146	159	0.02%	0.002%
26	5.672	747	752	759	rVB3	555	1167	0.11%	0.014%
27	5.757	765	766	770	rVB2	138	174	0.02%	0.002%
28	5.964	789	800	820	rBV2	352218	1025250	100.00%	12.519%
29	6.342	860	862	863	rVV	298	223	0.02%	0.003%
30	6.379	866	868	870	rVV2	477	446	0.04%	0.005%
31	6.476	880	884	885	rBV2	230	254	0.02%	0.003%
32	6.495	885	887	889	rVB	285	198	0.02%	0.002%
33	6.537	892	894	895	rBV	172	130	0.01%	0.002%
34	6.586	901	902	905	rVB2	178	122	0.01%	0.001%
35	6.757	920	930	944	rBV	254684	615814	60.06%	7.519%
36	7.123	983	990	999	rVB7	2869	7615	0.74%	0.093%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX050924\
 Data File : VX041431.D
 Acq On : 09 May 2024 12:42
 Operator : JC/MD
 Sample : VX0509WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK675

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML050924WMA.M
 Title : VOC Analysis

37	7.214	999	1005	1011	rBV3	705	1266	0.12%	0.015%
38	7.306	1011	1020	1037	rBV	213851	479406	46.76%	5.854%
39	7.543	1057	1059	1061	rVB	169	127	0.01%	0.002%
40	7.574	1061	1064	1065	rBV	178	161	0.02%	0.002%
41	7.641	1072	1075	1077	rBV2	134	122	0.01%	0.001%
42	7.824	1102	1105	1113	rVB3	519	1039	0.10%	0.013%
43	7.891	1115	1116	1119	rVV2	187	170	0.02%	0.002%
44	8.080	1146	1147	1149	rBV	178	134	0.01%	0.002%
45	8.116	1151	1153	1156	rVB2	168	188	0.02%	0.002%
46	8.324	1181	1187	1202	rBV	142208	238442	23.26%	2.912%
47	8.482	1211	1213	1215	rBV2	279	249	0.02%	0.003%
48	8.537	1217	1222	1224	rVB4	241	344	0.03%	0.004%
49	8.580	1224	1229	1232	rBV4	1474	2158	0.21%	0.026%
50	8.647	1233	1240	1250	rBV	565634	886381	86.46%	10.823%
51	8.872	1275	1277	1279	rVB	381	278	0.03%	0.003%
52	8.952	1284	1290	1305	rVV	100543	158028	15.41%	1.930%
53	9.153	1321	1323	1328	rVV2	799	1277	0.12%	0.016%
54	9.275	1340	1343	1348	rVB3	2677	3705	0.36%	0.045%
55	9.385	1356	1361	1379	rBV	283506	433616	42.29%	5.295%
56	9.610	1395	1398	1403	rVB3	1004	1454	0.14%	0.018%
57	9.702	1409	1413	1417	rBV2	2608	3302	0.32%	0.040%
58	9.811	1429	1431	1433	rBV	163	186	0.02%	0.002%
59	9.836	1433	1435	1437	rVV2	423	335	0.03%	0.004%
60	9.884	1441	1443	1445	rVB	234	209	0.02%	0.003%
61	10.055	1465	1471	1482	rBV	555856	804578	78.48%	9.824%
62	10.195	1491	1494	1500	rVB	2932	4448	0.43%	0.054%
63	10.305	1508	1512	1520	rVB	3109	4675	0.46%	0.057%
64	10.415	1528	1530	1532	rBV2	168	158	0.02%	0.002%
65	10.537	1546	1550	1552	rVB2	152	176	0.02%	0.002%
66	10.567	1552	1555	1557	rBV2	117	148	0.01%	0.002%
67	10.646	1561	1568	1582	rVV5	3434	9442	0.92%	0.115%
68	10.738	1582	1583	1586	rVB	228	126	0.01%	0.002%
69	10.775	1586	1589	1591	rBV	94	148	0.01%	0.002%
70	10.805	1591	1594	1599	rVV3	647	857	0.08%	0.010%
71	10.963	1616	1620	1624	rVV2	3548	4706	0.46%	0.057%
72	11.092	1637	1641	1650	rVB3	769	1433	0.14%	0.017%
73	11.152	1650	1651	1652	rBV	198	132	0.01%	0.002%
74	11.189	1652	1657	1664	rBV	420383	549269	53.57%	6.707%
75	11.354	1682	1684	1685	rVB	218	150	0.01%	0.002%
76	11.409	1691	1693	1697	rBV	225	202	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX050924\
 Data File : VX041431.D
 Acq On : 09 May 2024 12:42
 Operator : JC/MD
 Sample : VX0509WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK675

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML050924WMA.M
 Title : VOC Analysis

77	11.451	1697	1700	1707	rBV	3155	3781	0.37%	0.046%
78	11.628	1728	1729	1731	rBV2	177	130	0.01%	0.002%
79	11.689	1736	1739	1741	rBV2	134	139	0.01%	0.002%
80	11.707	1741	1742	1745	rBV2	336	245	0.02%	0.003%
81	11.756	1745	1750	1758	rBV2	3592	4553	0.44%	0.056%
82	11.933	1775	1779	1780	rBV	128	157	0.02%	0.002%
83	11.969	1782	1785	1788	rBV	5350	6527	0.64%	0.080%
84	12.018	1788	1793	1808	rVB	617931	800788	78.11%	9.778%
85	12.317	1837	1842	1852	rBV	603934	757483	73.88%	9.249%
86	12.664	1895	1899	1902	rBV2	122	181	0.02%	0.002%
87	12.872	1930	1933	1934	rBV	169	174	0.02%	0.002%
88	12.920	1939	1941	1942	rVV	187	131	0.01%	0.002%
89	12.951	1942	1946	1949	rVV4	678	995	0.10%	0.012%
90	13.116	1968	1973	1978	rBV2	5199	6865	0.67%	0.084%
91	13.420	2021	2023	2026	rBV	149	184	0.02%	0.002%
92	13.591	2047	2051	2058	rBV	6901	8822	0.86%	0.108%
93	13.780	2077	2082	2092	rBV	8861	13319	1.30%	0.163%
94	13.914	2101	2104	2107	rBV2	187	259	0.03%	0.003%
95	13.963	2107	2112	2121	rVV2	6531	9628	0.94%	0.118%
96	14.067	2126	2129	2130	rBV2	158	157	0.02%	0.002%
97	14.103	2133	2135	2136	rVB	272	149	0.01%	0.002%
98	14.128	2136	2139	2140	rBV2	312	267	0.03%	0.003%
99	14.365	2174	2178	2179	rBV2	188	200	0.02%	0.002%
100	14.609	2214	2218	2220	rBV3	299	340	0.03%	0.004%


Sum of corrected areas: 8189609

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX050924\
Data File : VX041431.D
Acq On : 09 May 2024 12:42
Operator : JC/MD
Sample : VX0509WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK675

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML050924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

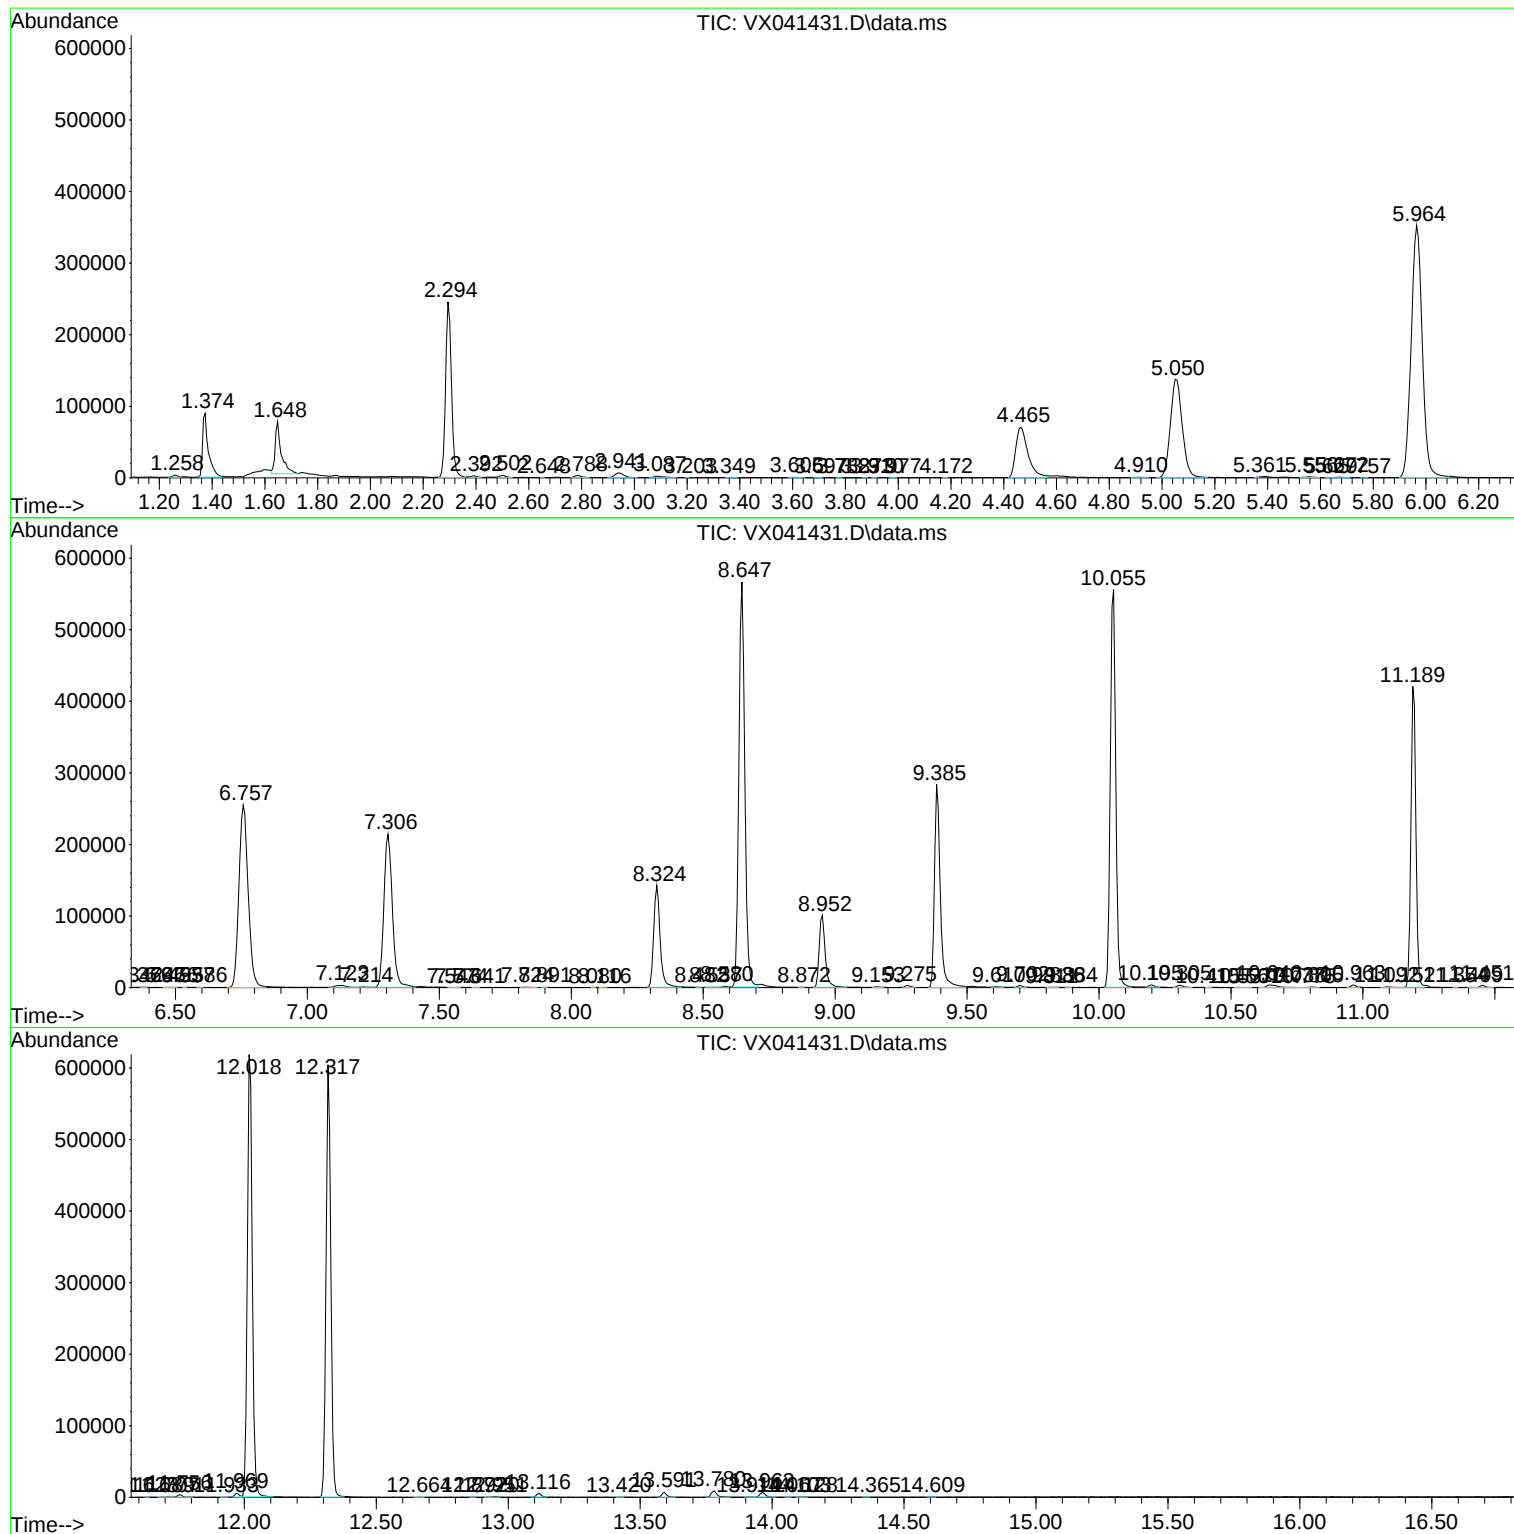

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX050924\
Data File : VX041431.D
Acq On : 09 May 2024 12:42
Operator : JC/MD
Sample : VX0509WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK675

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML050924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX050924\
Data File : VX041431.D
Acq On : 09 May 2024 12:42
Operator : JC/MD
Sample : VX0509WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK675

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML050924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc