

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX050924\
 Data File : VX041435.D
 Acq On : 09 May 2024 15:34
 Operator : JC/MD
 Sample : P2381-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E1D18

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML050924WMA.M
 Title : VOC Analysis

Signal : TIC: VX041435.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.258	25	28	32	rBV3	1952	2286	0.23%	0.030%
2	1.368	43	46	57	rBV	82028	114011	11.51%	1.516%
3	1.447	57	59	65	rVB4	1404	1842	0.19%	0.024%
4	1.599	72	84	85	rBV9	7009	22755	2.30%	0.303%
5	1.648	88	92	104	rVB	75580	113790	11.49%	1.513%
6	2.294	192	198	208	rBV	182878	281600	28.43%	3.745%
7	2.386	209	213	219	rVB	6732	10685	1.08%	0.142%
8	2.495	229	231	237	rVB2	466	756	0.08%	0.010%
9	2.575	237	244	251	rVB3	1308	3019	0.30%	0.040%
10	2.660	254	258	259	rBV2	233	262	0.03%	0.003%
11	2.697	260	264	265	rBV2	209	178	0.02%	0.002%
12	2.782	272	278	286	rBV4	1142	2180	0.22%	0.029%
13	2.940	297	304	313	rBV2	2359	5924	0.60%	0.079%
14	3.056	321	323	326	rBV2	76	106	0.01%	0.001%
15	3.136	331	336	338	rBV	134	175	0.02%	0.002%
16	3.318	364	366	370	rBV2	147	246	0.02%	0.003%
17	3.465	389	390	393	rBV	127	123	0.01%	0.002%
18	3.514	395	398	400	rVB2	154	157	0.02%	0.002%
19	3.568	406	407	410	rBV	144	156	0.02%	0.002%
20	3.623	414	416	418	rVB	193	153	0.02%	0.002%
21	3.648	418	420	421	rBV	202	139	0.01%	0.002%
22	3.696	427	428	430	rBV	142	114	0.01%	0.002%
23	3.739	433	435	439	rBV2	211	196	0.02%	0.003%
24	3.770	439	440	443	rVB	158	107	0.01%	0.001%
25	3.837	445	451	452	rBV2	139	209	0.02%	0.003%
26	4.044	484	485	490	rVV2	111	142	0.01%	0.002%
27	4.111	494	496	498	rVB	172	114	0.01%	0.002%
28	4.215	510	513	514	rBV2	250	292	0.03%	0.004%
29	4.379	537	540	545	rVB2	161	262	0.03%	0.003%
30	4.458	545	553	573	rBV	67755	213001	21.50%	2.832%
31	4.904	624	626	627	rBV2	138	115	0.01%	0.002%
32	5.050	639	650	669	rBV	126835	390855	39.46%	5.198%
33	5.318	692	694	696	rBV	168	160	0.02%	0.002%
34	5.391	699	706	716	rVB4	757	2311	0.23%	0.031%
35	5.513	724	726	727	rVV2	193	149	0.02%	0.002%
36	5.550	727	732	741	rVB3	891	2465	0.25%	0.033%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX050924\
 Data File : VX041435.D
 Acq On : 09 May 2024 15:34
 Operator : JC/MD
 Sample : P2381-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E1D18

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML050924WMA.M
 Title : VOC Analysis

37	5.964	788	800	828	rBV2	335646	990614	100.00%	13.173%
38	6.348	862	863	867	rBV2	388	401	0.04%	0.005%
39	6.446	877	879	880	rBV2	132	103	0.01%	0.001%
40	6.537	892	894	896	rVB2	202	175	0.02%	0.002%
41	6.556	896	897	905	rVB2	172	233	0.02%	0.003%
42	6.757	921	930	944	rBV	243045	588483	59.41%	7.826%
43	7.123	984	990	995	rVB5	1275	2778	0.28%	0.037%
44	7.208	1000	1004	1009	rBV4	506	981	0.10%	0.013%
45	7.306	1011	1020	1041	rBV	197667	438366	44.25%	5.829%
46	7.641	1073	1075	1076	rBV	137	97	0.01%	0.001%
47	7.677	1080	1081	1085	rVB2	218	176	0.02%	0.002%
48	7.720	1086	1088	1093	rBV2	102	193	0.02%	0.003%
49	8.074	1144	1146	1149	rVB2	120	97	0.01%	0.001%
50	8.183	1162	1164	1166	rBV2	177	144	0.01%	0.002%
51	8.324	1180	1187	1199	rBV	123439	211038	21.30%	2.806%
52	8.647	1234	1240	1262	rBV	509310	808073	81.57%	10.746%
53	8.952	1284	1290	1304	rBV	88345	141355	14.27%	1.880%
54	9.275	1337	1343	1348	rVB	2212	3513	0.35%	0.047%
55	9.317	1348	1350	1353	rVB2	134	96	0.01%	0.001%
56	9.384	1356	1361	1382	rBV	319000	483349	48.79%	6.427%
57	9.921	1446	1449	1450	rBV	163	180	0.02%	0.002%
58	10.049	1465	1470	1486	rBV	487721	696536	70.31%	9.262%
59	10.396	1526	1527	1530	rVB2	196	104	0.01%	0.001%
60	10.470	1537	1539	1540	rBV	167	117	0.01%	0.002%
61	10.622	1562	1564	1565	rBV2	135	92	0.01%	0.001%
62	10.646	1565	1568	1573	rVV4	438	735	0.07%	0.010%
63	10.793	1589	1592	1593	rBV2	228	213	0.02%	0.003%
64	10.878	1603	1606	1610	rVV	147	212	0.02%	0.003%
65	10.963	1617	1620	1623	rBV	208	324	0.03%	0.004%
66	11.067	1635	1637	1638	rVV	178	133	0.01%	0.002%
67	11.091	1638	1641	1645	rVB4	990	1423	0.14%	0.019%
68	11.189	1652	1657	1668	rBV	398463	516178	52.11%	6.864%
69	11.311	1674	1677	1684	rVB	2170	3022	0.31%	0.040%
70	11.384	1687	1689	1690	rVB	201	103	0.01%	0.001%
71	11.433	1693	1697	1699	rBV2	642	699	0.07%	0.009%
72	11.713	1738	1743	1744	rBV2	478	470	0.05%	0.006%
73	11.756	1747	1750	1754	rVB2	366	411	0.04%	0.005%
74	11.793	1754	1756	1758	rBV	123	108	0.01%	0.001%
75	11.975	1783	1786	1788	rBV4	820	904	0.09%	0.012%
76	12.018	1788	1793	1805	rVV	524583	679707	68.61%	9.039%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX050924\
 Data File : VX041435.D
 Acq On : 09 May 2024 15:34
 Operator : JC/MD
 Sample : P2381-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E1D18

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML050924WMA.M
 Title : VOC Analysis

77	12.219	1822	1826	1837	rVB	3838	6100	0.62%	0.081%
78	12.317	1837	1842	1856	rBV	593172	761552	76.88%	10.127%
79	12.500	1870	1872	1873	rVB2	240	127	0.01%	0.002%
80	12.591	1885	1887	1889	rBV2	260	238	0.02%	0.003%
81	12.634	1892	1894	1897	rVB2	207	176	0.02%	0.002%
82	12.664	1897	1899	1900	rBV	173	103	0.01%	0.001%
83	12.768	1912	1916	1919	rBV4	691	1118	0.11%	0.015%
84	12.859	1925	1931	1935	rBV4	861	1342	0.14%	0.018%
85	13.000	1950	1954	1957	rBV2	154	261	0.03%	0.003%
86	13.115	1969	1973	1976	rVB3	677	904	0.09%	0.012%
87	13.274	1997	1999	2000	rBV	140	101	0.01%	0.001%
88	13.378	2013	2016	2017	rBV2	155	149	0.02%	0.002%
89	13.451	2027	2028	2031	rBV	231	182	0.02%	0.002%
90	13.481	2031	2033	2034	rVV	211	126	0.01%	0.002%
91	13.597	2048	2052	2055	rVB2	1211	1471	0.15%	0.020%
92	13.695	2066	2068	2069	rBV	128	115	0.01%	0.002%
93	13.749	2073	2077	2078	rBV2	514	433	0.04%	0.006%
94	13.963	2110	2112	2115	rVB2	1024	940	0.09%	0.012%
95	14.097	2130	2134	2136	rBV2	230	357	0.04%	0.005%
96	14.121	2136	2138	2143	rVV3	282	374	0.04%	0.005%
97	14.255	2157	2160	2161	rBV	274	244	0.02%	0.003%
98	14.371	2177	2179	2181	rBV	219	148	0.01%	0.002%
99	14.792	2246	2248	2250	rBV3	355	245	0.02%	0.003%
100	15.072	2292	2294	2295	rBV	319	239	0.02%	0.003%


Sum of corrected areas: 7520016

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX050924\
Data File : VX041435.D
Acq On : 09 May 2024 15:34
Operator : JC/MD
Sample : P2381-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E1D18

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML050924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

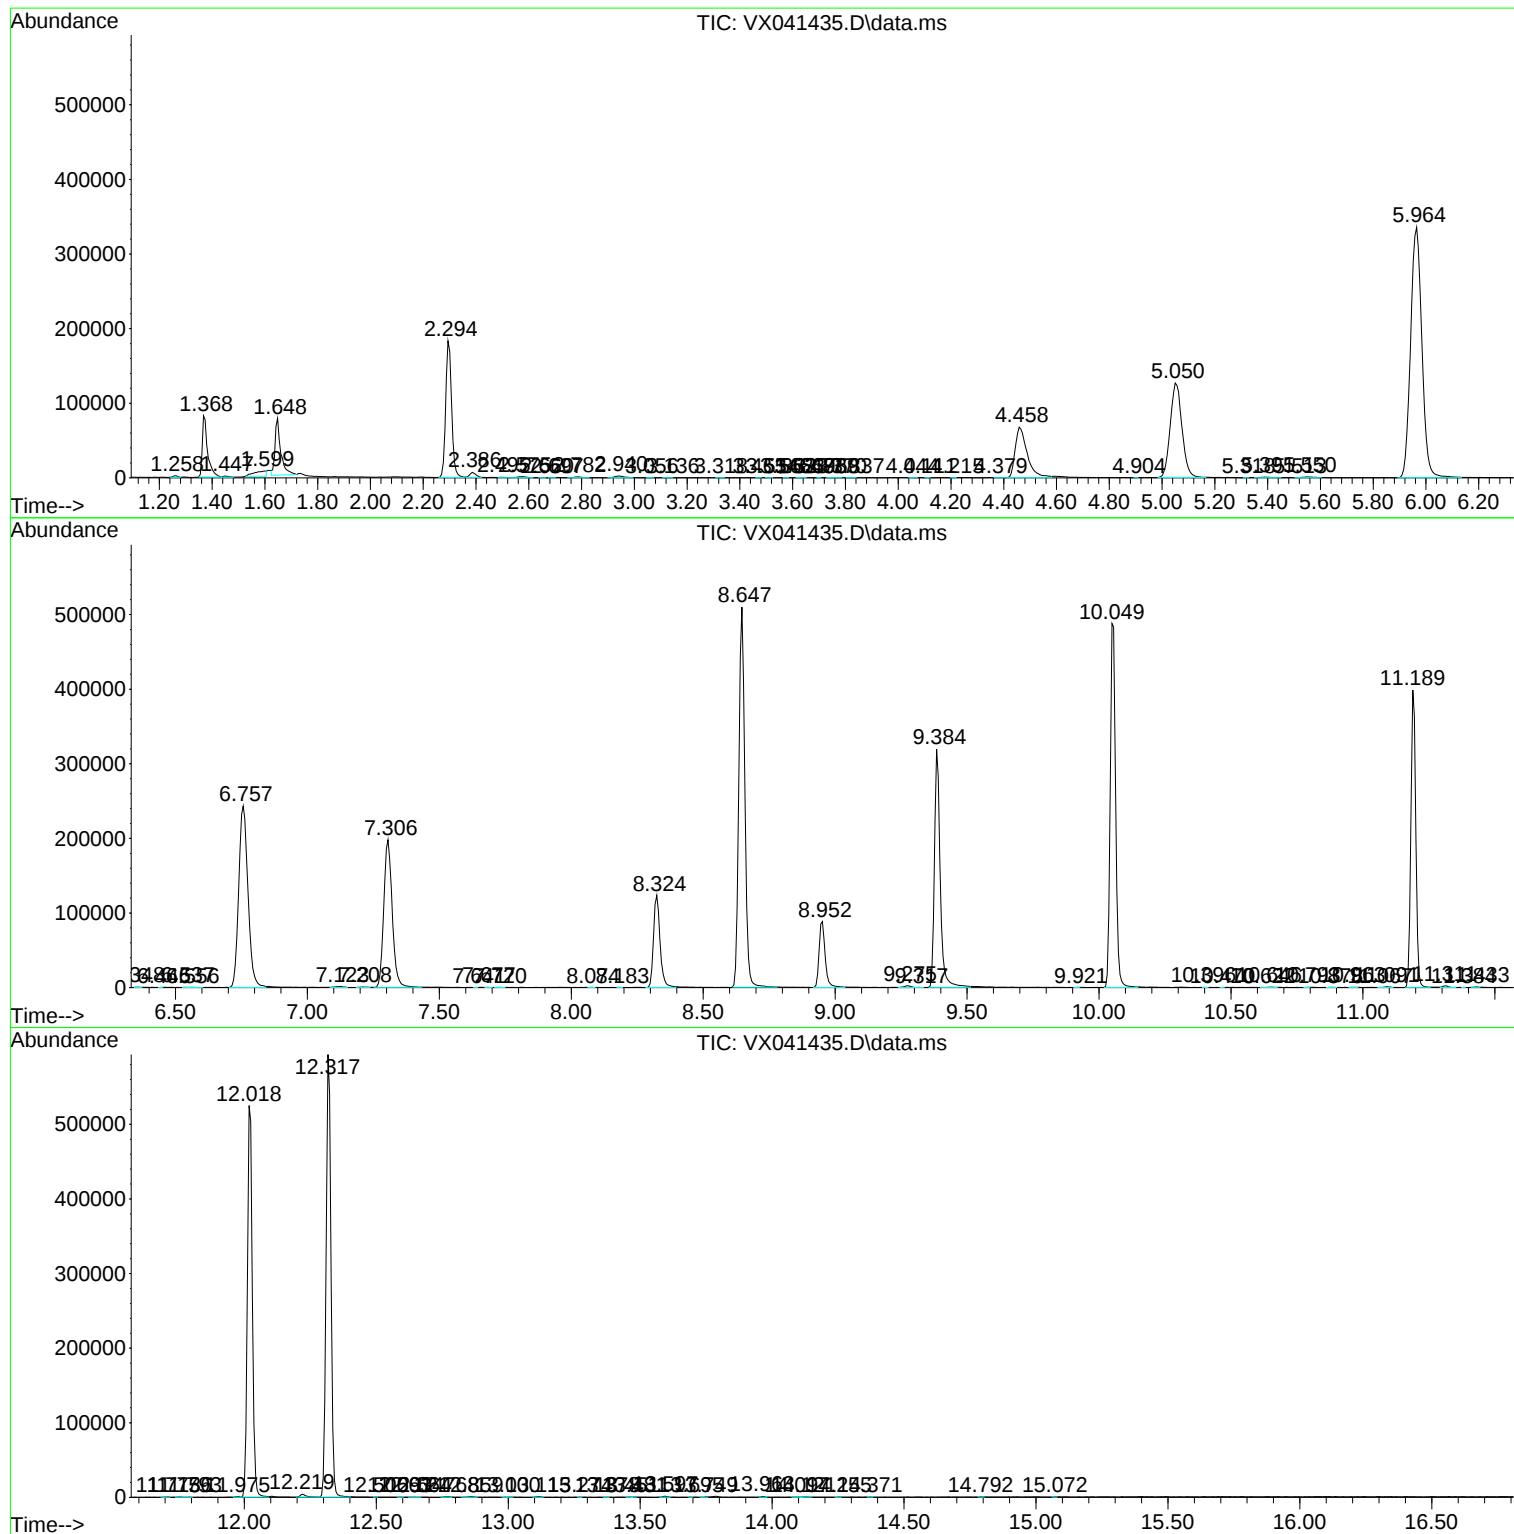

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX050924\
Data File : VX041435.D
Acq On : 09 May 2024 15:34
Operator : JC/MD
Sample : P2381-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E1D18

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML050924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX050924\
Data File : VX041435.D
Acq On : 09 May 2024 15:34
Operator : JC/MD
Sample : P2381-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E1D18

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML050924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc