

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX050924\
 Data File : VX041436.D
 Acq On : 09 May 2024 15:57
 Operator : JC/MD
 Sample : P2381-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML050924WMA.M
 Title : VOC Analysis

Signal : TIC: VX041436.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.258	25	28	32	rVB3	2182	2598	0.27%	0.036%
2	1.368	43	46	58	rBV	77776	109444	11.45%	1.505%
3	1.538	71	74	76	rBV2	5675	6952	0.73%	0.096%
4	1.648	88	92	107	rVB	73716	121168	12.68%	1.667%
5	2.294	192	198	209	rBV	208193	320107	33.49%	4.403%
6	2.392	210	214	220	rVB2	2227	3677	0.38%	0.051%
7	2.495	229	231	236	rBV3	577	925	0.10%	0.013%
8	2.544	236	239	240	rVV2	226	283	0.03%	0.004%
9	2.581	241	245	254	rVB3	1128	2346	0.25%	0.032%
10	2.684	260	262	264	rBV2	106	116	0.01%	0.002%
11	2.709	264	266	267	rBV	211	138	0.01%	0.002%
12	2.788	273	279	287	rVB2	2883	5372	0.56%	0.074%
13	2.940	301	304	312	rVB2	684	1183	0.12%	0.016%
14	3.245	351	354	357	rBV2	170	272	0.03%	0.004%
15	3.270	357	358	361	rVV	156	110	0.01%	0.002%
16	3.325	365	367	372	rVV2	165	249	0.03%	0.003%
17	3.483	391	393	398	rVB2	123	177	0.02%	0.002%
18	4.172	505	506	508	rBV	173	138	0.01%	0.002%
19	4.245	515	518	519	rVB2	145	121	0.01%	0.002%
20	4.324	525	531	532	rBV2	152	244	0.03%	0.003%
21	4.465	546	554	575	rBV	65128	214577	22.45%	2.952%
22	4.824	611	613	614	rBV	157	110	0.01%	0.002%
23	4.934	630	631	634	rVB2	141	117	0.01%	0.002%
24	4.958	634	635	637	rBV2	192	122	0.01%	0.002%
25	5.056	638	651	672	rVV	122619	378756	39.62%	5.210%
26	5.318	691	694	696	rVB2	175	185	0.02%	0.003%
27	5.397	700	707	715	rBV5	1070	2698	0.28%	0.037%
28	5.745	763	764	768	rBV	199	232	0.02%	0.003%
29	5.964	788	800	824	rBV2	324251	955910	100.00%	13.149%
30	6.354	862	864	865	rBV	235	144	0.02%	0.002%
31	6.537	892	894	897	rVB2	180	157	0.02%	0.002%
32	6.562	897	898	901	rBV2	145	136	0.01%	0.002%
33	6.604	903	905	908	rVV	157	110	0.01%	0.002%
34	6.757	921	930	948	rBV	243533	587474	61.46%	8.081%
35	7.117	984	989	995	rVB5	1145	2516	0.26%	0.035%
36	7.208	1000	1004	1011	rBV2	547	1178	0.12%	0.016%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX050924\
 Data File : VX041436.D
 Acq On : 09 May 2024 15:57
 Operator : JC/MD
 Sample : P2381-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML050924WMA.M
 Title : VOC Analysis

37	7.306	1011	1020	1039	rBV	192298	423206	44.27%	5.821%
38	7.482	1046	1049	1053	rBV5	609	887	0.09%	0.012%
39	7.769	1092	1096	1098	rBV2	162	259	0.03%	0.004%
40	8.019	1136	1137	1139	rBV	124	129	0.01%	0.002%
41	8.110	1150	1152	1157	rVB	169	185	0.02%	0.003%
42	8.147	1157	1158	1163	rBV2	139	217	0.02%	0.003%
43	8.324	1181	1187	1200	rBV	124278	202611	21.20%	2.787%
44	8.531	1218	1221	1222	rBV2	257	233	0.02%	0.003%
45	8.549	1222	1224	1225	rVB	228	120	0.01%	0.002%
46	8.586	1228	1230	1233	rVB	291	214	0.02%	0.003%
47	8.647	1233	1240	1257	rBV	497131	776911	81.27%	10.687%
48	8.952	1285	1290	1305	rBV	82956	129731	13.57%	1.785%
49	9.159	1322	1324	1326	rVB2	188	135	0.01%	0.002%
50	9.275	1337	1343	1350	rBV	2408	3852	0.40%	0.053%
51	9.384	1356	1361	1384	rBV	313301	479771	50.19%	6.599%
52	9.994	1458	1461	1465	rVB2	202	203	0.02%	0.003%
53	10.055	1465	1471	1491	rBV	441518	633651	66.29%	8.716%
54	10.268	1505	1506	1510	rBV2	182	198	0.02%	0.003%
55	10.305	1510	1512	1517	rVV3	434	674	0.07%	0.009%
56	10.616	1561	1563	1566	rBV2	132	117	0.01%	0.002%
57	10.646	1566	1568	1569	rBV	179	114	0.01%	0.002%
58	10.701	1576	1577	1579	rBV	160	135	0.01%	0.002%
59	10.799	1591	1593	1596	rBV2	98	119	0.01%	0.002%
60	10.823	1596	1597	1600	rBV	171	139	0.01%	0.002%
61	10.902	1608	1610	1612	rBV2	100	130	0.01%	0.002%
62	10.963	1617	1620	1623	rBV2	318	354	0.04%	0.005%
63	11.018	1626	1629	1631	rBV2	157	180	0.02%	0.002%
64	11.055	1633	1635	1638	rBV2	81	112	0.01%	0.002%
65	11.091	1638	1641	1645	rBV4	577	1006	0.11%	0.014%
66	11.189	1652	1657	1670	rBV	391834	503627	52.69%	6.928%
67	11.311	1673	1677	1682	rVV	2464	2947	0.31%	0.041%
68	11.347	1682	1683	1685	rVB	319	143	0.01%	0.002%
69	11.457	1697	1701	1705	rBV2	338	469	0.05%	0.006%
70	11.536	1711	1714	1716	rBV2	145	139	0.01%	0.002%
71	11.713	1740	1743	1745	rBV	322	266	0.03%	0.004%
72	11.762	1747	1751	1753	rBV3	409	484	0.05%	0.007%
73	11.908	1774	1775	1778	rBV2	118	120	0.01%	0.002%
74	11.975	1783	1786	1788	rVV2	490	497	0.05%	0.007%
75	12.018	1788	1793	1811	rVV	510123	658471	68.88%	9.058%
76	12.213	1824	1825	1831	rVB3	302	470	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX050924\
 Data File : VX041436.D
 Acq On : 09 May 2024 15:57
 Operator : JC/MD
 Sample : P2381-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML050924WMA.M
 Title : VOC Analysis

77	12.317	1837	1842	1860	rBV	562179	720323	75.35%	9.908%
78	12.762	1910	1915	1918	rVB2	310	338	0.04%	0.005%
79	12.786	1918	1919	1925	rVB2	155	152	0.02%	0.002%
80	12.926	1940	1942	1946	rVB2	133	112	0.01%	0.002%
81	12.969	1946	1949	1950	rVB	163	127	0.01%	0.002%
82	13.018	1954	1957	1960	rBV2	124	150	0.02%	0.002%
83	13.097	1965	1970	1971	rBV2	187	223	0.02%	0.003%
84	13.115	1971	1973	1979	rVB3	286	357	0.04%	0.005%
85	13.286	1997	2001	2002	rVB2	142	138	0.01%	0.002%
86	13.359	2010	2013	2017	rBV	128	200	0.02%	0.003%
87	13.408	2019	2021	2024	rBV2	141	192	0.02%	0.003%
88	13.548	2043	2044	2046	rBV2	172	133	0.01%	0.002%
89	13.603	2049	2053	2057	rBV4	479	789	0.08%	0.011%
90	13.780	2080	2082	2089	rBV2	452	822	0.09%	0.011%
91	13.853	2091	2094	2097	rBV	232	237	0.02%	0.003%
92	13.908	2101	2103	2105	rBV2	292	224	0.02%	0.003%
93	13.963	2110	2112	2116	rVB2	510	575	0.06%	0.008%
94	14.109	2131	2136	2138	rBV2	239	327	0.03%	0.004%
95	14.146	2141	2142	2145	rBV2	180	158	0.02%	0.002%
96	14.195	2148	2150	2151	rBV2	139	128	0.01%	0.002%
97	14.286	2163	2165	2166	rBV	179	116	0.01%	0.002%
98	14.316	2166	2170	2172	rBV3	206	333	0.03%	0.005%
99	14.408	2183	2185	2188	rBV3	206	229	0.02%	0.003%
100	14.853	2256	2258	2259	rBV2	277	162	0.02%	0.002%

Sum of corrected areas: 7269813




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX050924\
Data File : VX041436.D
Acq On : 09 May 2024 15:57
Operator : JC/MD
Sample : P2381-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML050924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

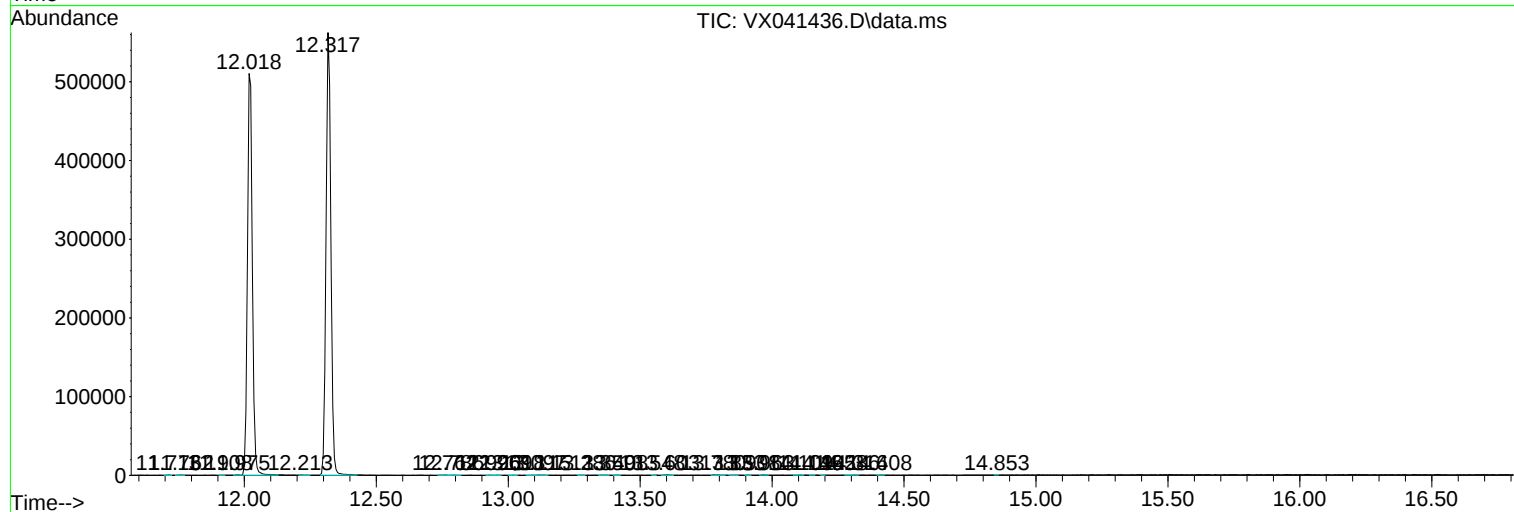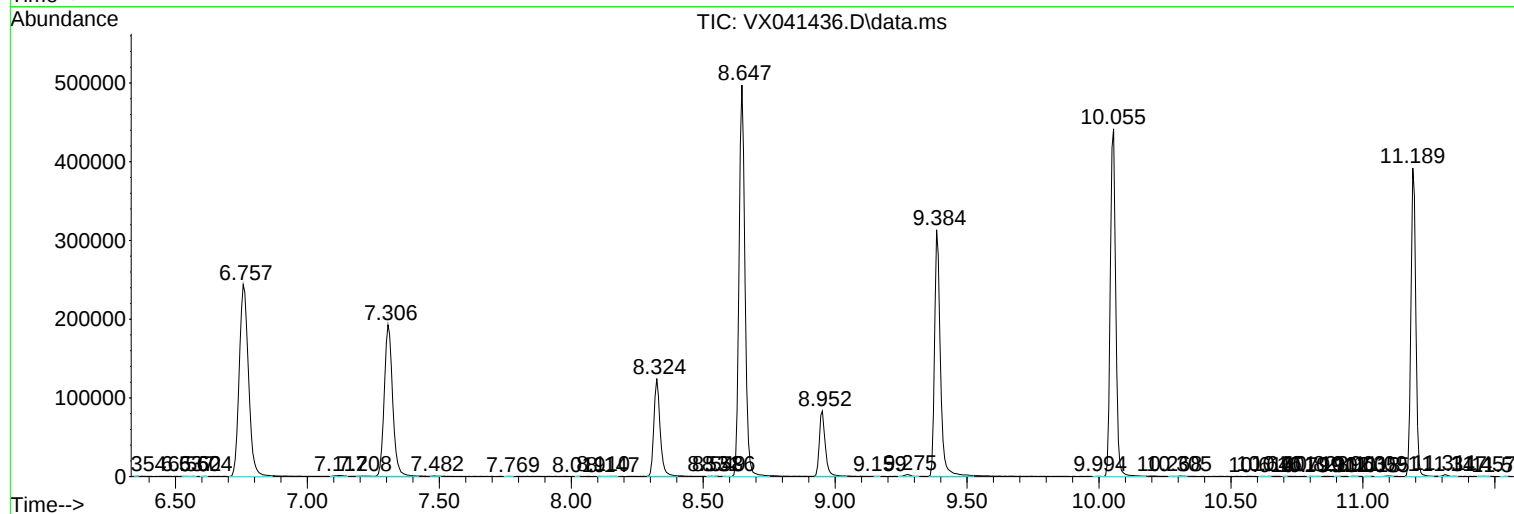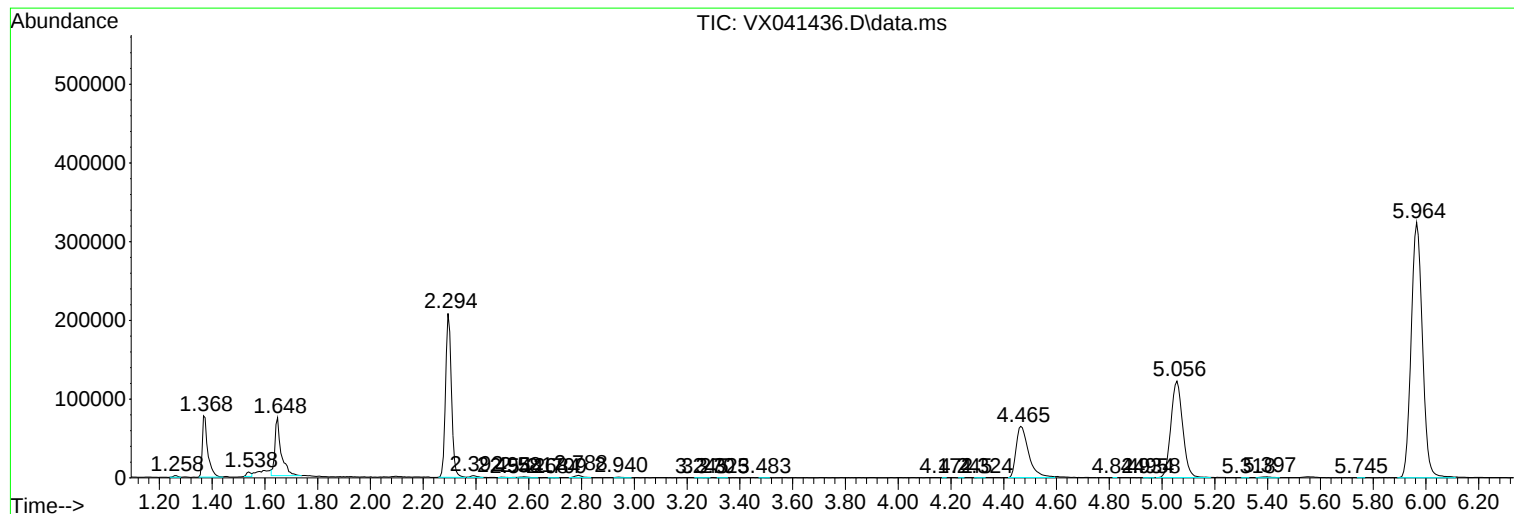

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX050924\
Data File : VX041436.D
Acq On : 09 May 2024 15:57
Operator : JC/MD
Sample : P2381-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML050924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX050924\
Data File : VX041436.D
Acq On : 09 May 2024 15:57
Operator : JC/MD
Sample : P2381-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML050924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc