
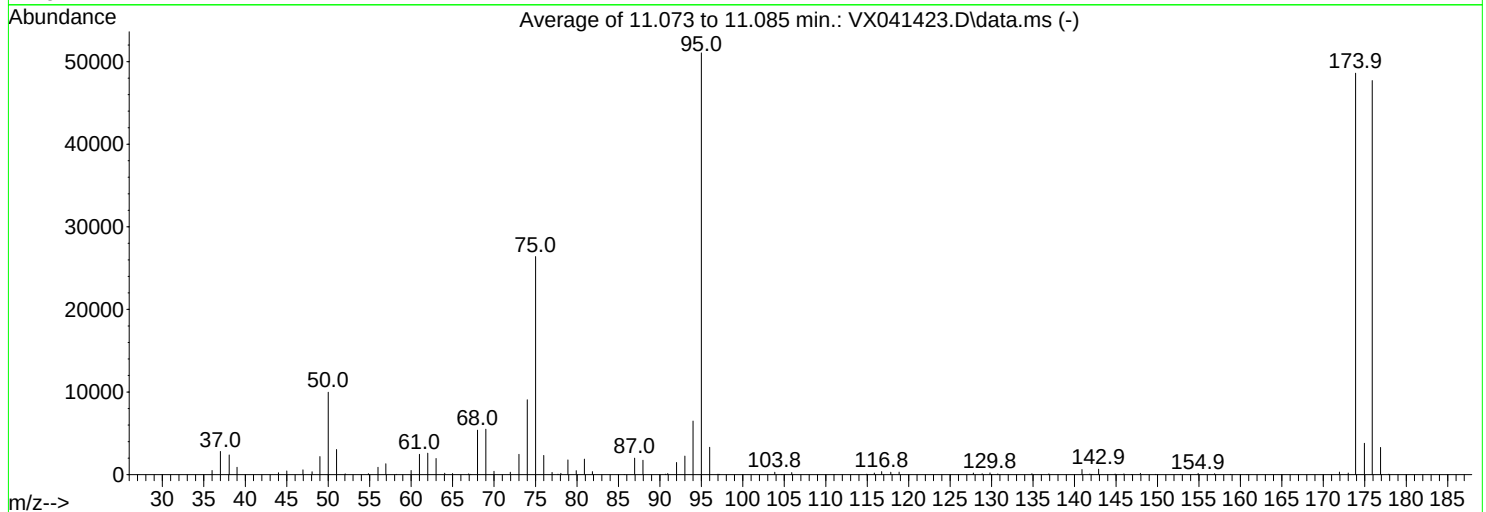


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX050924\
Data File : VX041423.D
Acq On : 09 May 2024 08:47
Operator : JC/MD
Sample : BFB675
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB675

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM050924WMA.M
Title : VOC Analysis
Last Update : Thu May 09 23:24:52 2024

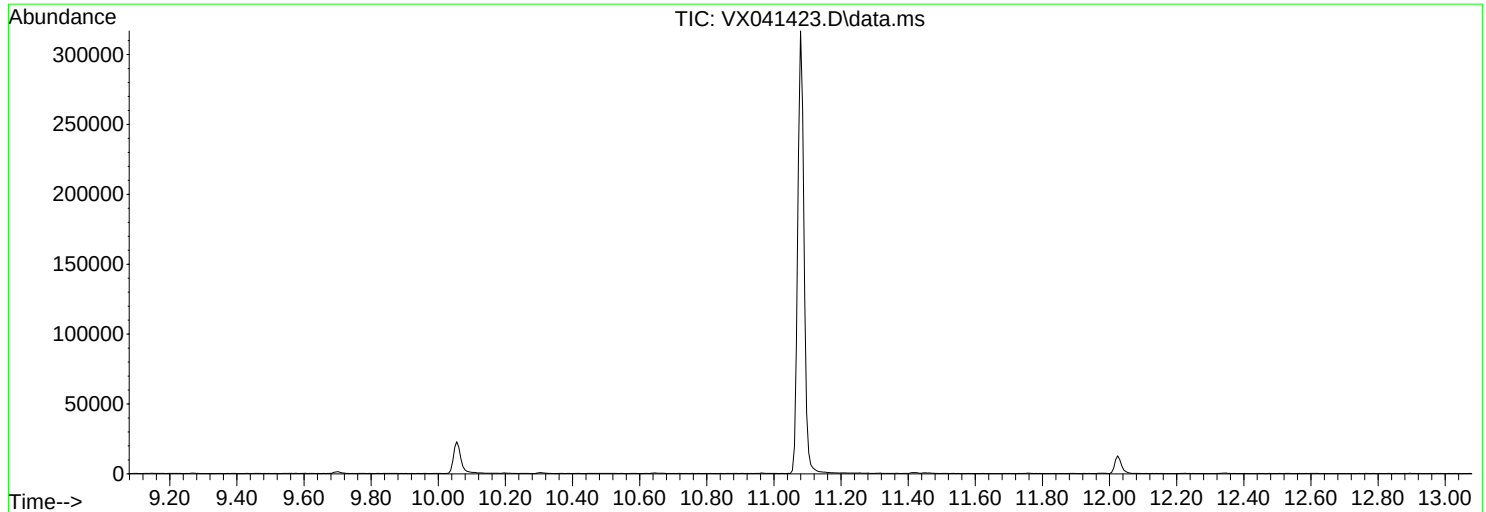

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.5	9969	PASS
75	95	30	80	51.7	26392	PASS
95	95	100	100	100.0	51061	PASS
96	95	5	9	6.5	3312	PASS
173	174	0.00	2	0.4	203	PASS
174	95	50	120	95.2	48595	PASS
175	174	5	9	7.8	3793	PASS
176	174	95	101	98.2	47709	PASS
177	176	5	9	6.9	3290	PASS

Scan 1633 (11.043 min): VX041423.D\data.ms
BFB675

m/z	Abundance
39.90	152.0
40.10	156.0
44.00	186.0

Instrument :
MSVOA_X
ClientSampleId :
BFB675

m/z	Abundance
36.00	447.0
37.00	2653.0
38.00	2434.0
39.00	948.0
39.90	199.0
44.10	353.0
45.00	468.0
47.00	536.0
48.00	346.0
49.00	2019.0
50.00	9739.0
51.00	2926.0
52.10	117.0
54.80	120.0
56.00	906.0
56.90	1243.0
60.00	502.0
61.00	2104.0
62.00	2498.0
63.00	1916.0
64.10	101.0
64.90	129.0
67.20	133.0
68.00	4826.0
69.00	5028.0
70.00	433.0
71.90	303.0
73.00	2428.0
74.00	8266.0
75.00	23392.0
76.00	2126.0
77.10	246.0
77.70	194.0
78.90	1667.0
80.00	476.0
80.90	1686.0
81.80	304.0
86.90	1788.0
87.90	1751.0
91.00	202.0
92.00	1226.0
93.00	1834.0
94.00	6024.0
95.00	45440.0
96.00	2906.0
97.00	169.0
103.90	274.0
105.10	74.0
105.90	231.0
115.00	60.0
115.90	193.0
116.70	324.0
117.90	186.0
118.80	304.0
127.80	202.0
128.80	67.0
129.90	138.0
130.90	76.0
134.90	118.0
136.90	83.0
140.90	574.0
141.80	96.0
142.90	593.0
144.90	66.0
145.90	121.0
147.90	91.0
155.00	131.0
156.90	51.0
172.00	229.0
173.90	36416.0
174.90	2937.0
175.90	36000.0
176.90	2812.0

Instrument :
MSVOA_X
ClientSampleId :
BFB675

m/z	Abundance
35.90	639.0
37.00	3468.0
38.10	2857.0
39.00	1037.0
40.00	143.0
44.00	509.0
45.00	591.0
47.00	723.0
48.10	420.0
49.00	2679.0
50.00	11747.0
51.00	3412.0
52.00	98.0
54.90	111.0
56.00	997.0
57.00	1585.0
58.20	98.0
60.00	503.0
61.00	3089.0
62.00	3049.0
63.00	2170.0
64.00	250.0
65.00	168.0
66.90	136.0
68.00	6183.0
69.00	6594.0
70.00	506.0
71.90	337.0
73.00	2766.0
74.00	11088.0
75.00	32008.0
76.00	2707.0
76.90	275.0
78.10	294.0
78.90	2132.0
79.80	527.0
80.90	2257.0
81.90	461.0
85.70	53.0
87.00	2270.0
88.00	2045.0
90.70	198.0
92.00	1724.0
93.00	2879.0
94.00	7636.0
95.00	59776.0
96.00	3999.0
97.20	104.0
103.80	360.0
104.70	85.0
105.00	68.0
105.90	281.0
111.00	72.0
114.80	80.0
115.70	216.0
116.80	440.0
117.90	294.0
118.90	333.0
127.90	210.0
128.90	120.0
129.70	231.0
130.70	111.0
134.80	113.0
136.90	110.0
140.90	677.0
141.90	118.0
142.90	775.0
144.90	119.0
146.00	75.0
146.90	54.0
147.90	227.0
149.80	56.0
152.80	70.0
154.80	151.0
156.90	124.0
158.80	79.0
160.80	72.0
171.90	355.0
173.90	57984.0
175.00	4464.0
175.90	55096.0
176.90	3823.0
177.90	105.0

Instrument :
MSVOA_X
ClientSampleId :
BFB675

m/z	Abundance
36.10	442.0
37.00	2291.0
38.00	1835.0
39.00	712.0
40.00	214.0
44.00	399.0
45.00	276.0
46.90	485.0
48.00	285.0
49.00	1861.0
50.00	8422.0
51.00	2772.0
52.00	94.0
54.90	134.0
56.00	779.0
57.00	1122.0
60.00	522.0
61.00	2199.0
62.00	2218.0
63.00	1787.0
64.00	163.0
65.10	111.0
67.00	137.0
68.00	5128.0
69.00	4885.0
70.10	260.0
72.00	262.0
73.00	2203.0
74.00	7859.0
75.00	23776.0
76.00	2145.0
77.00	284.0
78.00	161.0
78.90	1540.0
79.90	432.0
80.90	1707.0
81.90	371.0
86.90	1909.0
87.90	1428.0
90.90	190.0
92.00	1471.0
93.00	2000.0
94.00	5824.0
95.00	47968.0
96.00	3032.0
103.90	228.0
105.90	226.0
115.00	60.0
115.90	194.0
116.80	344.0
117.70	208.0
117.90	207.0
118.90	293.0
127.70	172.0
128.80	166.0
129.90	243.0
130.70	98.0
134.80	108.0
136.90	82.0
140.90	622.0
142.10	91.0
142.90	632.0
144.90	61.0
145.90	90.0
148.00	138.0
149.80	71.0
152.80	60.0
154.90	181.0
156.90	157.0
158.80	69.0
172.00	348.0
173.00	610.0
173.90	51384.0
175.00	3979.0
175.90	52032.0
176.90	3235.0
177.90	77.0

Instrument :
MSVOA_X
ClientSampleId :
BFB675