

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX051019\
 Data File : VX009473.D
 Acq On : 10 May 2019 11:18
 Operator : JC/SP
 Sample : K2803-01
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 SPDES-1

Quant Time: May 10 15:15:40 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA X\METHOD\624X050119W.M
 Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 QLast Update : Thu May 02 06:46:57 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Bromochloromethane	5.02	128	28779	30.00	ug/l	0.00
28) 1,4-Difluorobenzene	6.85	114	166003	30.00	ug/l	0.00
57) Chlorobenzene-d5	10.11	117	142910	30.00	ug/l	0.00

System Monitoring Compounds

27) 1,2-Dichloroethane-d4	6.06	65	71537	29.97	ug/l	0.00
Spiked Amount	30.000	Range	50 - 169	Recovery	=	99.90%
60) 4-Bromofluorobenzene	11.13	95	68201	28.08	ug/l	0.00
Spiked Amount	30.000	Range	56 - 143	Recovery	=	93.60%
63) Toluene-d8	8.71	98	204371	30.16	ug/l	0.00
Spiked Amount	30.000	Range	66 - 137	Recovery	=	100.53%


Target Compounds					Ovalue
25) Chloroform	5.20	83	6798	2.068 ug/l	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX051019\
Data File : VX009473.D
Acq On : 10 May 2019 11:18
Operator : JC/SP
Sample : K2803-01
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SPDES-1

Quant Time: May 10 15:15:40 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA X\METHOD\624X050119W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
QLast Update : Thu May 02 06:46:57 2019
Response via : Initial Calibration

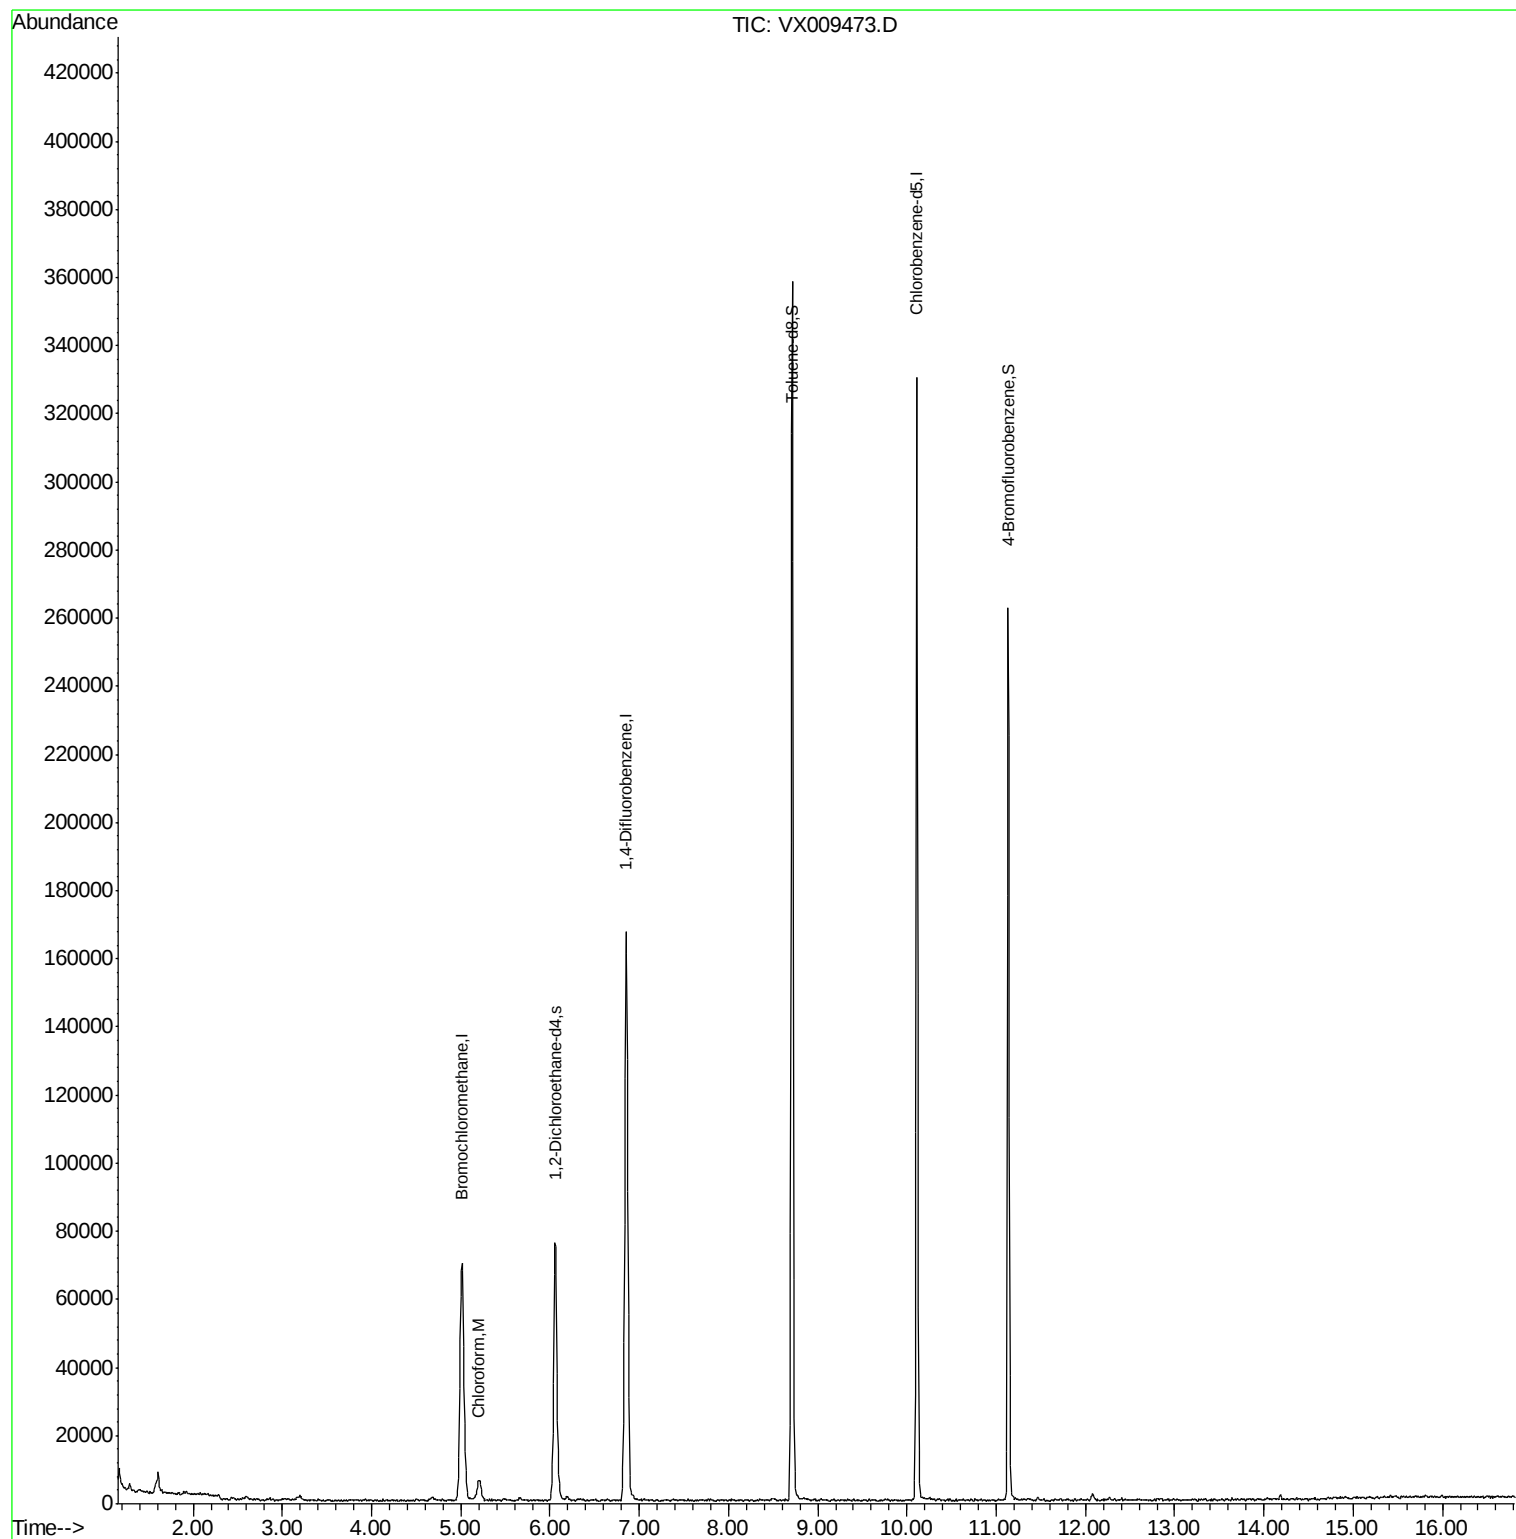

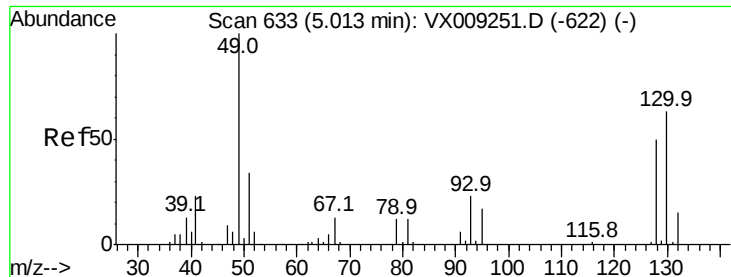

#1

Bromochloromethane

Concen: 30.000 ug/l

RT: 5.02 min Scan# 634

Delta R.T. 0.01 min

Lab File: VX009473.D

Acq: 10 May 2019 11:18

Instrument :

MSVOA_X

ClientSampleId :

SPDES-1


Tot Ion:128 Resp: 28779

Ion Ratio Lower Upper

128 100

49 198.6 0.0 515.0




130 130.7 0.0 323.3

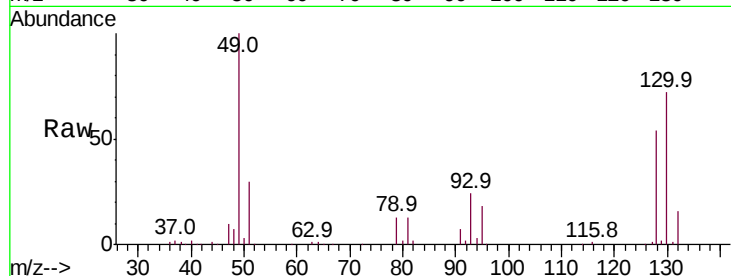

Abundance Ion 128.00 (127.70 to 128.70): V

Ion 49.00 (48.70 to 49.70): VX0

Ion 130.00 (129.70 to 130.70): V

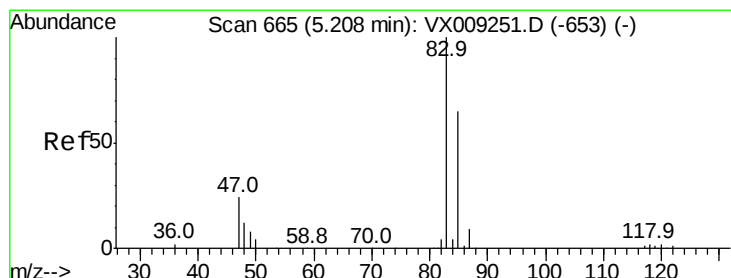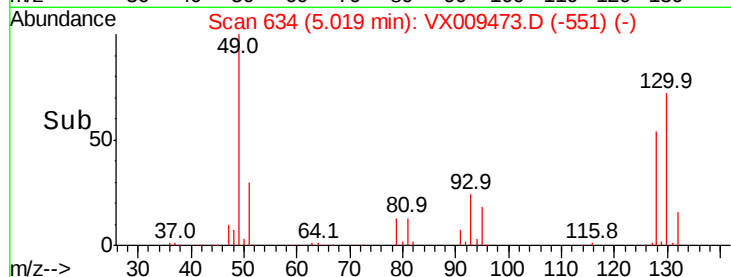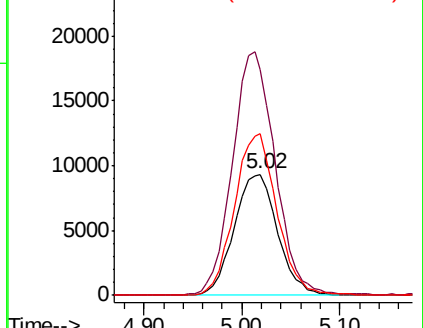

#25

Chloroform

Concen: 2.068 ug/l

RT: 5.20 min Scan# 664

Delta R.T. -0.01 min

Lab File: VX009473.D


Acq: 10 May 2019 11:18

Tgt Ion: 83 Resp: 6798

Ion Ratio Lower Upper



83 100


85 66.2 51.9 77.9

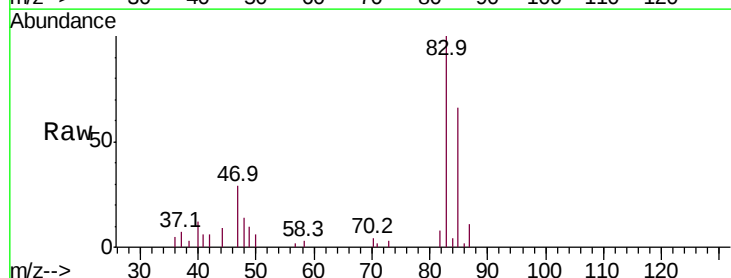

Abundance Ion 83.00 (82.70 to 83.70): VX0

Ion 85.00 (84.70 to 85.70): VX0



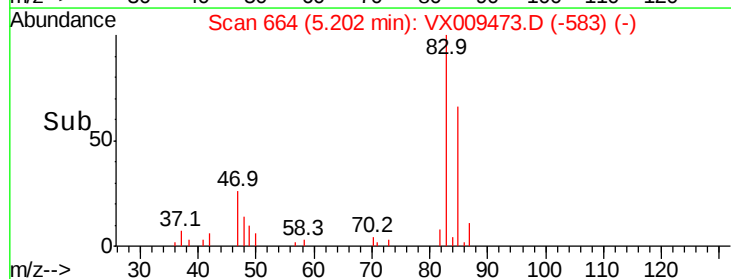
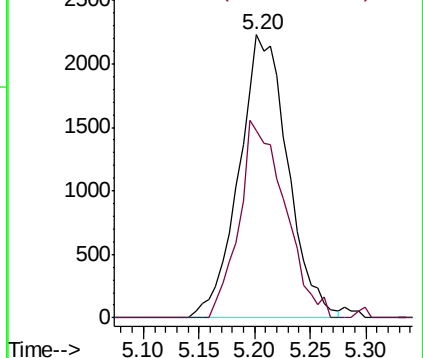


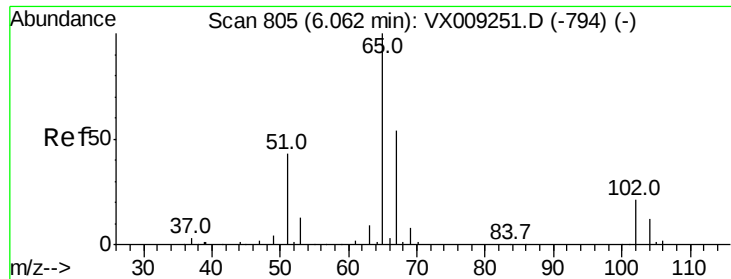

#27
 1,2-Dichloroethane-d4
 Concen: 29.965 ug/l
 RT: 6.06 min Scan# 804
 Delta R.T. -0.01 min
 Lab File: VX009473.D
 Acq: 10 May 2019 11:18




Instrument :
 MSVOA_X
 ClientSampleId :
 SPDES-1


Tot Ion: 65 Resp: 71537
 Ion Ratio Lower Upper
 65 100
 67 54.0 43.1 64.7

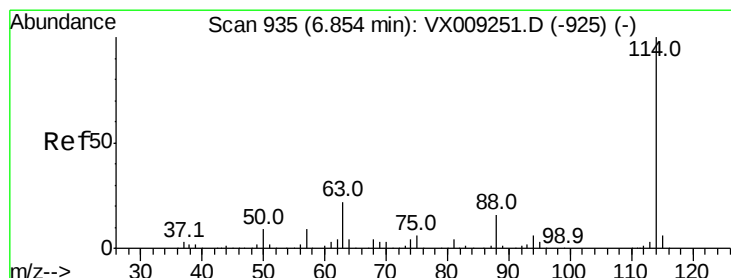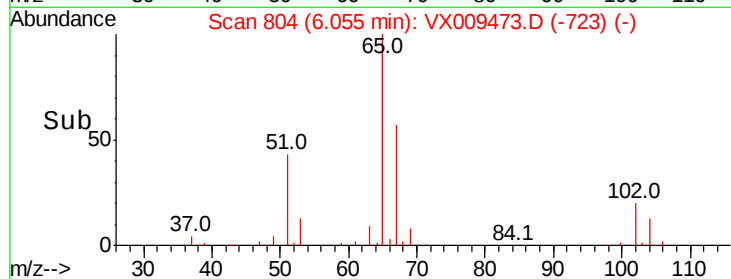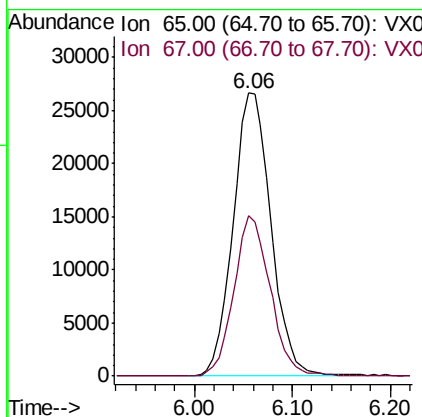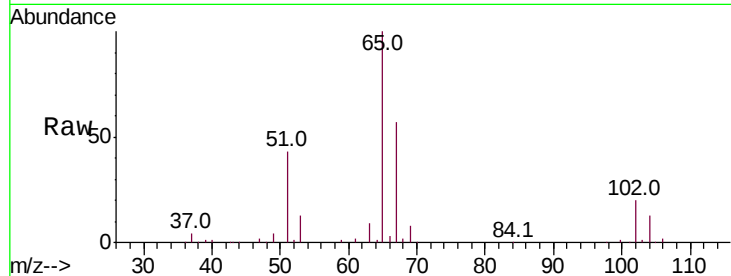

#28
 1,4-Difluorobenzene
 Concen: 30.000 ug/l
 RT: 6.85 min Scan# 935
 Delta R.T. -0.00 min
 Lab File: VX009473.D
 Acq: 10 May 2019 11:18

Tgt Ion: 114 Resp: 166003
 Ion Ratio Lower Upper
 114 100
 63 23.1 18.0 27.0
 88 16.2 13.4 20.0

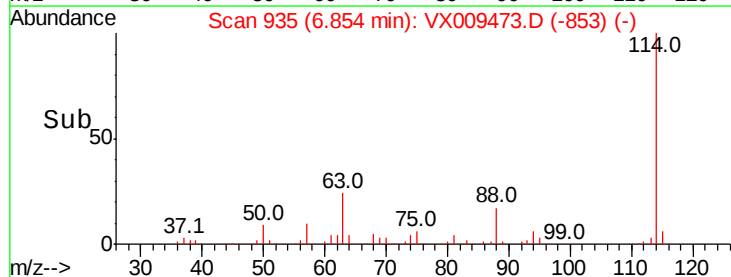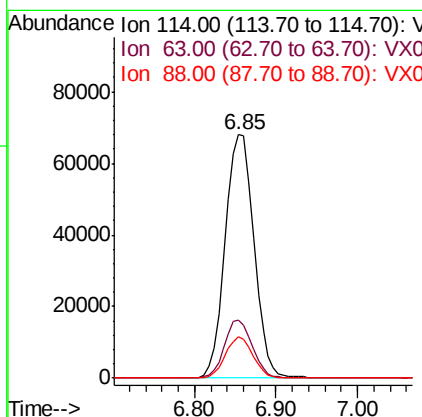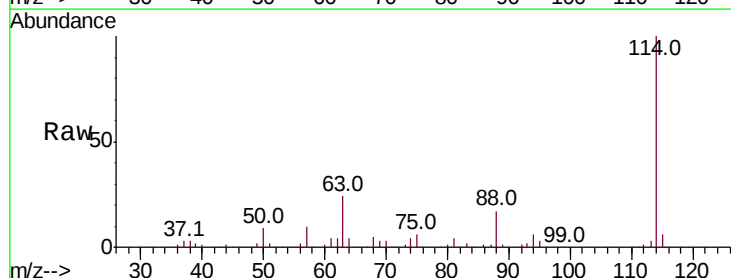


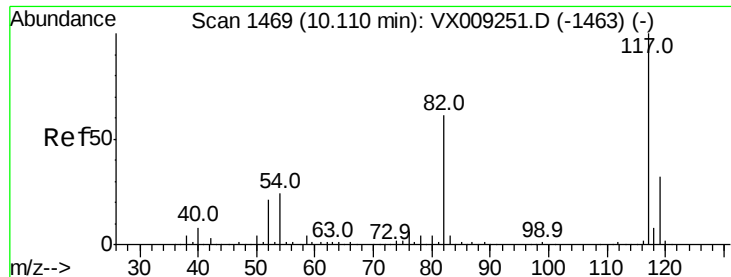




#57
Chlorobenzene-d5
Concen: 30.000 ug/l
RT: 10.11 min Scan# 1469
Delta R.T. -0.00 min
Lab File: VX009473.D
Acq: 10 May 2019 11:18

Instrument :
MSVOA_X
ClientSampleId :
SPDES-1

Tot Ion:117 Resp: 142910
Ion Ratio Lower Upper
117 100
82 59.4 47.8 71.8
119 32.6 25.6 38.4

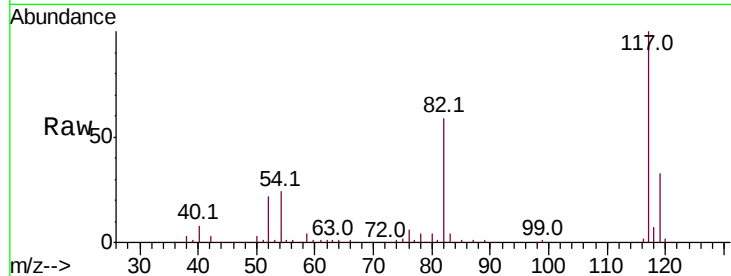


Abundance Ion 117.00 (116.70 to 117.70): V
Ion 82.00 (81.70 to 82.70): VX0
Ion 119.00 (118.70 to 119.70): V

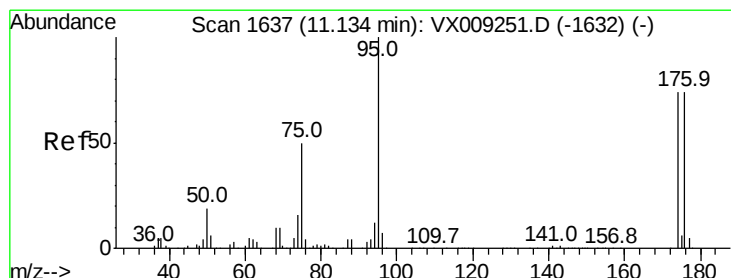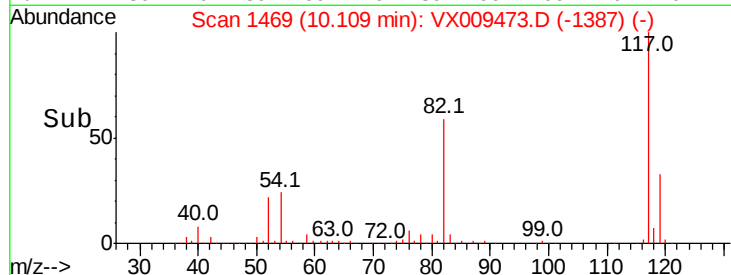
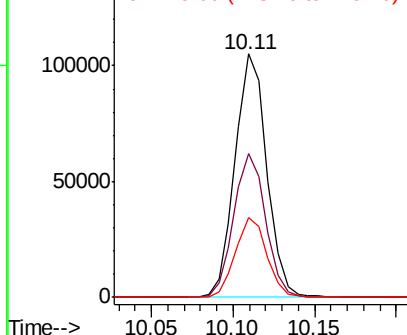



#60
4-Bromofluorobenzene
Concen: 28.085 ug/l
RT: 11.13 min Scan# 1637
Delta R.T. -0.00 min
Lab File: VX009473.D
Acq: 10 May 2019 11:18

Tgt Ion: 95 Resp: 68201
Ion Ratio Lower Upper
95 100
174 81.8 63.6 95.4
176 79.6 62.4 93.6

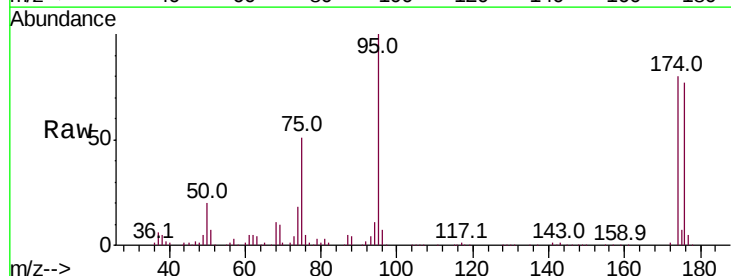

Abundance Ion 95.00 (94.70 to 95.70): VX0
Ion 174.00 (173.70 to 174.70): V
Ion 176.00 (175.70 to 176.70): V

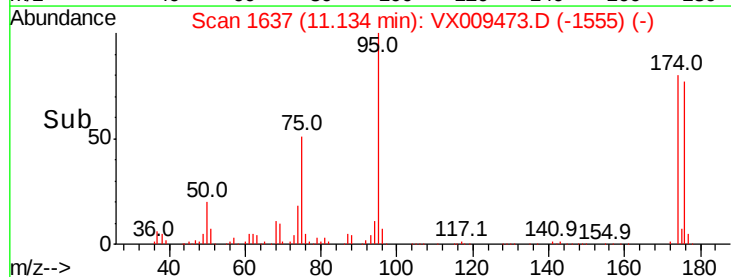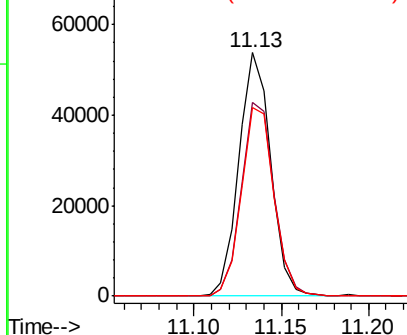

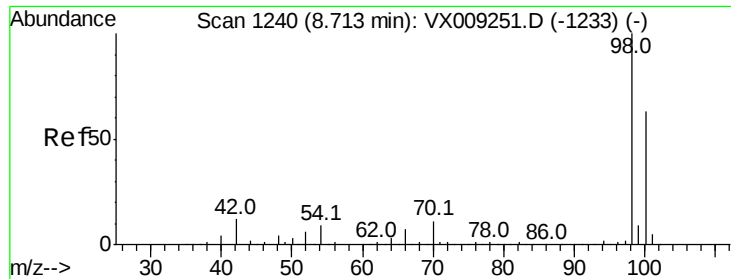

#63

Toluene-d8

Concen: 30.163 ug/l

RT: 8.71 min Scan# 1240

Delta R.T. -0.00 min

Lab File: VX009473.D

Acq: 10 May 2019 11:18

Instrument :

MSVOA_X

ClientSampleId :

SPDES-1

Tot Ion: 98 Resp: 204371

Ion Ratio Lower Upper

98 100

100 64.3 52.3 78.5

