


Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX051019\
Data File : VX009483.D
Acq On : 10 May 2019 15:31
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X042919W.M
Title : SW846 8260
Last Update : Thu May 09 07:31:15 2019

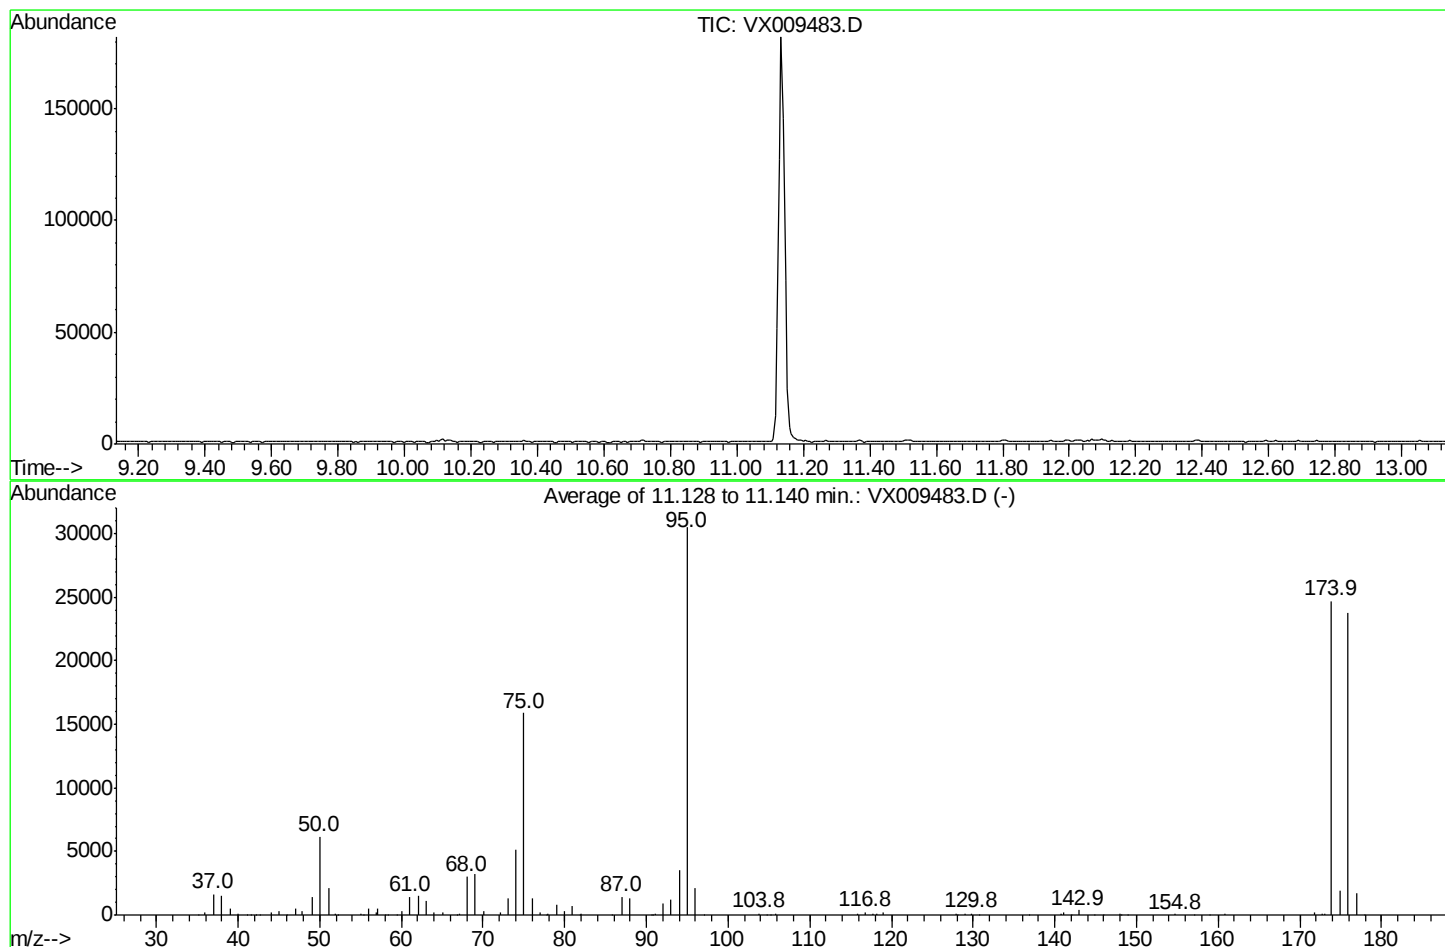

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1629

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.3	6194	PASS
75	95	30	60	52.1	15908	PASS
95	95	100	100	100.0	30509	PASS
96	95	5	9	6.9	2120	PASS
173	174	0.00	2	0.5	127	PASS
174	95	50	100	80.9	24696	PASS
175	174	5	9	7.8	1920	PASS
176	174	95	101	96.4	23802	PASS
177	176	5	9	7.0	1672	PASS