


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051021\
 Data File : VX021880.D
 Acq On : 10 May 2021 16:43
 Operator : JC/MD
 Sample : BFB69
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB169

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR051021WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Tue May 11 02:59:37 2021

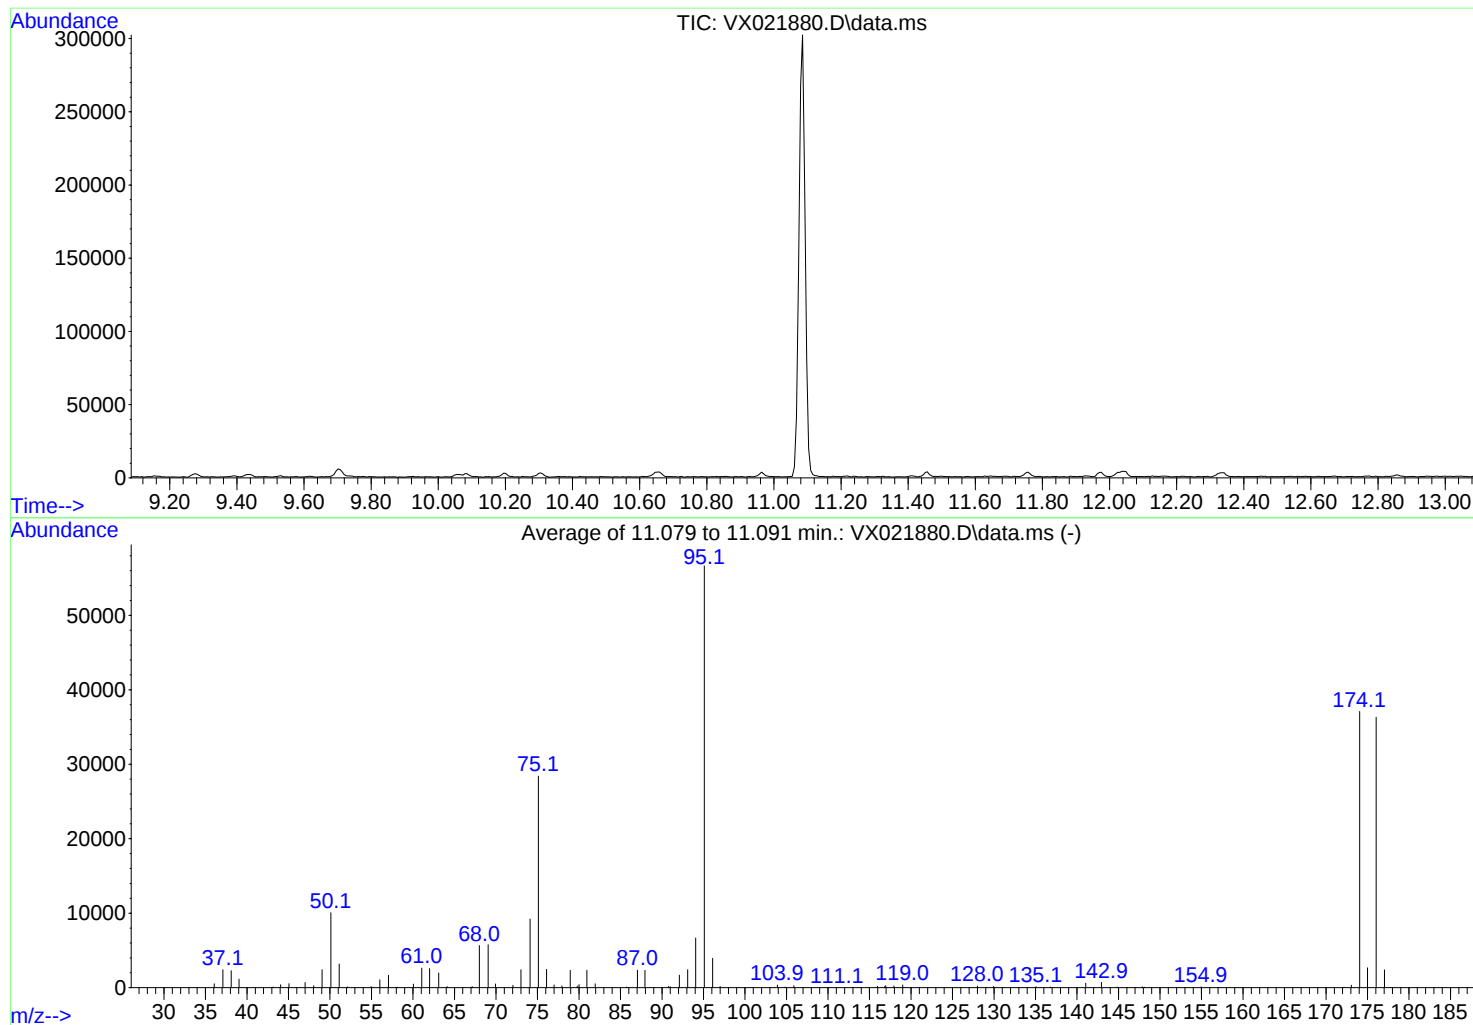

AutoFind: Scans 1639, 1640, 1641; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.7	10053	PASS
75	95	30	80	50.2	28416	PASS
95	95	100	100	100.0	56648	PASS
96	95	5	9	6.9	3925	PASS
173	174	0.00	2	0.9	332	PASS
174	95	50	120	65.5	37091	PASS
175	174	5	9	7.2	2666	PASS
176	174	95	105	97.9	36307	PASS
177	176	5	10	6.6	2387	PASS

m/z	Abundance
39.90	183.0
41.00	66.0
44.00	544.0

Instrument :
MSVOA_X
ClientSampleId :
BFB169

m/z	Abundance
36.00	431.0
37.00	1501.0
38.10	1623.0
39.00	857.0
39.90	144.0
41.10	51.0
43.20	113.0
44.10	863.0
45.00	365.0
45.90	52.0
47.10	510.0
48.10	227.0
49.10	1718.0
50.00	7088.0
51.10	2280.0
52.20	77.0
55.20	205.0
56.10	744.0
57.10	1273.0
58.10	74.0
60.00	269.0
61.00	1980.0
62.00	1682.0
63.10	1390.0
64.00	107.0
67.10	172.0
68.00	4188.0
69.10	3904.0
70.00	395.0
72.00	239.0
73.10	1591.0
74.10	6452.0
75.10	19952.0
76.10	1818.0
77.00	335.0
78.00	255.0
79.00	1617.0
80.00	495.0
81.00	1699.0
82.00	415.0
86.00	89.0
87.00	1694.0
88.00	1456.0
90.80	206.0
92.10	1016.0
93.10	1701.0
94.10	5103.0
95.10	42984.0
96.00	2831.0
97.00	141.0
103.80	272.0
104.90	58.0
105.90	140.0
112.00	81.0
113.00	58.0
115.00	80.0
115.90	189.0
116.90	335.0
118.00	177.0
119.00	243.0
128.10	190.0
129.90	222.0
131.10	55.0
135.10	136.0
141.00	466.0
143.00	666.0
144.90	87.0
147.90	153.0
155.00	112.0
171.90	63.0
173.10	305.0
174.10	32800.0
175.00	2351.0
176.10	32864.0
177.00	2118.0

Instrument :
MSVOA_X
ClientSampleId :
BFB169

m/z	Abundance
36.10	602.0
37.10	2628.0
38.10	2680.0
39.00	1219.0
40.00	174.0
43.10	53.0
44.10	797.0
45.10	704.0
46.00	65.0
47.00	757.0
48.00	273.0
49.00	2806.0
50.10	11769.0
51.10	3601.0
52.10	125.0
54.90	216.0
56.00	1109.0
57.00	1738.0
58.10	118.0
60.00	617.0
61.00	2990.0
62.00	2974.0
63.10	2146.0
64.20	224.0
67.20	191.0
68.00	6691.0
69.00	6742.0
69.90	619.0
72.10	374.0
73.00	3000.0
74.10	10603.0
75.10	33112.0
76.10	2810.0
77.00	418.0
77.90	215.0
79.00	2697.0
80.00	716.0
80.90	2811.0
81.90	605.0
83.00	69.0
85.80	161.0
87.00	2739.0
88.00	3156.0
91.00	308.0
92.10	2268.0
93.10	3014.0
94.00	7827.0
95.10	67072.0
96.10	4395.0
97.00	122.0
103.90	429.0
104.80	55.0
105.90	284.0
107.00	94.0
113.00	63.0
114.90	62.0
116.00	225.0
117.00	529.0
117.90	273.0
119.00	484.0
128.00	254.0
129.00	110.0
130.00	144.0
131.10	67.0
135.00	158.0
136.80	160.0
141.00	774.0
142.10	83.0
142.90	816.0
144.90	88.0
146.00	55.0
147.80	163.0
155.00	119.0
157.10	66.0
172.10	144.0
173.00	388.0
174.00	44408.0
175.00	3143.0
176.00	42752.0
177.10	2875.0
177.80	61.0

Instrument :
MSVOA_X
ClientSampleId :
BFB169

m/z	Abundance
36.00	484.0
37.10	3114.0
38.10	2522.0
39.10	1371.0
39.90	191.0
41.20	123.0
43.10	110.0
44.10	1112.0
45.00	551.0
47.00	808.0
48.10	300.0
49.10	2676.0
50.10	11302.0
51.10	3675.0
52.00	102.0
55.00	263.0
56.00	1342.0
57.10	1972.0
57.90	152.0
60.10	531.0
61.10	2871.0
62.00	3030.0
63.10	2411.0
64.10	130.0
67.00	192.0
68.00	6046.0
69.10	6637.0
70.00	443.0
72.00	355.0
73.00	2629.0
74.10	10593.0
75.10	32184.0
76.10	2750.0
77.00	352.0
78.00	262.0
78.90	2640.0
79.80	650.0
81.00	2523.0
81.90	498.0
83.00	61.0
85.70	103.0
87.10	2591.0
87.90	2354.0
90.80	317.0
92.10	1725.0
93.10	2516.0
94.10	7026.0
95.10	59888.0
96.10	4550.0
97.00	165.0
104.00	338.0
104.90	138.0
105.90	366.0
111.10	91.0
113.00	96.0
115.00	59.0
116.00	202.0
116.80	392.0
118.00	244.0
119.00	345.0
127.90	234.0
129.10	79.0
130.00	95.0
135.00	90.0
136.80	110.0
141.10	551.0
142.10	74.0
143.00	635.0
144.80	64.0
146.10	58.0
148.10	168.0
148.80	68.0
154.90	103.0
172.20	59.0
173.00	303.0
174.00	34064.0
175.00	2503.0
176.00	33304.0
177.00	2167.0

Instrument :
MSVOA_X
ClientSampleId :
BFB169