

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051023\
 Data File : VX035579.D
 Acq On : 10 May 2023 12:02
 Operator : JC/MD
 Sample : VX0510WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0510WBL01

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X042523W.M
 Title : SW846 8260

Signal : TIC: VX035579.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.385	692	705	719	rBV2	170062	502060	34.46%	5.543%
2	5.550	719	732	746	rVV	296080	833504	57.22%	9.202%
3	5.952	788	798	812	rBV	166722	441157	30.28%	4.871%
4	6.757	919	930	948	rBV	447841	1077888	73.99%	11.900%
5	8.647	1232	1240	1256	rBV	936703	1456767	100.00%	16.083%
6	10.055	1465	1471	1480	rBV	913042	1280202	87.88%	14.134%
7	11.079	1634	1639	1650	rVB	847806	1046903	71.86%	11.558%
8	12.018	1788	1793	1803	rBV	1032625	1304809	89.57%	14.406%
9	13.542	2031	2043	2055	rBV5	21254	79905	5.49%	0.882%
10	14.024	2117	2122	2129	rVB8	6434	15460	1.06%	0.171%
11	15.182	2303	2312	2316	rBV6	27404	73193	5.02%	0.808%
12	15.255	2321	2324	2328	rVV3	18910	25316	1.74%	0.280%
13	15.323	2332	2335	2340	rVB2	14054	18167	1.25%	0.201%
14	15.542	2364	2371	2381	rBV	268803	407741	27.99%	4.502%
15	15.688	2391	2395	2405	rVB9	13866	33268	2.28%	0.367%
16	15.981	2438	2443	2446	rBV7	10774	19391	1.33%	0.214%
17	16.469	2516	2523	2536	rVB	227866	418373	28.72%	4.619%
18	16.645	2548	2552	2563	rVB	8810	23450	1.61%	0.259%




Sum of corrected areas: 9057554

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051023\
Data File : VX035579.D
Acq On : 10 May 2023 12:02
Operator : JC/MD
Sample : VX0510WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0510WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X042523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

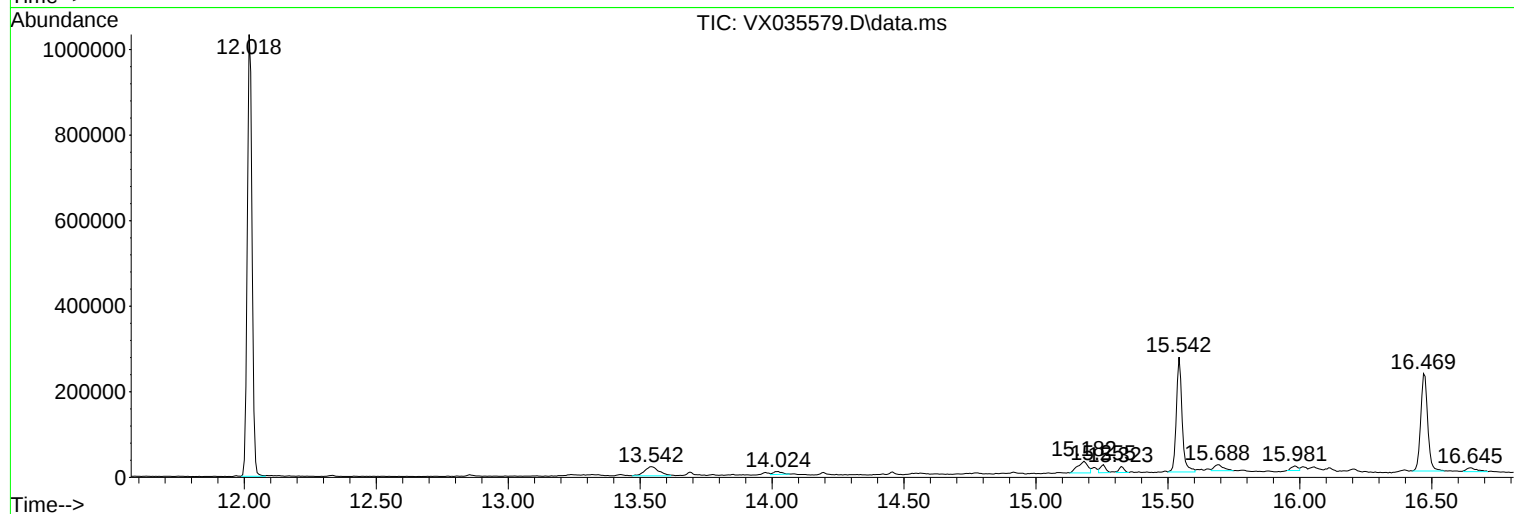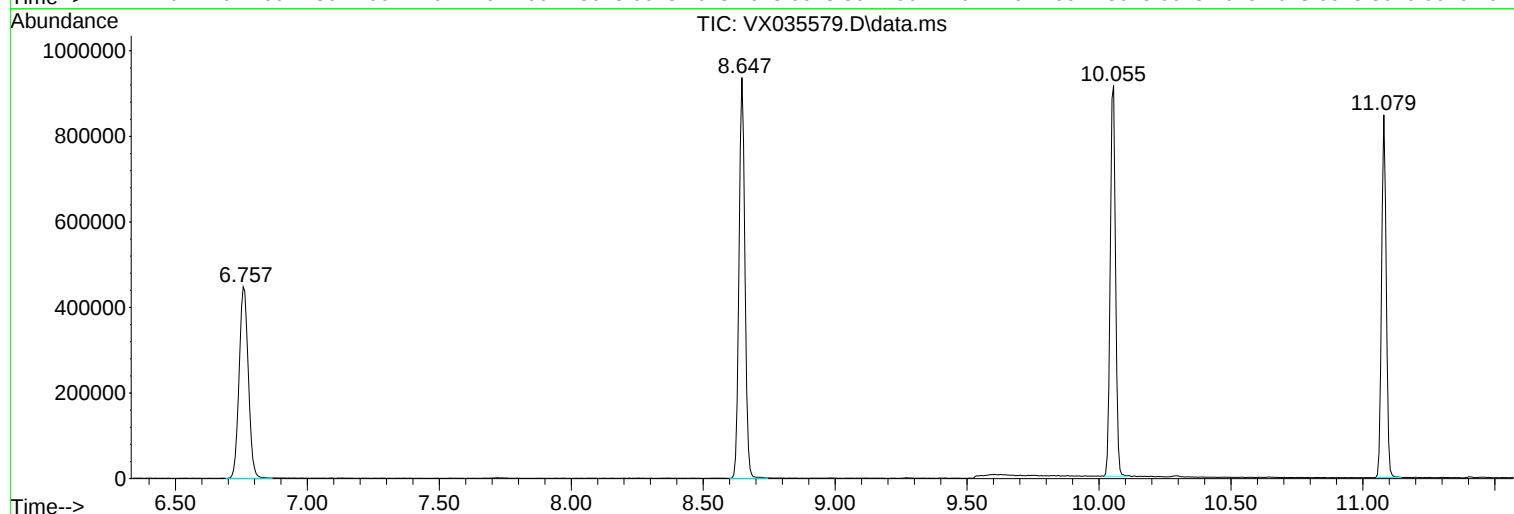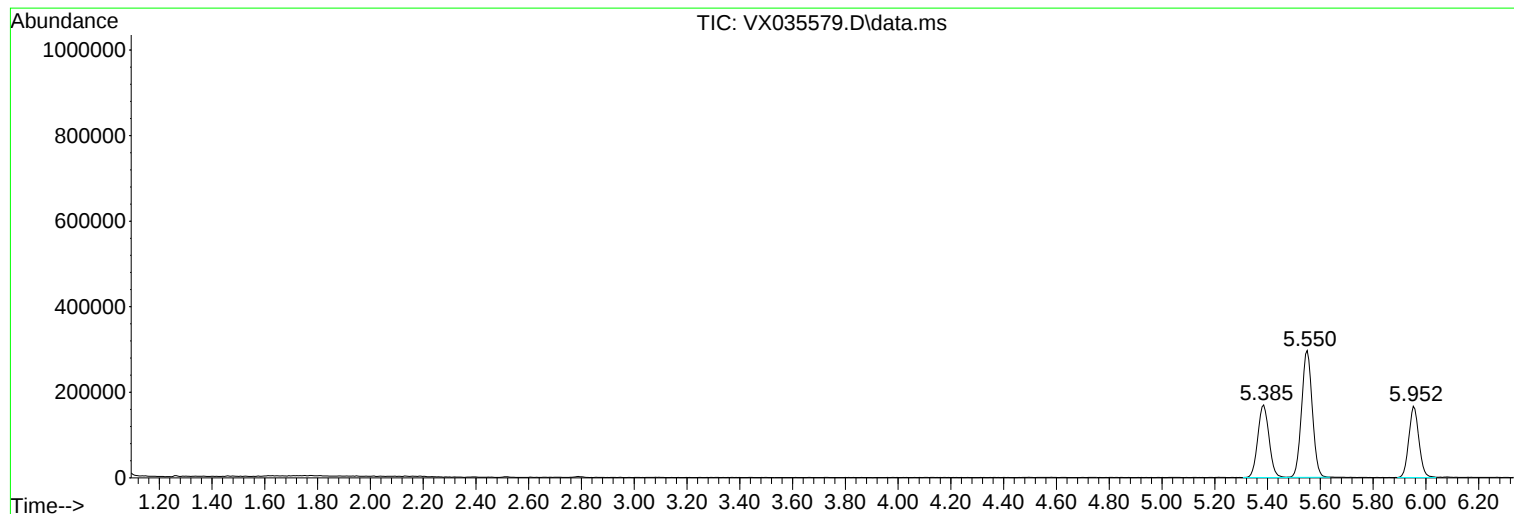

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051023\
Data File : VX035579.D
Acq On : 10 May 2023 12:02
Operator : JC/MD
Sample : VX0510WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0510WBL01










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X042523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Dodecane, 1-chloro- Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
15.542	15.62 ug/l	407741	1,4-Dichlorobenzene-d4	12.018

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Dodecane, 1-chloro-	204	C12H25Cl	000112-52-7	96
2			1-Chloroundecane	190	C11H23Cl	002473-03-2	91
3			Decane, 1-chloro-	176	C10H21Cl	001002-69-3	80
4			Tetradecane, 1-chloro-	232	C14H29Cl	002425-54-9	53
5			Nonane, 1-chloro-	162	C9H19Cl	002473-01-0	47

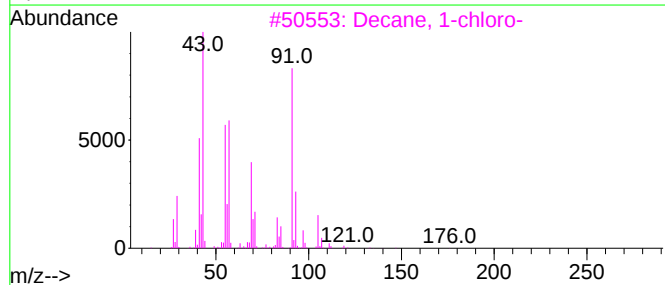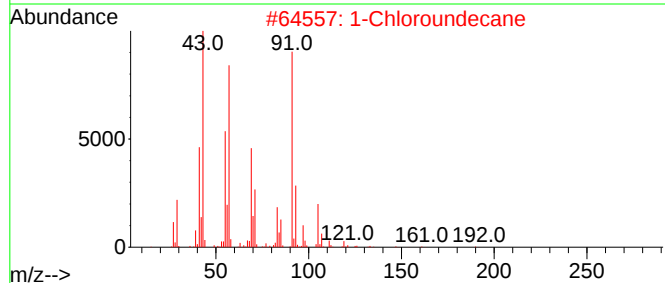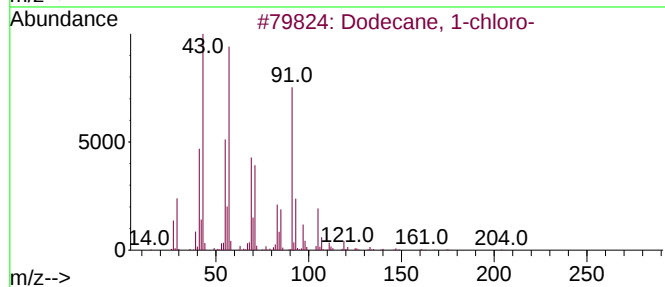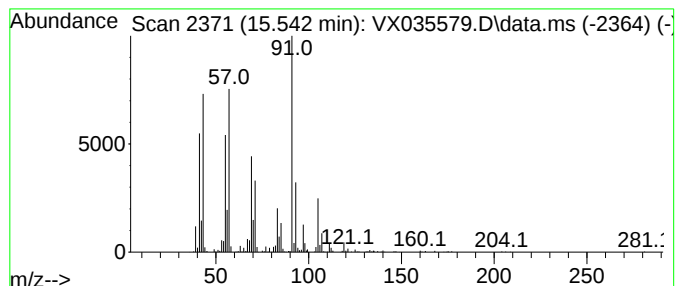

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051023\
Data File : VX035579.D
Acq On : 10 May 2023 12:02
Operator : JC/MD
Sample : VX0510WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0510WBL01










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X042523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Tetradecane, 1-chloro- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
16.469	16.03 ug/l	418373	1,4-Dichlorobenzene-d4	12.018

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Dodecane, 1-chloro-	204	C12H25Cl	000112-52-7	91
2			Tetradecane, 1-chloro-	232	C14H29Cl	002425-54-9	87
3			1-Chloroundecane	190	C11H23Cl	002473-03-2	64
4			1-Decanol, 2-hexyl-	242	C16H34O	002425-77-6	49
5			Oxalic acid, allyl dodecyl ester	298	C17H30O4	1000309-24-0	49

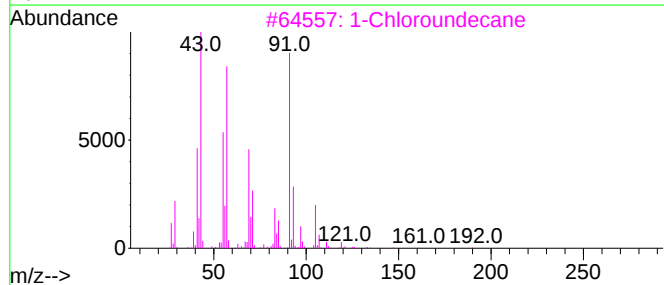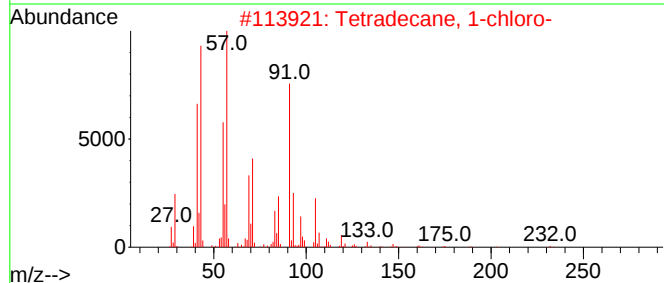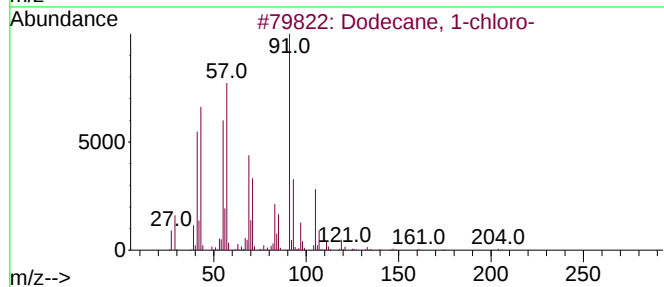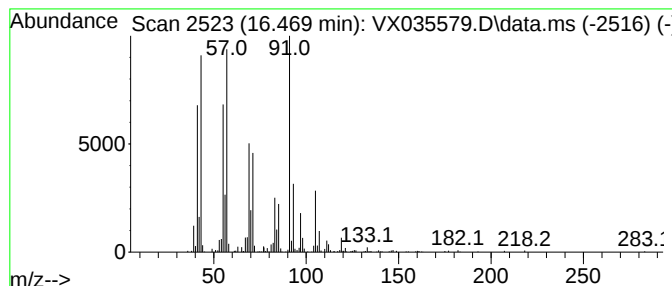

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051023\
Data File : VX035579.D
Acq On : 10 May 2023 12:02
Operator : JC/MD
Sample : VX0510WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0510WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X042523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Dodecane, 1-chl...	15.542	15.6	ug/l	407741	4	12.018	1304810	50.0
Tetradecane, 1-...	16.469	16.0	ug/l	418373	4	12.018	1304810	50.0