

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051023\
 Data File : VX035587.D
 Acq On : 10 May 2023 15:37
 Operator : JC/MD
 Sample : 02648-03DL 5X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 ORA-1636DL

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X042523W.M
 Title : SW846 8260

Signal : TIC: VX035587.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.142	6	9	19	rVB	37304	38025	2.17%	0.245%
2	1.264	26	29	41	rBV	116254	116811	6.68%	0.754%
3	1.373	41	47	53	rVV	575125	659469	37.70%	4.254%
4	1.428	53	56	58	rVV	53464	54179	3.10%	0.349%
5	1.453	58	60	64	rVV	26795	29629	1.69%	0.191%
6	1.495	64	67	74	rVB	49298	53694	3.07%	0.346%
7	1.751	104	109	121	rVB	184826	246007	14.06%	1.587%
8	1.959	138	143	154	rVV3	76403	152053	8.69%	0.981%
9	2.068	156	161	168	rVV	56492	99618	5.69%	0.643%
10	2.166	172	177	181	rVV	33786	64225	3.67%	0.414%
11	2.215	181	185	195	rVB	111924	171774	9.82%	1.108%
12	2.385	208	213	222	rVB	13046	25260	1.44%	0.163%
13	2.751	262	273	277	rBV	38296	77057	4.40%	0.497%
14	2.867	287	292	304	rVB	41666	91848	5.25%	0.592%
15	3.111	318	332	347	rVB2	43679	109354	6.25%	0.705%
16	3.745	429	436	445	rVB5	7274	24293	1.39%	0.157%
17	4.300	520	527	541	rVB2	24212	69996	4.00%	0.452%
18	4.562	559	570	585	rBV	11971	35787	2.05%	0.231%
19	5.196	663	674	686	rVB4	8855	28287	1.62%	0.182%
20	5.385	691	705	714	rBV2	173422	506398	28.95%	3.267%
21	5.470	714	719	722	rVV3	18108	45311	2.59%	0.292%
22	5.549	723	732	751	rVB	308385	873950	49.95%	5.638%
23	5.952	788	798	804	rBV	175398	447699	25.59%	2.888%
24	6.037	804	812	827	rVB	664029	1749482	100.00%	11.285%
25	6.238	833	845	854	rVB10	5930	23389	1.34%	0.151%
26	6.757	920	930	946	rBV	461355	1109053	63.39%	7.154%
27	8.646	1232	1240	1246	rBV	938640	1502296	85.87%	9.691%
28	8.720	1246	1252	1260	rVB	809991	1274244	72.84%	8.220%
29	10.055	1465	1471	1478	rBV	956568	1320105	75.46%	8.516%
30	10.195	1489	1494	1499	rBV	26033	34593	1.98%	0.223%
31	10.299	1505	1511	1520	rVB	144415	197303	11.28%	1.273%
32	10.640	1562	1567	1573	rBV	117336	151126	8.64%	0.975%
33	11.079	1634	1639	1650	rBV	841198	1070348	61.18%	6.904%
34	11.378	1683	1688	1690	rBV	30795	40079	2.29%	0.259%
35	11.451	1696	1700	1706	rVB	34020	40786	2.33%	0.263%
36	11.609	1722	1726	1732	rVB	19344	24434	1.40%	0.158%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051023\
 Data File : VX035587.D
 Acq On : 10 May 2023 15:37
 Operator : JC/MD
 Sample : 02648-03DL 5X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 ORA-1636DL

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X042523W.M
 Title : SW846 8260

37	11.750	1745	1749	1755	rVB	51154	63658	3.64%	0.411%
38	12.018	1788	1793	1800	rBV	1037296	1330649	76.06%	8.584%
39	12.085	1800	1804	1809	rVB	48118	56983	3.26%	0.368%
40	12.243	1822	1830	1833	rBV2	29164	46522	2.66%	0.300%
41	12.316	1837	1842	1849	rVB2	29126	41473	2.37%	0.268%
42	12.609	1886	1890	1894	rBV	30249	37106	2.12%	0.239%
43	12.701	1900	1905	1914	rVB3	16669	28890	1.65%	0.186%
44	12.847	1924	1929	1934	rVB3	15628	20662	1.18%	0.133%
45	12.920	1934	1941	1944	rBV2	22892	29271	1.67%	0.189%
46	12.963	1944	1948	1953	rVB	31680	38049	2.17%	0.245%
47	13.292	1997	2002	2007	rVB2	49726	64354	3.68%	0.415%
48	13.420	2019	2023	2030	rVB	25841	35839	2.05%	0.231%
49	13.548	2039	2044	2047	rVV4	26942	54251	3.10%	0.350%
50	13.585	2047	2050	2056	rVV3	23000	41334	2.36%	0.267%
51	13.664	2060	2063	2070	rVB3	13452	26443	1.51%	0.171%
52	14.072	2126	2130	2135	rVB	14286	18889	1.08%	0.122%
53	14.225	2146	2155	2160	rBV5	24533	69165	3.95%	0.446%
54	14.371	2175	2179	2183	rVB2	15049	18597	1.06%	0.120%
55	14.481	2189	2197	2201	rBV5	15512	26646	1.52%	0.172%
56	14.633	2215	2222	2226	rBV3	16347	31677	1.81%	0.204%
57	15.182	2303	2312	2320	rBV7	30291	94815	5.42%	0.612%
58	15.255	2321	2324	2331	rVB2	17669	25196	1.44%	0.163%
59	15.322	2331	2335	2340	rBV4	12876	19154	1.09%	0.124%
60	15.542	2365	2371	2380	rBV	235991	357513	20.44%	2.306%
61	15.980	2438	2443	2446	rBV5	10626	18696	1.07%	0.121%
62	16.468	2517	2523	2536	rVB	194780	348581	19.92%	2.249%




Sum of corrected areas: 15502375

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051023\
Data File : VX035587.D
Acq On : 10 May 2023 15:37
Operator : JC/MD
Sample : 02648-03DL 5X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
ORA-1636DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X042523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

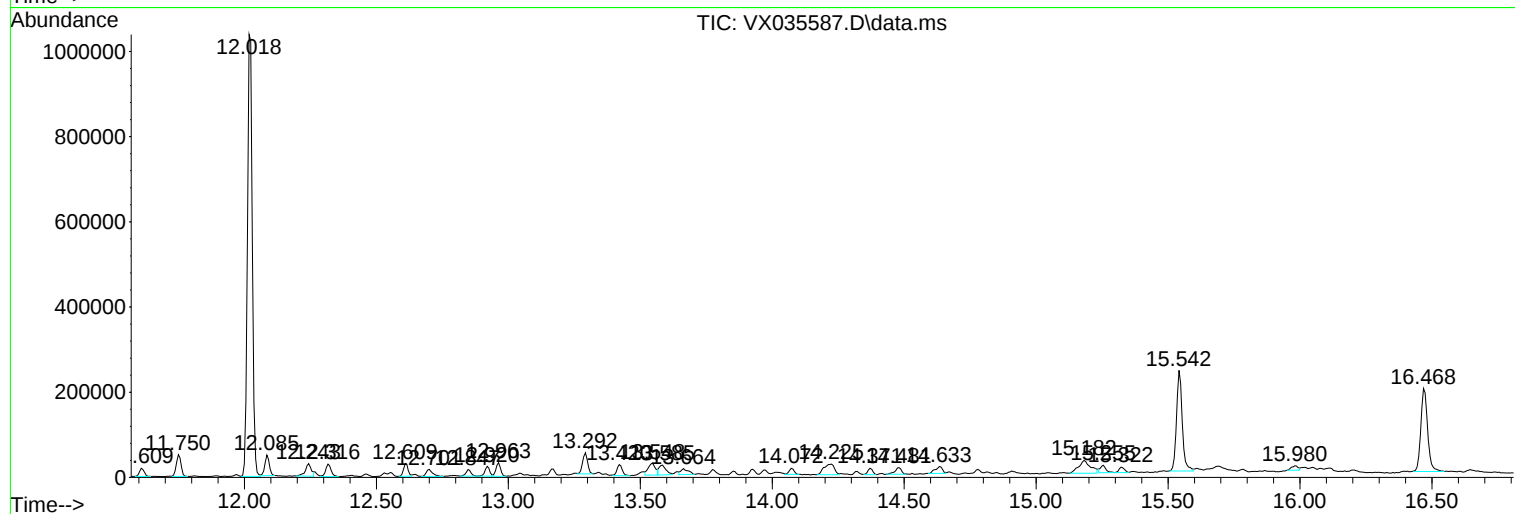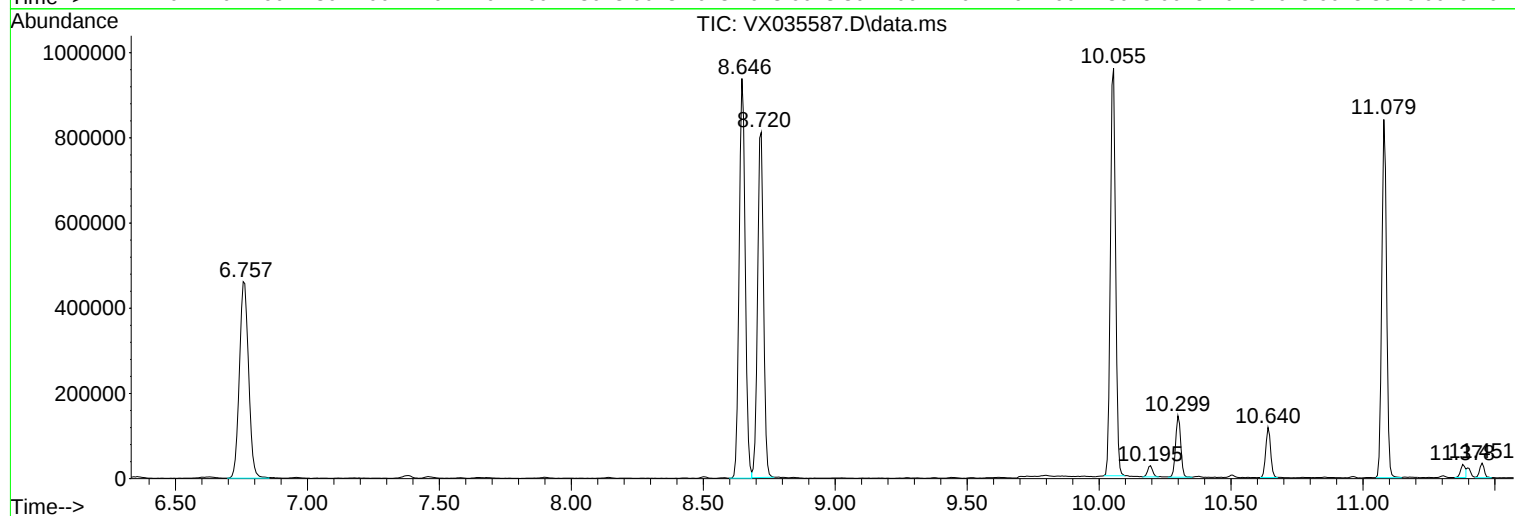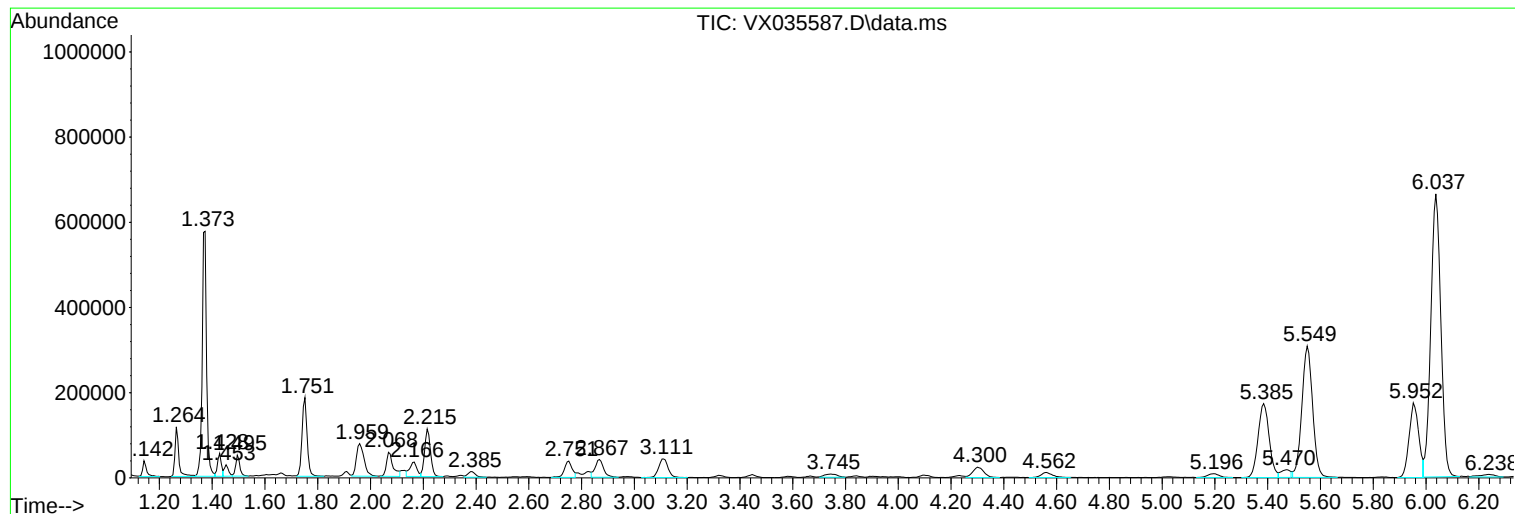

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051023\
Data File : VX035587.D
Acq On : 10 May 2023 15:37
Operator : JC/MD
Sample : 02648-03DL 5X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
ORA-1636DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X042523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051023\
Data File : VX035587.D
Acq On : 10 May 2023 15:37
Operator : JC/MD
Sample : 02648-03DL 5X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
ORA-1636DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X042523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc