

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051023\
 Data File : VX035594.D
 Acq On : 10 May 2023 18:19
 Operator : JC/MD
 Sample : 02743-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 DRUM-A-WATER

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X042523W.M
 Title : SW846 8260

Signal : TIC: VX035594.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.385	693	705	719	rBV	178713	520969	33.59%	5.694%
2	5.550	719	732	748	rVB	320188	894830	57.69%	9.780%
3	5.952	787	798	813	rBV	176622	469314	30.26%	5.130%
4	6.757	920	930	944	rBV	478572	1146690	73.93%	12.533%
5	8.647	1233	1240	1250	rBV	1009693	1551104	100.00%	16.953%
6	10.055	1465	1471	1482	rBV	999472	1359406	87.64%	14.858%
7	11.079	1634	1639	1650	rBV	877134	1085572	69.99%	11.865%
8	12.018	1788	1793	1804	rBV	1058787	1320132	85.11%	14.429%
9	13.524	2032	2040	2048	rBV8	9432	32479	2.09%	0.355%
10	15.176	2302	2311	2317	rBV8	19689	61413	3.96%	0.671%
11	15.255	2321	2324	2329	rVV2	14530	21186	1.37%	0.232%
12	15.542	2365	2371	2382	rBV	209617	327656	21.12%	3.581%
13	15.688	2391	2395	2407	rVB10	11673	29778	1.92%	0.325%
14	15.975	2436	2442	2446	rBV8	9263	21415	1.38%	0.234%
15	16.469	2516	2523	2538	rVB	167188	307353	19.82%	3.359%


Sum of corrected areas: 9149297

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051023\
Data File : VX035594.D
Acq On : 10 May 2023 18:19
Operator : JC/MD
Sample : 02743-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DRUM-A-WATER

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X042523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

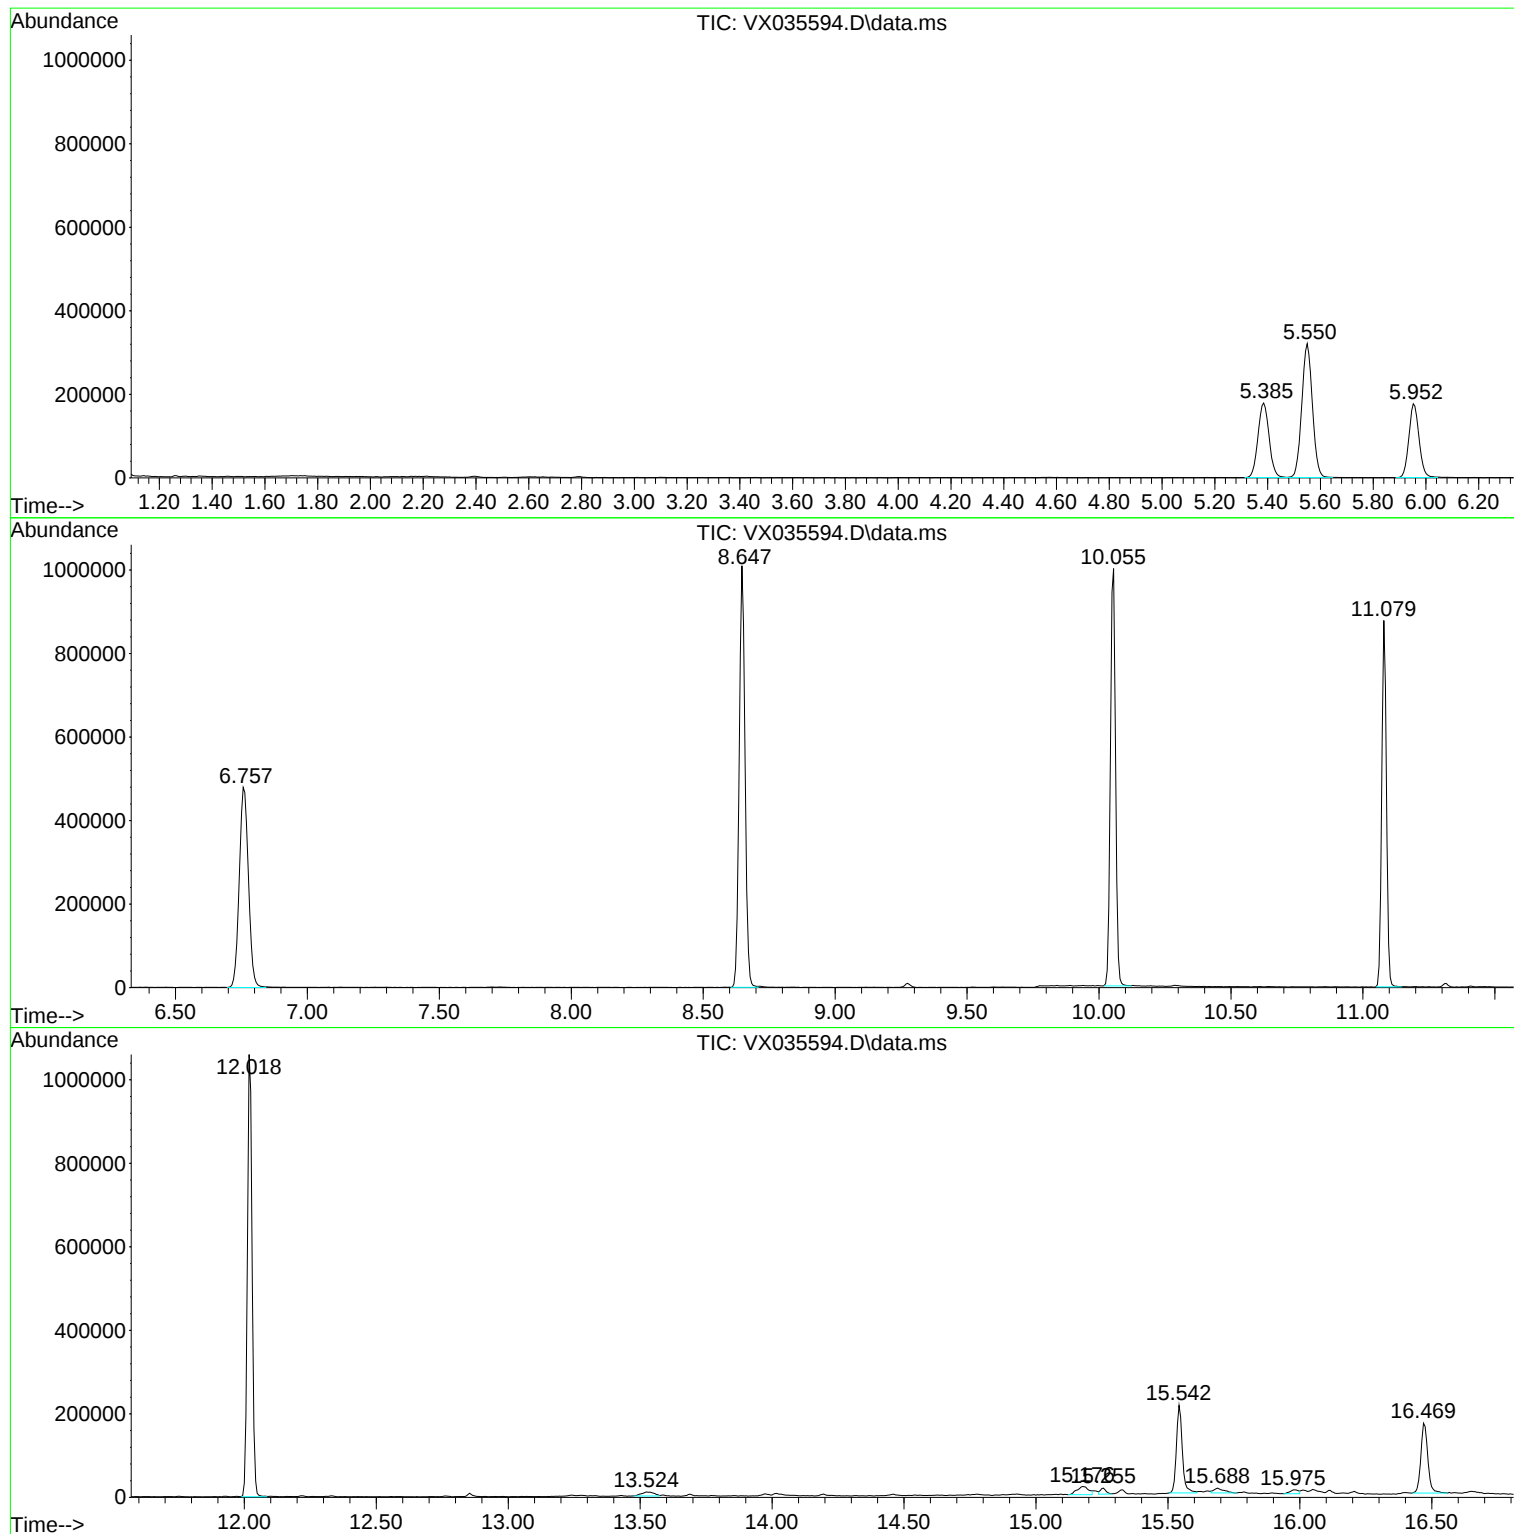

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051023\
Data File : VX035594.D
Acq On : 10 May 2023 18:19
Operator : JC/MD
Sample : 02743-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DRUM-A-WATER










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X042523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Dodecane, 1-chloro- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
15.542	12.41 ug/l	327656	1,4-Dichlorobenzene-d4	12.018

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Dodecane, 1-chloro-	204	C12H25Cl	000112-52-7	98
2			1-Chloroundecane	190	C11H23Cl	002473-03-2	91
3			Tetradecane, 1-chloro-	232	C14H29Cl	002425-54-9	64
4			Dodecane, 1-fluoro-	188	C12H25F	000334-68-9	46
5			Heptane, 1-chloro-	134	C7H15Cl	000629-06-1	30

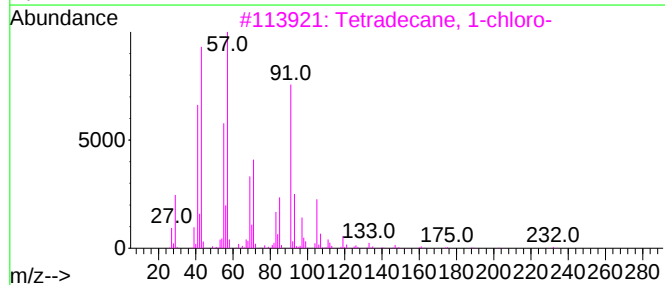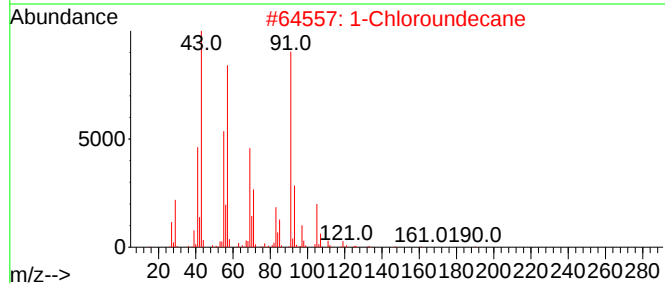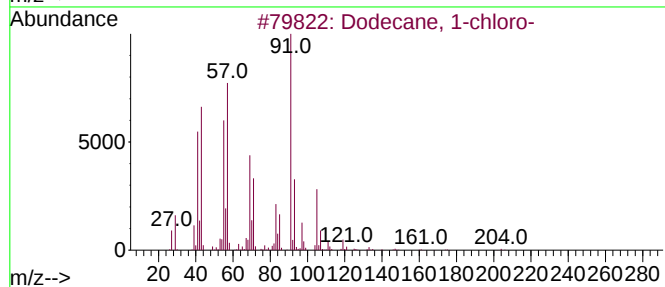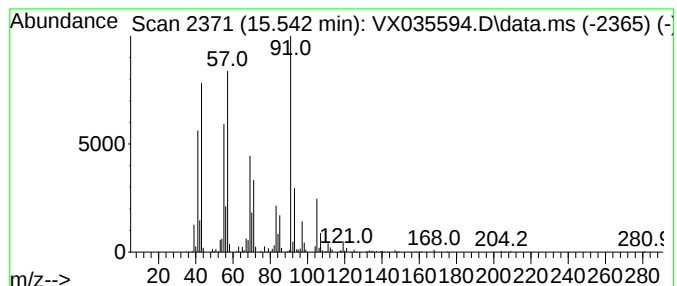

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051023\
Data File : VX035594.D
Acq On : 10 May 2023 18:19
Operator : JC/MD
Sample : 02743-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DRUM-A-WATER










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X042523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Tetradecane, 1-chloro- Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
16.468	11.64 ug/l	307353	1,4-Dichlorobenzene-d4	12.018

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Dodecane, 1-chloro-	204	C12H25Cl	000112-52-7	87
2			Tetradecane, 1-chloro-	232	C14H29Cl	002425-54-9	83
3			Oxalic acid, allyl dodecyl ester	298	C17H30O4	1000309-24-0	58
4			Oxalic acid, allyl pentadecyl ester	340	C20H36O4	1000309-24-3	52
5			Decane, 1-chloro-	176	C10H21Cl	001002-69-3	49

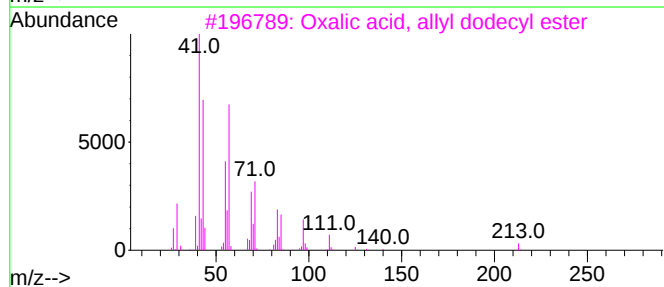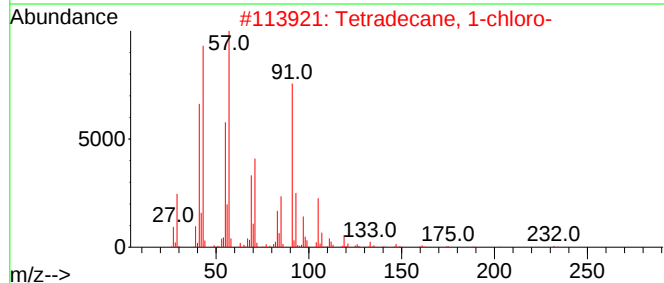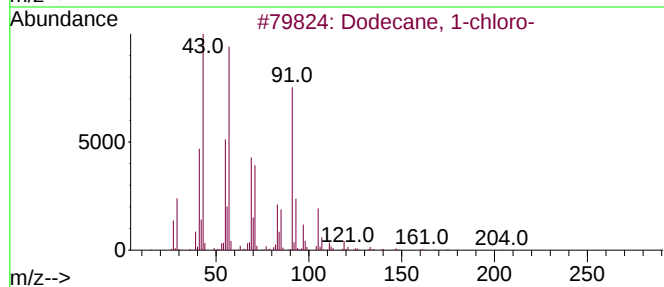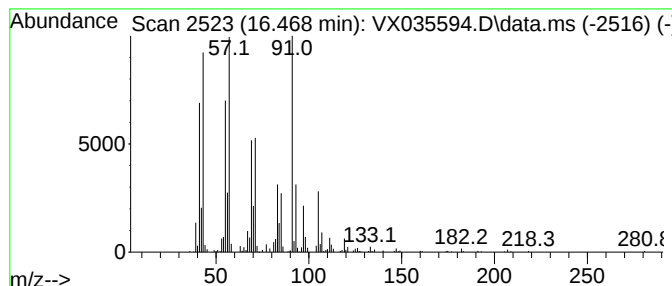

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051023\
Data File : VX035594.D
Acq On : 10 May 2023 18:19
Operator : JC/MD
Sample : 02743-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DRUM-A-WATER

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X042523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Dodecane, 1-chl...	15.542	12.4	ug/l	327656	4	12.018	1320130	50.0
Tetradecane, 1-...	16.468	11.6	ug/l	307353	4	12.018	1320130	50.0