

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051024\
 Data File : VX041447.D
 Acq On : 10 May 2024 09:07
 Operator : JC/MD
 Sample : VX0510MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: May 10 23:16:50 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML050924WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri May 10 23:16:04 2024
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.757	114	260308	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	254480	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.018	152	121150	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	78133	52.923	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	105.840%	
7) Chloroethane-d5	1.666	69	65351	60.334	ug/L	0.02
Spiked Amount 50.000	Range 70	- 130	Recovery	=	120.660%	
11) 1,1-Dichloroethene-d2	2.307	65	39859	53.643	ug/L	0.01
Spiked Amount 50.000	Range 60	- 125	Recovery	=	107.280%	
21) 2-Butanone-d5	4.452	46	149091	135.456	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130	Recovery	=	135.460%#	
24) Chloroform-d	5.056	84	175369	53.717	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	107.440%	
26) 1,2-Dichloroethane-d4	5.952	65	120248	51.202	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	102.400%	
32) Benzene-d6	5.970	84	346863	49.893	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	99.780%	
36) 1,2-Dichloropropane-d6	7.306	67	96743	46.833	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	93.660%	
41) Toluene-d8	8.647	98	270921	37.730	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	75.460%#	
43) trans-1,3-Dichloroprop...	8.946	79	44227	42.736	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	85.480%	
47) 2-Hexanone-d5	9.384	63	90162	93.668	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	93.670%	
56) 1,1,2,2-Tetrachloroeth...	11.189	84	142992	43.986	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	87.980%	
66) 1,2-Dichlorobenzene-d4	12.317	152	128096	51.746	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	103.500%	
Target Compounds					Qvalue	
37) 1,2-Dichloropropane	7.306	63	11621	6.481	ug/L #	85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051024\
Data File : VX041447.D
Acq On : 10 May 2024 09:07
Operator : JC/MD
Sample : VX0510MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: May 10 23:16:50 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML050924WMA.M
Quant Title : VOC Analysis
QLast Update : Fri May 10 23:16:04 2024
Response via : Initial Calibration

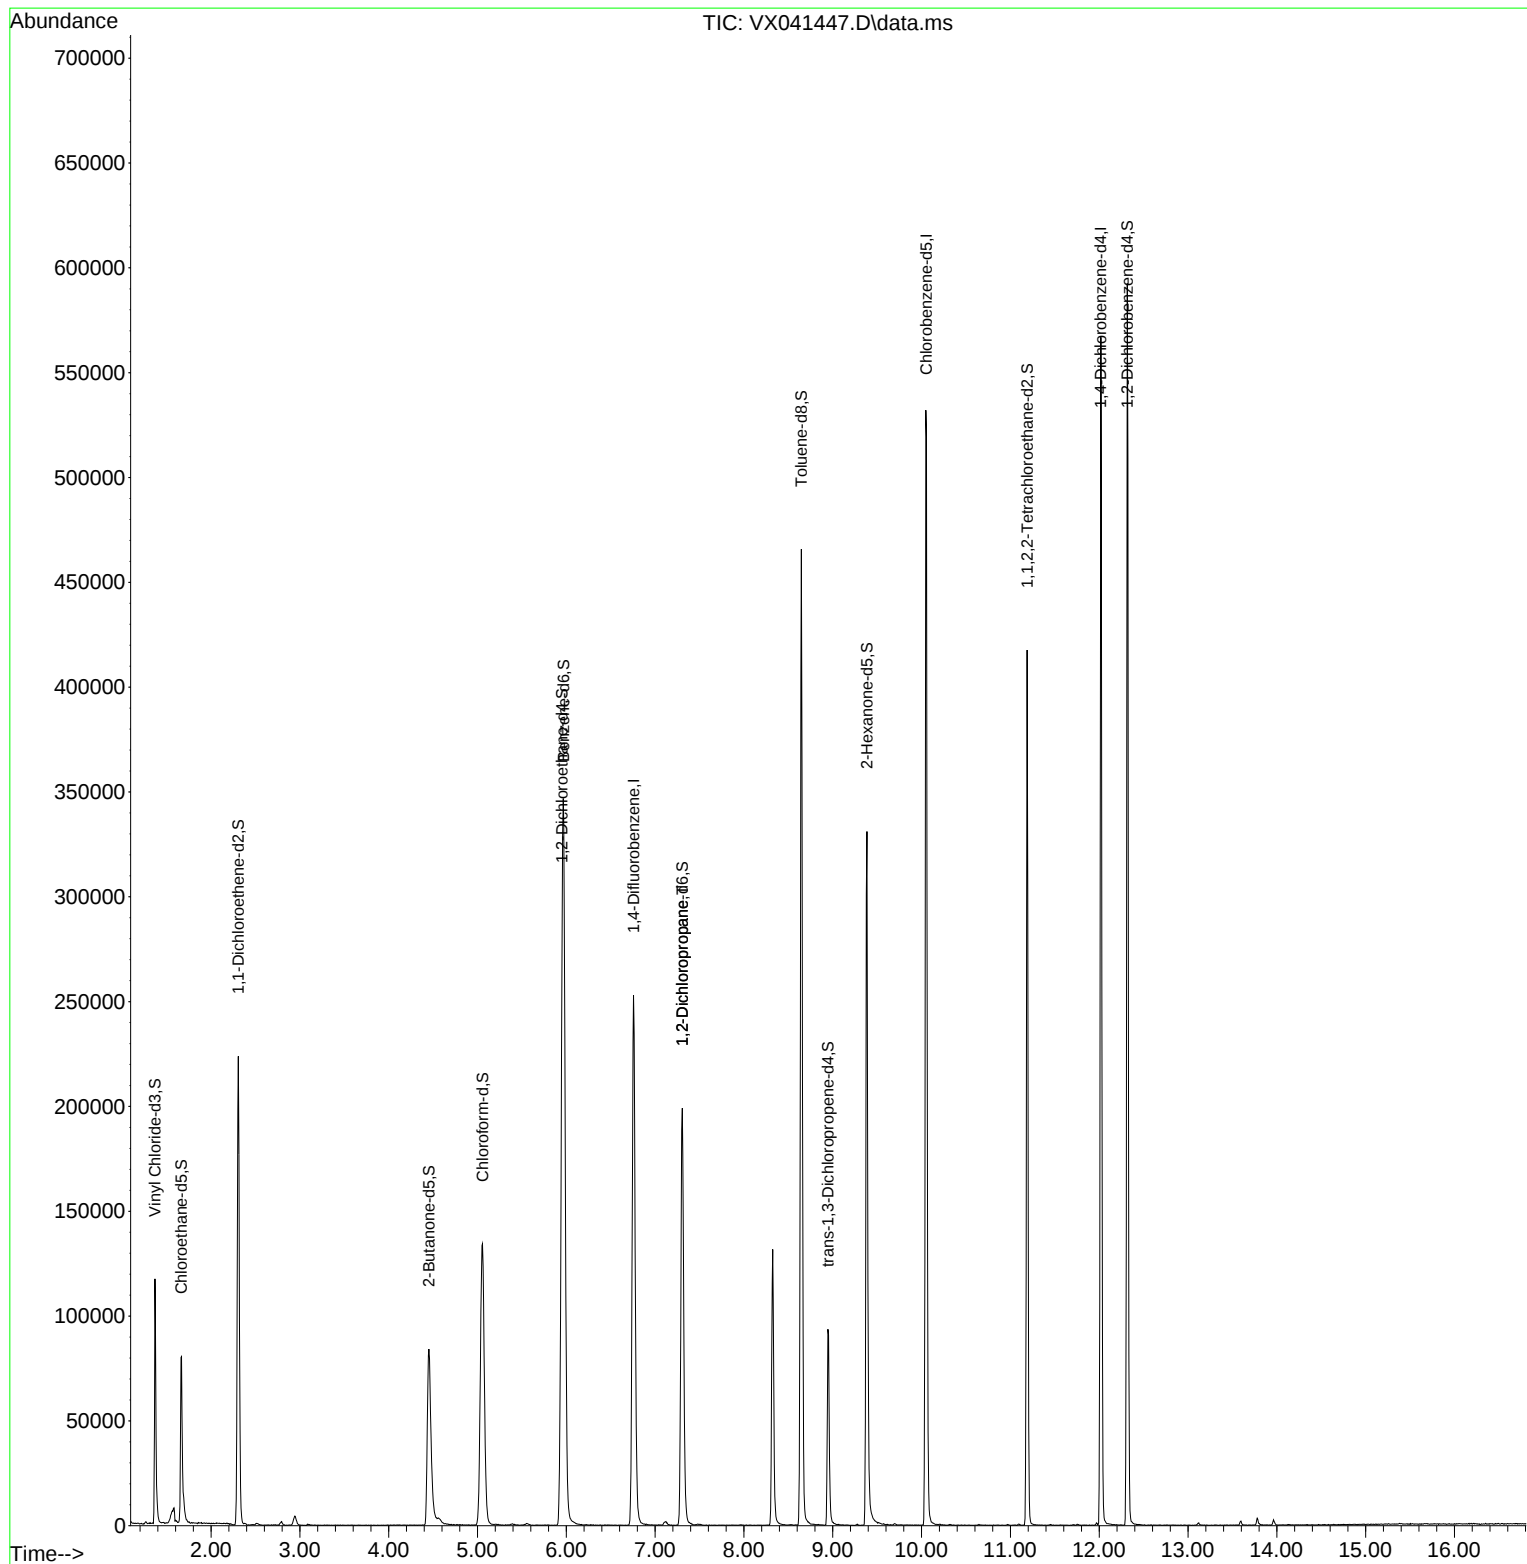

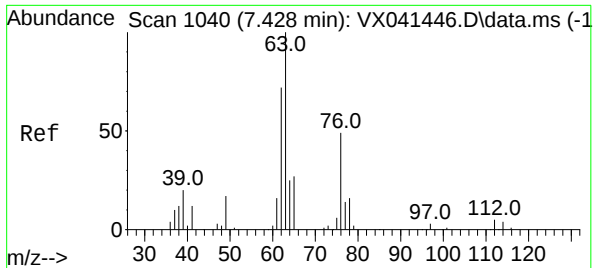

#37
 1,2-Dichloropropane
 Concen: 6.481 ug/L
 RT: 7.306 min Scan# 10
 Delta R.T. -0.122 min
 Lab File: VX041447.D
 Acq: 10 May 2024 09:07

Instrument :
 MSVOA_X
 ClientSampleId :

Tgt Ion: 63 Resp: 11621
 Ion Ratio Lower Upper
 63 100
 112 0.0 4.1 6.1#

