
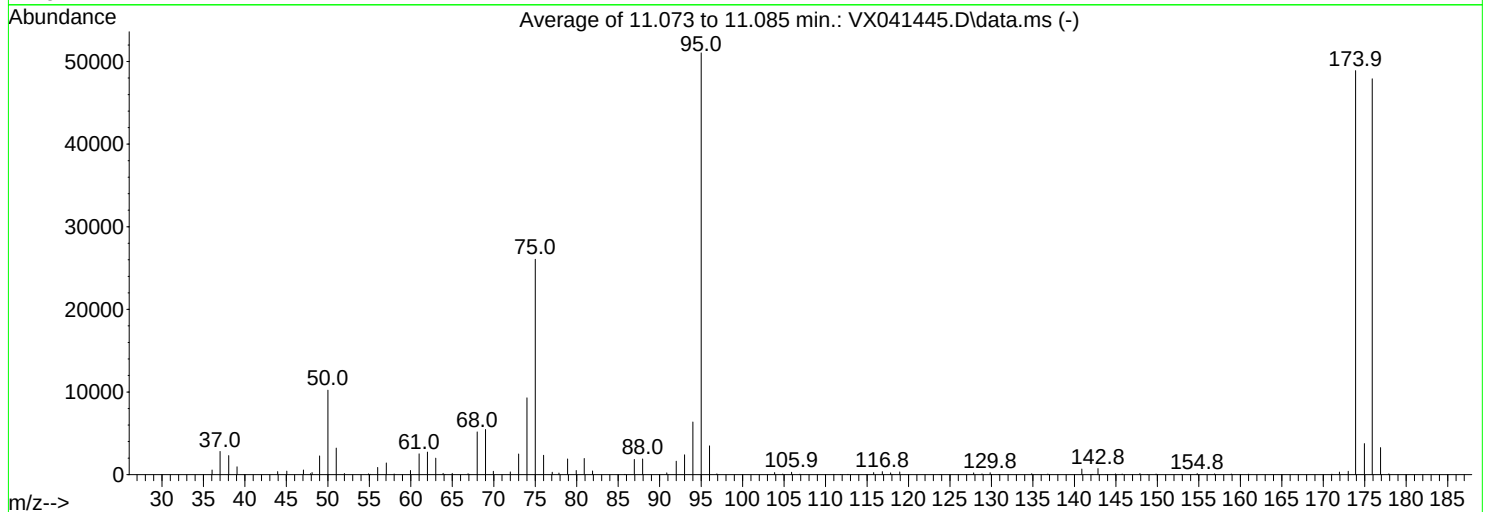


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051024\
Data File : VX041445.D
Acq On : 10 May 2024 08:09
Operator : JC/MD
Sample : BFB676
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB676

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM050924WMA.M
Title : VOC Analysis
Last Update : Fri May 10 23:16:04 2024

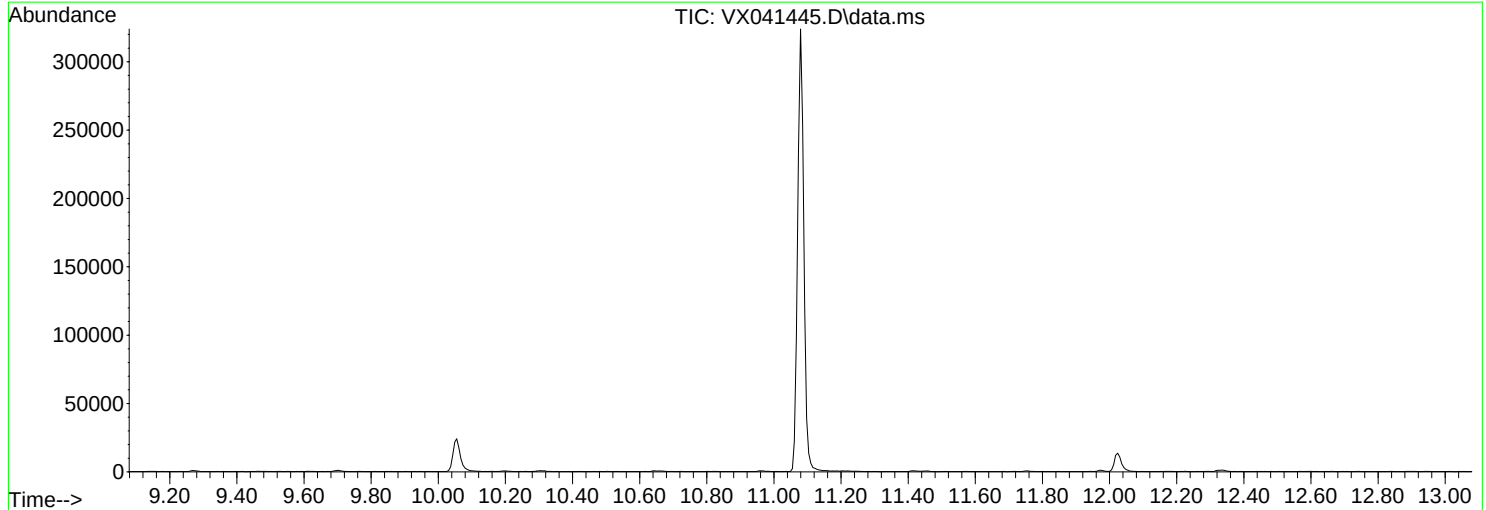

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.0	10230	PASS
75	95	30	80	51.1	26072	PASS
95	95	100	100	100.0	51048	PASS
96	95	5	9	6.8	3486	PASS
173	174	0.00	2	0.8	404	PASS
174	95	50	120	95.8	48904	PASS
175	174	5	9	7.7	3752	PASS
176	174	95	101	97.9	47899	PASS
177	176	5	9	6.8	3273	PASS

m/z	Abundance
39.90	183.0
44.00	89.0

Instrument :
MSVOA_X
ClientSampleId :
BFB676

m/z	Abundance
36.10	619.0
37.00	2892.0
38.00	2231.0
39.10	1019.0
39.90	230.0
43.90	572.0
45.00	427.0
47.10	541.0
47.90	356.0
49.00	2076.0
50.00	10282.0
51.00	3199.0
52.00	166.0
54.90	140.0
56.00	807.0
57.00	1390.0
58.00	91.0
59.90	470.0
61.00	2537.0
62.00	2626.0
63.00	1922.0
63.90	206.0
65.00	213.0
66.90	122.0
68.00	4729.0
69.00	5053.0
69.90	421.0
72.00	392.0
73.00	2476.0
74.00	8897.0
75.00	24056.0
76.00	2310.0
77.10	289.0
77.80	132.0
78.90	1976.0
79.90	456.0
80.90	1848.0
81.90	429.0
87.00	1737.0
87.90	1794.0
90.90	183.0
92.00	1380.0
93.00	2437.0
94.00	5563.0
95.00	46040.0
96.00	3113.0
96.90	107.0
103.90	257.0
105.90	192.0
115.80	180.0
116.90	333.0
117.80	155.0
119.00	317.0
128.00	176.0
128.90	81.0
129.90	263.0
134.80	110.0
136.80	61.0
140.90	552.0
142.00	65.0
142.80	668.0
145.00	72.0
145.80	80.0
147.90	116.0
148.80	57.0
149.80	55.0
154.80	95.0
156.80	73.0
171.10	56.0
172.00	278.0
173.90	37712.0
174.90	2791.0
175.90	36088.0
176.90	2572.0
177.90	76.0

Instrument :
MSVOA_X
ClientSampleId :
BFB676

m/z	Abundance
36.00	626.0
37.00	3133.0
38.00	2753.0
39.00	1017.0
40.00	171.0
44.00	476.0
45.00	532.0
47.00	647.0
48.10	405.0
49.00	2725.0
50.00	12299.0
51.00	3736.0
52.00	174.0
55.10	107.0
56.00	936.0
57.00	1733.0
58.00	136.0
60.00	611.0
61.00	2858.0
62.00	3245.0
63.00	2446.0
63.90	256.0
64.90	142.0
66.90	217.0
68.00	6172.0
69.00	6738.0
70.00	477.0
71.90	321.0
73.00	2937.0
74.00	11053.0
75.00	30720.0
76.00	2837.0
76.90	330.0
77.80	220.0
78.90	2153.0
80.00	665.0
80.90	2415.0
81.90	535.0
85.80	54.0
87.00	2178.0
88.00	2263.0
90.90	291.0
92.00	1909.0
93.00	2681.0
94.00	7747.0
95.00	61008.0
96.00	4393.0
96.90	132.0
103.90	325.0
104.80	119.0
105.90	402.0
106.90	76.0
111.00	53.0
111.80	52.0
112.70	62.0
114.90	54.0
115.80	344.0
116.80	391.0
117.90	260.0
119.00	359.0
123.80	66.0
127.80	252.0
128.90	114.0
129.90	240.0
130.90	77.0
134.90	103.0
136.80	121.0
140.90	813.0
142.20	98.0
142.90	922.0
144.90	107.0
145.70	77.0
147.90	131.0
149.90	119.0
152.90	71.0
154.80	144.0
156.90	107.0
158.90	125.0
161.00	101.0
171.00	97.0
171.90	359.0
173.00	665.0
173.90	59000.0
174.90	4640.0
175.90	57424.0
176.90	3776.0
177.90	126.0

Instrument :
MSVOA_X
ClientSampleId :
BFB676

m/z	Abundance
36.00	444.0
37.00	2374.0
38.10	1932.0
39.10	819.0
40.00	176.0
44.00	348.0
45.10	335.0
47.00	514.0
48.10	380.0
49.00	1972.0
50.00	8108.0
51.00	2726.0
51.90	88.0
54.90	177.0
56.00	892.0
57.10	1106.0
60.00	435.0
61.00	2180.0
62.00	2311.0
63.00	1611.0
64.10	146.0
65.10	135.0
67.10	132.0
68.00	4608.0
69.00	4585.0
70.00	332.0
72.10	291.0
73.00	2102.0
74.00	7943.0
75.00	23440.0
76.00	1894.0
77.10	230.0
77.90	206.0
78.90	1582.0
79.90	404.0
80.90	1585.0
81.90	361.0
85.80	51.0
86.90	1619.0
87.90	1613.0
90.70	187.0
92.00	1582.0
93.00	2072.0
94.00	5790.0
95.00	46096.0
96.00	2952.0
97.00	65.0
103.70	170.0
104.90	92.0
105.90	258.0
106.90	82.0
111.00	54.0
112.70	66.0
115.80	219.0
116.80	366.0
117.90	199.0
118.90	336.0
127.80	208.0
128.80	120.0
129.80	209.0
130.90	61.0
134.90	126.0
136.80	78.0
140.90	676.0
142.90	637.0
143.80	51.0
144.90	98.0
145.70	53.0
147.90	169.0
149.80	65.0
152.90	59.0
154.80	150.0
157.00	107.0
158.90	87.0
161.00	88.0
171.90	272.0
173.00	548.0
173.90	50000.0
175.00	3826.0
175.90	50184.0
176.90	3470.0
177.90	64.0

Instrument :
MSVOA_X
ClientSampleId :
BFB676