
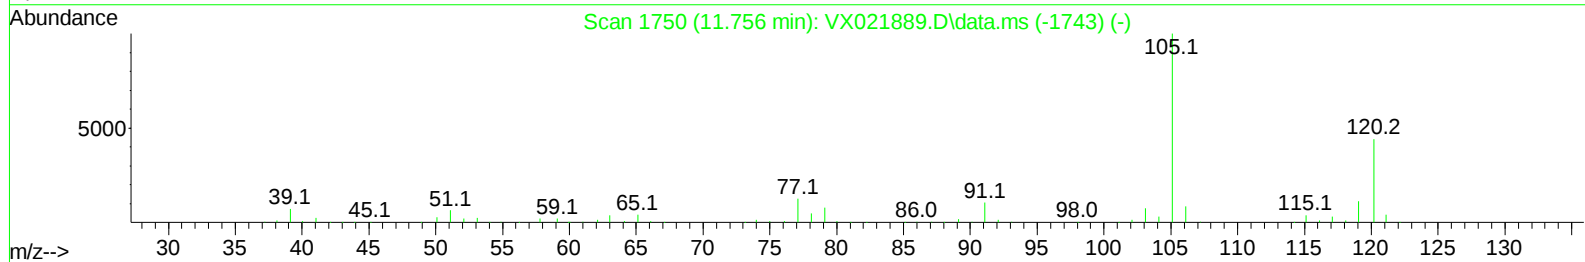
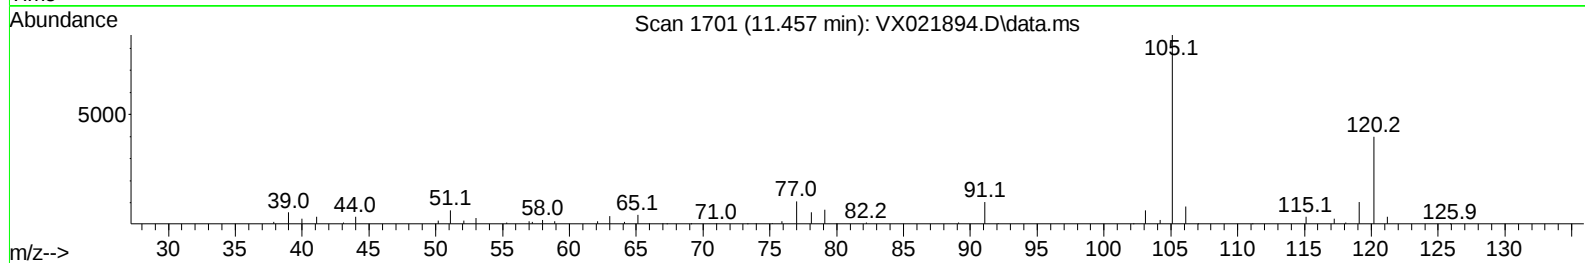


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051121\
 Data File : VX021894.D
 Acq On : 11 May 2021 13:19
 Operator : JC/MD
 Sample : M2336-06
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Quant Time: May 12 03:39:43 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR051021WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed May 12 03:37:54 2021
 Response via : Initial Calibration

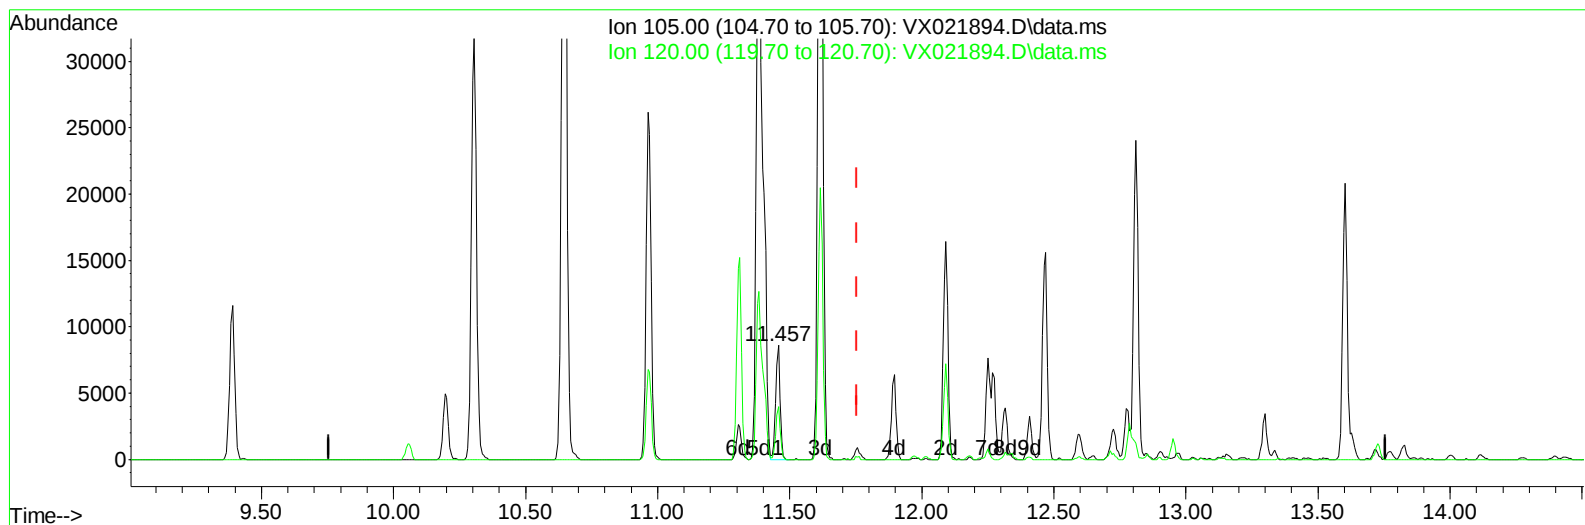




TIC: VX021894.D\data.ms

(63) 1,2,4-Trimethylbenzene (T)**11.457min (-0.299) 0.40 ug/L****response 10113**

Ion	Exp%	Act%
105.00	100.00	100.00
120.00	45.50	47.36
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051121\
Data File : VX021894.D
Acq On : 11 May 2021 13:19
Operator : JC/MD
Sample : M2336-06
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Quant Time: May 12 03:39:43 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR051021WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed May 12 03:37:54 2021
Response via : Initial Calibration

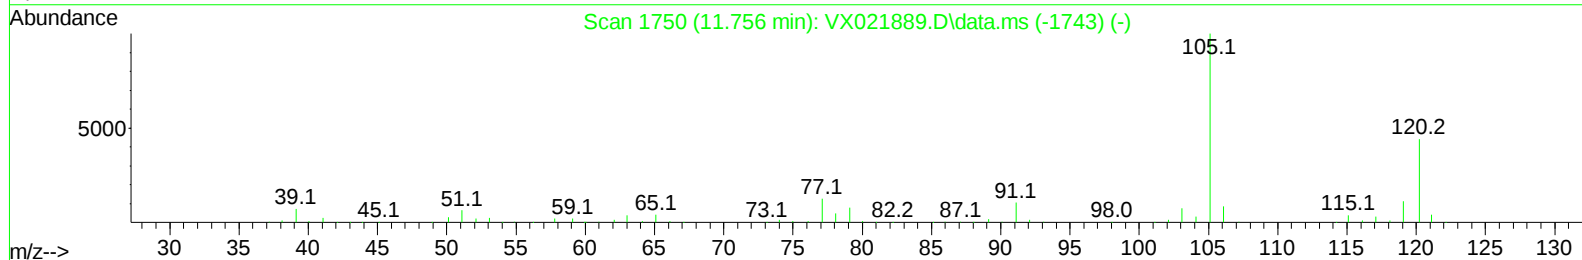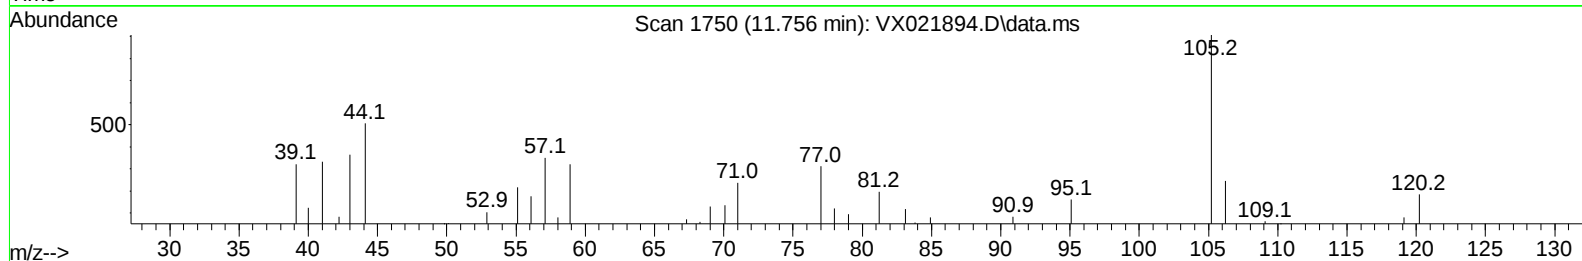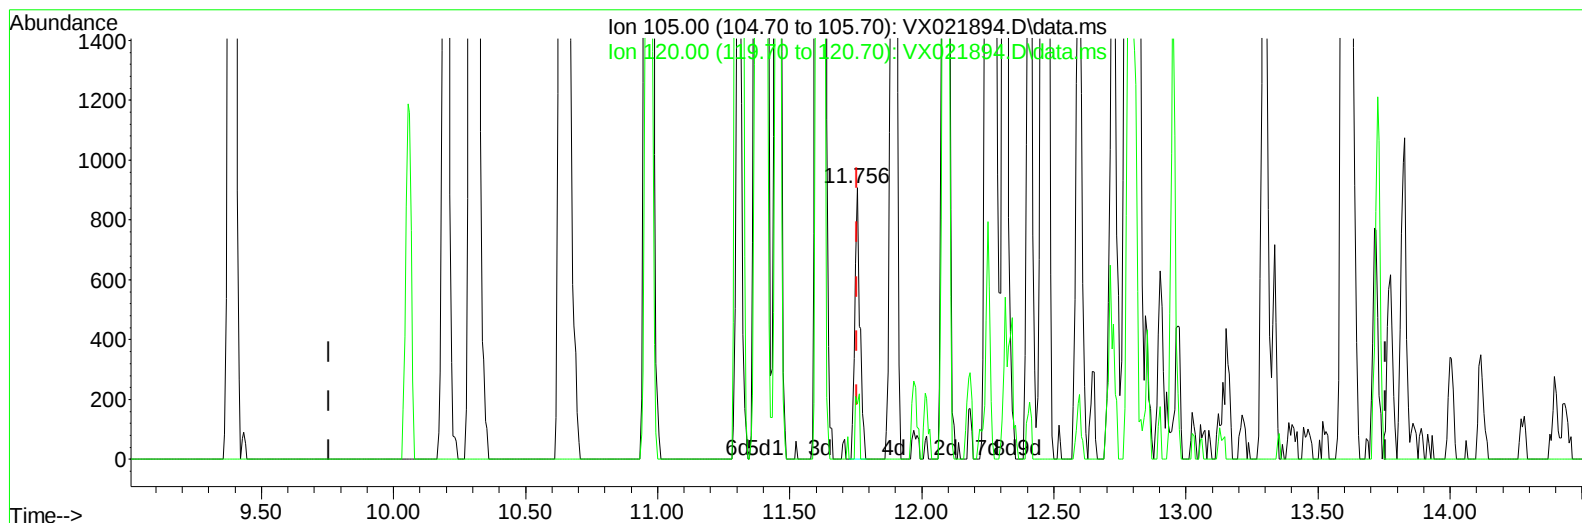

TIC: VX021894.D\data.ms

(63) 1,2,4-Trimethylbenzene (T)

11.756min (0.000) 0.05 ug/L m

response 1154

Ion	Exp%	Act%
105.00	100.00	100.00
120.00	45.50	415.08#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051121\
 Data File : VX021894.D
 Acq On : 11 May 2021 13:19
 Operator : JC/MD
 Sample : M2336-06
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Quant Time: May 12 03:39:43 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR051021WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed May 12 03:37:54 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.769	114	83392	5.00	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	72788	5.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	34465	5.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	30830	4.30	ug/L	0.00
Spiked Amount 5.000	Range 40 - 130		Recovery =	86.00%		
7) Chloroethane-d5	1.672	69	27300	4.76	ug/L	0.00
Spiked Amount 5.000	Range 65 - 130		Recovery =	95.20%		
11) 1,1-Dichloroethene-d2	2.306	63	34012	2.86	ug/L	0.00
Spiked Amount 5.000	Range 60 - 125		Recovery =	57.20%#		
20) 2-Butanone-d5	4.471	46	83693	51.29	ug/L	0.00
Spiked Amount 50.000	Range 40 - 130		Recovery =	102.58%		
24) Chloroform-d	5.068	84	55723	4.53	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	90.60%		
26) 1,2-Dichloroethane-d4	5.964	65	29488	4.67	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	93.40%		
32) Benzene-d6	5.983	84	117597	4.88	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	97.60%		
36) 1,2-Dichloropropane-d6	7.318	67	37367	5.05	ug/L	0.00
Spiked Amount 5.000	Range 60 - 140		Recovery =	101.00%		
41) Toluene-d8	8.653	98	107510	4.91	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	98.20%		
43) trans-1,3-Dichloroprop...	8.952	79	16085	4.82	ug/L	0.00
Spiked Amount 5.000	Range 55 - 130		Recovery =	96.40%		
46) 2-Hexanone-d5	9.391	63	71914	50.65	ug/L	0.00
Spiked Amount 50.000	Range 45 - 130		Recovery =	101.30%		
56) 1,1,2,2-Tetrachloroeth...	11.195	84	28269	4.95	ug/L	0.00
Spiked Amount 5.000	Range 65 - 120		Recovery =	99.00%		
66) 1,2-Dichlorobenzene-d4	12.323	152	35537	4.92	ug/L	0.00
Spiked Amount 5.000	Range 80 - 120		Recovery =	98.40%		
Target Compounds						
						Qvalue
5) Vinyl chloride	1.374	62	2219	0.27	ug/L #	77
8) Chloroethane	1.691	64	1491	0.30	ug/L	98
13) Acetone	2.404	43	29677	35.54	ug/L	96
18) trans-1,2-Dichloroethene	3.087	96	1290	0.20	ug/L	71
19) 1,1-Dichloroethane	3.617	63	16851	1.51	ug/L	96
21) 2-Butanone	4.580	43	9213	5.99	ug/L	90
22) cis-1,2-Dichloroethene	4.495	96	12468	1.78	ug/L	91
27) 1,2-Dichloroethane	6.092	62	4466	0.66	ug/L	100
29) 1,1,1-Trichloroethane	5.391	97	665	0.07	ug/L #	82
30) Cyclohexane	5.477	56	10463	0.97	ug/L #	88
33) Benzene	6.050	78	59337	2.36	ug/L	100
34) Trichloroethene	7.129	95	3479	0.53	ug/L	92
35) Methylcyclohexane	7.385	83	6357	0.57	ug/L #	79
42) Toluene	8.720	91	54176	2.03	ug/L	97
47) Tetrachloroethene	9.275	164	648	0.15	ug/L	88
51) Chlorobenzene	10.079	112	46945	2.83	ug/L	98
52) Ethylbenzene	10.195	91	141450	4.74	ug/L	99
53) m,p-xylene	10.305	106	97449	8.50	ug/L	99

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051121\
 Data File : VX021894.D
 Acq On : 11 May 2021 13:19
 Operator : JC/MD
 Sample : M2336-06
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Quant Time: May 12 03:39:43 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR051021WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed May 12 03:37:54 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
54) o-xylene	10.646	106	206113	18.60	ug/L	94
60) Isopropylbenzene	10.963	105	34273	1.17	ug/L	99
62) 1,3,5-Trimethylbenzene	11.457	105	10113	0.41	ug/L	99
63) 1,2,4-Trimethylbenzene	11.756	105	1154m	0.05	ug/L	
64) 1,3-Dichlorobenzene	11.975	146	3032	0.25	ug/L	95
65) 1,4-Dichlorobenzene	12.042	146	9179	0.77	ug/L	99
67) 1,2-Dichlorobenzene	12.335	146	109724	9.94	ug/L	98
70) 1,2,4-trichlorobenzene	13.591	180	2568	0.35	ug/L	98
72) 1,2,3-Trichlorobenzene	13.963	180	1158	0.18	ug/L	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051121\
Data File : VX021894.D
Acq On : 11 May 2021 13:19
Operator : JC/MD
Sample : M2336-06
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Quant Time: May 12 03:39:43 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR051021WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed May 12 03:37:54 2021
Response via : Initial Calibration

