

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051121\
 Data File : VX021903.D
 Acq On : 11 May 2021 16:43
 Operator : JC/MD
 Sample : M2337-09
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BG6K6

Quant Time: May 12 03:41:56 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR051021WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed May 12 03:37:54 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.769	114	76945	5.00	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	69780	5.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	31984	5.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	28628	4.33	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	86.60%
7) Chloroethane-d5	1.672	69	24967	4.71	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	94.20%
11) 1,1-Dichloroethene-d2	2.306	63	37788	3.44	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	68.80%
20) 2-Butanone-d5	4.465	46	73364	48.72	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	97.44%
24) Chloroform-d	5.068	84	54011	4.76	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.20%
26) 1,2-Dichloroethane-d4	5.964	65	28002	4.80	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.00%
32) Benzene-d6	5.983	84	112354	4.86	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.20%
36) 1,2-Dichloropropane-d6	7.312	67	34935	4.93	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	98.60%
41) Toluene-d8	8.653	98	101063	4.81	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.20%
43) trans-1,3-Dichloroprop...	8.952	79	13879	4.33	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	86.60%
46) 2-Hexanone-d5	9.384	63	64222	47.18	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	94.36%
56) 1,1,2,2-Tetrachloroeth...	11.195	84	25731	4.70	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	94.00%
66) 1,2-Dichlorobenzene-d4	12.323	152	33265	4.96	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	99.20%
Target Compounds					Qvalue	
13) Acetone	2.392	43	2978	3.87	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051121\
Data File : VX021903.D
Acq On : 11 May 2021 16:43
Operator : JC/MD
Sample : M2337-09
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BG6K6


Quant Time: May 12 03:41:56 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR051021WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed May 12 03:37:54 2021
Response via : Initial Calibration

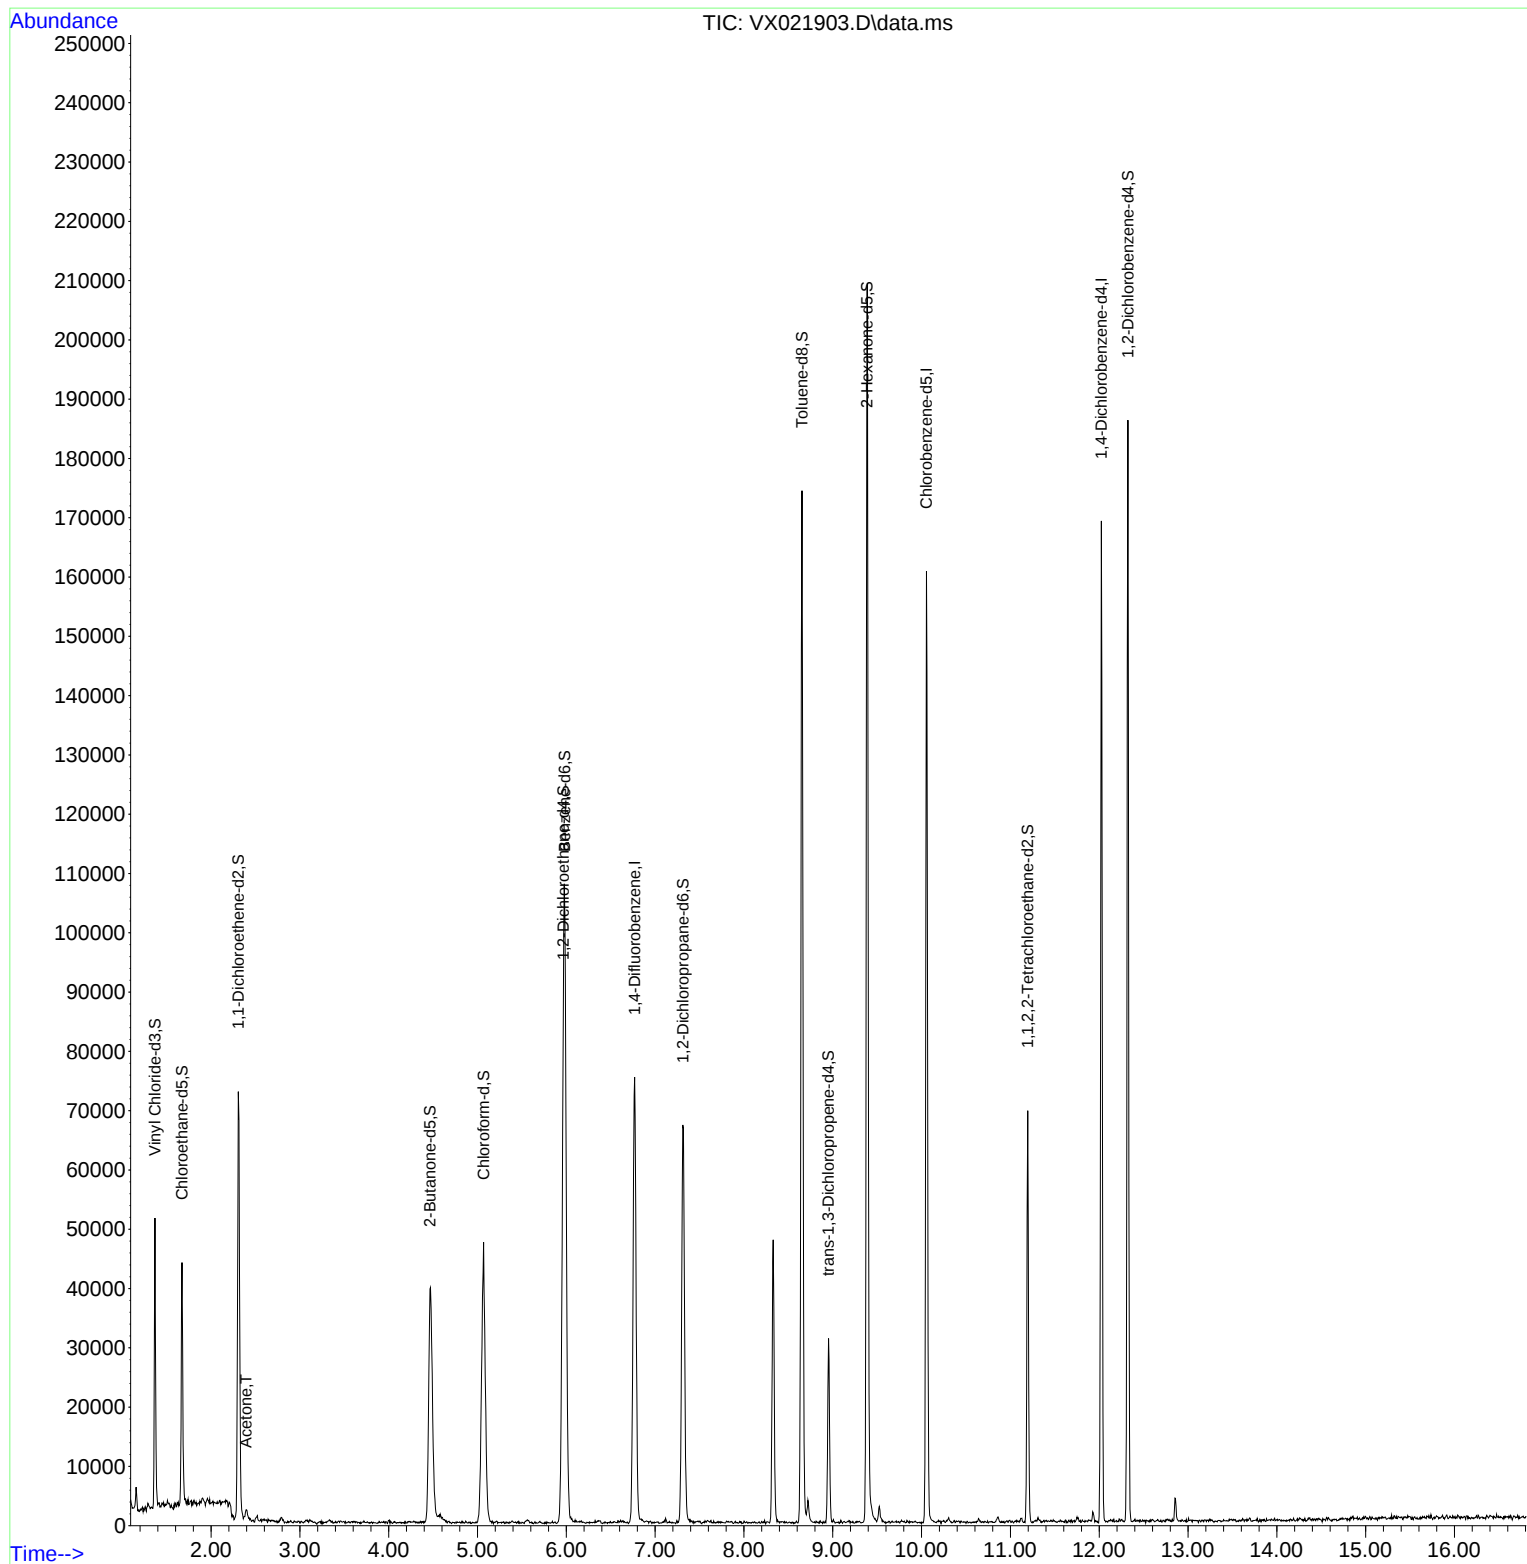

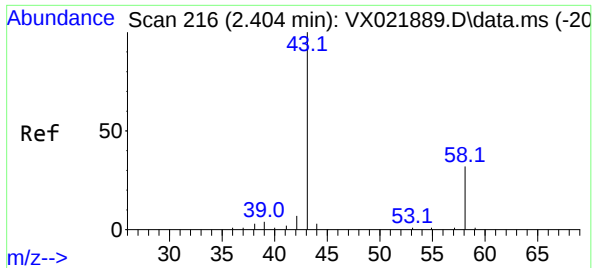

#13
Acetone
Concen: 3.87 ug/L
RT: 2.392 min Scan# 214
Delta R.T. -0.012 min
Lab File: VX021903.D
Acq: 11 May 2021 16:43

Instrument :
MSVOA_X
ClientSampleId :
BG6K6

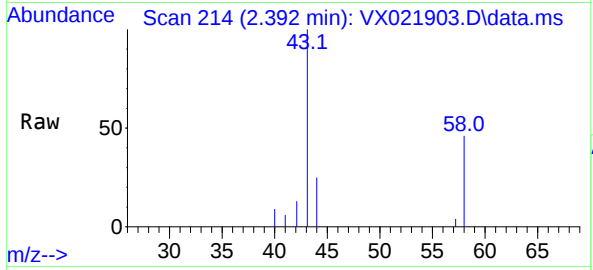

Tgt Ion: 43 Resp: 2978
Ion Ratio Lower Upper
43 100
58 30.8 0.0 66.4

