

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051121\
 Data File : VX021910.D
 Acq On : 11 May 2021 19:27
 Operator : JC/MD
 Sample : M2339-06
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0AW5

Quant Time: May 12 03:43:18 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR051021WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed May 12 03:37:54 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.769	114	77243	5.00	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	68760	5.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	31311	5.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	28126	4.24	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	84.80%
7) Chloroethane-d5	1.673	69	23212	4.36	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	87.20%
11) 1,1-Dichloroethene-d2	2.307	63	36128	3.28	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	65.60%
20) 2-Butanone-d5	4.471	46	75426	49.90	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	99.80%
24) Chloroform-d	5.068	84	51038	4.48	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.60%
26) 1,2-Dichloroethane-d4	5.958	65	28065	4.79	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	95.80%
32) Benzene-d6	5.983	84	108071	4.74	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.80%
36) 1,2-Dichloropropane-d6	7.318	67	34116	4.88	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	97.60%
41) Toluene-d8	8.653	98	96376	4.66	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.20%
43) trans-1,3-Dichloroprop...	8.952	79	13927	4.41	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	88.20%
46) 2-Hexanone-d5	9.385	63	65357	48.72	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	97.44%
56) 1,1,2,2-Tetrachloroeth...	11.195	84	25510	4.73	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	94.60%
66) 1,2-Dichlorobenzene-d4	12.323	152	31127	4.74	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	94.80%
Target Compounds						
13) Acetone	2.398	43	1797	2.32	ug/L	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051121\
Data File : VX021910.D
Acq On : 11 May 2021 19:27
Operator : JC/MD
Sample : M2339-06
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0AW5

Quant Time: May 12 03:43:18 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR051021WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed May 12 03:37:54 2021
Response via : Initial Calibration

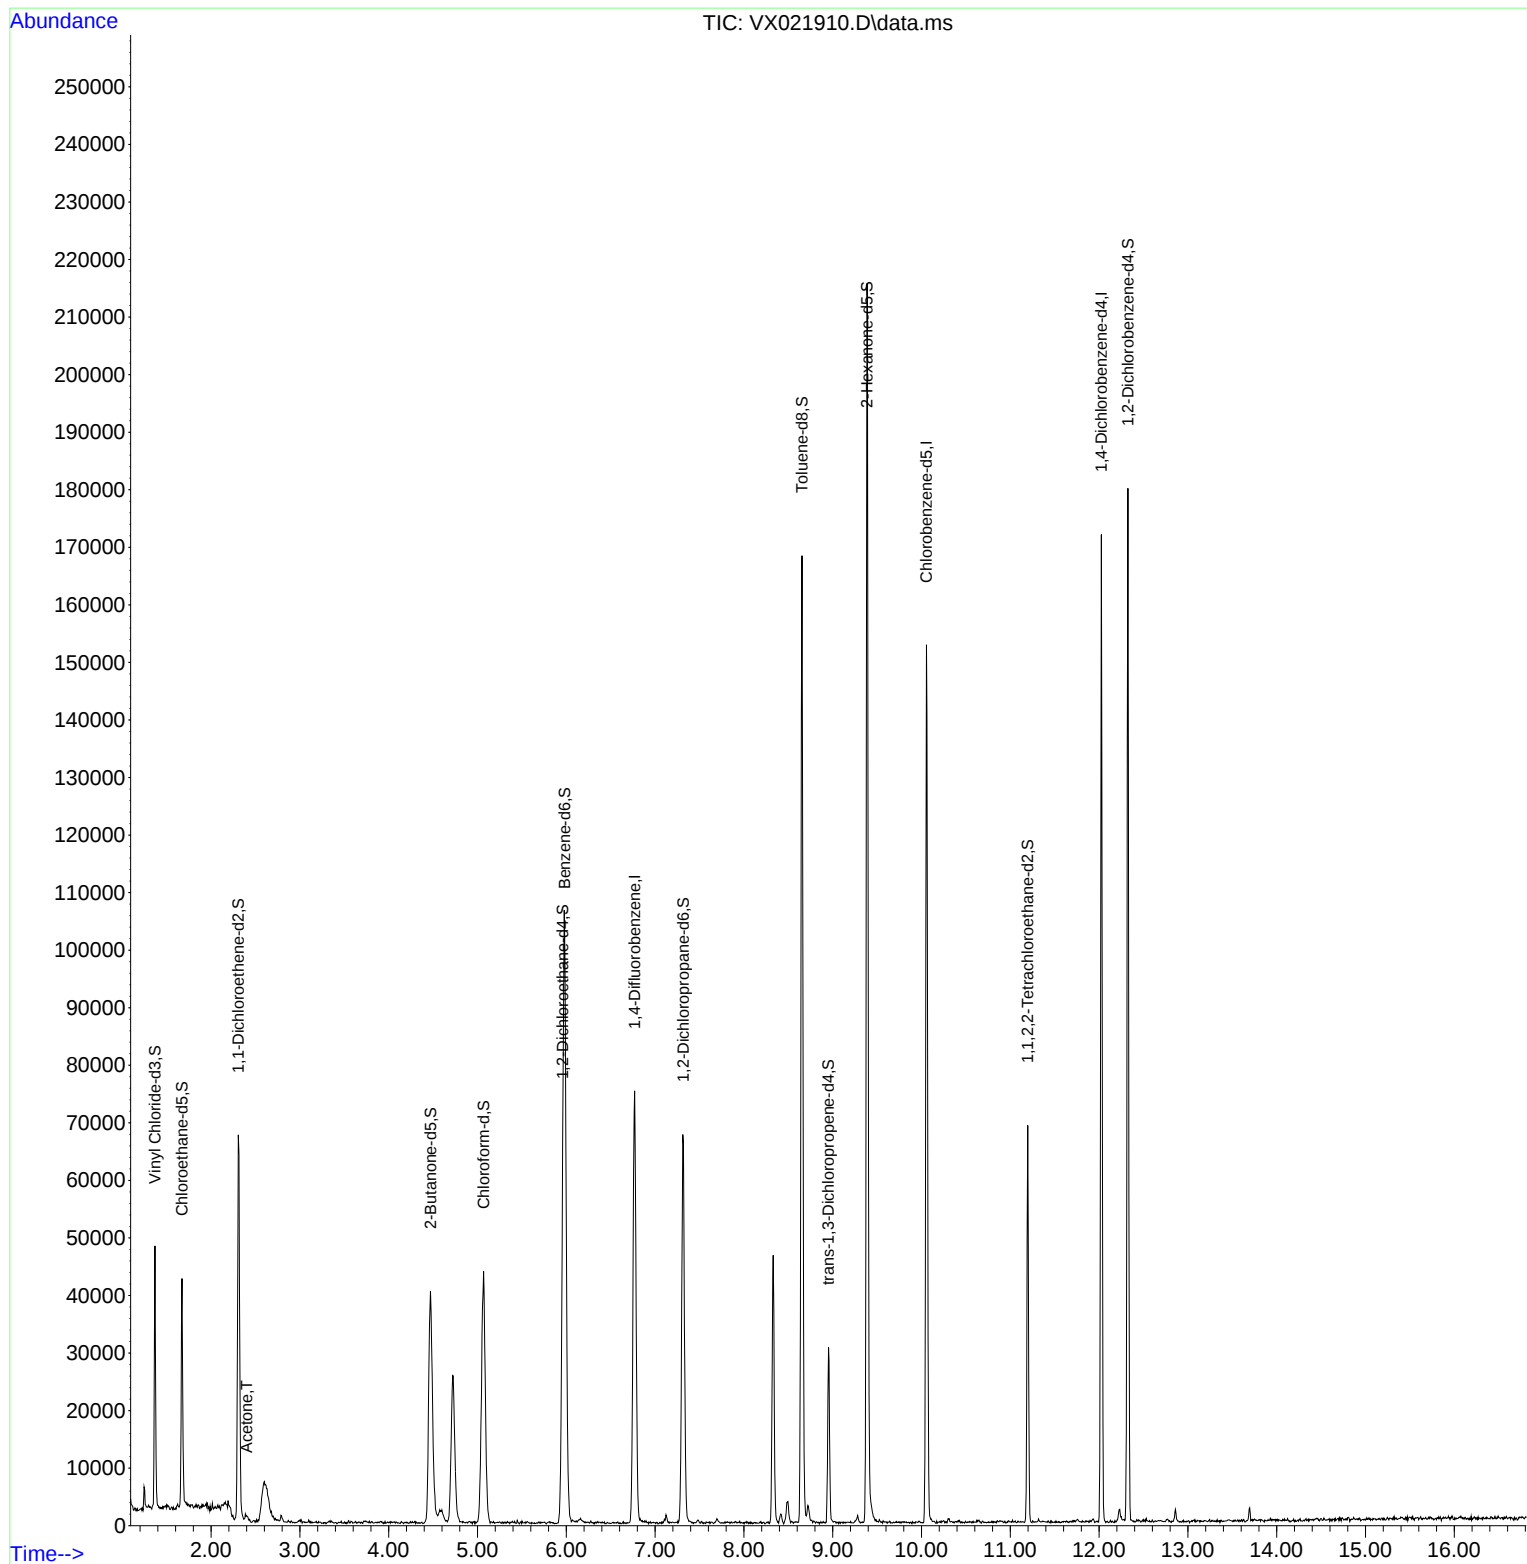

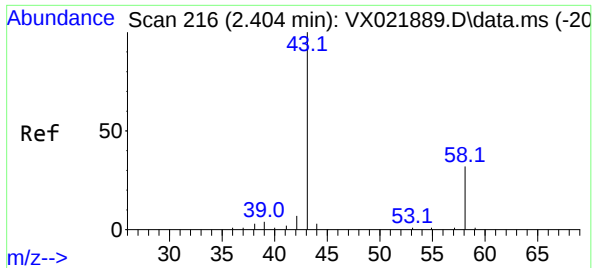

#13
 Acetone
 Concen: 2.32 ug/L
 RT: 2.398 min Scan# 215
 Delta R.T. -0.006 min
 Lab File: VX021910.D
 Acq: 11 May 2021 19:27

Instrument :
 MSVOA_X
 ClientSampleId :
 C0AW5

Tgt Ion: 43 Resp: 1797
 Ion Ratio Lower Upper
 43 100
 58 32.2 0.0 66.4

