

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051121\
 Data File : VX021913.D
 Acq On : 11 May 2021 21:00
 Operator : JC/MD
 Sample : VX0511WBL02
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK302

Quant Time: May 12 06:27:17 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR051021WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed May 12 06:12:28 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.769	114	77515	5.00	ug/L	0.00
28) Chlorobenzene-d5	10.061	117	70058	5.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	32167	5.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.367	65	25863	3.88	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	77.60%
7) Chloroethane-d5	1.672	69	22942	4.30	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	86.00%
11) 1,1-Dichloroethene-d2	2.306	63	33242	3.01	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	60.20%
20) 2-Butanone-d5	4.477	46	75820	49.99	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	99.98%
24) Chloroform-d	5.062	84	49219	4.30	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	86.00%
26) 1,2-Dichloroethane-d4	5.964	65	26725	4.55	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.00%
32) Benzene-d6	5.976	84	100978	4.35	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	87.00%
36) 1,2-Dichloropropane-d6	7.318	67	32252	4.53	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	90.60%
41) Toluene-d8	8.653	98	87224	4.14	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	82.80%
43) trans-1,3-Dichloroprop...	8.952	79	12948	4.03	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	80.60%
46) 2-Hexanone-d5	9.384	63	66131	48.39	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	96.78%
56) 1,1,2,2-Tetrachloroeth...	11.195	84	24833	4.52	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	90.40%
66) 1,2-Dichlorobenzene-d4	12.323	152	29655	4.40	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	88.00%
Target Compounds						
16) Methylene chloride	2.800	84	2254	0.29	ug/L	Qvalue 94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051121\
Data File : VX021913.D
Acq On : 11 May 2021 21:00
Operator : JC/MD
Sample : VX0511WBL02
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK302


Quant Time: May 12 06:27:17 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR051021WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed May 12 06:12:28 2021
Response via : Initial Calibration

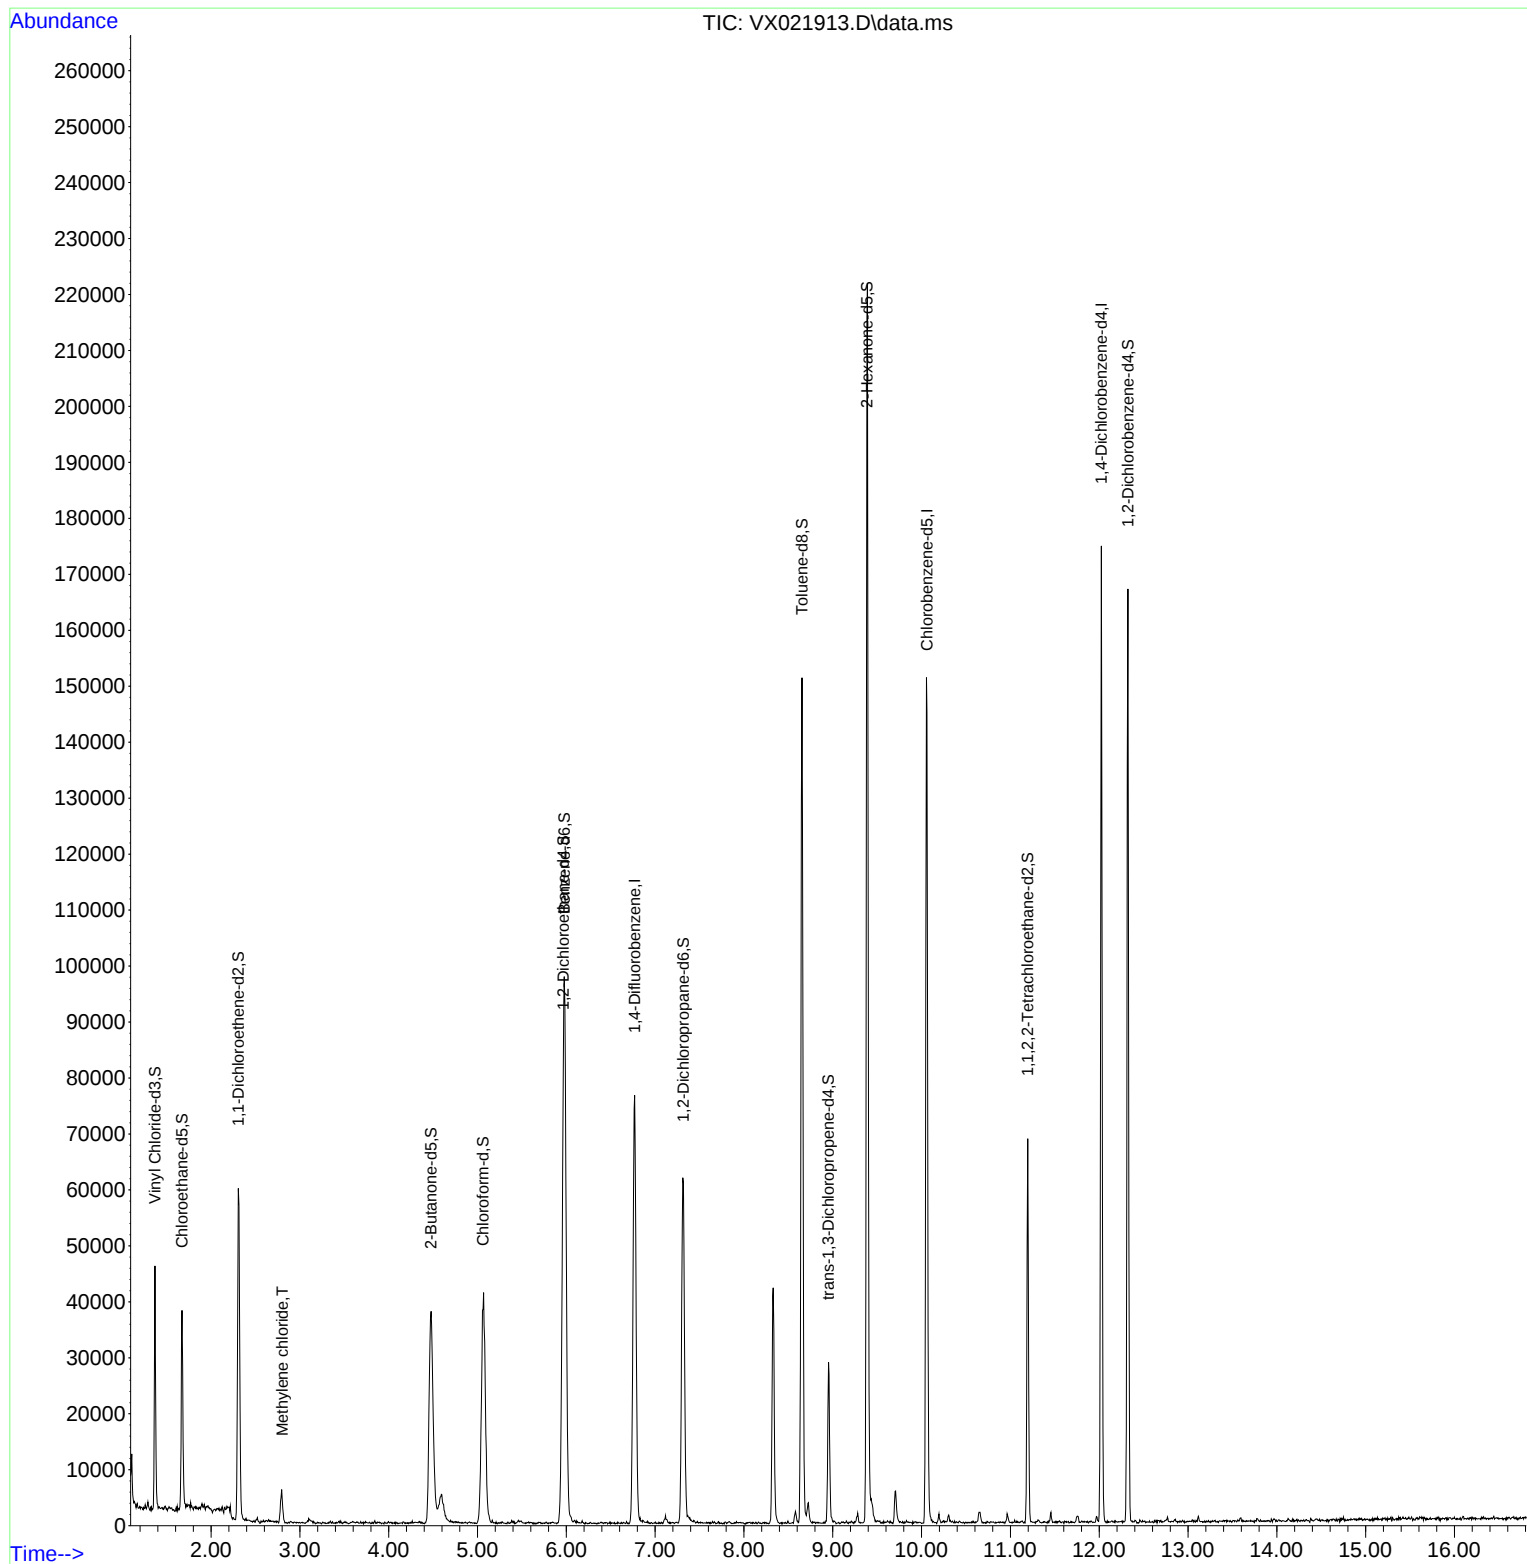

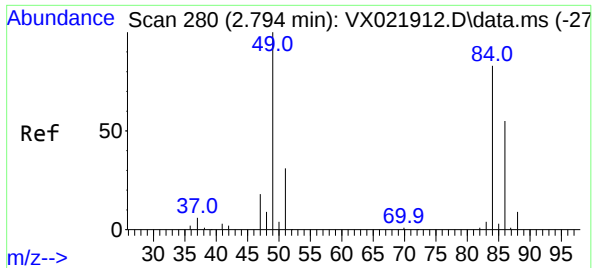

#16
Methylene chloride
Concen: 0.29 ug/L
RT: 2.800 min Scan# 281
Delta R.T. 0.006 min
Lab File: VX021913.D
Acq: 11 May 2021 21:00

Instrument :
MSVOA_X
ClientSampleId :
VBLK302

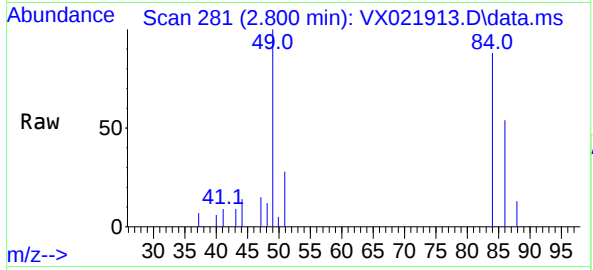

Tgt Ion: 84 Resp: 2254

Ion	Ratio	Lower	Upper
84	100		
86	61.7	46.3	86.1
49	113.7	84.4	156.7

