

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051121\
 Data File : VX021917.D
 Acq On : 11 May 2021 22:34
 Operator : JC/MD
 Sample : M2336-08
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Quant Time: May 12 06:28:07 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR051021WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed May 12 06:12:28 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.769	114	76543	5.00	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	69871	5.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	32128	5.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	25631	3.90	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	78.00%
7) Chloroethane-d5	1.673	69	22212	4.22	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	84.40%
11) 1,1-Dichloroethene-d2	2.307	63	32997	3.02	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	60.40%
20) 2-Butanone-d5	4.471	46	76663	51.18	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	102.36%
24) Chloroform-d	5.068	84	48555	4.30	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	86.00%
26) 1,2-Dichloroethane-d4	5.964	65	26932	4.64	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.80%
32) Benzene-d6	5.983	84	101505	4.38	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	87.60%
36) 1,2-Dichloropropane-d6	7.312	67	31274	4.41	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	88.20%
41) Toluene-d8	8.653	98	87027	4.14	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	82.80%
43) trans-1,3-Dichloroprop...	8.952	79	12698	3.96	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	79.20%
46) 2-Hexanone-d5	9.385	63	65186	47.82	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	95.64%
56) 1,1,2,2-Tetrachloroeth...	11.195	84	24104	4.40	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	88.00%
66) 1,2-Dichlorobenzene-d4	12.323	152	30909	4.59	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	91.80%
Target Compounds						
16) Methylene chloride	2.794	84	2133	0.28	ug/L	Qvalue 89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051121\
Data File : VX021917.D
Acq On : 11 May 2021 22:34
Operator : JC/MD
Sample : M2336-08
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Time: May 12 06:28:07 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR051021WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed May 12 06:12:28 2021
Response via : Initial Calibration

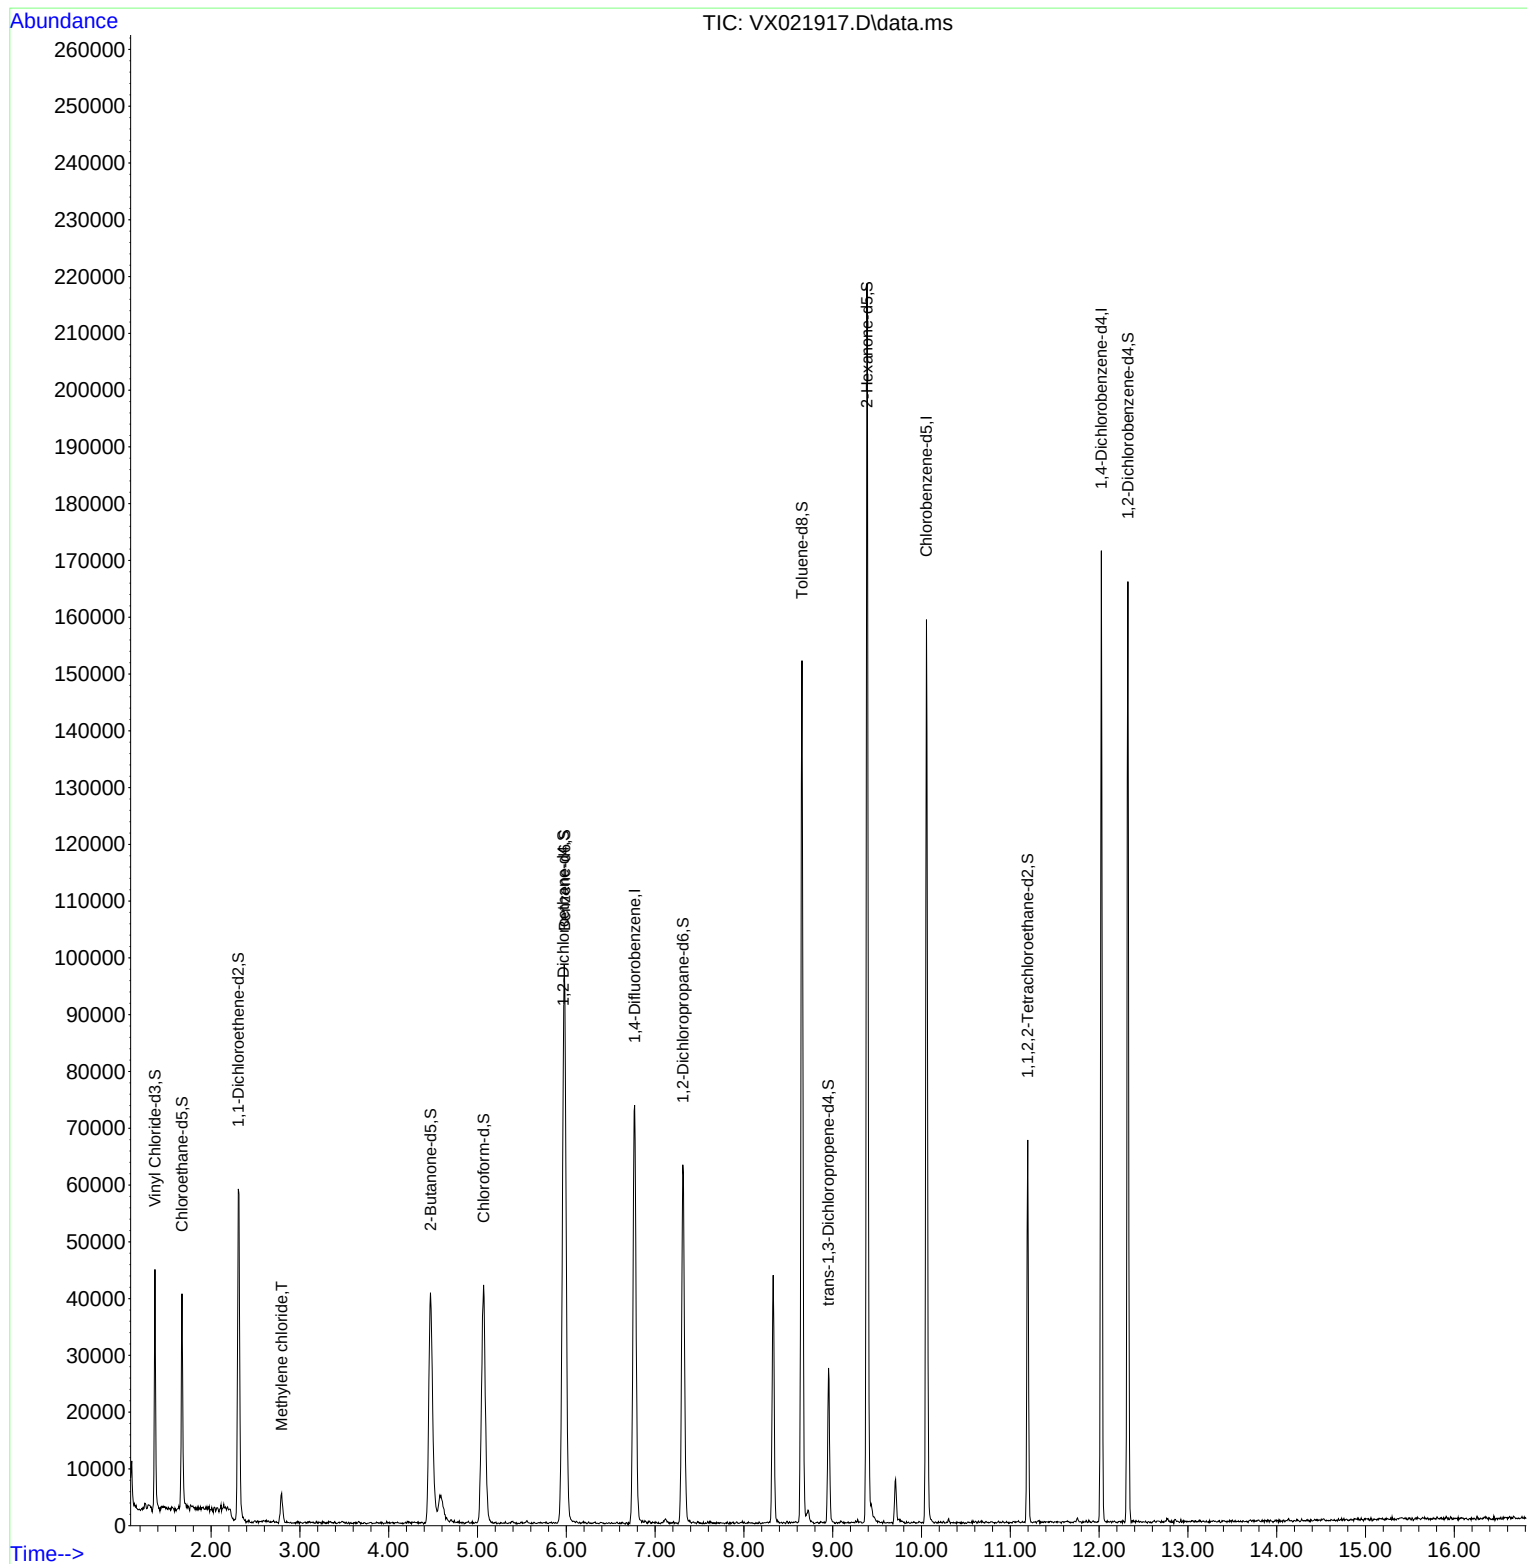

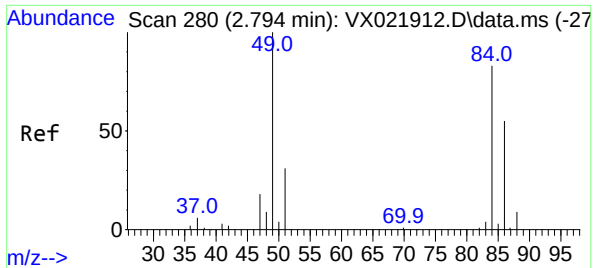

#16
Methylene chloride
Concen: 0.28 ug/L
RT: 2.794 min Scan# 280
Delta R.T. 0.000 min
Lab File: VX021917.D
Acq: 11 May 2021 22:34

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Tgt Ion: 84 Resp: 2133

Ion	Ratio	Lower	Upper
84	100		
86	77.7	46.3	86.1
49	131.5	84.4	156.7

