

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051121\
 Data File : VX021918.D
 Acq On : 11 May 2021 22:57
 Operator : JC/MD
 Sample : M2337-12
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Quant Time: May 12 06:28:17 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR051021WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed May 12 06:12:28 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.769	114	78868	5.00	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	70193	5.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	33184	5.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	26228	3.87	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	77.40%
7) Chloroethane-d5	1.672	69	23146	4.26	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	85.20%
11) 1,1-Dichloroethene-d2	2.306	63	33579	2.99	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	59.80%#
20) 2-Butanone-d5	4.471	46	76273	49.42	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	98.84%
24) Chloroform-d	5.062	84	49237	4.23	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	84.60%
26) 1,2-Dichloroethane-d4	5.964	65	26793	4.48	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	89.60%
32) Benzene-d6	5.977	84	101414	4.36	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	87.20%
36) 1,2-Dichloropropane-d6	7.318	67	32386	4.54	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	90.80%
41) Toluene-d8	8.653	98	87332	4.13	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	82.60%
43) trans-1,3-Dichloroprop...	8.952	79	13148	4.08	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	81.60%
46) 2-Hexanone-d5	9.391	63	65743	48.01	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	96.02%
56) 1,1,2,2-Tetrachloroeth...	11.195	84	25270	4.59	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	91.80%
66) 1,2-Dichlorobenzene-d4	12.323	152	30115	4.33	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	86.60%
Target Compounds						Qvalue
16) Methylene chloride	2.788	84	2229	0.29	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051121\
Data File : VX021918.D
Acq On : 11 May 2021 22:57
Operator : JC/MD
Sample : M2337-12
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Time: May 12 06:28:17 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR051021WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed May 12 06:12:28 2021
Response via : Initial Calibration

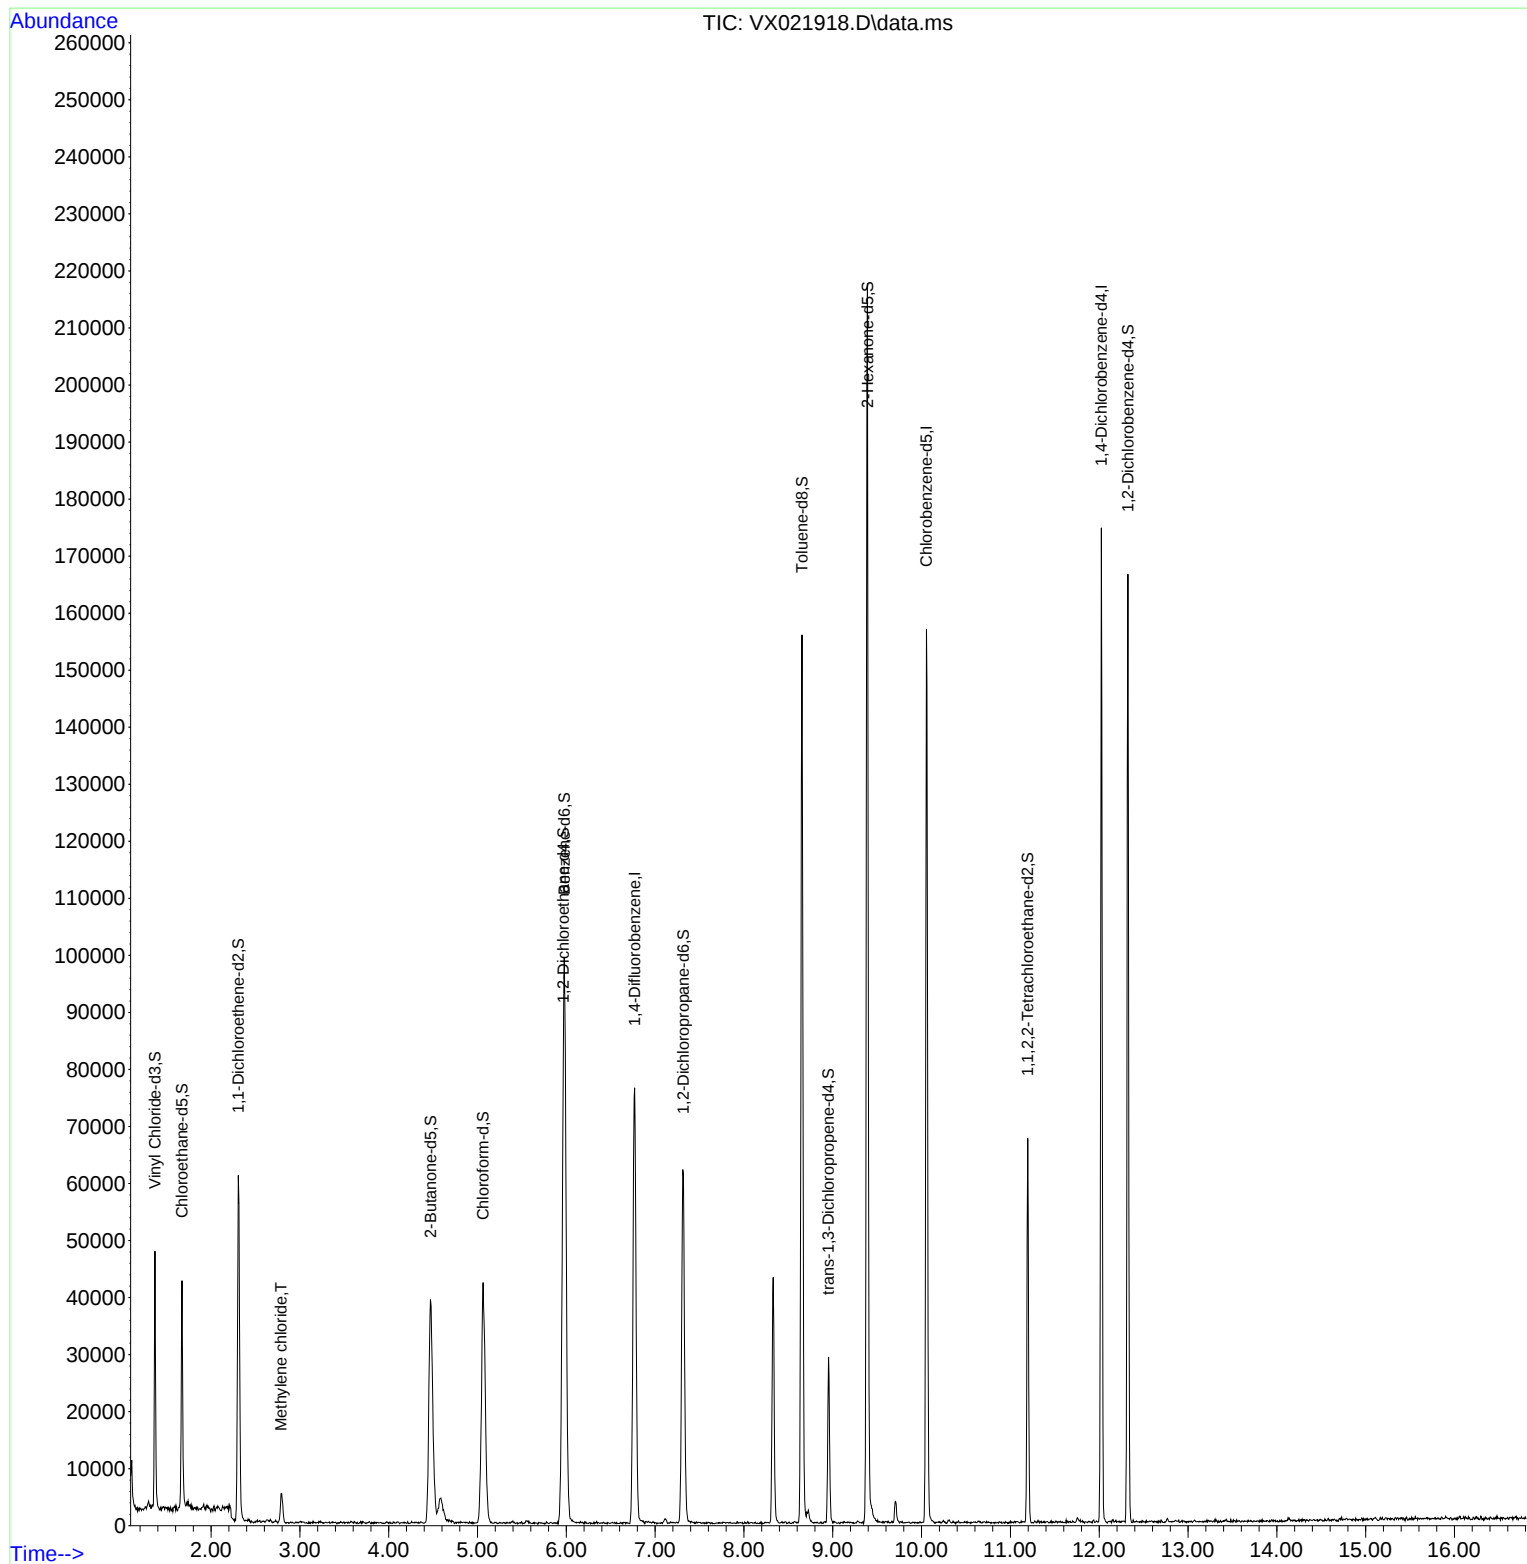

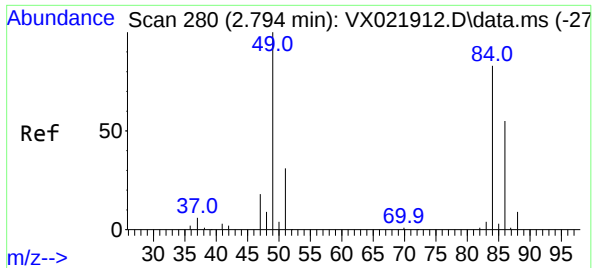

#16
Methylene chloride
Concen: 0.29 ug/L
RT: 2.788 min Scan# 279
Delta R.T. -0.006 min
Lab File: VX021918.D
Acq: 11 May 2021 22:57

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Tgt Ion: 84 Resp: 2229

Ion	Ratio	Lower	Upper
84	100		
86	58.4	46.3	86.1
49	122.6	84.4	156.7

