

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051121\
 Data File : VX021919.D
 Acq On : 11 May 2021 23:21
 Operator : JC/MD
 Sample : M2339-08
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Quant Time: May 12 06:28:27 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR051021WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed May 12 06:12:28 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.769	114	77349	5.00	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	69762	5.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	32293	5.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.367	65	25835	3.89	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	77.80%	
7) Chloroethane-d5	1.672	69	22649	4.25	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	85.00%	
11) 1,1-Dichloroethene-d2	2.306	63	32762	2.97	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	59.40%#	
20) 2-Butanone-d5	4.471	46	75194	49.68	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	99.36%	
24) Chloroform-d	5.068	84	48646	4.26	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	85.20%	
26) 1,2-Dichloroethane-d4	5.964	65	26472	4.52	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	90.40%	
32) Benzene-d6	5.976	84	100146	4.33	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	86.60%	
36) 1,2-Dichloropropane-d6	7.311	67	31774	4.48	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	89.60%	
41) Toluene-d8	8.653	98	87566	4.17	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	83.40%	
43) trans-1,3-Dichloroprop...	8.951	79	12840	4.01	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	80.20%	
46) 2-Hexanone-d5	9.390	63	64978	47.75	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	95.50%	
56) 1,1,2,2-Tetrachloroeth...	11.195	84	23979	4.38	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	87.60%	
66) 1,2-Dichlorobenzene-d4	12.323	152	28922	4.27	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	85.40%	
Target Compounds						Qvalue
16) Methylene chloride	2.794	84	2275	0.30	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051121\
Data File : VX021919.D
Acq On : 11 May 2021 23:21
Operator : JC/MD
Sample : M2339-08
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Time: May 12 06:28:27 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR051021WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed May 12 06:12:28 2021
Response via : Initial Calibration

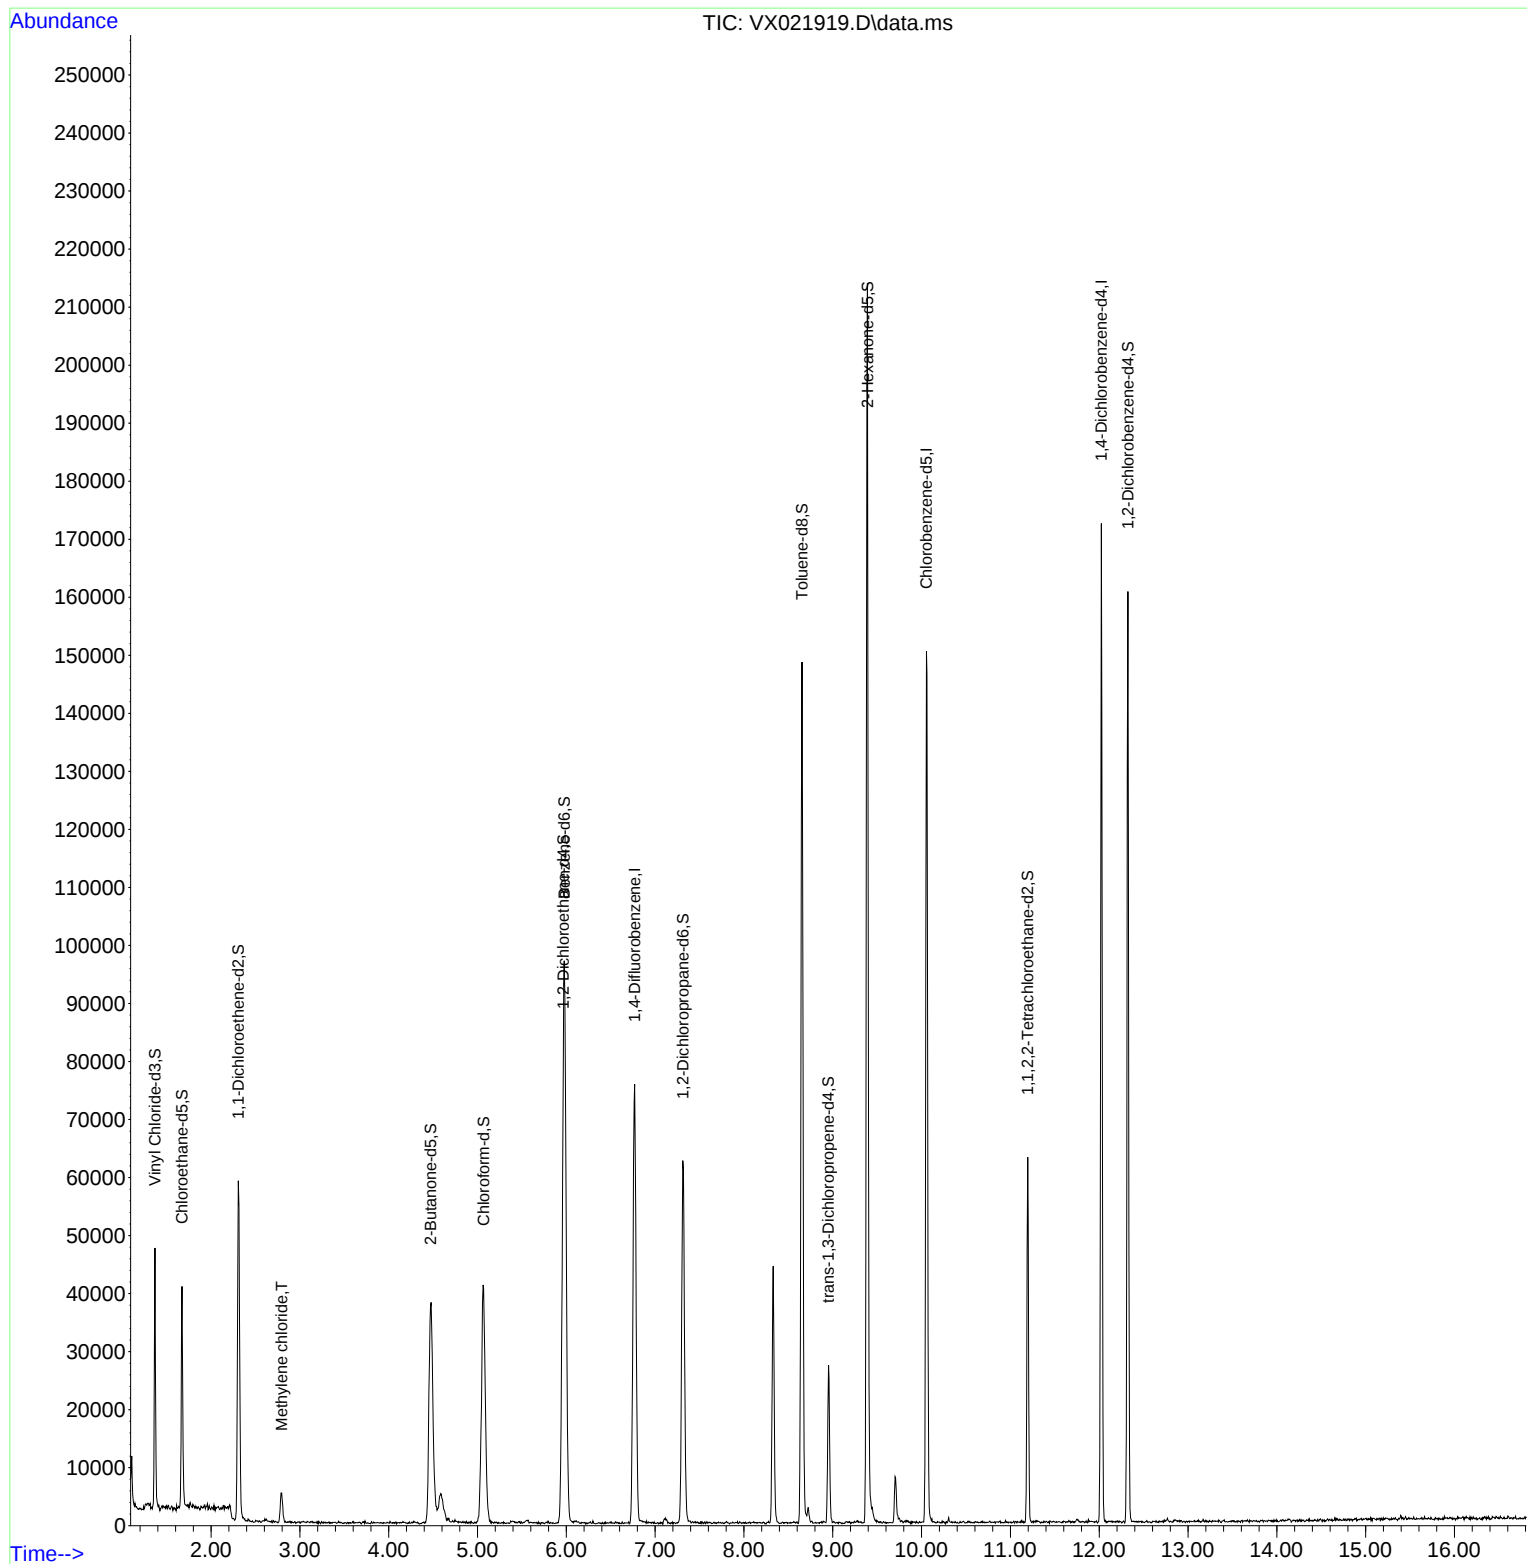

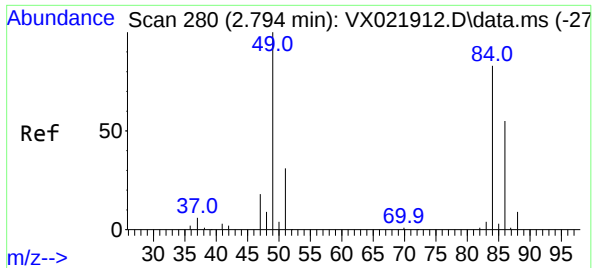

#16
Methylene chloride
Concen: 0.30 ug/L
RT: 2.794 min Scan# 280
Delta R.T. -0.000 min
Lab File: VX021919.D
Acq: 11 May 2021 23:21

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Tgt Ion:	84	Resp:	2275
Ion	Ratio	Lower	Upper
84	100		
86	71.0	46.3	86.1
49	116.9	84.4	156.7

