

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051121\
 Data File : VX021911.D
 Acq On : 11 May 2021 19:50
 Operator : JC/MD
 Sample : M2339-07
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0AW6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR051021WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VX021911.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	54	rVB	46023	44642	14.10%	1.719%
2	1.672	91	96	101	rBV	38548	46056	14.54%	1.773%
3	2.306	194	200	210	rVV	67683	106451	33.61%	4.099%
4	2.398	210	215	220	rVB2	1713	3546	1.12%	0.137%
5	2.581	237	245	246	rBV	3904	6720	2.12%	0.259%
6	2.599	246	248	263	rVB2	3991	11997	3.79%	0.462%
7	2.867	286	292	301	rBV2	6112	12538	3.96%	0.483%
8	4.465	544	554	565	rBV	41375	123078	38.86%	4.739%
9	4.580	565	573	586	rVV2	4907	17829	5.63%	0.687%
10	4.721	589	596	607	rVB3	4677	13097	4.14%	0.504%
11	5.068	642	653	666	rBV2	43262	129461	40.88%	4.985%
12	5.976	788	802	815	rBV2	105686	307540	97.11%	11.842%
13	6.769	921	932	944	rBV	74330	177484	56.04%	6.834%
14	7.318	1012	1022	1032	rBV2	65883	145091	45.81%	5.587%
15	8.330	1179	1188	1196	rBV	45632	76999	24.31%	2.965%
16	8.488	1208	1214	1224	rBV4	2813	5378	1.70%	0.207%
17	8.653	1235	1241	1249	rBV	165143	259451	81.92%	9.991%
18	8.720	1249	1252	1258	rVB4	3738	6404	2.02%	0.247%
19	8.952	1282	1290	1297	rBV	30216	44215	13.96%	1.703%
20	9.384	1355	1361	1370	rBV	216019	316700	100.00%	12.195%
21	10.055	1464	1471	1484	rBV	149880	211395	66.75%	8.140%
22	10.659	1563	1570	1578	rVB2	3763	5705	1.80%	0.220%
23	11.195	1653	1658	1664	rVB	70962	86227	27.23%	3.320%
24	12.024	1789	1794	1803	rVB	169306	207897	65.64%	8.006%
25	12.225	1823	1827	1834	rBV4	2770	5256	1.66%	0.202%
26	12.323	1838	1843	1851	rVB	183605	225764	71.29%	8.694%




Sum of corrected areas: 2596921

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051121\
Data File : VX021911.D
Acq On : 11 May 2021 19:50
Operator : JC/MD
Sample : M2339-07
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0AW6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR051021WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

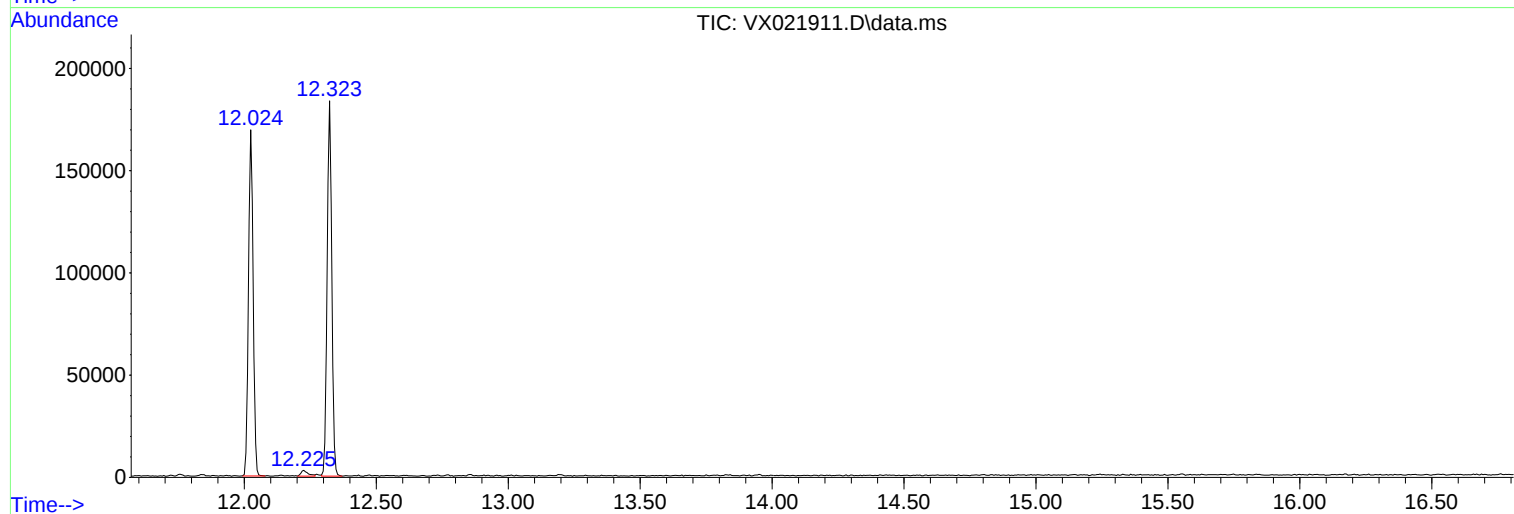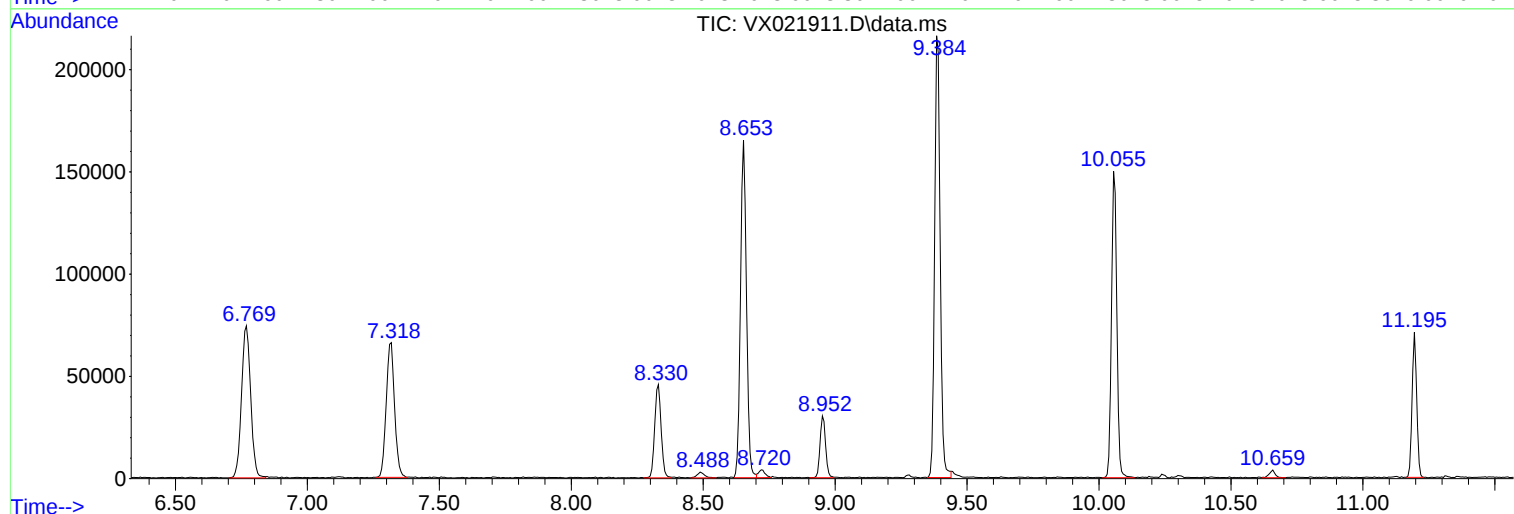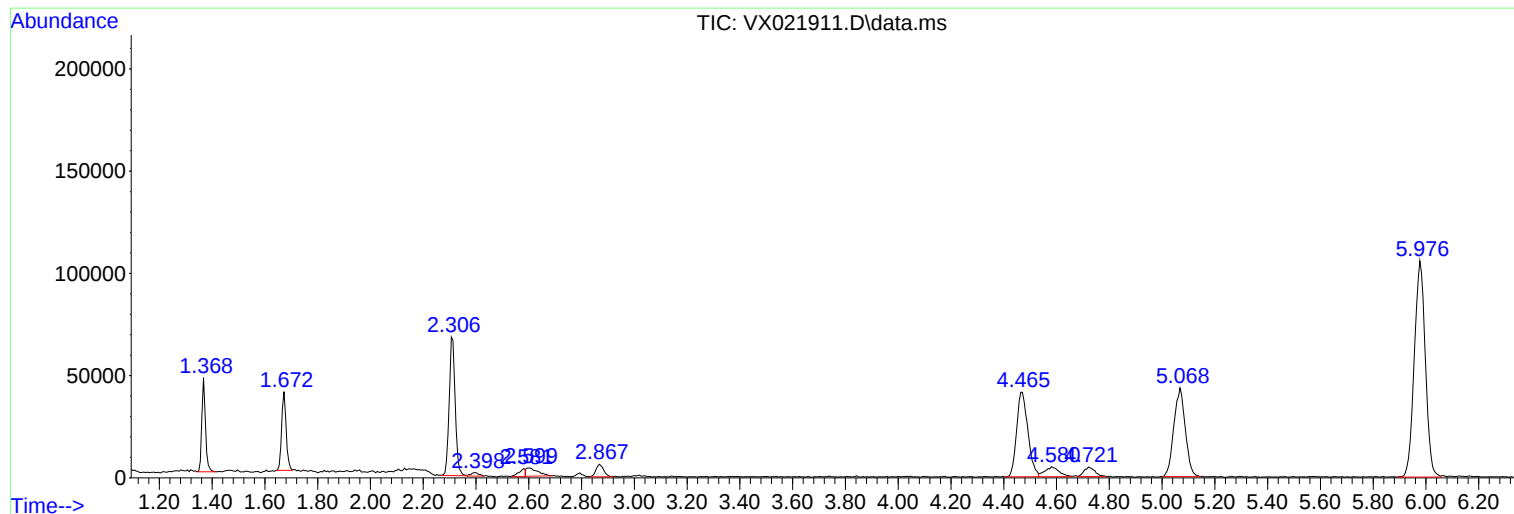

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051121\
Data File : VX021911.D
Acq On : 11 May 2021 19:50
Operator : JC/MD
Sample : M2339-07
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0AW6










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR051021WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown-01 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.580	0.50 ug/L	17829	1,4-Difluorobenzene	6.769

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Formamide, N-methylthio	75	C2H5NS	018952-41-5	9
2			tert-Butyldimethylsilanol	132	C6H16OSi	018173-64-3	9
3			Aminoacetaldehyde dimethyl acetal	105	C4H11NO2	022483-09-6	4
4			Ethanethioamide	75	C2H5NS	000062-55-5	4
5			Silanol, trimethyl-	90	C3H10OSi	001066-40-6	4

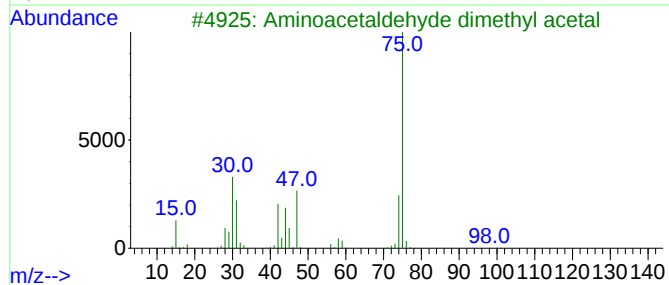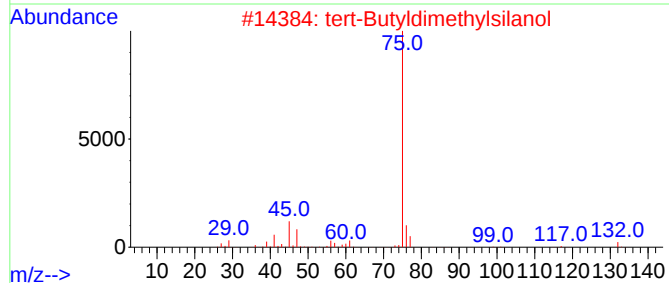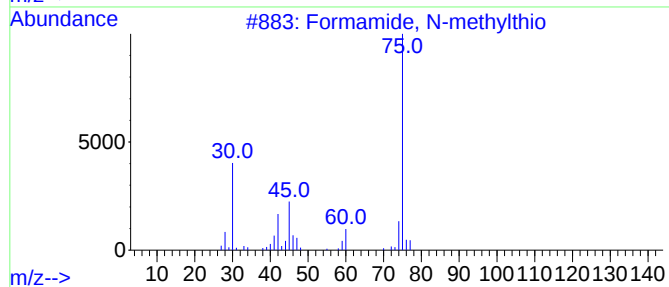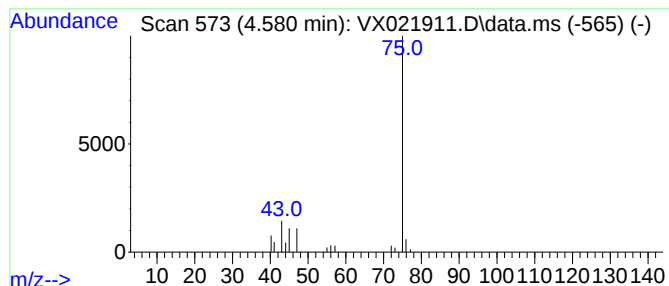

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051121\
Data File : VX021911.D
Acq On : 11 May 2021 19:50
Operator : JC/MD
Sample : M2339-07
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0AW6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR051021WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	4.580	0.5	ug/L	17829	1	6.769	177484	5.0