

m/z	Abundance
39.90	116.0
42.20	71.0
44.10	390.0
91.00	58.0

Instrument :
MSVOA_X
ClientSampleId :
BFB170

m/z	Abundance
36.00	407.0
37.10	1431.0
38.00	1567.0
39.00	645.0
40.00	209.0
41.00	67.0
42.90	157.0
44.10	787.0
44.90	334.0
46.90	290.0
47.90	277.0
49.00	1557.0
50.10	6987.0
51.10	2077.0
52.00	66.0
55.00	139.0
56.00	871.0
57.00	1246.0
57.90	139.0
60.00	384.0
61.00	1922.0
62.00	1603.0
63.00	1457.0
64.00	144.0
64.30	75.0
67.00	87.0
68.10	3544.0
69.10	4001.0
70.10	299.0
72.10	240.0
73.00	1690.0
74.10	7003.0
75.10	19848.0
76.10	1618.0
76.90	150.0
78.10	297.0
78.90	1572.0
79.90	386.0
81.00	1760.0
81.90	403.0
86.10	64.0
87.00	1973.0
87.90	1338.0
91.00	120.0
92.10	1383.0
93.10	1660.0
94.10	5005.0
95.10	40072.0
96.00	2701.0
104.00	260.0
105.10	162.0
105.90	184.0
110.90	58.0
116.00	267.0
117.10	270.0
118.00	195.0
119.00	269.0
127.90	163.0
128.90	67.0
130.00	157.0
135.10	99.0
141.00	596.0
142.00	70.0
143.00	367.0
145.10	68.0
146.00	60.0
148.00	87.0
155.10	132.0
172.90	381.0
174.00	31368.0
175.00	2362.0
176.00	31976.0
177.10	1700.0

Instrument :
MSVOA_X
ClientSampleId :
BFB170

m/z	Abundance
36.10	400.0
37.10	3273.0
38.10	2985.0
39.10	1080.0
40.00	117.0
41.20	85.0
43.10	104.0
44.00	866.0
45.10	618.0
47.10	979.0
48.00	342.0
49.10	2683.0
50.10	11551.0
51.10	3541.0
52.20	190.0
55.10	345.0
56.10	1131.0
57.00	2134.0
58.00	103.0
60.10	674.0
61.00	2970.0
62.10	3108.0
63.00	2535.0
63.90	197.0
67.00	261.0
68.10	6701.0
69.10	7064.0
70.00	742.0
72.00	440.0
73.00	3350.0
74.10	10276.0
75.10	33144.0
76.10	2724.0
77.10	295.0
78.10	340.0
79.00	2778.0
80.00	773.0
81.00	2794.0
81.90	627.0
82.90	72.0
86.10	73.0
87.00	2645.0
88.00	2893.0
91.00	247.0
92.00	1880.0
93.00	2719.0
94.10	7678.0
95.10	66352.0
96.10	4041.0
96.90	139.0
103.00	77.0
104.00	403.0
104.90	135.0
105.90	271.0
111.10	80.0
115.90	227.0
117.10	333.0
117.90	414.0
118.90	426.0
128.00	315.0
129.20	56.0
129.90	135.0
131.10	77.0
135.10	132.0
137.00	91.0
141.00	748.0
142.10	102.0
142.90	589.0
145.10	117.0
146.10	77.0
148.10	92.0
155.10	178.0
157.00	80.0
159.10	55.0
173.00	283.0
174.00	44280.0
175.10	3169.0
176.10	43136.0
177.00	2839.0

Instrument :
MSVOA_X
ClientSampleId :
BFB170

m/z	Abundance
36.10	449.0
37.00	2851.0
38.10	2908.0
39.10	1068.0
40.10	156.0
41.30	130.0
43.00	103.0
44.00	931.0
45.00	717.0
47.10	834.0
48.10	417.0
49.00	2674.0
50.10	11259.0
51.10	4006.0
52.10	170.0
55.00	230.0
56.00	1204.0
57.10	1881.0
58.00	111.0
60.10	422.0
61.00	2948.0
62.00	3105.0
63.10	2281.0
64.00	210.0
67.20	206.0
68.10	6233.0
69.00	6888.0
70.10	446.0
72.00	272.0
73.10	2631.0
74.10	10249.0
75.10	32736.0
76.10	2799.0
76.80	286.0
77.20	408.0
77.80	302.0
78.90	2632.0
80.00	650.0
80.90	2651.0
81.90	613.0
85.90	71.0
87.00	2419.0
88.10	2280.0
91.00	200.0
92.00	2012.0
93.10	2643.0
94.10	7352.0
95.10	62824.0
96.10	4475.0
97.00	176.0
103.00	66.0
104.00	382.0
104.90	126.0
105.90	299.0
107.10	66.0
111.30	77.0
115.80	156.0
117.00	434.0
118.00	328.0
119.10	286.0
124.10	56.0
128.00	242.0
129.80	173.0
131.00	91.0
135.00	99.0
137.20	77.0
140.90	744.0
142.10	103.0
143.10	551.0
146.10	71.0
148.00	104.0
155.00	81.0
157.00	81.0
159.10	81.0
161.10	84.0
172.90	330.0
174.00	35088.0
175.00	2603.0
176.00	33632.0
177.10	2268.0



Instrument :
MSVOA_X
ClientSampleId :
BFB170

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051121\
 Data File : VX021888.D
 Acq On : 11 May 2021 09:20
 Operator : JC/MD
 Sample : BFB70
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB170

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR051021WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Wed May 12 06:12:28 2021

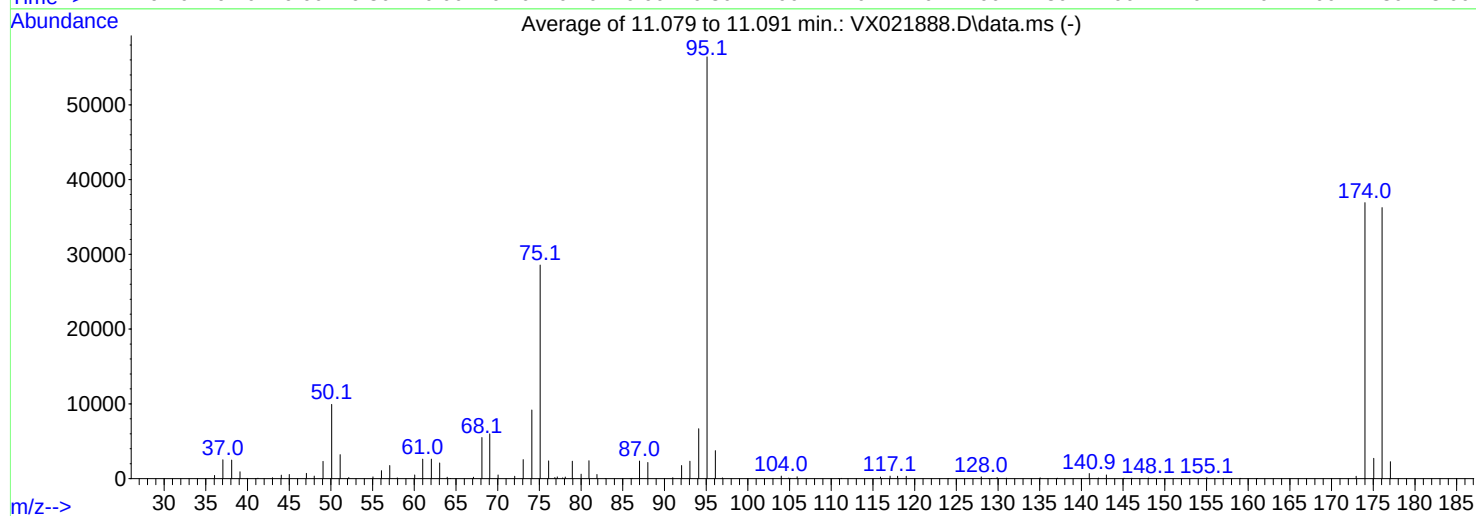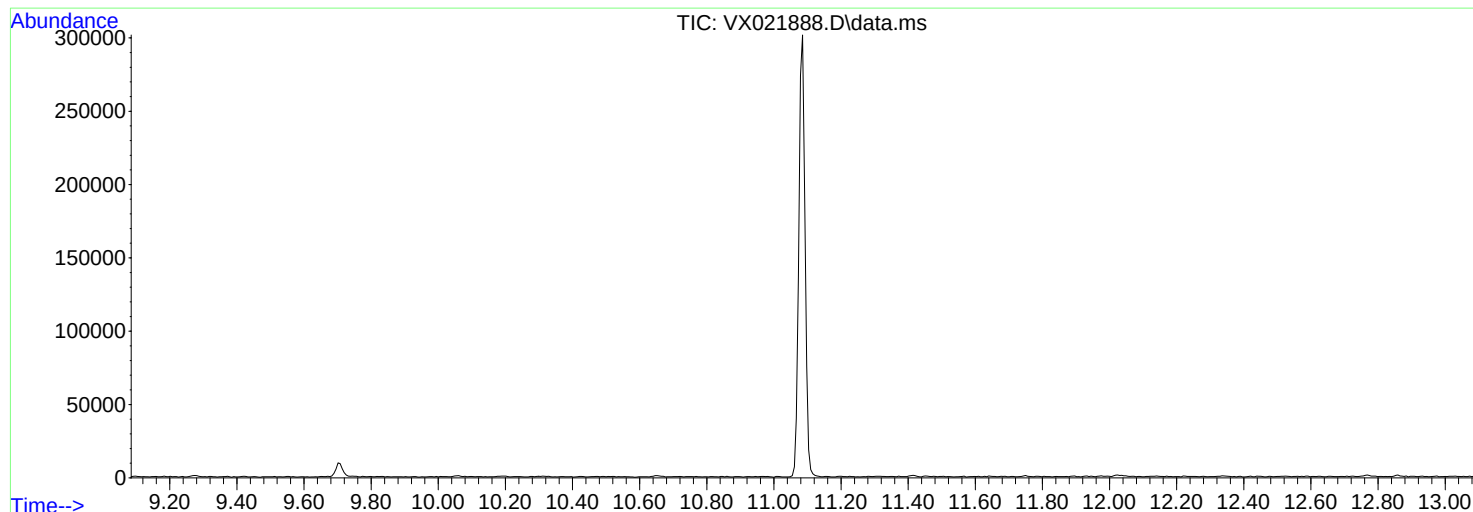

AutoFind: Scans 1639, 1640, 1641; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.6	9932	PASS
75	95	30	80	50.7	28576	PASS
95	95	100	100	100.0	56416	PASS
96	95	5	9	6.6	3739	PASS
173	174	0.00	2	0.9	331	PASS
174	95	50	120	65.4	36912	PASS
175	174	5	9	7.3	2711	PASS
176	174	95	105	98.2	36248	PASS
177	176	5	10	6.3	2269	PASS