

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051122\
 Data File : VX028620.D
 Acq On : 11 May 2022 14:13
 Operator : JC/MD
 Sample : N2761-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TWP05

Quant Time: May 12 04:55:50 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X042822W.M
 Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 QLast Update : Fri Apr 29 06:09:36 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Bromochloromethane	4.904	128	49981	30.000	ug/l	0.00
28) 1,4-Difluorobenzene	6.763	114	266547	30.000	ug/l	0.00
57) Chlorobenzene-d5	10.055	117	241008	30.000	ug/l	0.00
System Monitoring Compounds						
27) 1,2-Dichloroethane-d4	5.958	65	103057	32.422	ug/l	0.00
Spiked Amount	30.000	Range	91 - 110	Recovery	=	108.067%
60) 4-Bromofluorobenzene	11.085	95	101486	27.077	ug/l	0.00
Spiked Amount	30.000	Range	63 - 112	Recovery	=	90.267%
63) Toluene-d8	8.653	98	314340	30.788	ug/l	0.00
Spiked Amount	30.000	Range	91 - 112	Recovery	=	102.633%
Target Compounds						
15) Acetone	2.374	58	1369	3.530	ug/l	Qvalue 90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051122\
Data File : VX028620.D
Acq On : 11 May 2022 14:13
Operator : JC/MD
Sample : N2761-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TWP05

Quant Time: May 12 04:55:50 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X042822W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
QLast Update : Fri Apr 29 06:09:36 2022
Response via : Initial Calibration




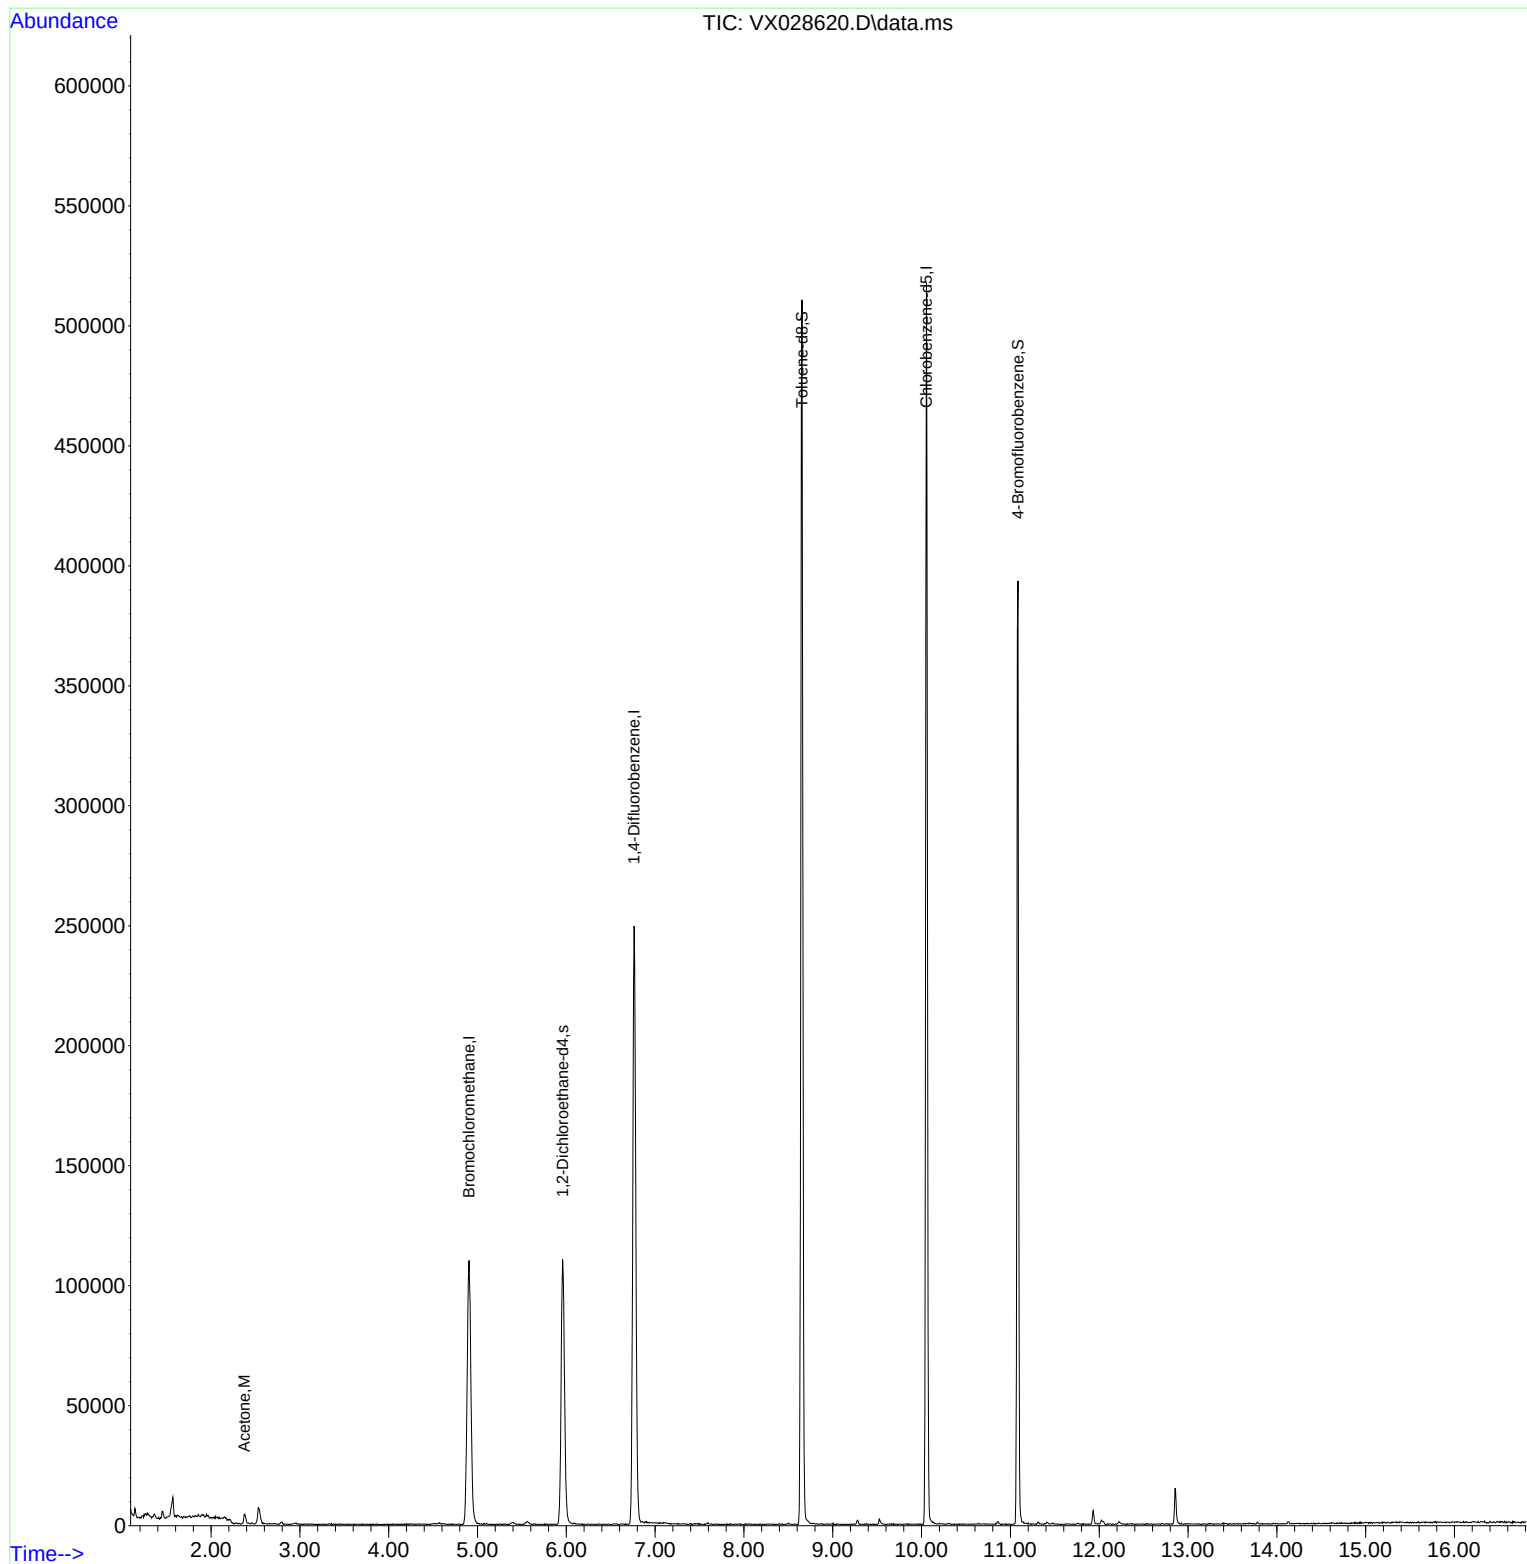


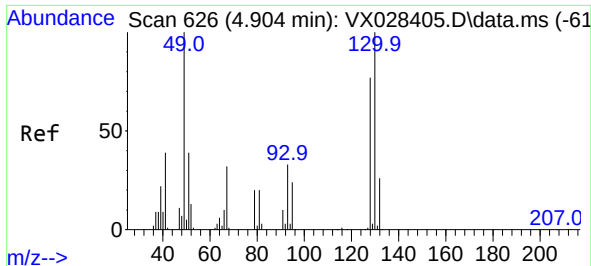

#1
Bromochloromethane
Concen: 30.000 ug/l
RT: 4.904 min Scan# 61
Delta R.T. -0.000 min
Lab File: VX028620.D
Acq: 11 May 2022 14:13




Instrument :
MSVOA_X
ClientSampleId :
TWP05


Tgt Ion:128 Resp: 49981
Ion Ratio Lower Upper
128 100
49 130.3 0.0 358.3
130 129.2 0.0 319.3

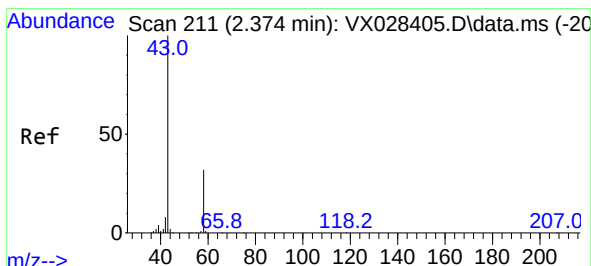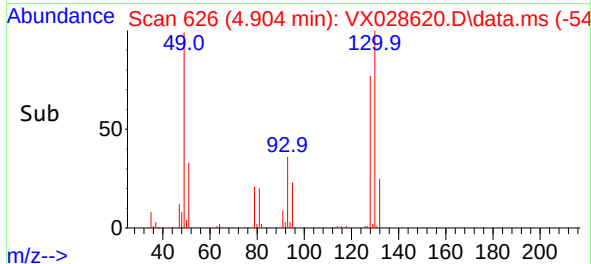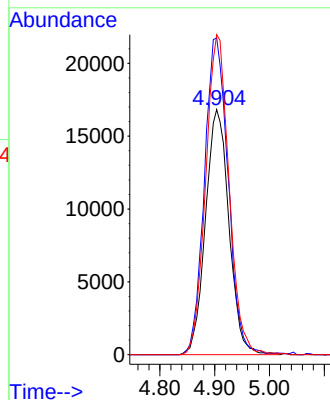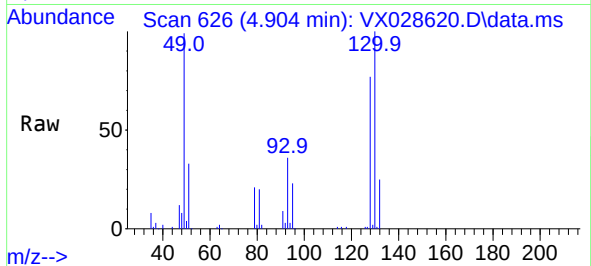

#15
Acetone
Concen: 3.530 ug/l
RT: 2.374 min Scan# 211
Delta R.T. -0.000 min
Lab File: VX028620.D
Acq: 11 May 2022 14:13

Tgt Ion: 58 Resp: 1369
Ion Ratio Lower Upper
58 100
43 293.1 250.2 375.2


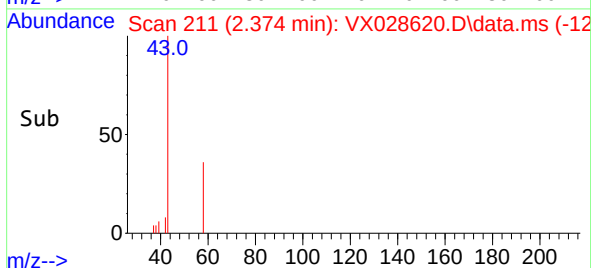
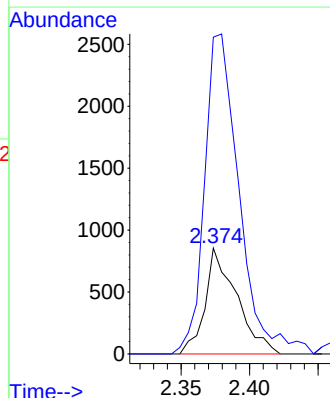
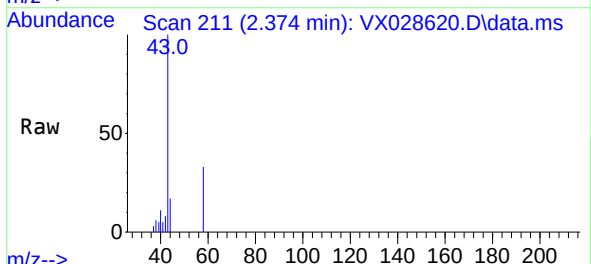


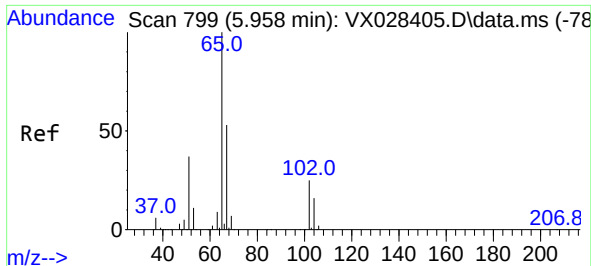

#27
1,2-Dichloroethane-d4
Concen: 32.422 ug/l
RT: 5.958 min Scan# 799
Delta R.T. -0.000 min
Lab File: VX028620.D
Acq: 11 May 2022 14:13




Instrument :
MSVOA_X
ClientSampleId :
TWP05


Tgt Ion: 65 Resp: 103057
Ion Ratio Lower Upper
65 100
67 51.5 42.3 63.5

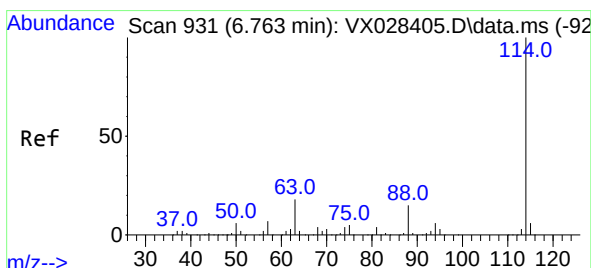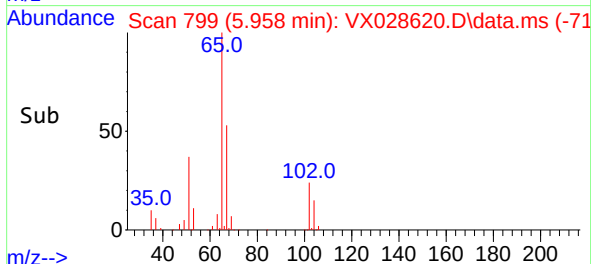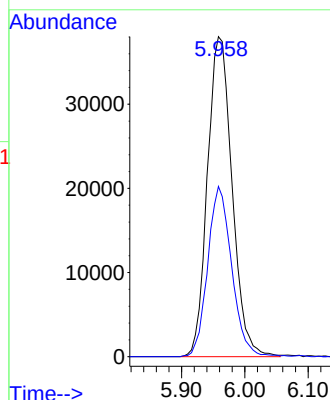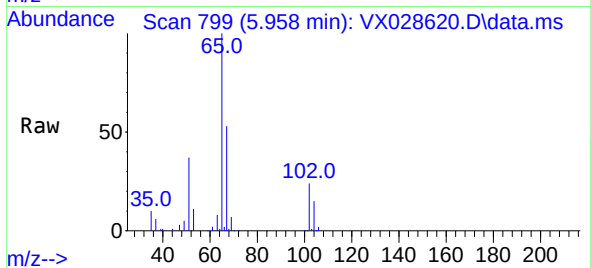

#28
1,4-Difluorobenzene
Concen: 30.000 ug/l
RT: 6.763 min Scan# 931
Delta R.T. -0.000 min
Lab File: VX028620.D
Acq: 11 May 2022 14:13

Tgt Ion: 114 Resp: 266547
Ion Ratio Lower Upper
114 100
63 18.3 15.3 22.9
88 14.9 12.2 18.4


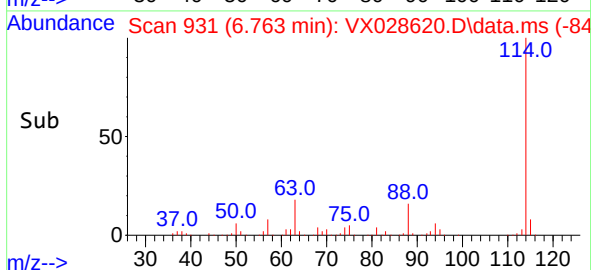
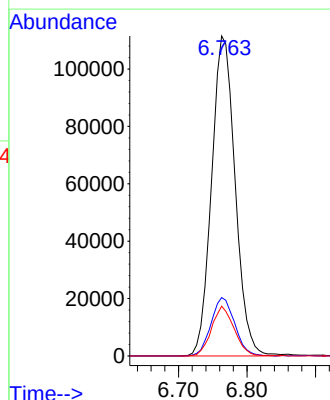
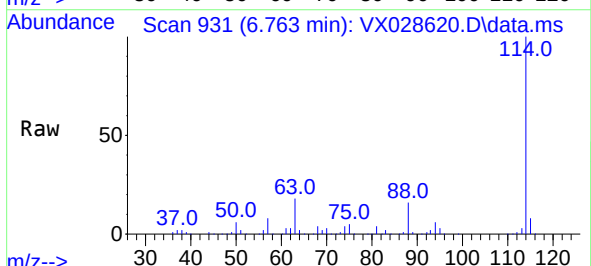


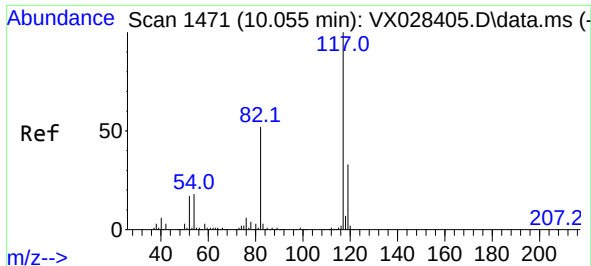

#57
Chlorobenzene-d5
Concen: 30.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX028620.D
Acq: 11 May 2022 14:13




Instrument :
MSVOA_X
ClientSampleId :
TWP05


Tgt Ion:117 Resp: 241008
Ion Ratio Lower Upper
117 100
82 52.0 42.3 63.5
119 31.9 26.2 39.2

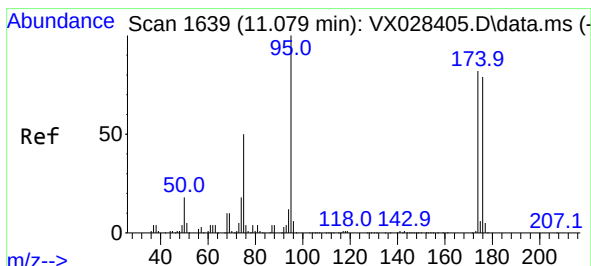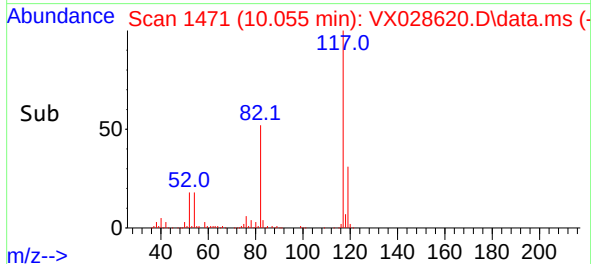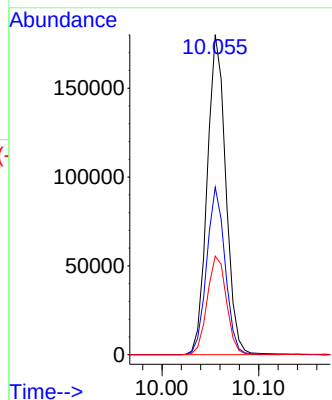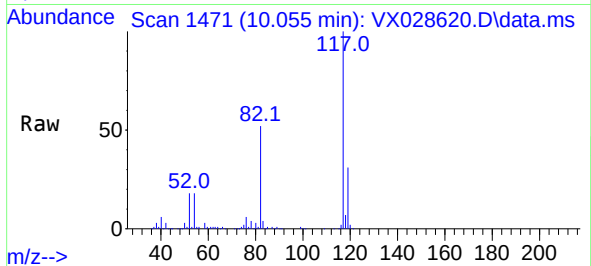

#60
4-Bromofluorobenzene
Concen: 27.077 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.006 min
Lab File: VX028620.D
Acq: 11 May 2022 14:13

Tgt Ion: 95 Resp: 101486
Ion Ratio Lower Upper
95 100
174 88.1 65.4 98.2
176 83.2 63.4 95.0

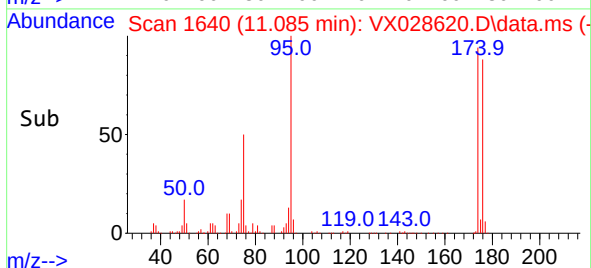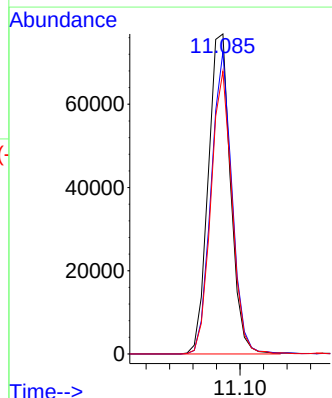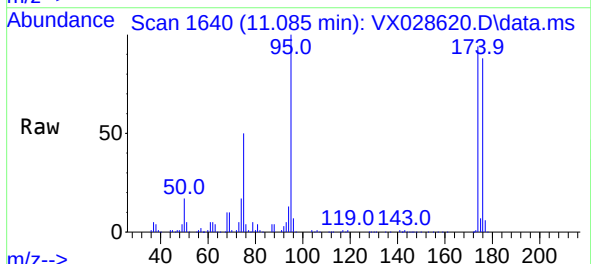

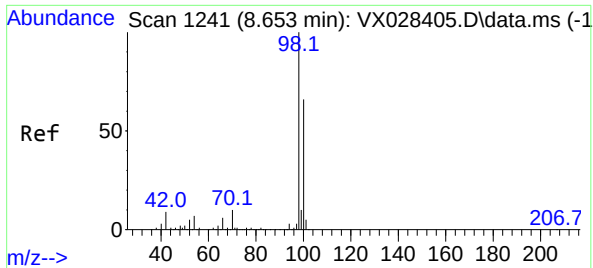

#63
Toluene-d8
Concen: 30.788 ug/l
RT: 8.653 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX028620.D
Acq: 11 May 2022 14:13

Instrument :
MSVOA_X
ClientSampleId :
TWP05

Tgt Ion: 98 Resp: 314340
Ion Ratio Lower Upper
98 100
100 64.4 51.4 77.2

