
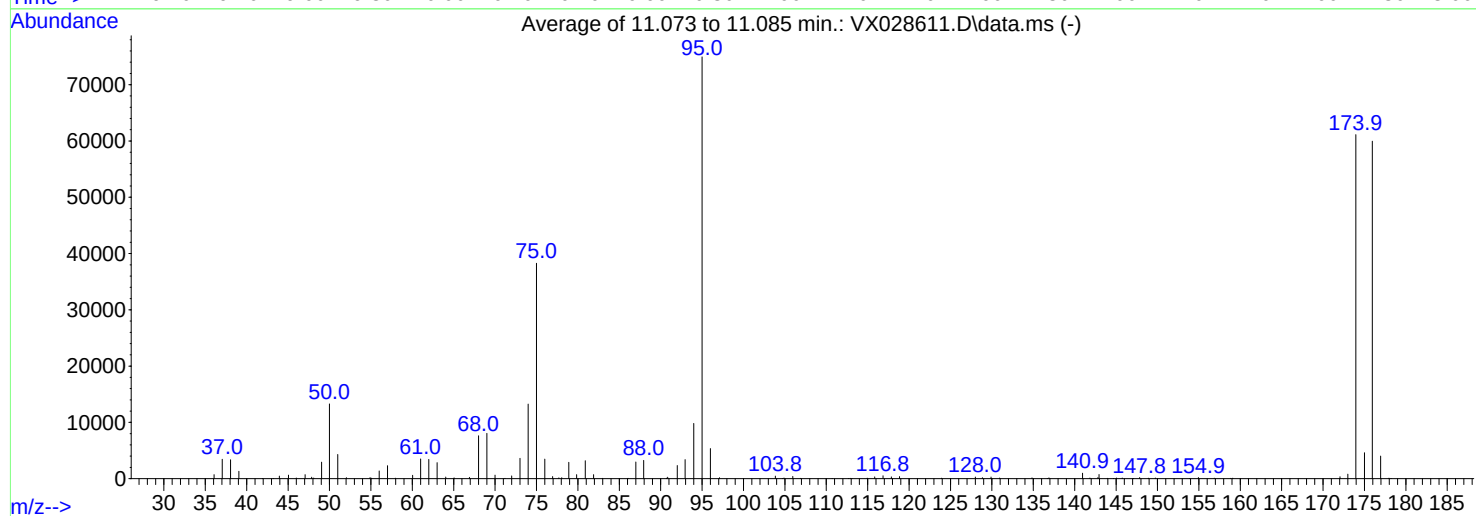


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051122\
 Data File : VX028611.D
 Acq On : 11 May 2022 10:11
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X042822W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Fri Apr 29 06:09:36 2022

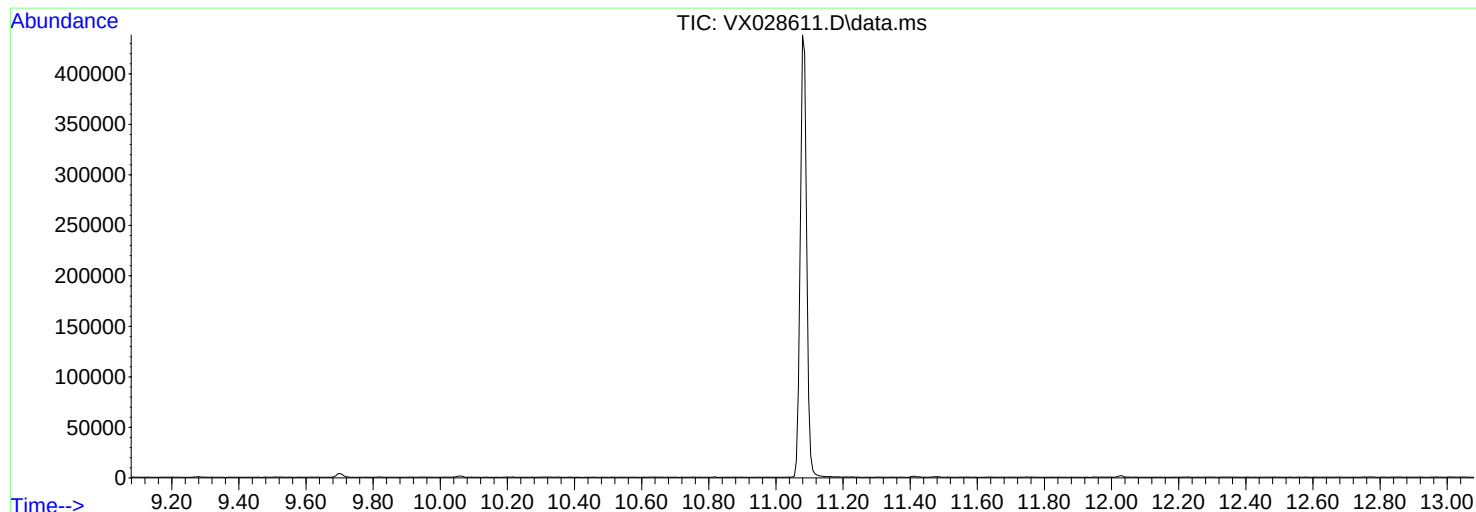

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.7	13283	PASS
75	95	30	60	51.1	38264	PASS
95	95	100	100	100.0	74952	PASS
96	95	5	9	7.1	5339	PASS
173	174	0.00	2	1.3	791	PASS
174	95	50	100	81.6	61141	PASS
175	174	5	9	7.5	4597	PASS
176	174	95	101	98.1	59968	PASS
177	176	5	9	6.7	4026	PASS