

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051123\
 Data File : VX035618.D
 Acq On : 11 May 2023 19:23
 Operator : JC/MD
 Sample : 02755-01 50X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 A5560

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051123W.M
 Title : SW846 8260

Signal : TIC: VX035618.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.385	694	705	720	rBV	126256	367077	32.27%	5.685%
2	5.550	720	732	746	rVV2	216463	616456	54.20%	9.547%
3	5.958	788	799	816	rBV	150250	405863	35.68%	6.286%
4	6.763	919	931	945	rBV	350342	845866	74.37%	13.100%
5	8.647	1232	1240	1248	rBV	731846	1137423	100.00%	17.615%
6	10.055	1465	1471	1485	rBV	744215	1013622	89.12%	15.698%
7	11.079	1634	1639	1649	rBV	618646	786889	69.18%	12.187%
8	12.018	1788	1793	1802	rBV	713398	933655	82.09%	14.460%
9	13.140	1971	1977	1984	rBV2	7681	12838	1.13%	0.199%
10	15.176	2302	2311	2317	rBV9	7786	26575	2.34%	0.412%
11	15.249	2321	2323	2331	rVV6	6846	11415	1.00%	0.177%
12	15.542	2364	2371	2384	rBV	96697	158875	13.97%	2.461%
13	15.981	2436	2443	2447	rBV8	4288	11409	1.00%	0.177%
14	16.468	2516	2523	2535	rBV	67166	129002	11.34%	1.998%




Sum of corrected areas: 6456965

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051123\
Data File : VX035618.D
Acq On : 11 May 2023 19:23
Operator : JC/MD
Sample : 02755-01 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
A5560

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

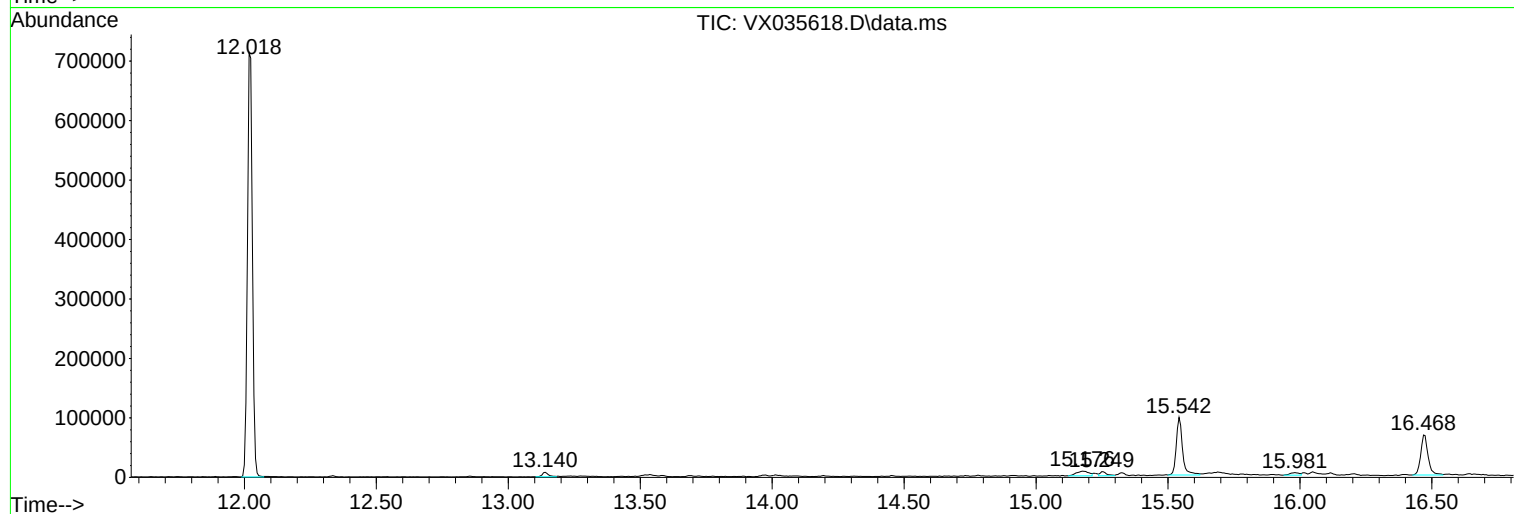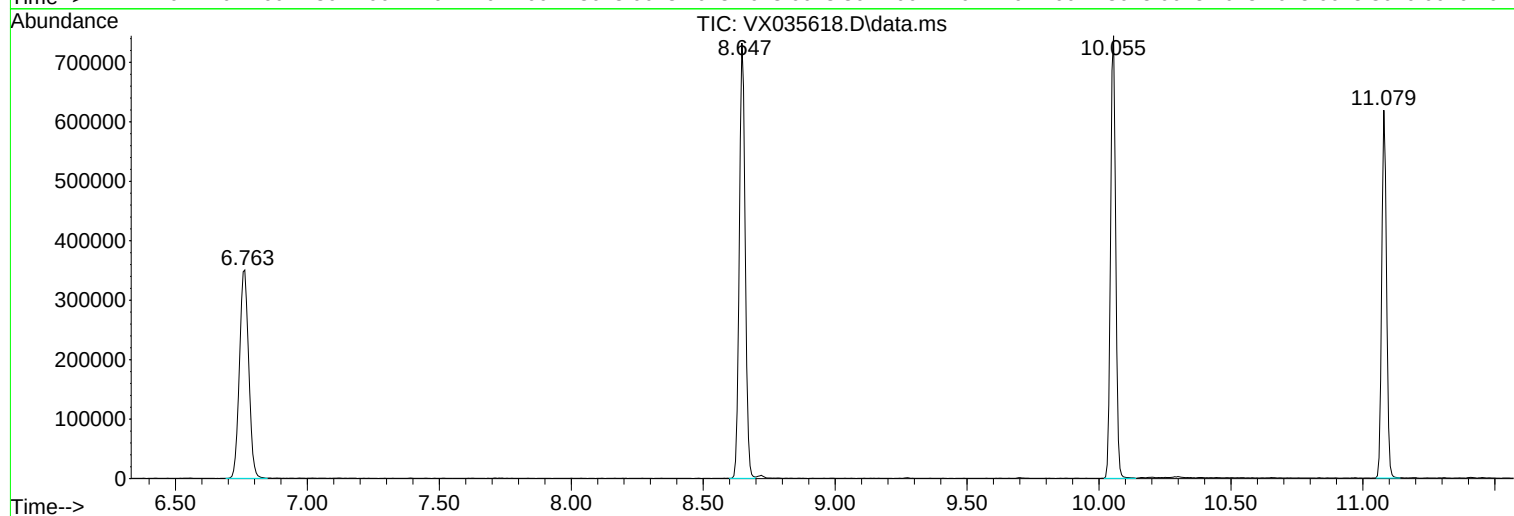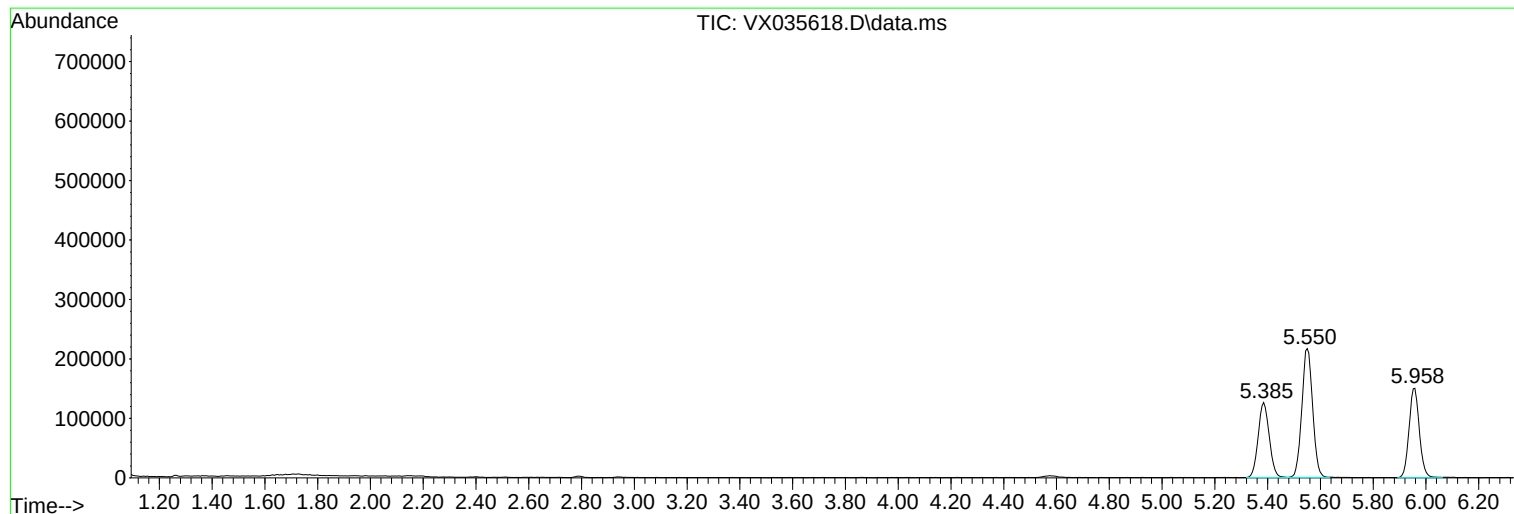

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051123\
Data File : VX035618.D
Acq On : 11 May 2023 19:23
Operator : JC/MD
Sample : 02755-01 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
A5560










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Dodecane, 1-chloro- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
15.542	8.51 ug/l	158875	1,4-Dichlorobenzene-d4	12.024

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Dodecane, 1-chloro-	204	C12H25Cl	000112-52-7	91
2			Tetradecane, 1-chloro-	232	C14H29Cl	002425-54-9	86
3			1-Chloroundecane	190	C11H23Cl	002473-03-2	78
4			Decane, 1-chloro-	176	C10H21Cl	001002-69-3	53
5			1-Octanol, 2-butyl-	186	C12H26O	003913-02-8	52

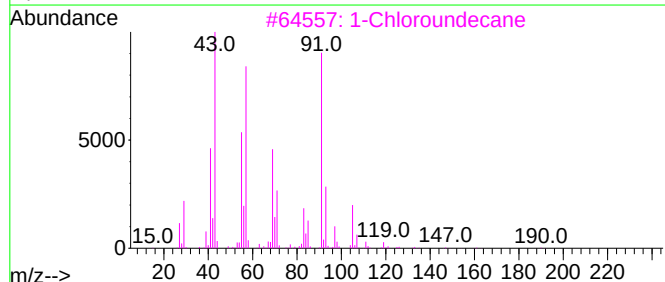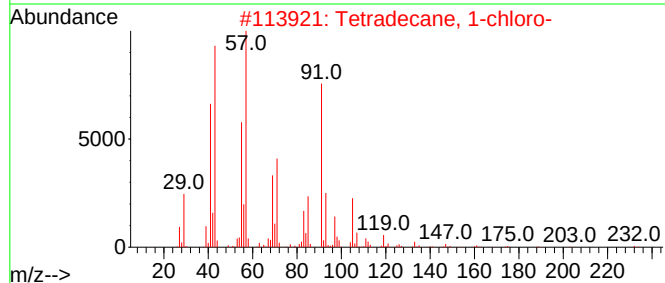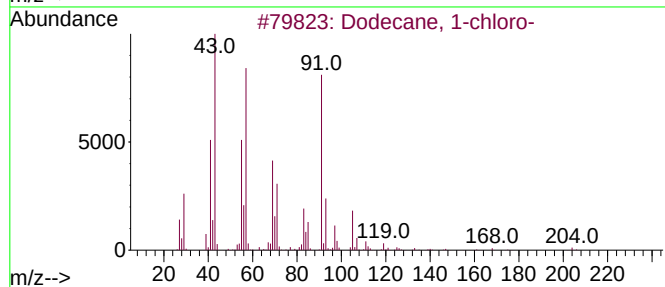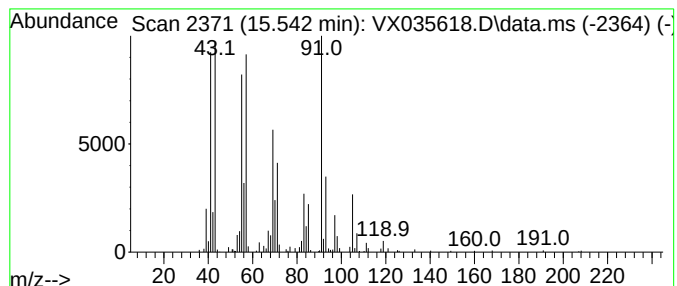

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051123\
Data File : VX035618.D
Acq On : 11 May 2023 19:23
Operator : JC/MD
Sample : 02755-01 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
A5560










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Oxalic acid, allyl dodecyl ... Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
16.468	6.91 ug/l	129002	1,4-Dichlorobenzene-d4	12.024

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Dodecane, 1-chloro-	204	C12H25Cl	000112-52-7	64
2			Oxalic acid, allyl dodecyl ester	298	C17H30O4	1000309-24-0	62
3			Tetradecane, 1-chloro-	232	C14H29Cl	002425-54-9	53
4			Oxalic acid, allyl pentadecyl ester	340	C20H36O4	1000309-24-3	52
5			Decane, 1-chloro-	176	C10H21Cl	001002-69-3	52

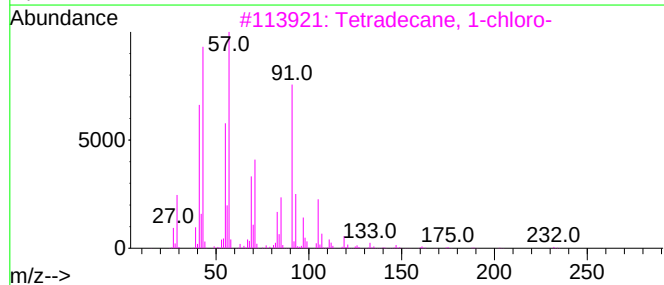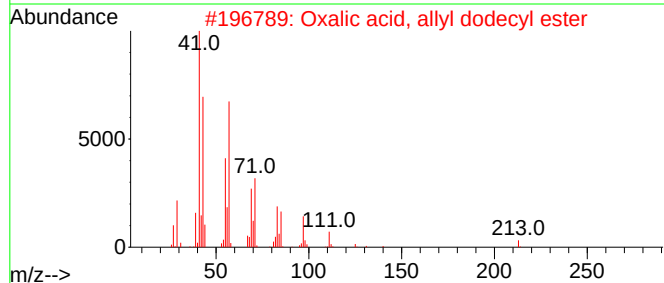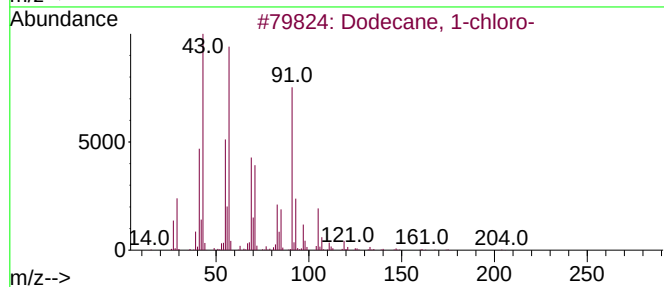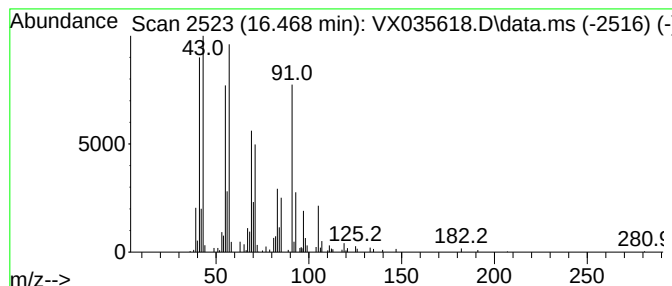

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051123\
Data File : VX035618.D
Acq On : 11 May 2023 19:23
Operator : JC/MD
Sample : 02755-01 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
A5560

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Dodecane, 1-chl...	15.542	8.5	ug/l	158875	4	12.024	933655	50.0
Oxalic acid, al...	16.468	6.9	ug/l	129002	4	12.024	933655	50.0