

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051123\
 Data File : VX035620.D
 Acq On : 11 May 2023 20:10
 Operator : JC/MD
 Sample : 02752-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 230510054-02-VOA

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051123W.M
 Title : SW846 8260

Signal : TIC: VX035620.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.386	206	213	221	rVB3	5911	11887	1.03%	0.133%
2	2.977	298	310	328	rBV	199073	664351	57.82%	7.416%
3	4.562	557	570	585	rBV	258356	866877	75.44%	9.676%
4	5.007	632	643	662	rBV2	190231	608515	52.96%	6.793%
5	5.385	691	705	717	rBV	133718	379591	33.03%	4.237%
6	5.550	720	732	747	rVB	221663	623883	54.29%	6.964%
7	5.952	788	798	812	rBV	154054	415693	36.18%	4.640%
8	6.239	833	845	857	rBV4	5543	23242	2.02%	0.259%
9	6.757	919	930	942	rBV	357567	854516	74.37%	9.538%
10	8.555	1221	1225	1233	rVB2	6685	13959	1.21%	0.156%
11	8.647	1233	1240	1248	rBV	752794	1149072	100.00%	12.826%
12	10.055	1465	1471	1477	rBV	737052	1007980	87.72%	11.252%
13	10.311	1499	1513	1517	rBV7	9300	23419	2.04%	0.261%
14	10.518	1542	1547	1558	rBV5	5336	12242	1.07%	0.137%
15	11.079	1634	1639	1646	rBV	627344	783758	68.21%	8.749%
16	11.506	1704	1709	1716	rBV	35932	53963	4.70%	0.602%
17	11.969	1780	1785	1788	rBV	10190	12546	1.09%	0.140%
18	12.018	1788	1793	1801	rVB	697413	916801	79.79%	10.234%
19	12.518	1872	1875	1882	rVB5	10261	17924	1.56%	0.200%
20	12.762	1906	1915	1919	rBV2	19628	35684	3.11%	0.398%
21	12.945	1937	1945	1950	rVV10	4752	11839	1.03%	0.132%
22	13.231	1988	1992	1997	rVB5	10597	12400	1.08%	0.138%
23	13.384	2012	2017	2020	rBV2	11555	15180	1.32%	0.169%
24	13.469	2026	2031	2035	rBV5	7525	12179	1.06%	0.136%
25	13.585	2045	2050	2057	rVB3	14984	22723	1.98%	0.254%
26	13.768	2076	2080	2086	rVB3	14675	21618	1.88%	0.241%
27	15.176	2301	2311	2315	rBV8	9433	25533	2.22%	0.285%
28	15.353	2331	2340	2344	rVB5	11114	23159	2.02%	0.259%
29	15.542	2363	2371	2378	rBV2	105770	165113	14.37%	1.843%
30	15.609	2378	2382	2387	rBV	23600	35181	3.06%	0.393%
31	16.469	2517	2523	2533	rBV	74268	137774	11.99%	1.538%




Sum of corrected areas: 8958602

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051123\
Data File : VX035620.D
Acq On : 11 May 2023 20:10
Operator : JC/MD
Sample : 02752-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
230510054-02-VOA

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

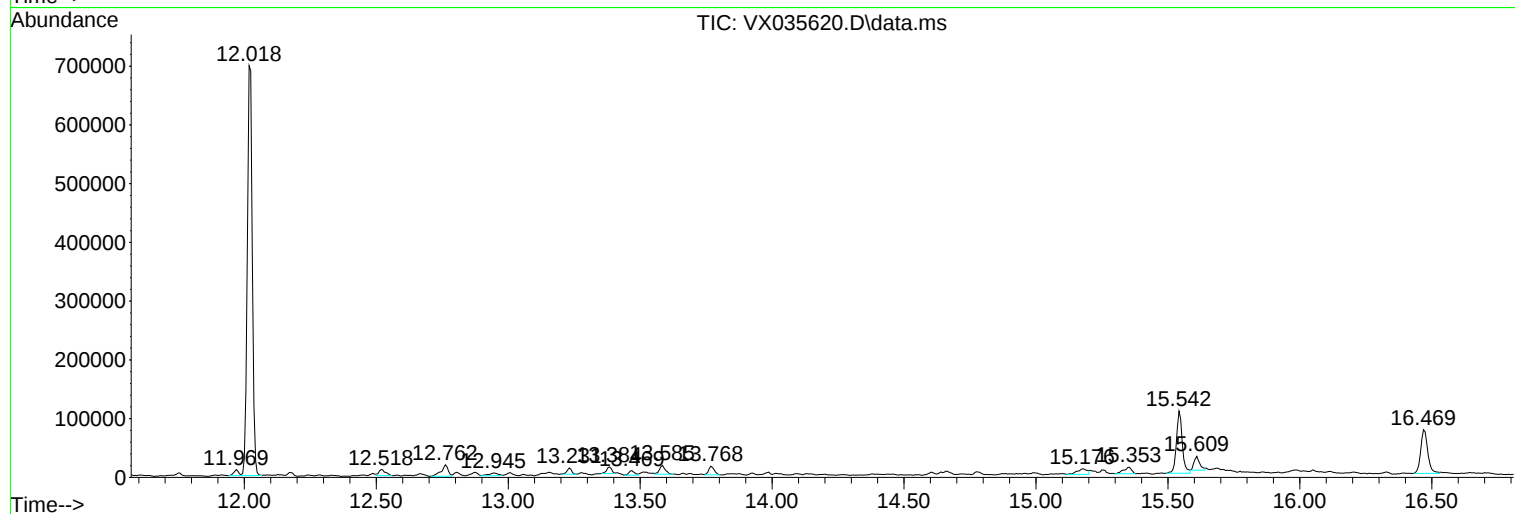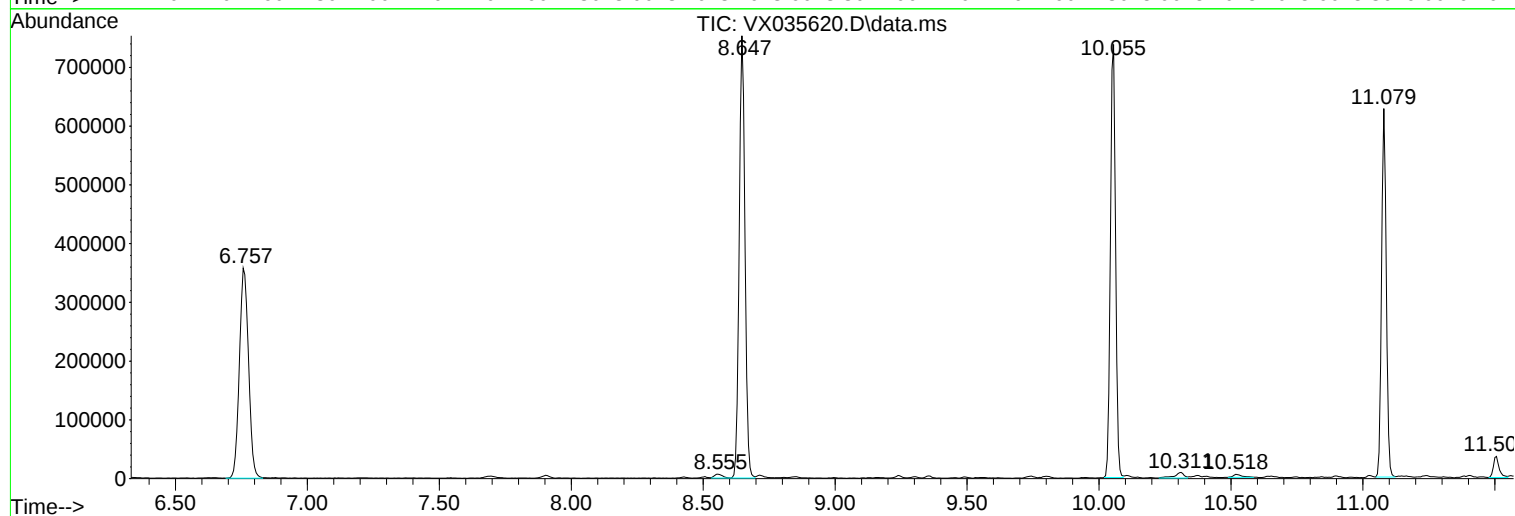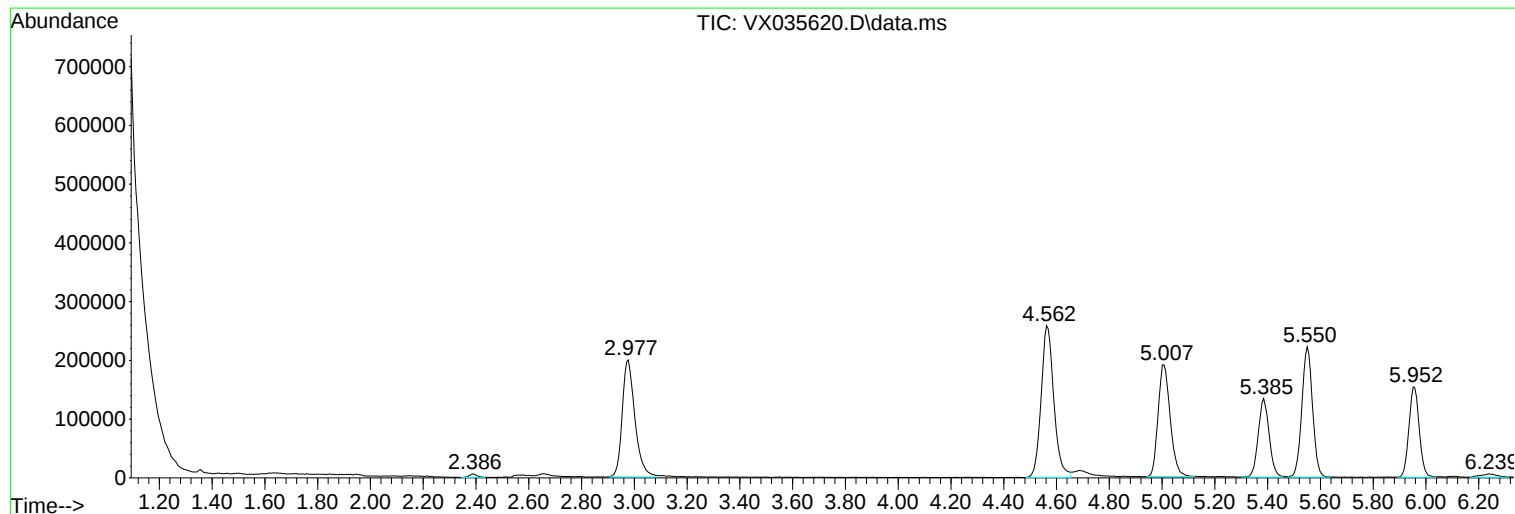

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051123\
Data File : VX035620.D
Acq On : 11 May 2023 20:10
Operator : JC/MD
Sample : 02752-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
230510054-02-VOA

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051123\
Data File : VX035620.D
Acq On : 11 May 2023 20:10
Operator : JC/MD
Sample : 02752-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
230510054-02-VOA

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------