
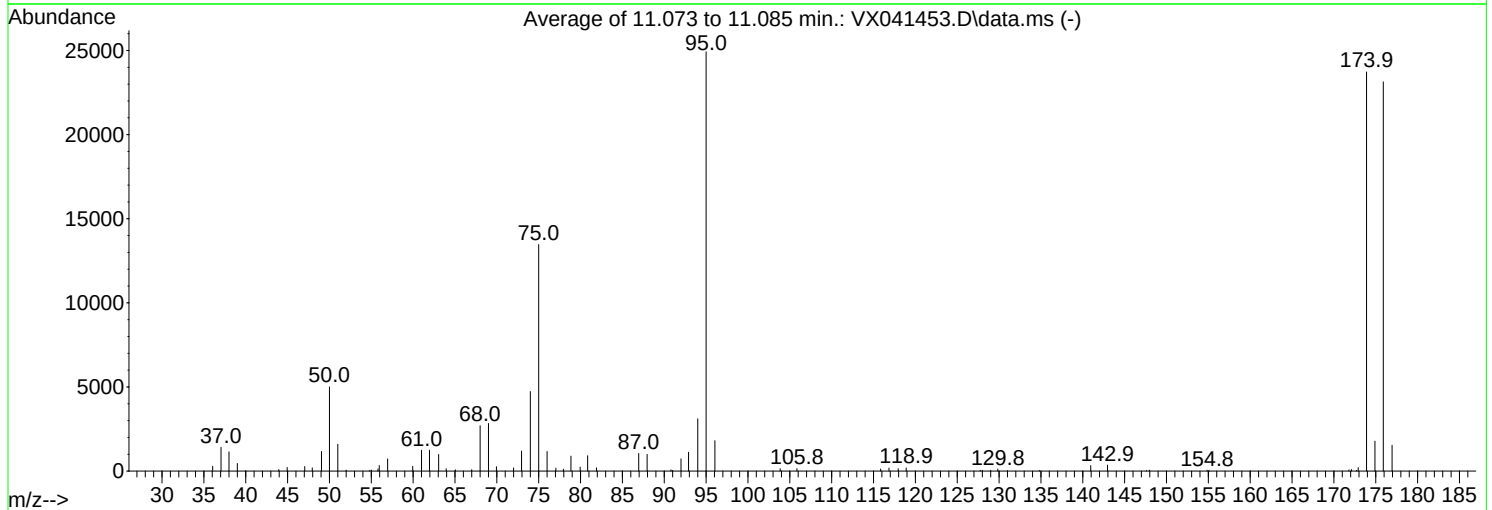


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051124\
Data File : VX041453.D
Acq On : 10 May 2024 12:20
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X043024W.M
Title : SW846 8260
Last Update : Wed May 08 06:03:16 2024

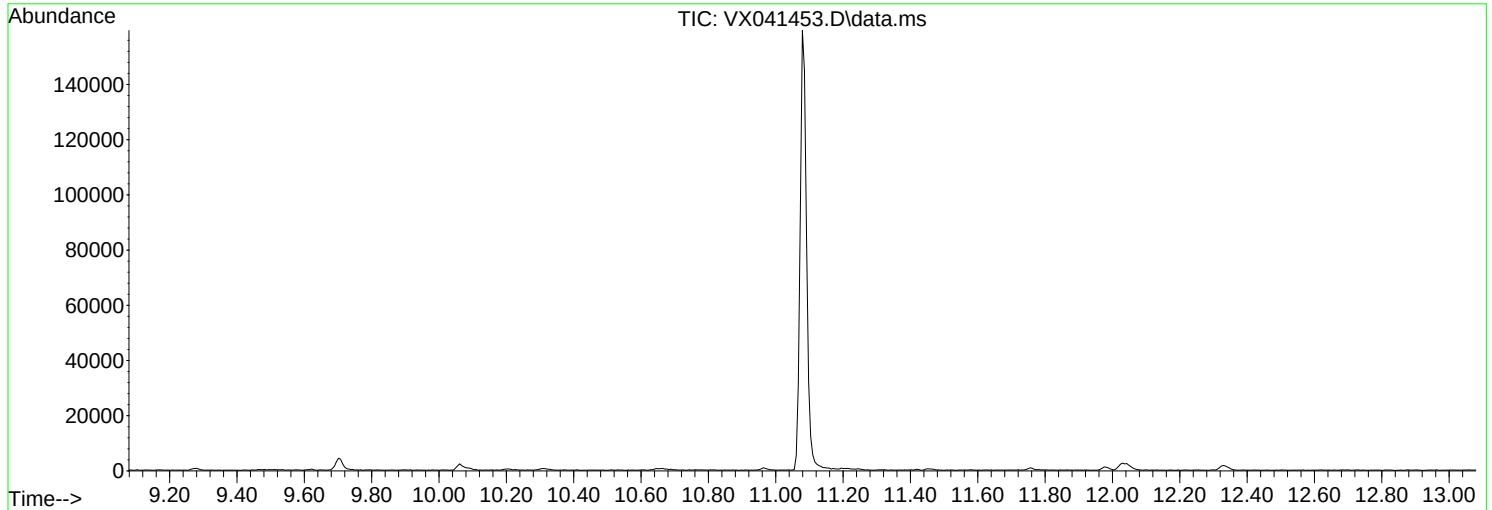

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.1	5006	PASS
75	95	30	60	54.0	13465	PASS
95	95	100	100	100.0	24928	PASS
96	95	5	9	7.2	1805	PASS
173	174	0.00	2	0.9	206	PASS
174	95	50	100	95.2	23725	PASS
175	174	5	9	7.5	1782	PASS
176	174	95	101	97.5	23141	PASS
177	176	5	9	6.6	1535	PASS