

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051221\
 Data File : VX021927.D
 Acq On : 12 May 2021 15:13
 Operator : JC/MD
 Sample : M2339-02DL 5X
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0AW0DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR051021WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VX021927.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.367	42	46	53	rVB	50956	48372	12.26%	1.673%
2	1.672	91	96	103	rBV	38125	44052	11.16%	1.524%
3	1.892	127	132	141	rVB	37210	54375	13.78%	1.881%
4	2.306	194	200	209	rBV	71844	111530	28.27%	3.858%
5	2.788	274	279	288	rVB3	5548	10907	2.76%	0.377%
6	4.489	546	558	569	rBV2	26609	99674	25.26%	3.448%
7	5.068	639	653	667	rVB	39868	125810	31.89%	4.352%
8	5.976	787	802	817	rBV2	103506	300182	76.08%	10.384%
9	6.769	922	932	946	rBV	77217	181999	46.13%	6.296%
10	7.134	986	992	998	rVB5	2492	5597	1.42%	0.194%
11	7.317	1013	1022	1034	rVB2	60990	138455	35.09%	4.789%
12	8.329	1179	1188	1198	rBV	46954	75887	19.23%	2.625%
13	8.652	1234	1241	1250	rBV	177188	275700	69.87%	9.537%
14	8.726	1250	1253	1262	rVB4	2949	4781	1.21%	0.165%
15	8.951	1285	1290	1301	rBV	28767	42917	10.88%	1.485%
16	9.274	1337	1343	1356	rBV	259694	394570	100.00%	13.649%
17	9.390	1356	1362	1379	rVB	181515	268250	67.99%	9.279%
18	10.055	1466	1471	1481	rBV	149576	212605	53.88%	7.354%
19	11.195	1653	1658	1665	rVB	57605	73271	18.57%	2.535%
20	12.024	1789	1794	1800	rBV	173854	209068	52.99%	7.232%
21	12.323	1835	1843	1850	rVB	172199	212911	53.96%	7.365%




Sum of corrected areas: 2890913

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051221\
Data File : VX021927.D
Acq On : 12 May 2021 15:13
Operator : JC/MD
Sample : M2339-02DL 5X
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0AW0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR051021WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

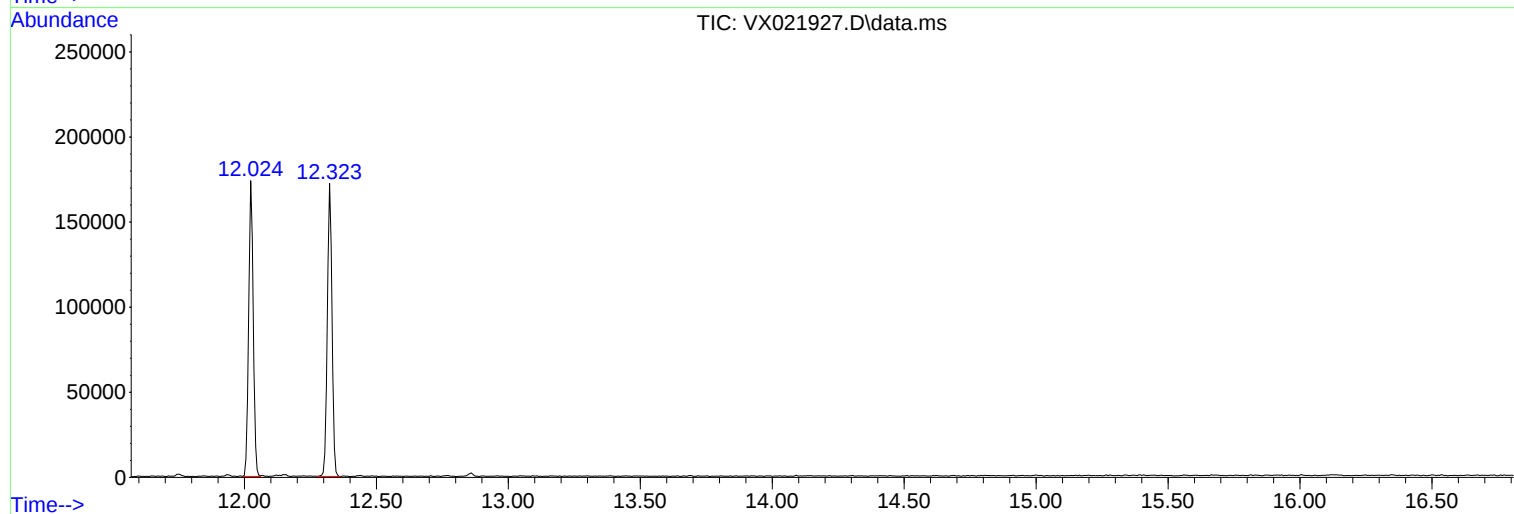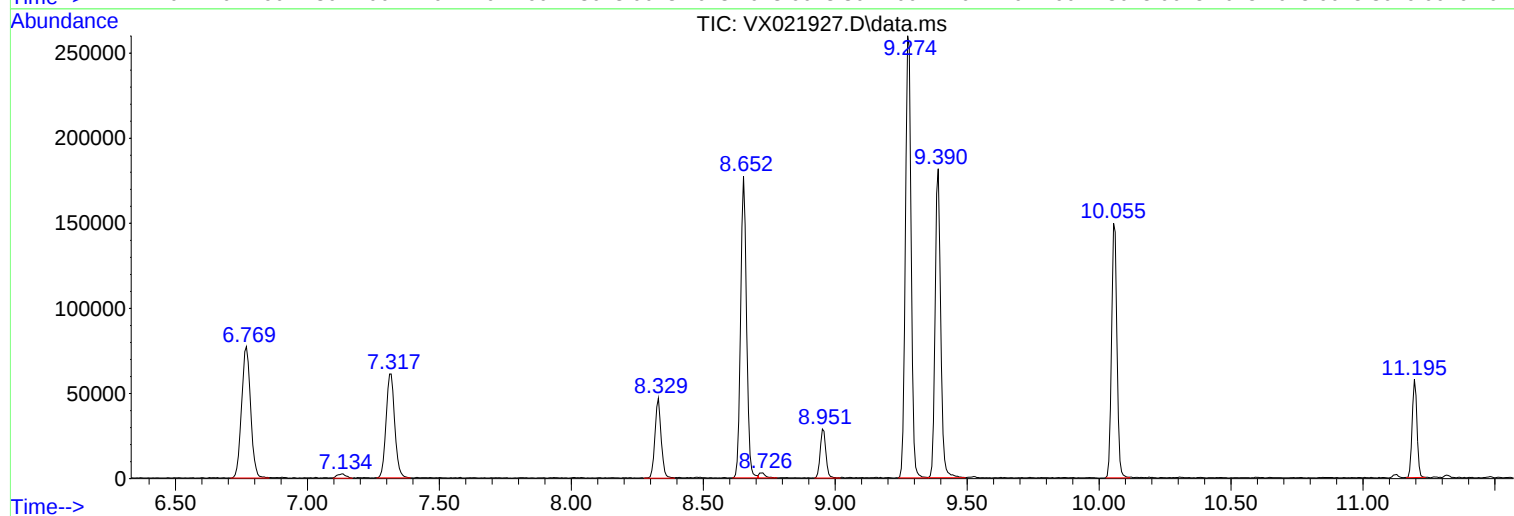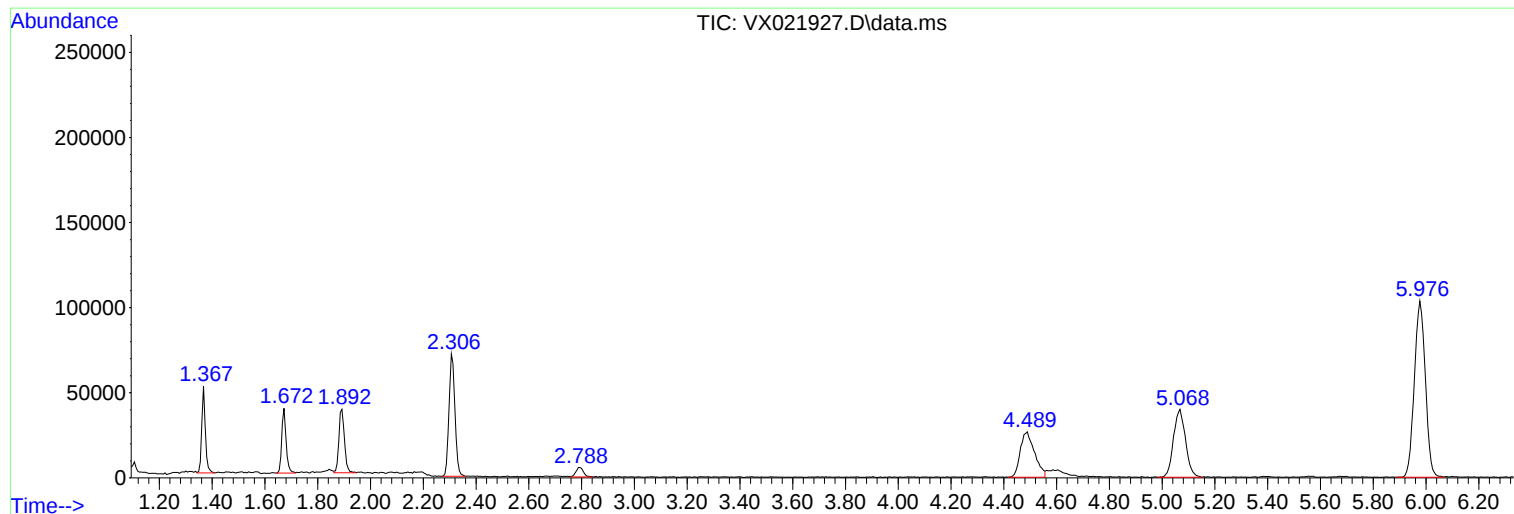

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051221\
Data File : VX021927.D
Acq On : 12 May 2021 15:13
Operator : JC/MD
Sample : M2339-02DL 5X
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0AW0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR051021WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051221\
Data File : VX021927.D
Acq On : 12 May 2021 15:13
Operator : JC/MD
Sample : M2339-02DL 5X
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0AW0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR051021WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
