
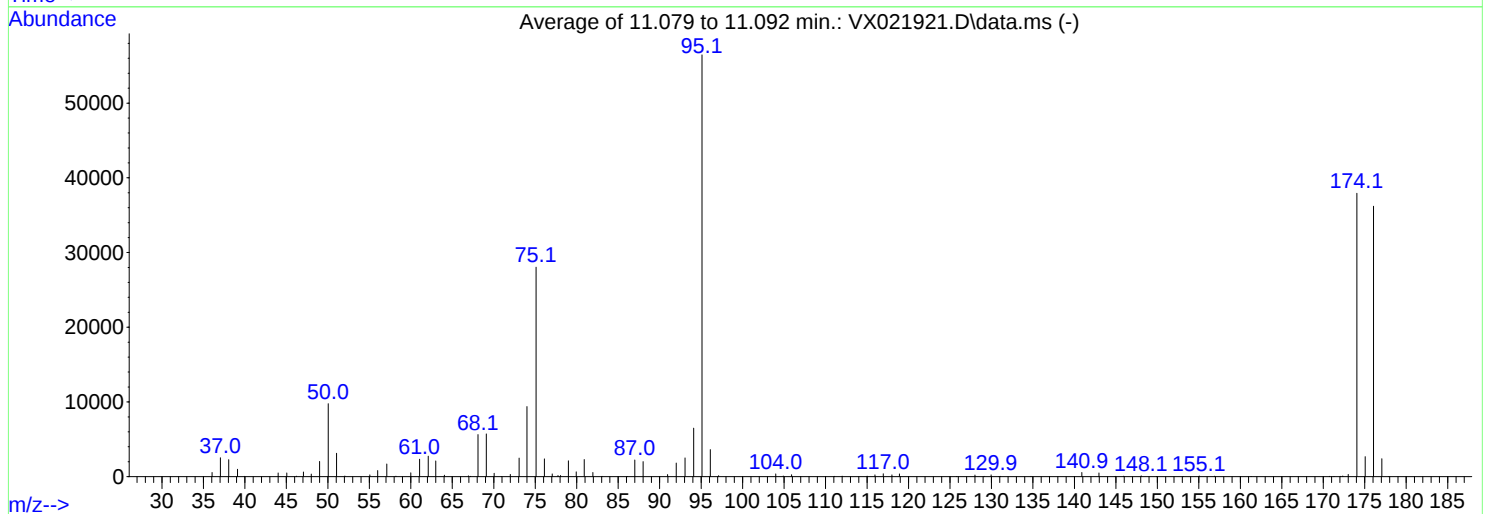


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051221\
 Data File : VX021921.D
 Acq On : 12 May 2021 09:25
 Operator : JC/MD
 Sample : BFB71
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB171

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR051021WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Thu May 13 01:12:16 2021

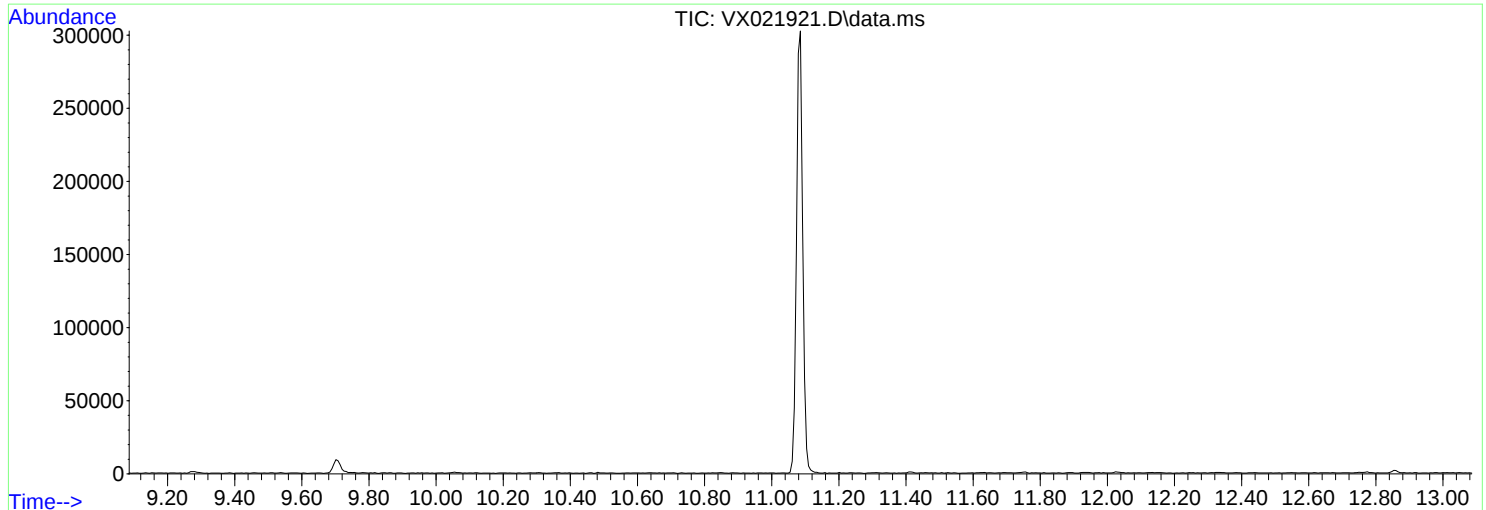

AutoFind: Scans 1639, 1640, 1641; Background Corrected with Scan 1631

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.3	9761	PASS
75	95	30	80	49.7	28035	PASS
95	95	100	100	100.0	56461	PASS
96	95	5	9	6.4	3615	PASS
173	174	0.00	2	0.8	304	PASS
174	95	50	120	67.2	37939	PASS
175	174	5	9	7.1	2683	PASS
176	174	95	105	95.4	36200	PASS
177	176	5	10	6.7	2408	PASS

Scan 1631 (11.031 min): VX021921.D\data.ms
BFB71

m/z	Abundance
40.00	135.0
43.00	72.0
44.10	413.0

Instrument :
MSVOA_X
ClientSampleId :
BFB171

m/z	Abundance
36.10	278.0
37.00	1519.0
38.10	1284.0
39.10	550.0
40.00	120.0
44.00	634.0
45.00	379.0
46.20	57.0
47.00	409.0
48.10	239.0
49.10	1262.0
50.00	5740.0
51.00	1804.0
55.10	161.0
55.90	456.0
57.10	1045.0
60.00	314.0
61.00	1549.0
62.10	1586.0
63.10	1295.0
64.10	190.0
67.20	116.0
68.10	3507.0
69.00	3804.0
70.00	385.0
72.10	194.0
73.00	1549.0
74.10	6719.0
75.10	17856.0
76.10	1314.0
77.10	276.0
77.80	273.0
78.90	1328.0
80.00	382.0
80.90	1561.0
82.00	511.0
86.10	88.0
87.00	1240.0
87.90	1315.0
91.00	119.0
92.00	1117.0
93.10	1604.0
94.10	4297.0
95.10	37816.0
96.00	2281.0
97.00	71.0
103.90	254.0
104.80	71.0
105.90	244.0
115.00	65.0
115.80	150.0
117.00	293.0
117.90	137.0
118.90	282.0
128.00	179.0
130.00	155.0
131.00	59.0
134.70	80.0
141.00	349.0
142.90	463.0
144.90	86.0
148.10	142.0
155.10	140.0
157.00	52.0
172.40	105.0
173.10	314.0
174.00	28736.0
175.00	2122.0
176.00	28496.0
177.00	1887.0

Instrument :
MSVOA_X
ClientSampleId :
BFB171

m/z	Abundance
36.10	640.0
37.10	2754.0
38.00	2753.0
39.10	1204.0
39.90	133.0
43.20	100.0
44.00	1184.0
45.10	488.0
46.20	120.0
47.10	826.0
47.90	358.0
49.00	2534.0
50.10	11074.0
51.10	3716.0
52.10	125.0
55.10	322.0
56.00	900.0
57.10	2027.0
58.20	99.0
60.00	583.0
61.10	2544.0
62.10	3095.0
63.00	2491.0
64.00	202.0
67.00	154.0
68.10	6536.0
69.10	6733.0
70.00	509.0
72.00	370.0
73.00	3073.0
74.00	11136.0
75.10	32488.0
76.10	2791.0
77.00	391.0
78.00	203.0
79.00	2514.0
79.90	743.0
80.90	2574.0
81.90	514.0
83.10	86.0
87.00	2678.0
88.00	2447.0
90.90	230.0
92.00	2271.0
93.10	2929.0
94.10	7807.0
95.10	66632.0
96.10	4372.0
97.10	212.0
104.00	500.0
104.90	119.0
105.80	265.0
111.10	76.0
112.00	65.0
116.00	240.0
117.00	518.0
118.00	292.0
118.90	447.0
125.80	73.0
128.00	270.0
129.10	79.0
129.90	401.0
131.10	95.0
134.80	82.0
137.00	56.0
140.90	708.0
142.90	471.0
144.90	53.0
146.00	110.0
148.10	88.0
149.90	50.0
153.10	88.0
155.00	68.0
156.90	68.0
161.30	85.0
170.70	58.0
172.30	132.0
172.90	331.0
174.00	46544.0
175.10	3309.0
176.10	43552.0
177.10	2933.0

Instrument :
MSVOA_X
ClientSampleId :
BFB171

m/z	Abundance
36.00	768.0
37.00	3327.0
38.10	2798.0
39.10	1196.0
40.00	276.0
43.20	74.0
44.00	888.0
45.00	633.0
47.00	607.0
48.00	438.0
49.00	2346.0
50.00	12469.0
51.00	3839.0
52.00	148.0
55.00	216.0
56.00	1108.0
57.10	1984.0
58.20	98.0
60.00	664.0
61.00	2934.0
62.10	3565.0
63.00	2496.0
64.00	176.0
66.90	180.0
68.10	6873.0
69.10	6635.0
70.10	473.0
70.90	74.0
72.00	325.0
73.10	2819.0
74.00	10306.0
75.10	33760.0
76.10	3023.0
77.00	414.0
77.70	210.0
78.10	266.0
79.00	2517.0
80.00	815.0
80.90	2771.0
81.90	625.0
83.00	54.0
87.00	2750.0
88.10	2303.0
91.00	508.0
92.00	2070.0
93.00	3003.0
94.10	7347.0
95.10	64936.0
96.10	4193.0
97.20	86.0
104.00	354.0
105.00	92.0
106.00	297.0
107.00	54.0
111.00	89.0
112.00	116.0
115.00	137.0
116.00	290.0
116.90	327.0
118.00	309.0
118.90	380.0
128.00	215.0
129.10	66.0
130.10	168.0
130.90	92.0
140.90	597.0
143.10	567.0
145.90	67.0
148.00	127.0
155.00	64.0
156.90	100.0
170.80	59.0
171.30	63.0
172.10	137.0
173.00	268.0
174.10	38536.0
175.00	2617.0
176.00	36552.0
177.10	2405.0
177.90	54.0

Instrument :
MSVOA_X
ClientSampleId :
BFB171