


Bromomethane

Response Ratio

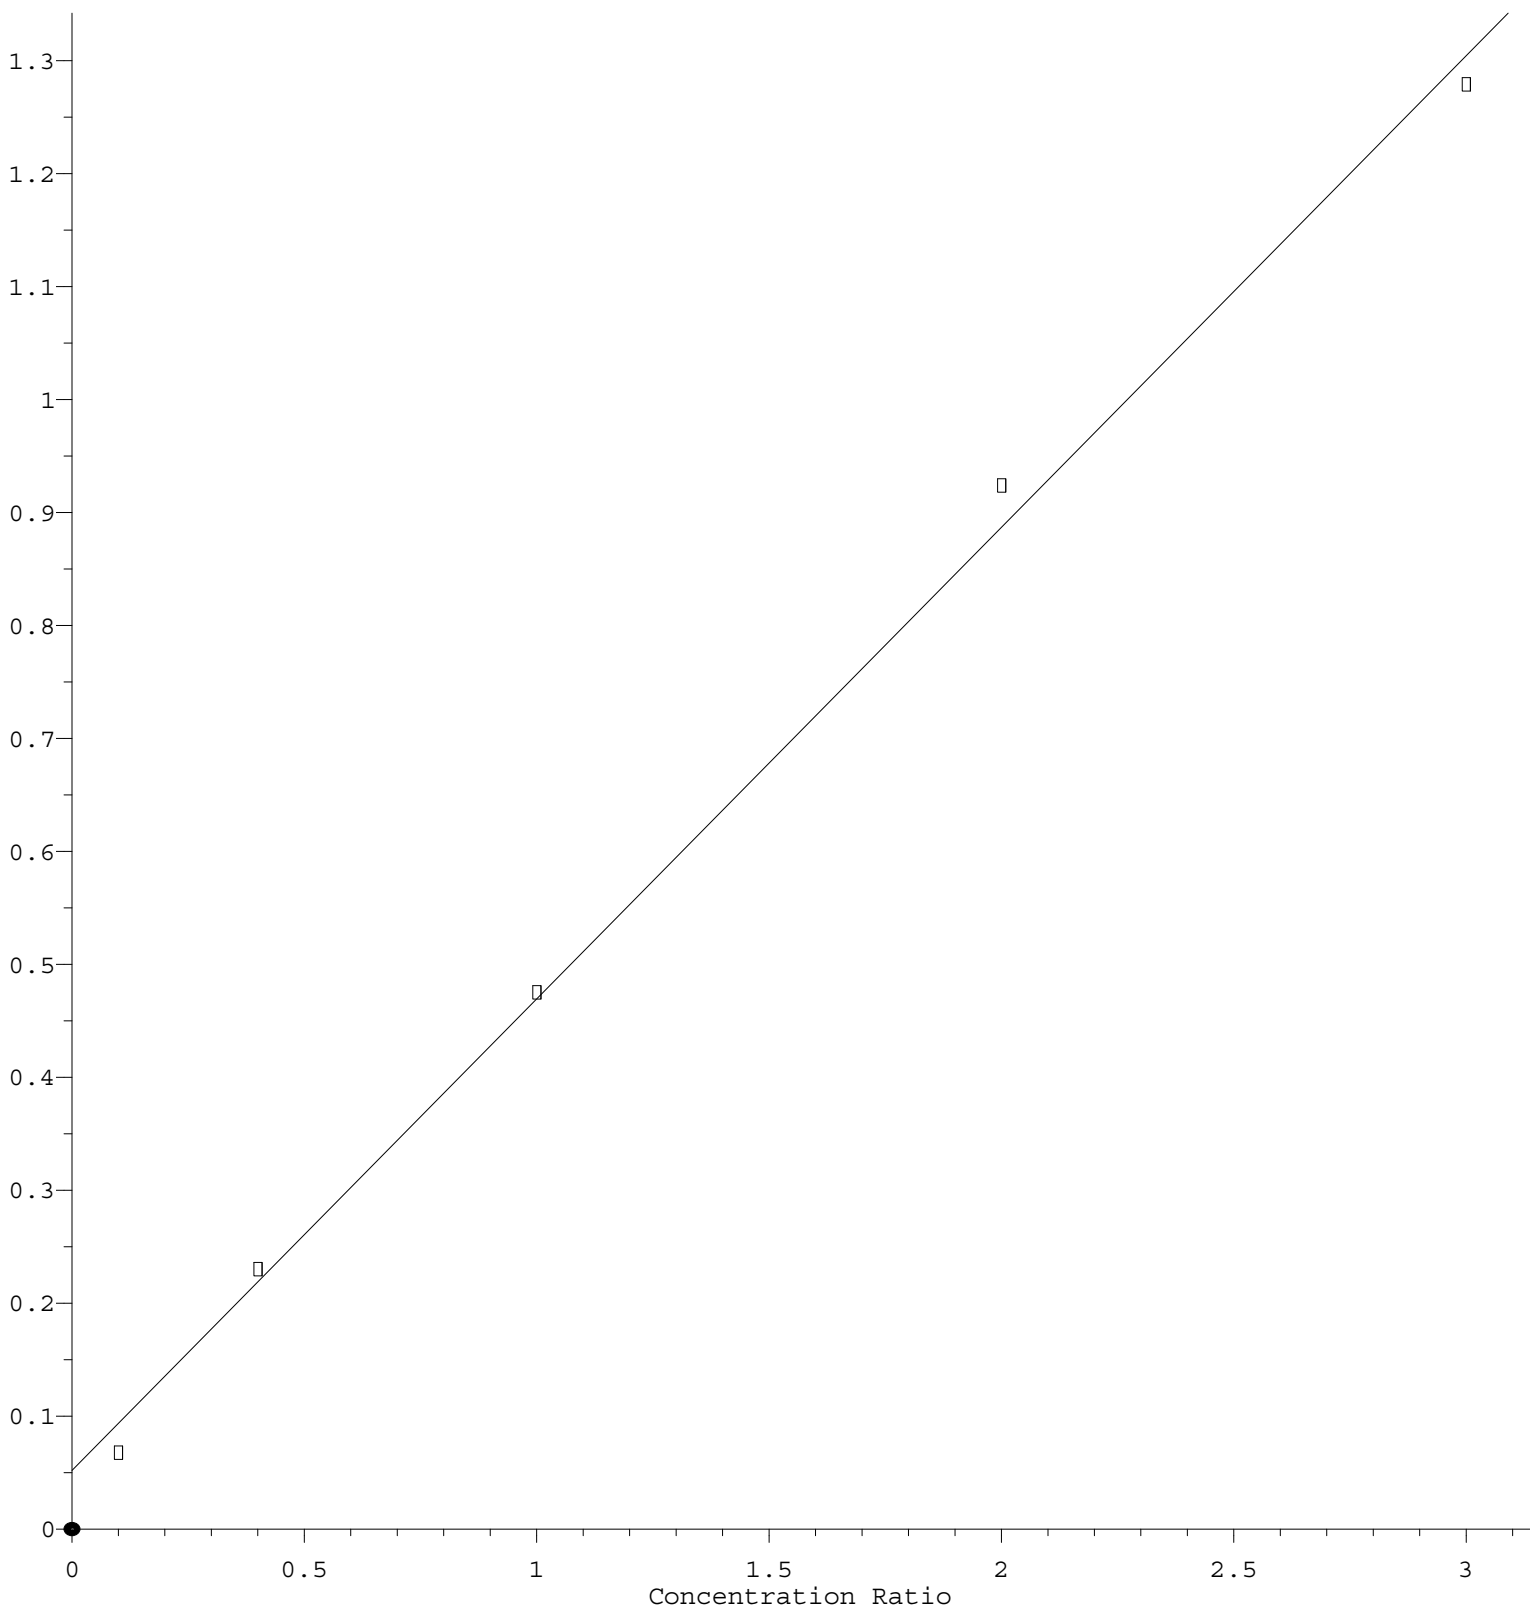

$$\text{Response} = 4.179\text{e-}001 * \text{Amt} + 5.201\text{e-}002$$


Coef of Det (r^2) = 0.997158 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X051222W.M

Calibration Table Last Updated: Thu May 12 14:58:53 2022

Chloroethane


Response Ratio

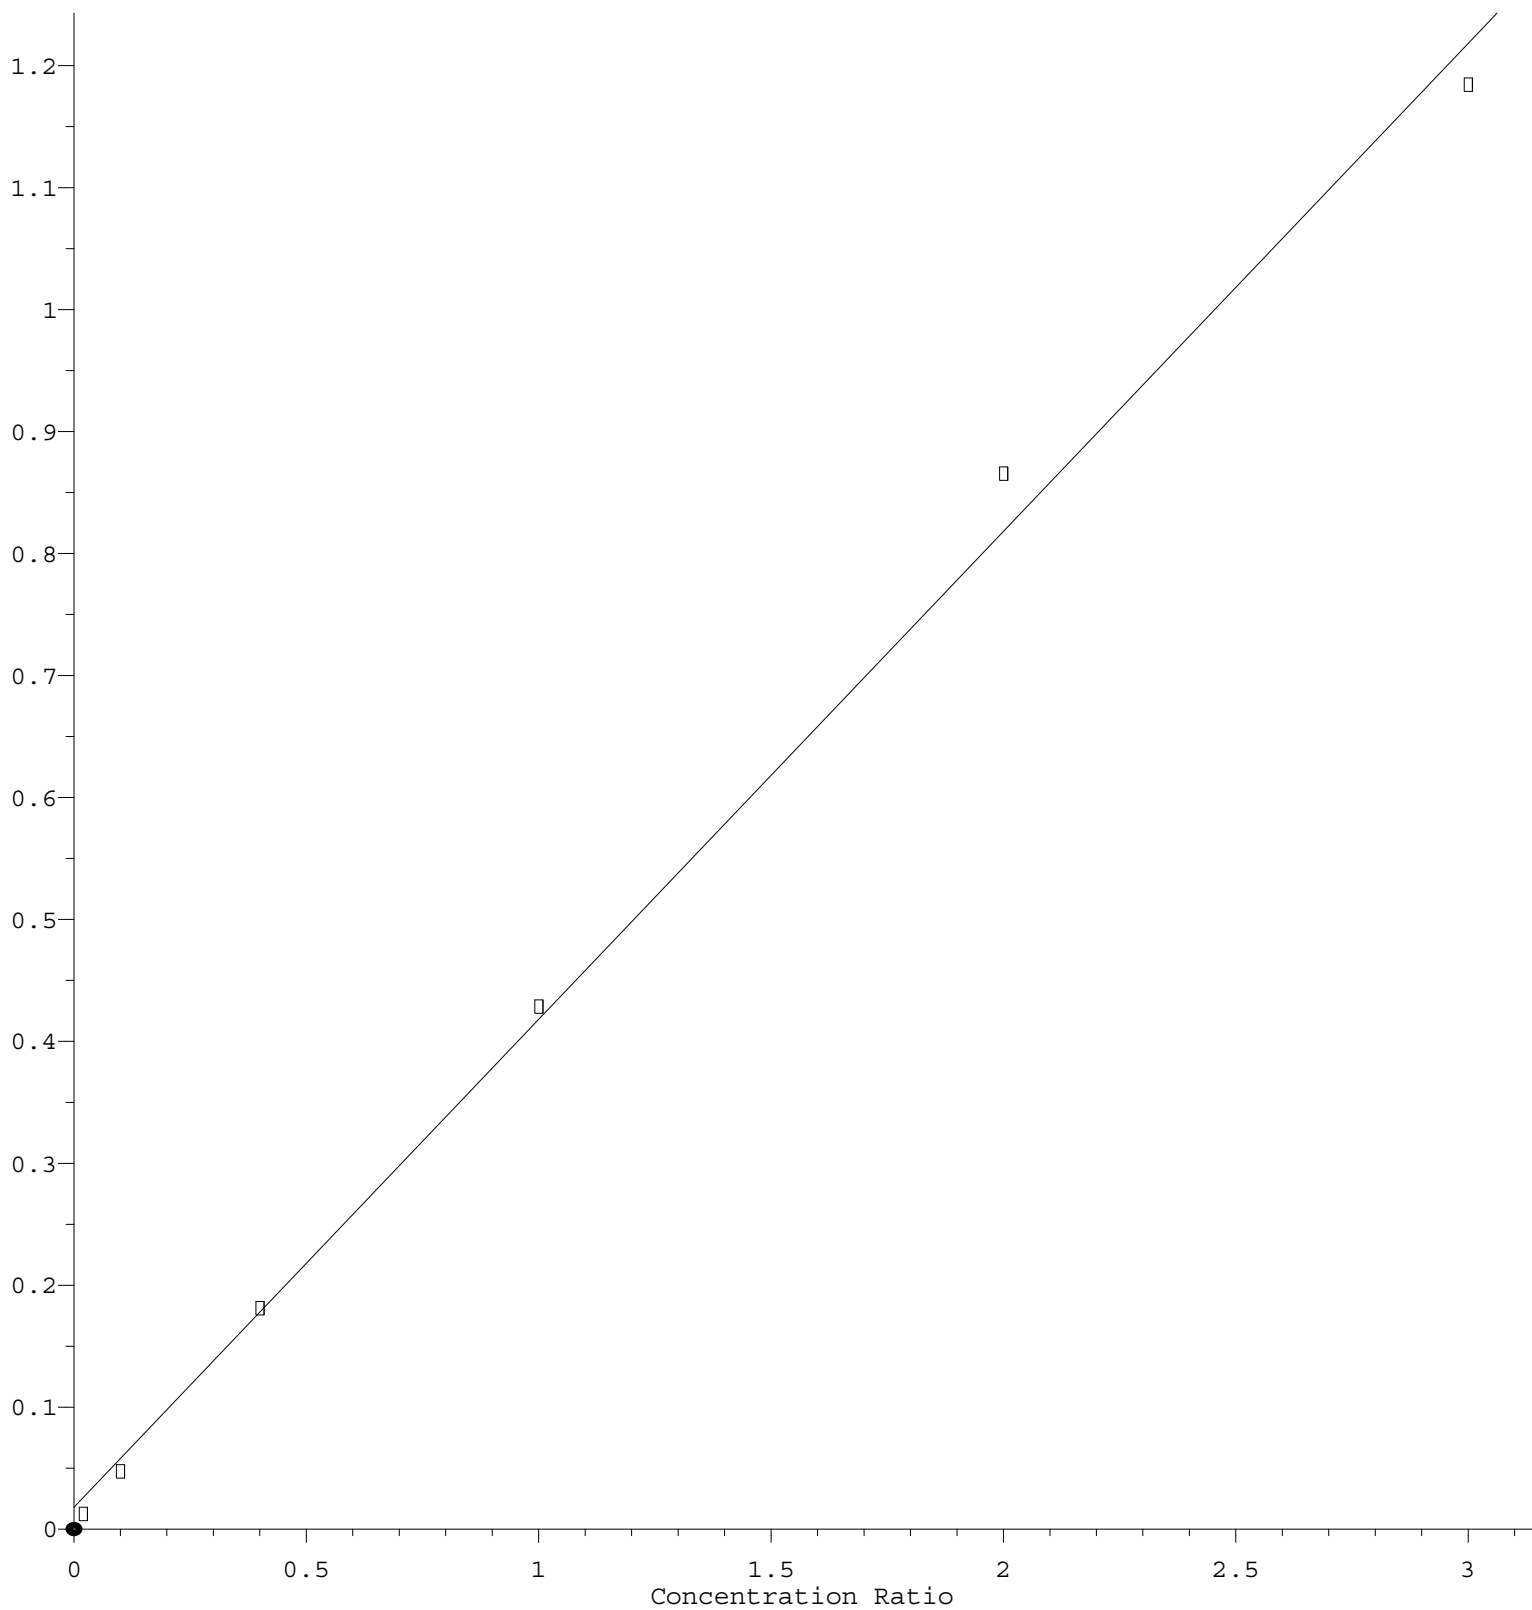

Response = $4.001\text{e-}001 \cdot \text{Amt} + 1.842\text{e-}002$
Coef of Det (r^2) = 0.996661 Curve Fit: Linear
Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X051222W.M
Calibration Table Last Updated: Thu May 12 14:58:53 2022

Tert butyl alcohol

Response Ratio

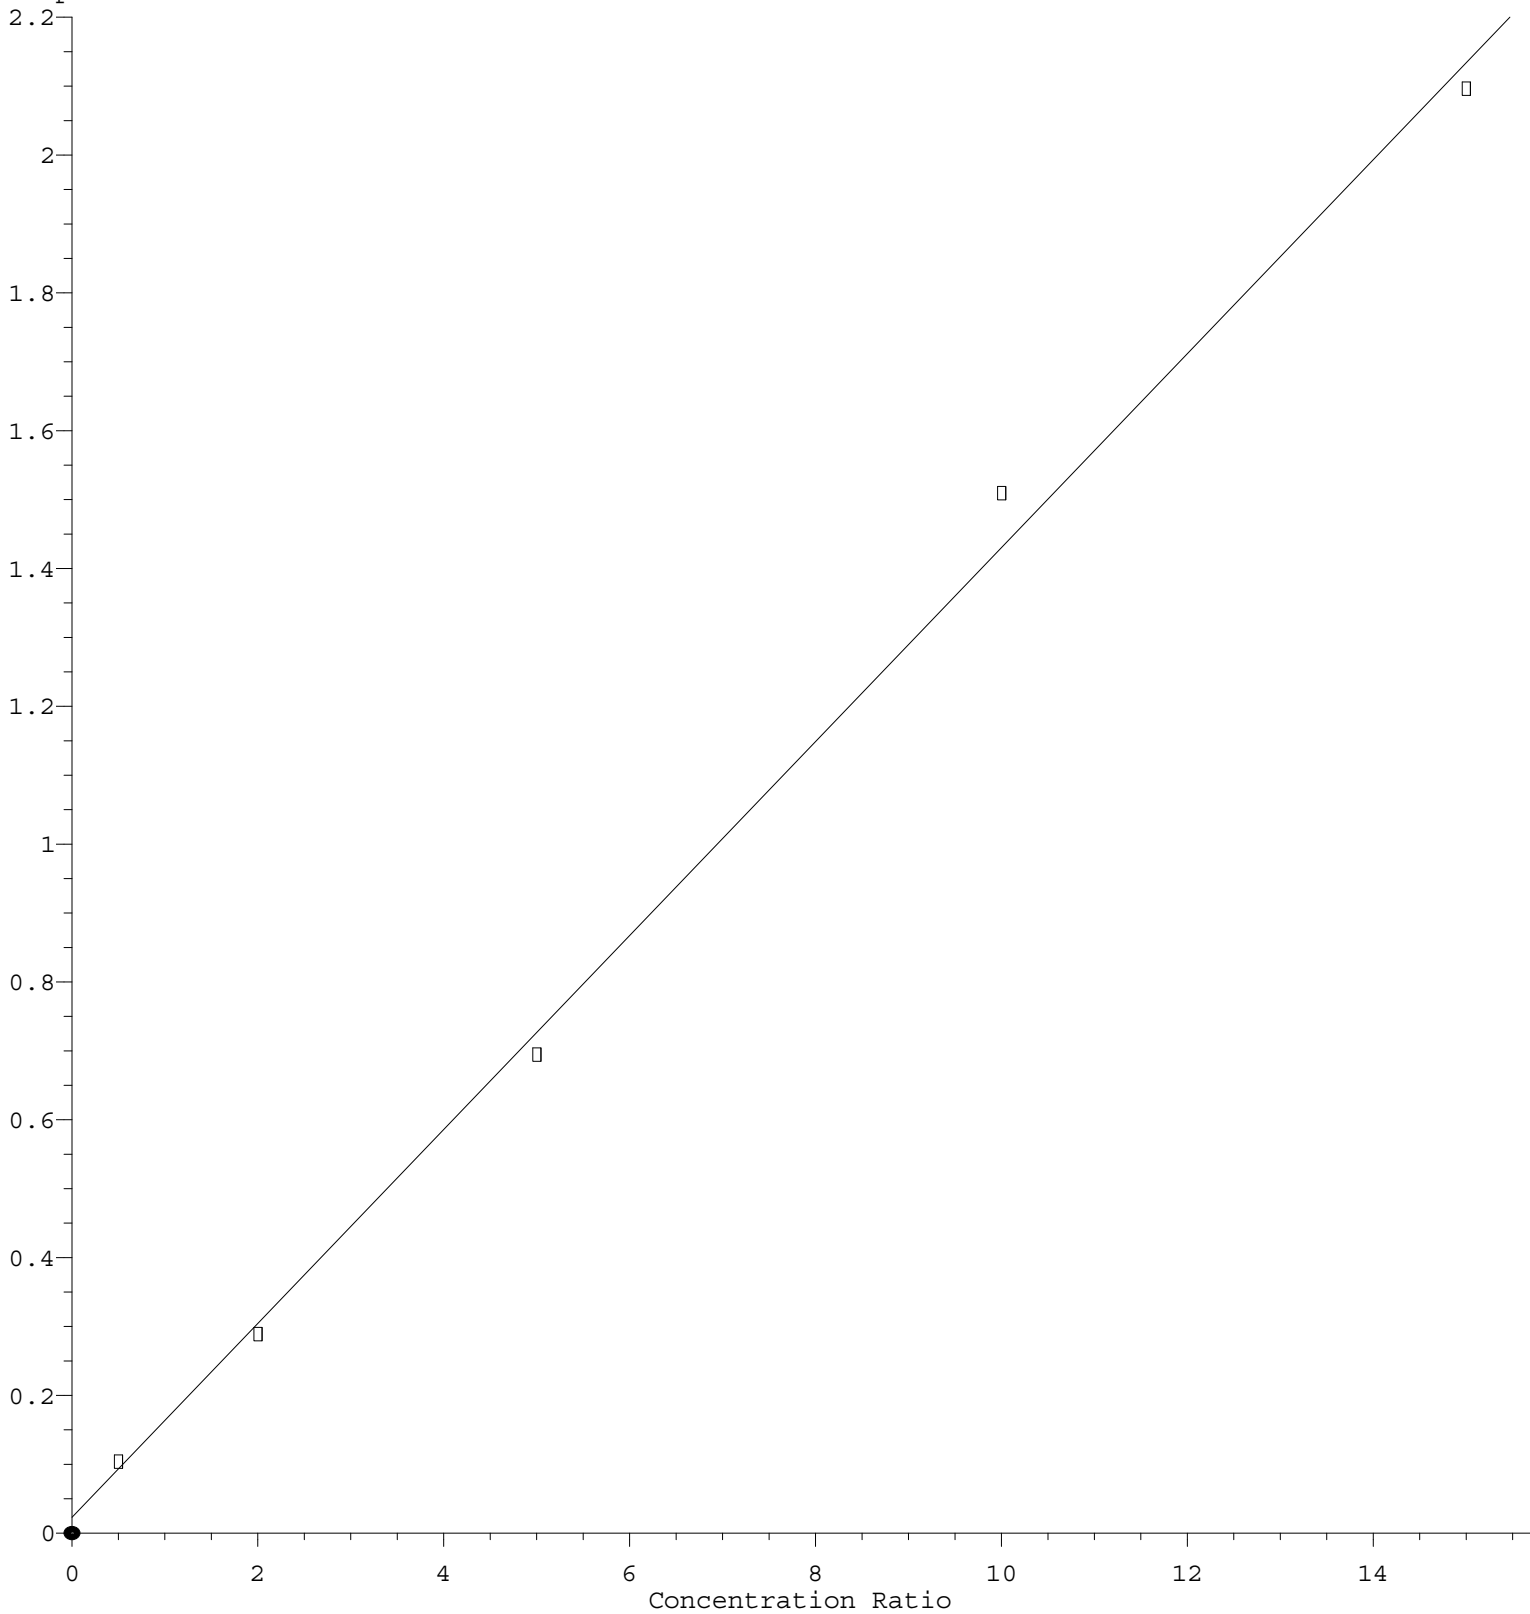

$$\text{Response} = 1.408\text{e-}001 * \text{Amt} + 2.321\text{e-}002$$


Coef of Det (r^2) = 0.996821 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X051222W.M

Calibration Table Last Updated: Thu May 12 14:58:53 2022

1,3-Dichloropropane

Response Ratio

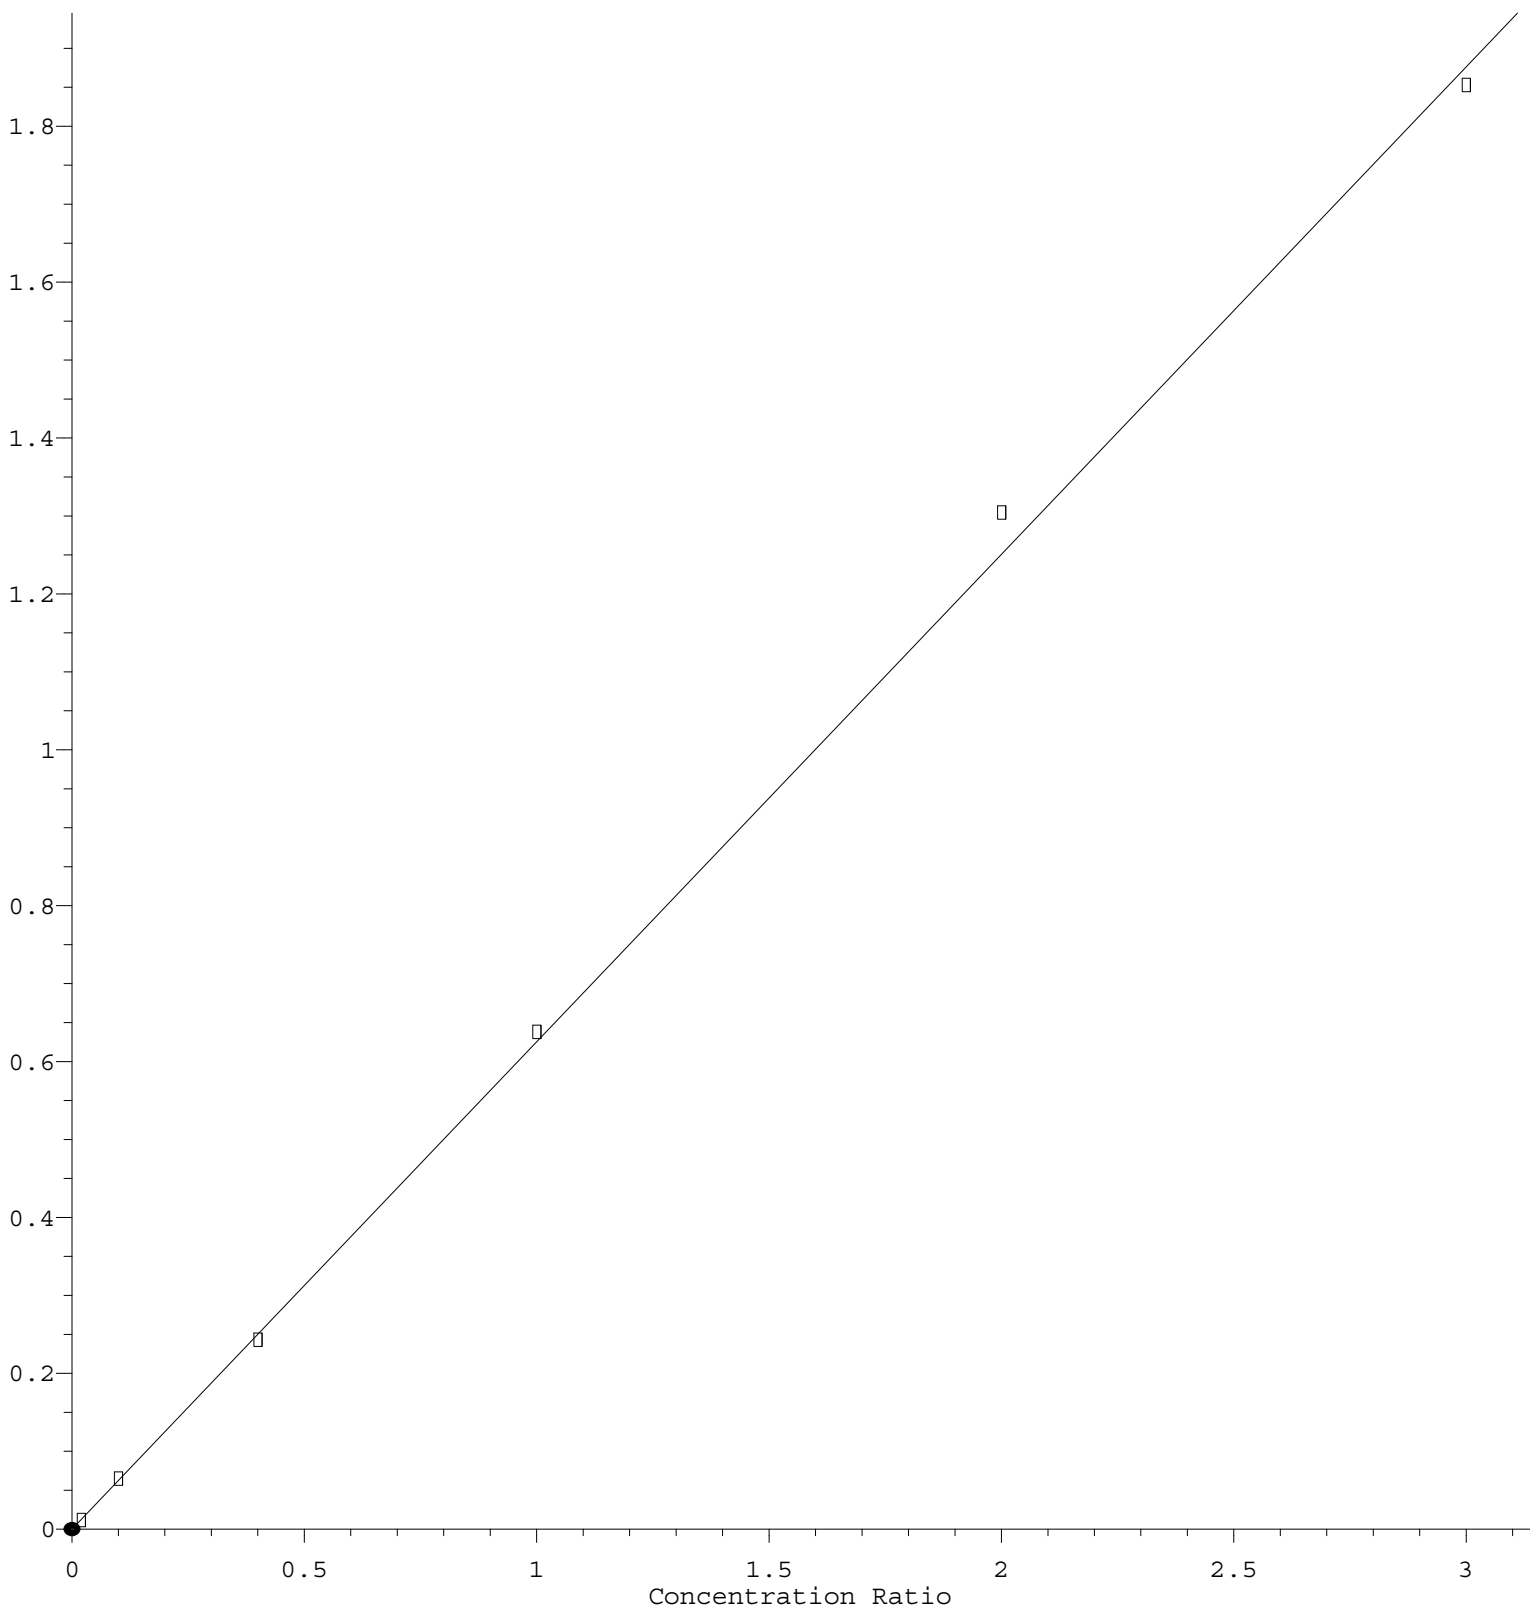

$$\text{Response} = 6.256\text{e-}001 * \text{Amt}$$


RF Rel Std Dev = 4.025% Curve Fit: Avg RF

Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X051222W.M

Calibration Table Last Updated: Thu May 12 14:58:53 2022

Bromoform


Response Ratio

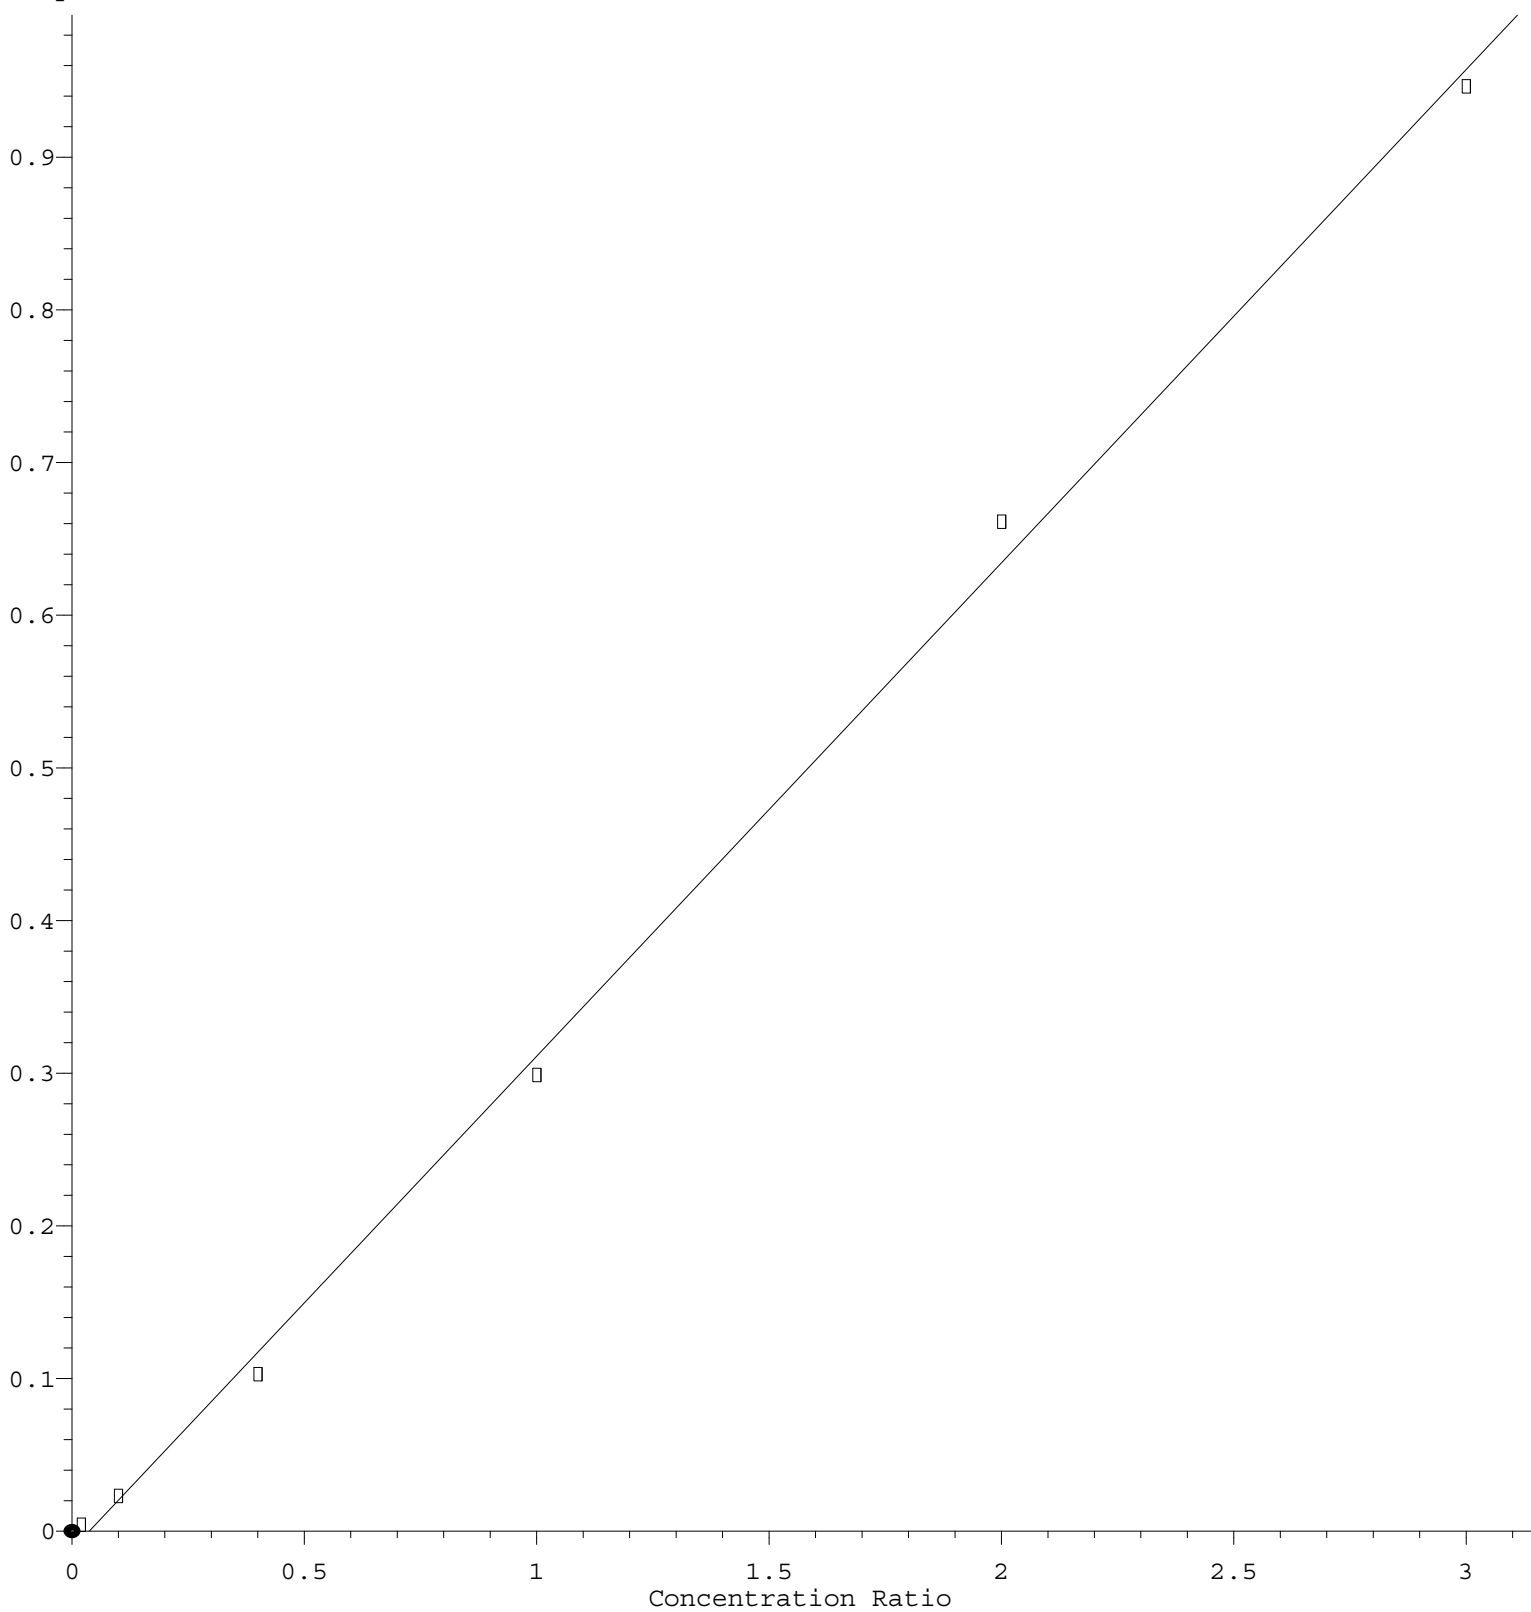

Response = 3.233e-001 * Amt - 1.196e-002
 Coef of Det (r^2) = 0.998240 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X051222W.M
 Calibration Table Last Updated: Thu May 12 14:58:53 2022

trans-1,4-Dichloro-2-butene

Response Ratio

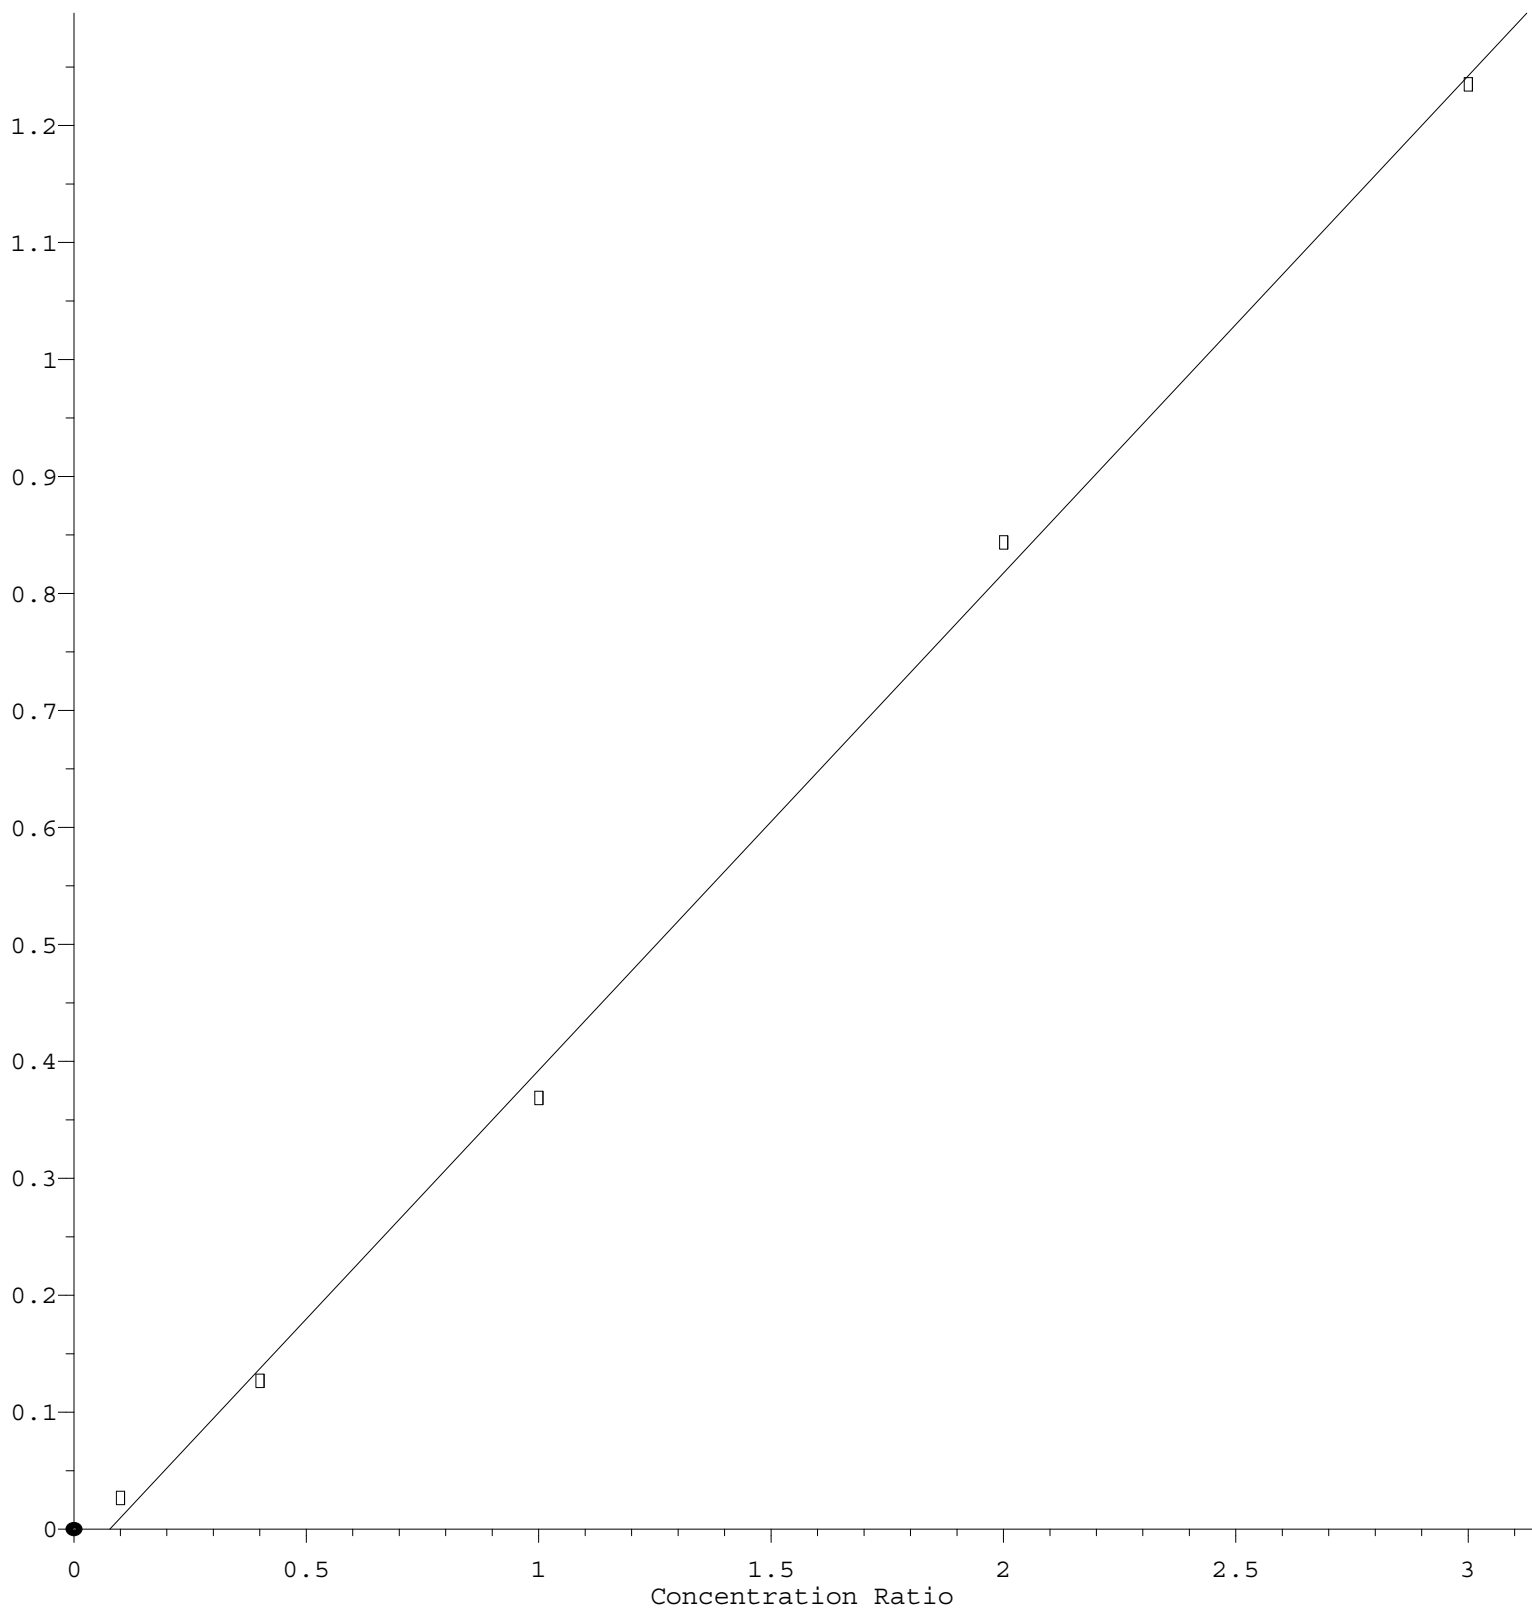

$$\text{Response} = 4.254\text{e-}001 * \text{Amt} - 3.293\text{e-}002$$


Coef of Det (r^2) = 0.998367 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X051222W.M

Calibration Table Last Updated: Thu May 12 14:58:53 2022

t-1,3-Dichloropropene

Response Ratio

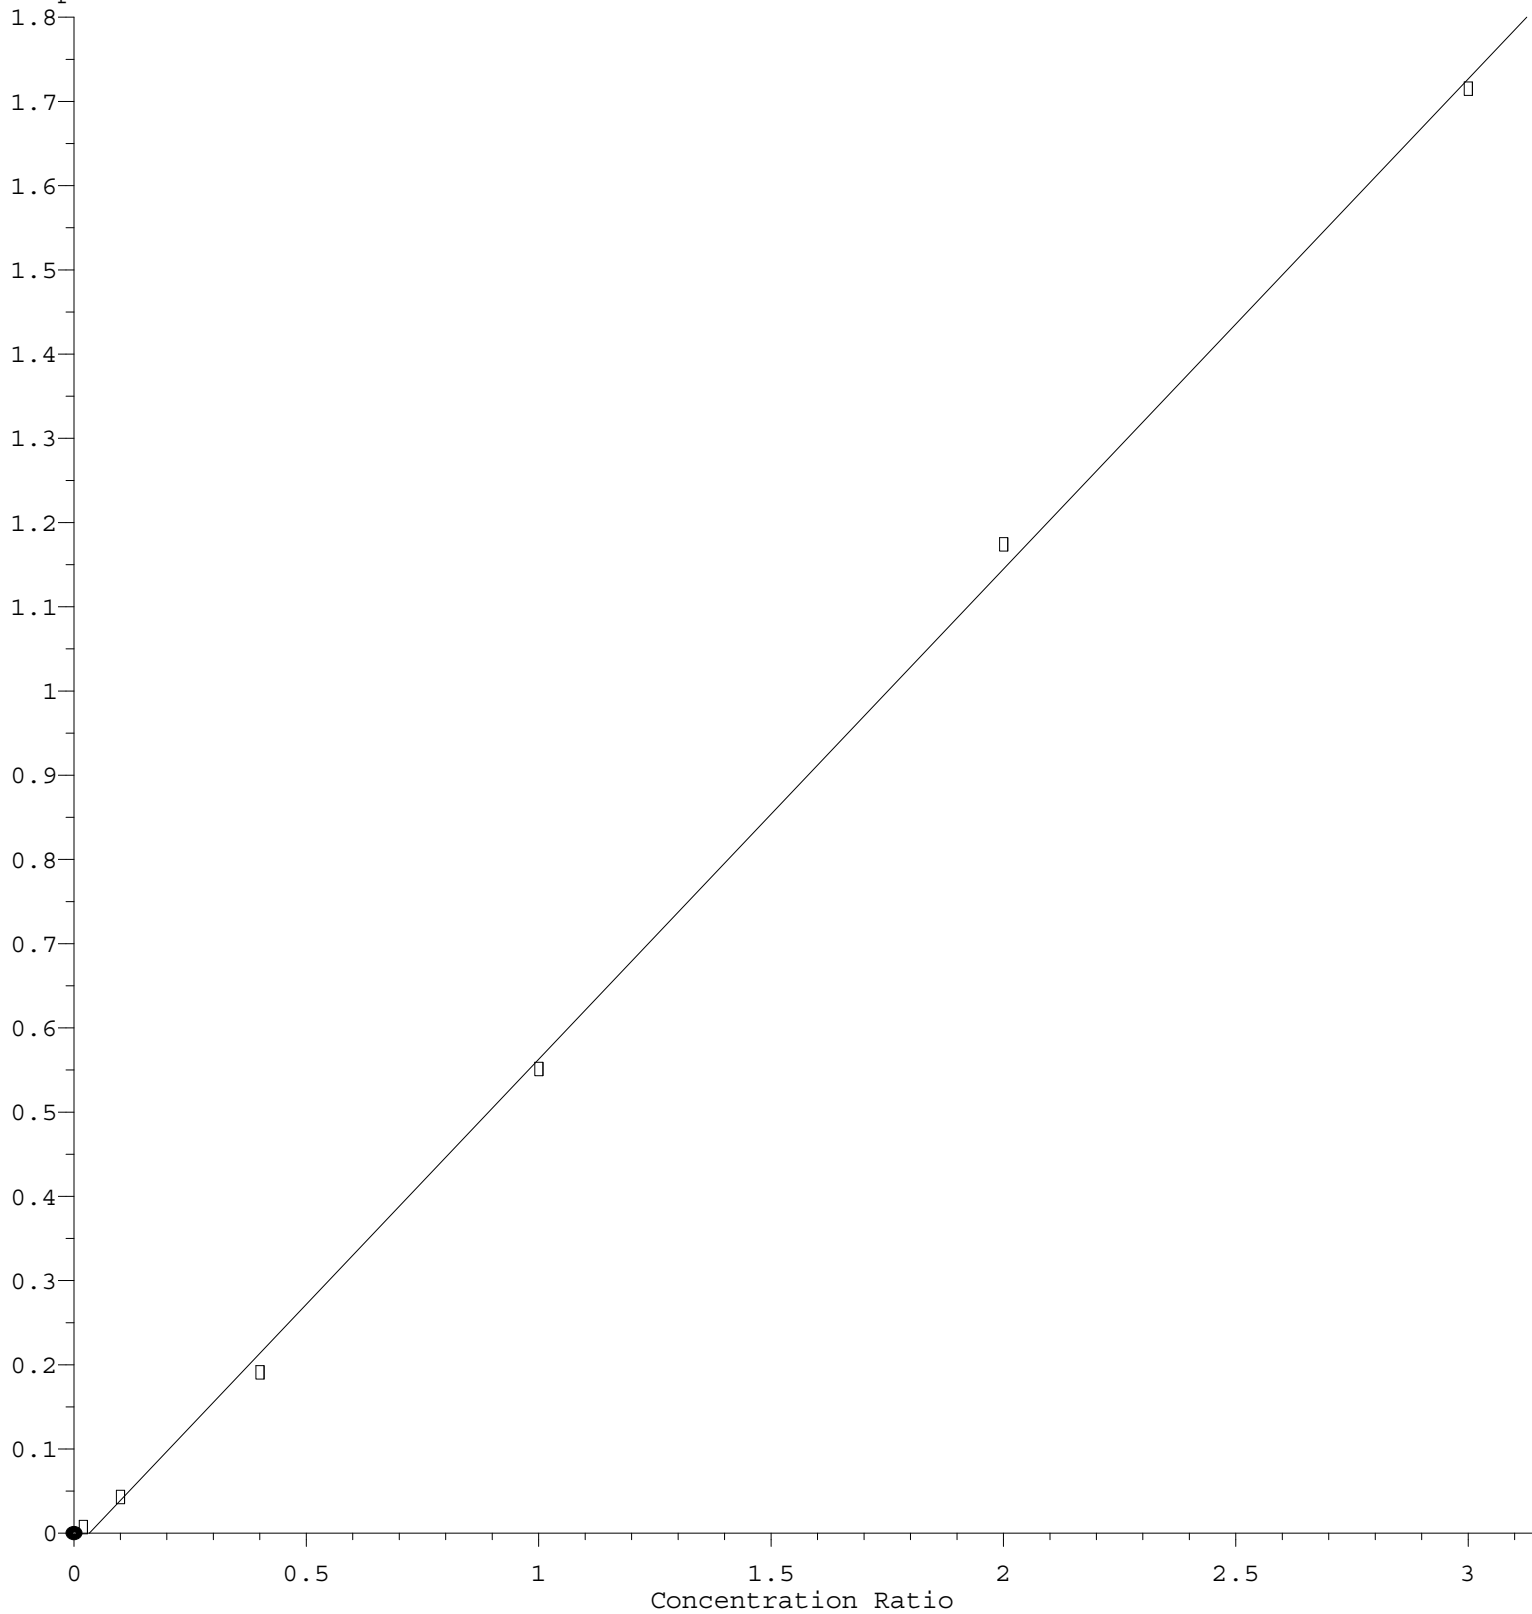

$$\text{Response} = 5.822\text{e-}001 * \text{Amt} - 1.910\text{e-}002$$

Coef of Det (r^2) = 0.999216 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X051222W.M

Calibration Table Last Updated: Thu May 12 14:58:53 2022