


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051222\
Data File : VX028622.D
Acq On : 11 May 2022 15:23
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051222W.M
Title : SW846 8260
Last Update : Thu May 12 14:58:53 2022

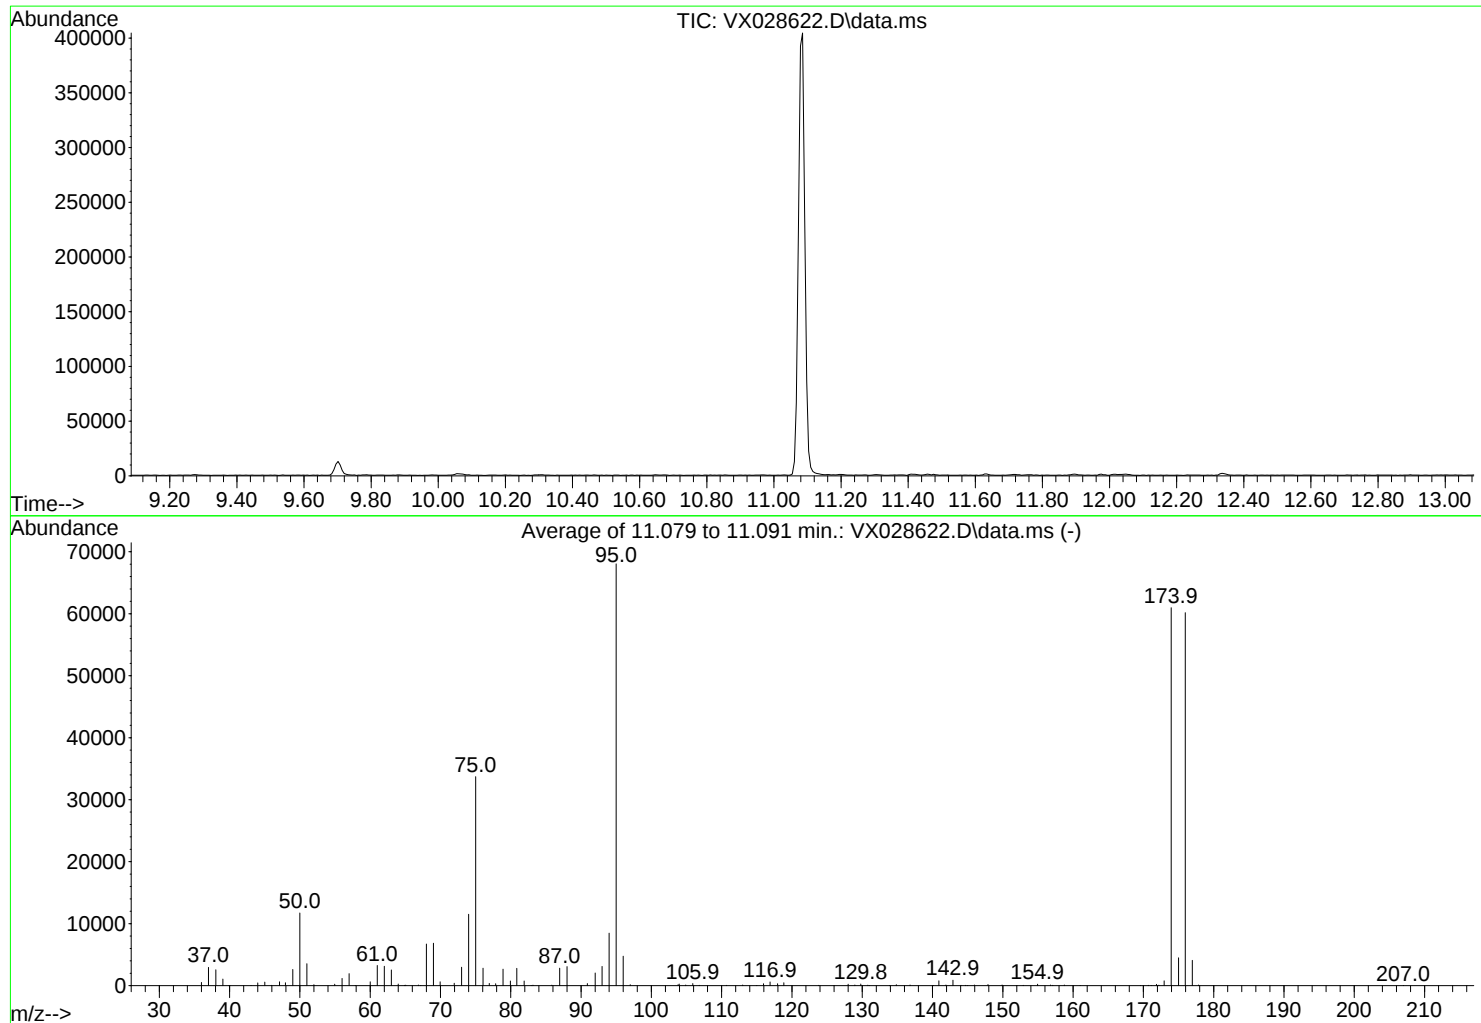

AutoFind: Scans 1639, 1640, 1641; Background Corrected with Scan 1632

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.2	11718	PASS
75	95	30	60	49.5	33712	PASS
95	95	100	100	100.0	68056	PASS
96	95	5	9	7.0	4741	PASS
173	174	0.00	2	1.3	765	PASS
174	95	50	100	89.6	60984	PASS
175	174	5	9	7.4	4495	PASS
176	174	95	101	98.7	60173	PASS
177	176	5	9	6.8	4071	PASS