
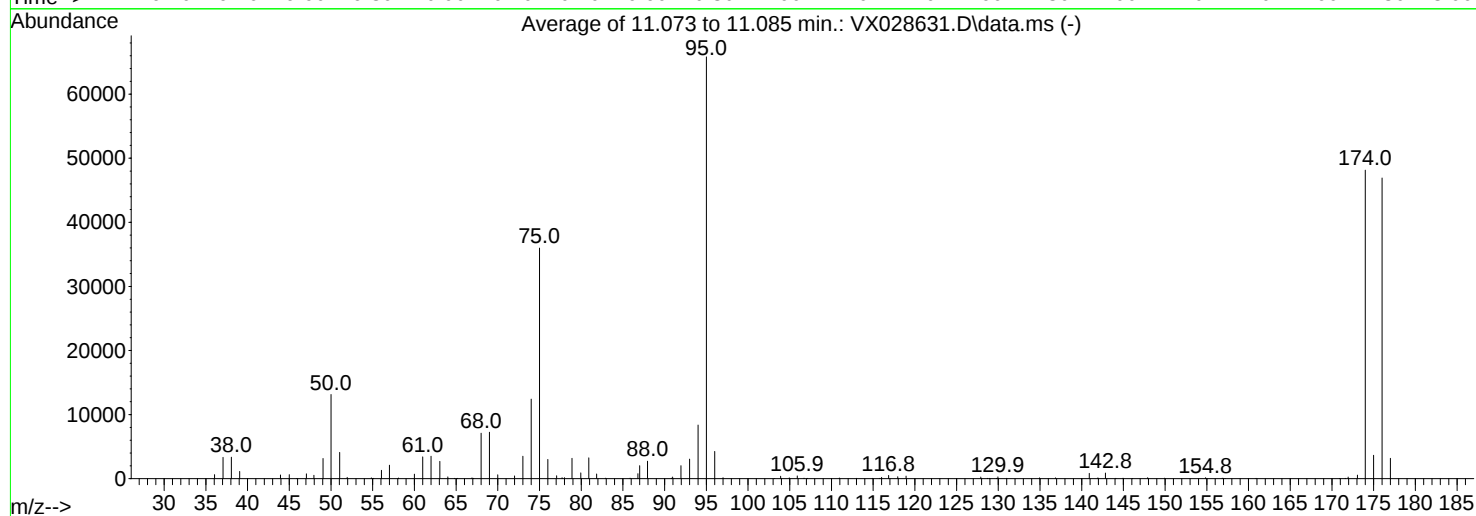


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051222\
Data File : VX028631.D
Acq On : 12 May 2022 09:35
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051222W.M
Title : SW846 8260
Last Update : Thu May 12 14:58:53 2022

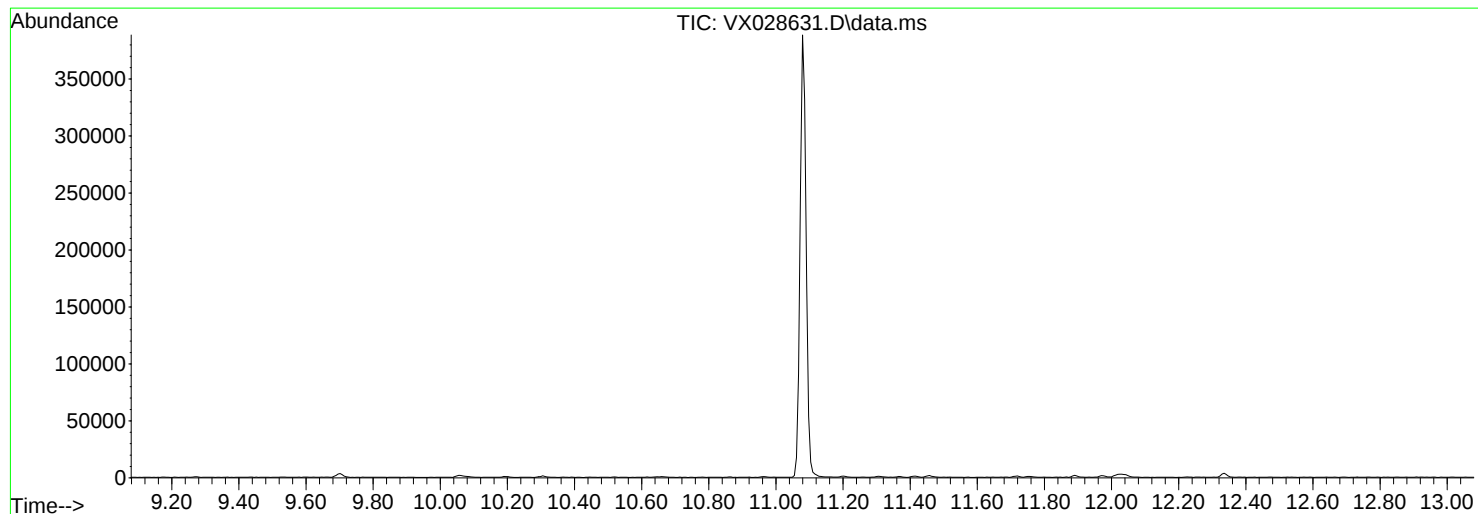

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1631

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.0	13140	PASS
75	95	30	60	54.7	35979	PASS
95	95	100	100	100.0	65821	PASS
96	95	5	9	6.4	4245	PASS
173	174	0.00	2	1.2	562	PASS
174	95	50	100	73.1	48147	PASS
175	174	5	9	7.6	3652	PASS
176	174	95	101	97.4	46904	PASS
177	176	5	9	6.8	3186	PASS