

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051223\
 Data File : VX035639.D
 Acq On : 12 May 2023 15:41
 Operator : JC/MD
 Sample : 02777-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 STORAGE-BLANK-SAMPLE-MANAG

Quant Time: May 15 01:57:28 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051123W.M
 Quant Title : SW846 8260
 QLast Update : Thu May 11 13:57:54 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.550	168	198165	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	6.763	114	364619	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	331591	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	150490	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	164141	47.480	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	94.960%
35) Dibromofluoromethane	5.385	113	116186	47.250	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	94.500%
50) Toluene-d8	8.647	98	431420	47.492	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	94.980%
62) 4-Bromofluorobenzene	11.079	95	179824	49.164	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	98.320%
Target Compounds						
16) Acetone	2.392	43	1774	1.194	ug/l	Qvalue 92

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051223\
Data File : VX035639.D
Acq On : 12 May 2023 15:41
Operator : JC/MD
Sample : 02777-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SAMPLE-MANAG

Quant Time: May 15 01:57:28 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051123W.M
Quant Title : SW846 8260
QLast Update : Thu May 11 13:57:54 2023
Response via : Initial Calibration



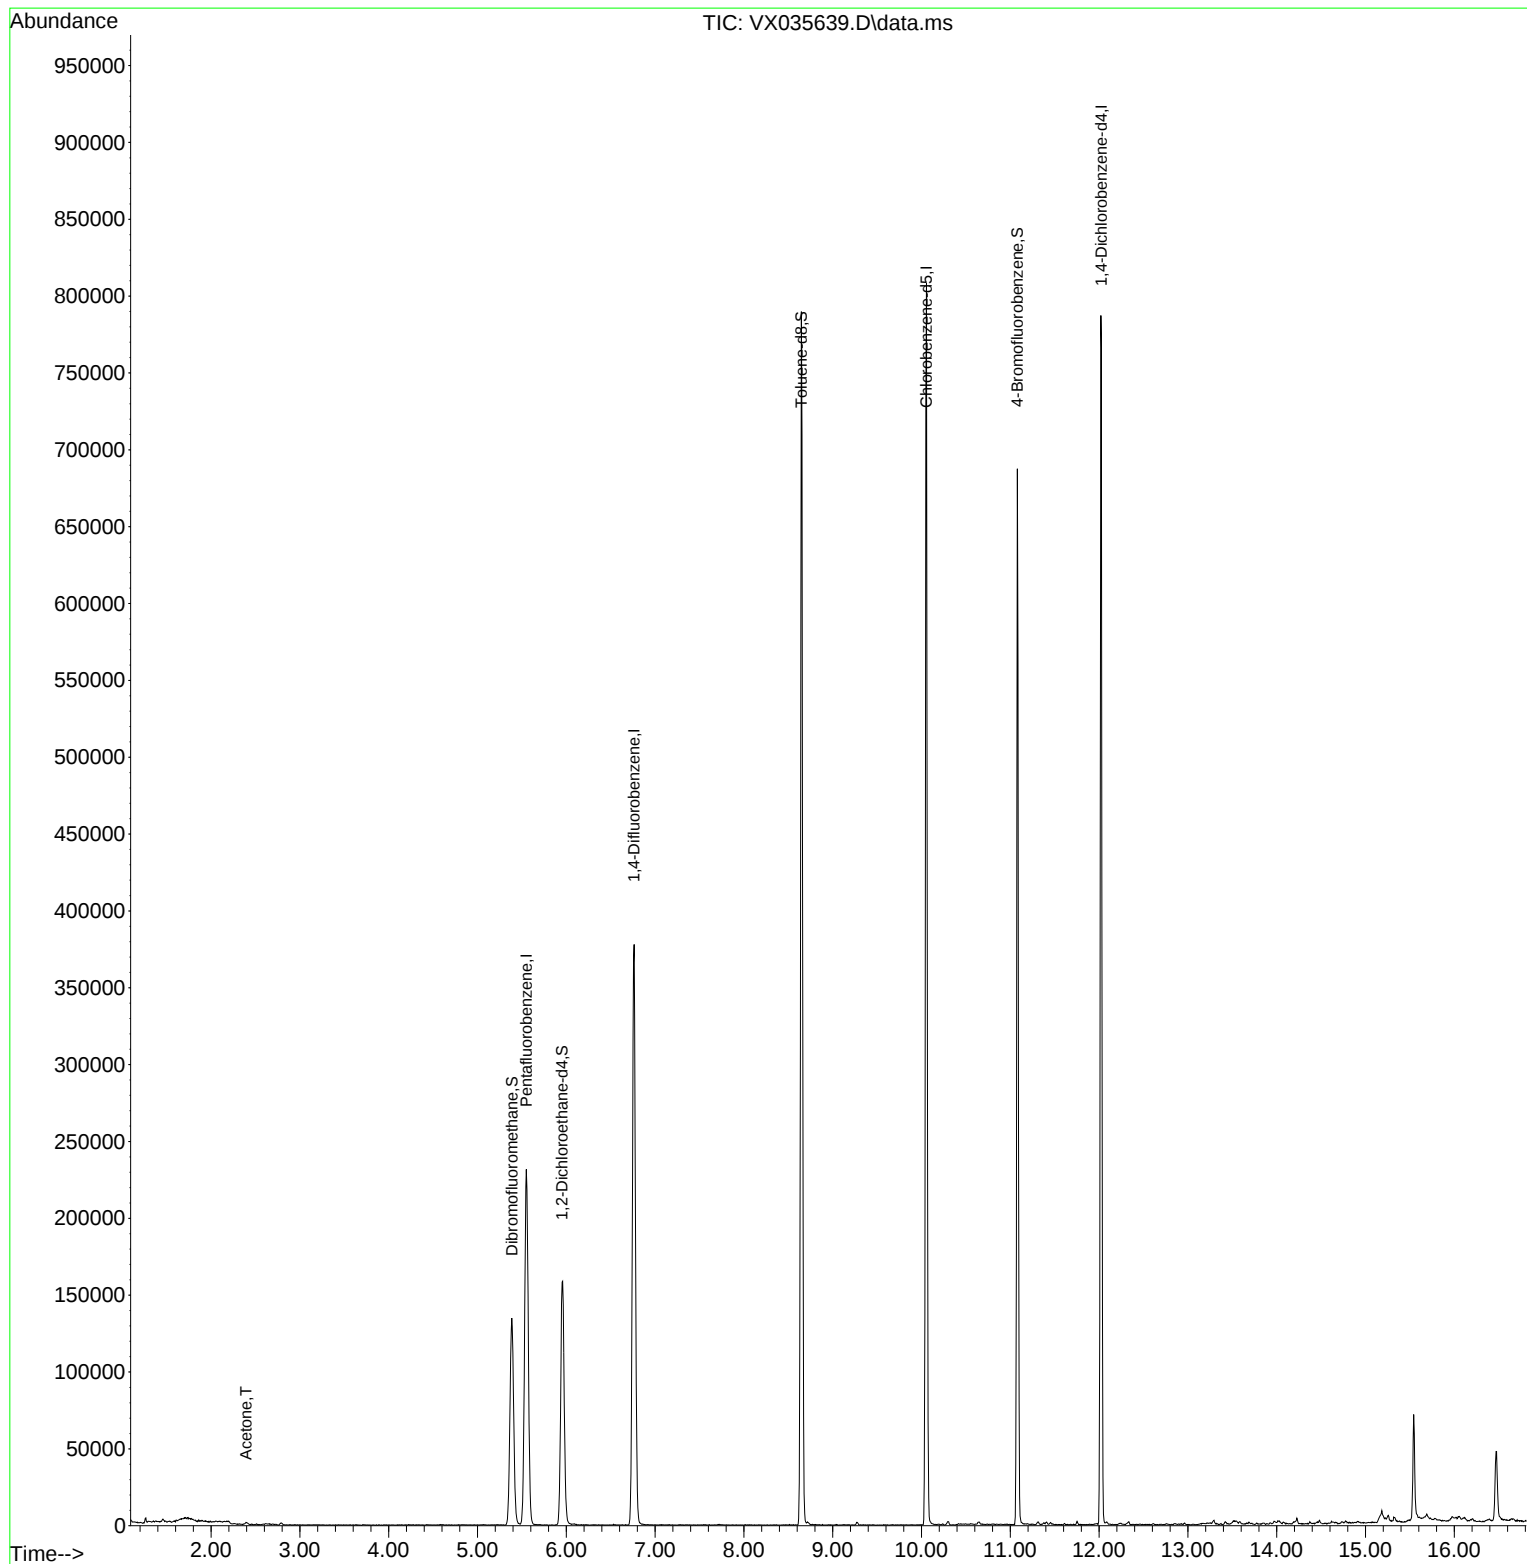




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX035639.D
Acq: 12 May 2023 15:41




Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SAMPLE-MANAG


Tgt Ion:168 Resp: 198165
Ion Ratio Lower Upper
168 100
99 69.9 45.7 68.5#

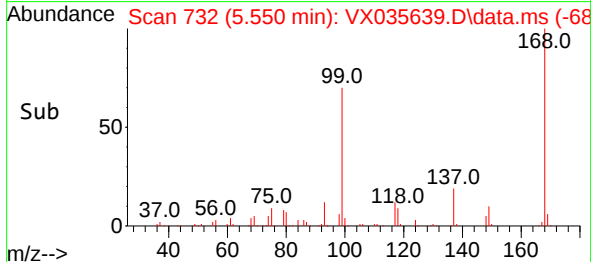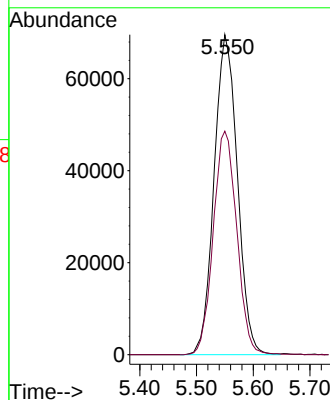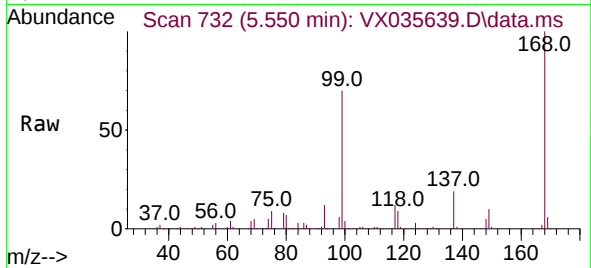

#16
Acetone
Concen: 1.194 ug/l
RT: 2.392 min Scan# 214
Delta R.T. -0.000 min
Lab File: VX035639.D
Acq: 12 May 2023 15:41

Tgt Ion: 43 Resp: 1774
Ion Ratio Lower Upper
43 100
58 26.5 24.7 37.1

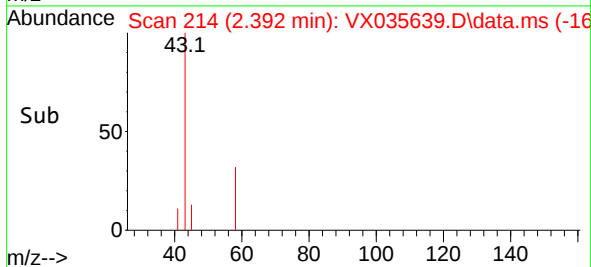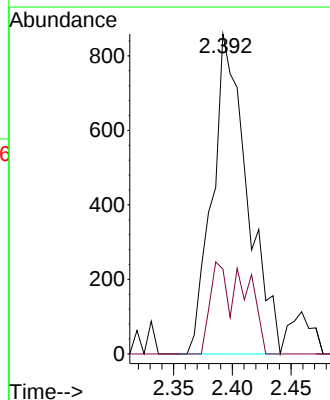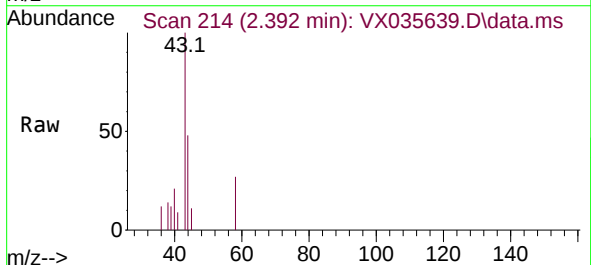

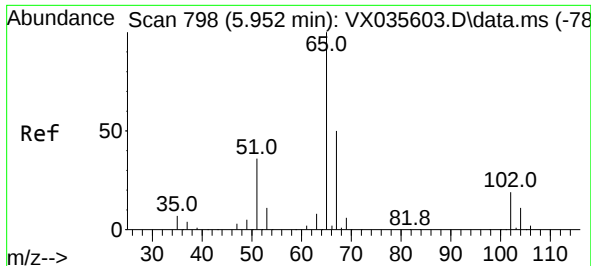

#33

1,2-Dichloroethane-d4

Concen: 47.480 ug/l

RT: 5.952 min Scan# 798

Delta R.T. 0.000 min

Lab File: VX035639.D

Acq: 12 May 2023 15:41

Instrument :

MSVOA_X

ClientSampleId :





STORAGE-BLANK-SAMPLE-MANAG

Tgt Ion: 65 Resp: 164141

Ion Ratio Lower Upper

65 100

67 49.8 0.0 104.0

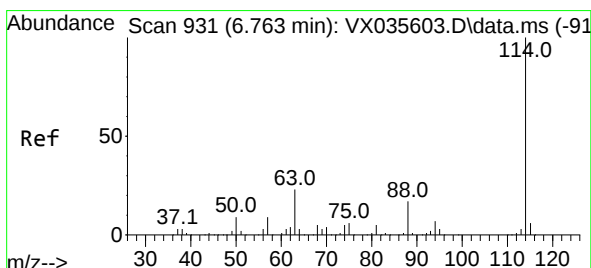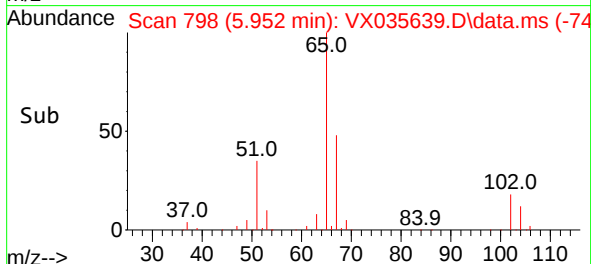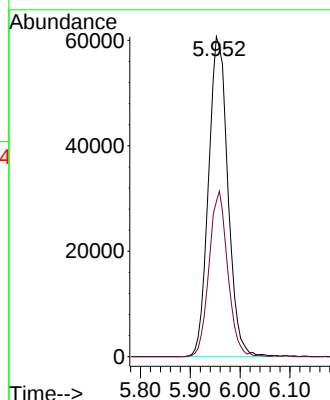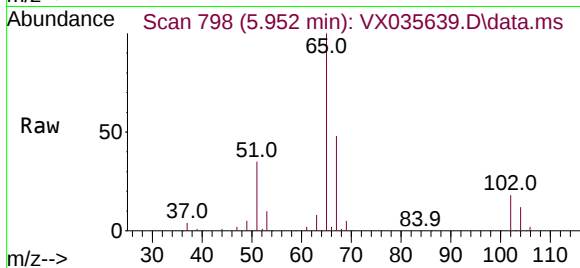

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.763 min Scan# 931

Delta R.T. 0.000 min

Lab File: VX035639.D

Acq: 12 May 2023 15:41




Tgt Ion: 114 Resp: 364619


Ion Ratio Lower Upper

114 100

63 22.5 0.0 42.2

88 17.4 0.0 33.2

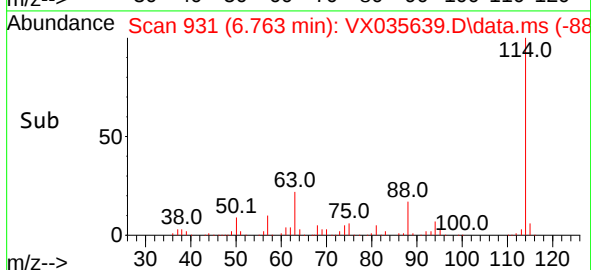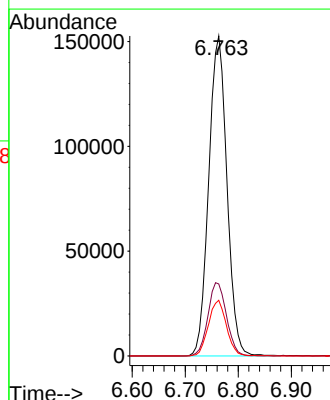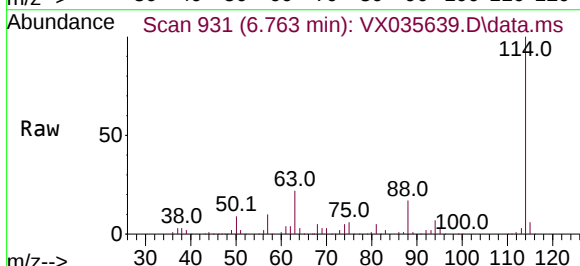

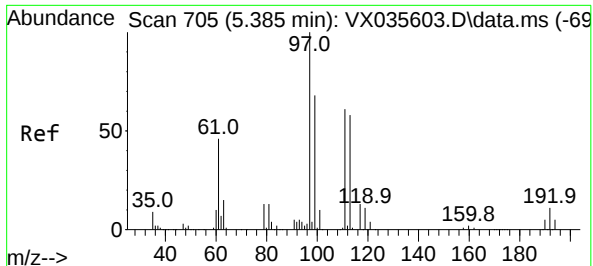

#35

Dibromofluoromethane

Concen: 47.250 ug/l

RT: 5.385 min Scan# 705

Delta R.T. 0.000 min

Lab File: VX035639.D


Acq: 12 May 2023 15:41

Instrument :

MSVOA_X

ClientSampleId :

STORAGE-BLANK-SAMPLE-MANAG

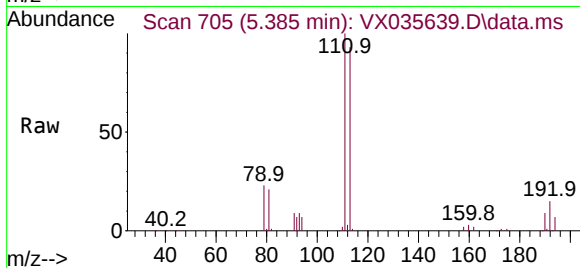




Tgt Ion:113 Resp: 116186

Ion Ratio Lower Upper

113 100

111 104.9 83.7 125.5

192 17.2 15.4 23.2

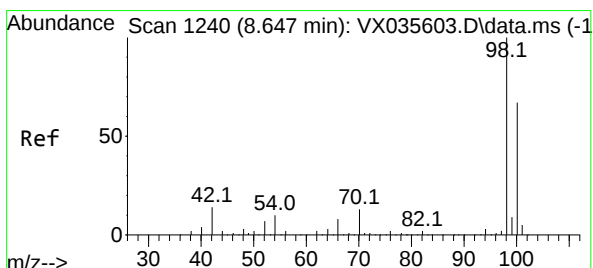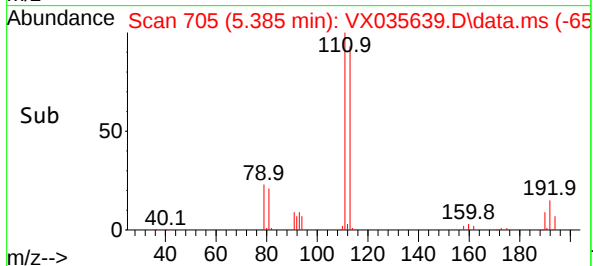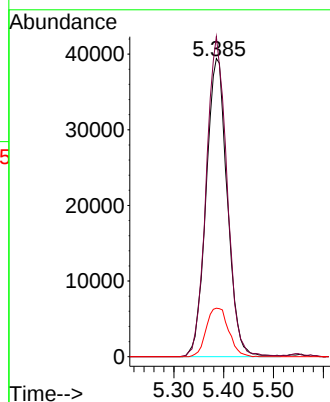

#50

Toluene-d8

Concen: 47.492 ug/l

RT: 8.647 min Scan# 1240

Delta R.T. -0.000 min

Lab File: VX035639.D




Acq: 12 May 2023 15:41


Tgt Ion: 98 Resp: 431420

Ion Ratio Lower Upper

98 100

100 67.3 52.5 78.7


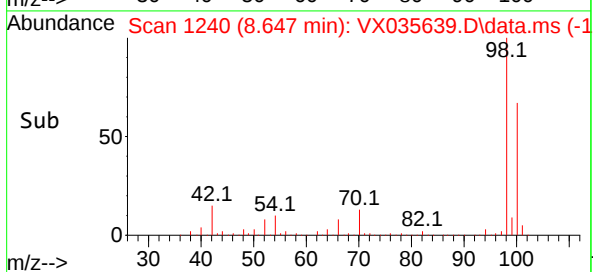
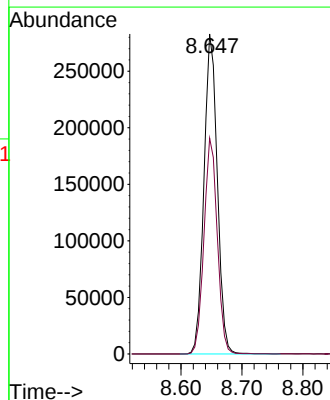
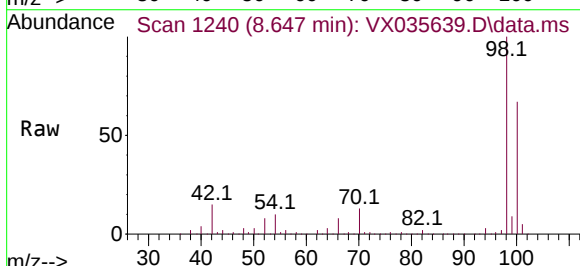


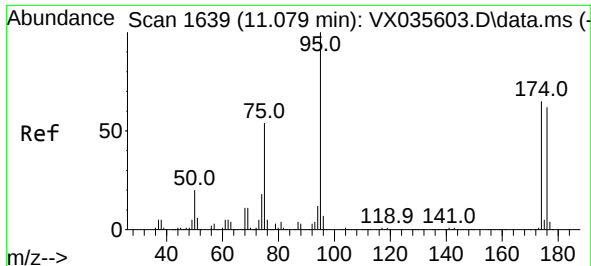

#62
4-Bromofluorobenzene
Concen: 49.164 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX035639.D
Acq: 12 May 2023 15:41




Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SAMPLE-MANAG


Tgt Ion: 95 Resp: 179824
Ion Ratio Lower Upper
95 100
174 65.2 0.0 147.4
176 63.3 0.0 140.6

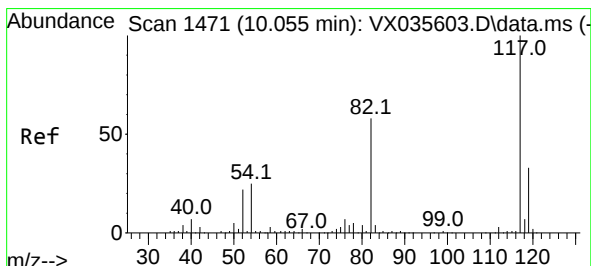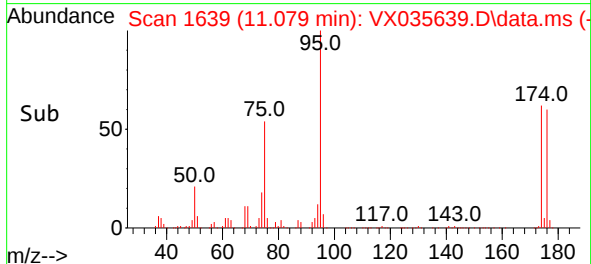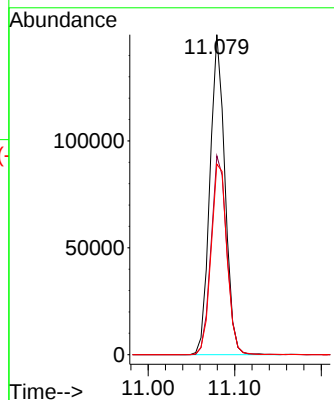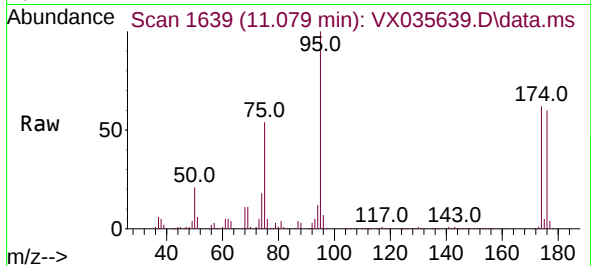

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX035639.D
Acq: 12 May 2023 15:41

Tgt Ion: 117 Resp: 331591
Ion Ratio Lower Upper
117 100
82 60.7 45.0 67.4
119 32.3 26.0 39.0

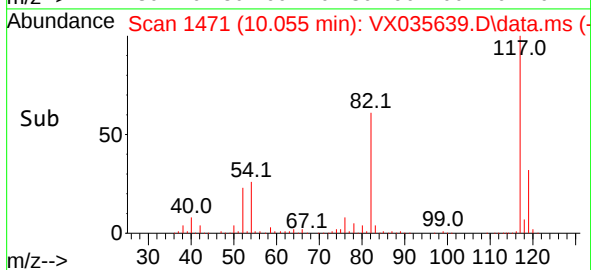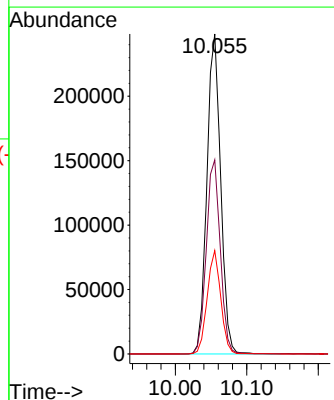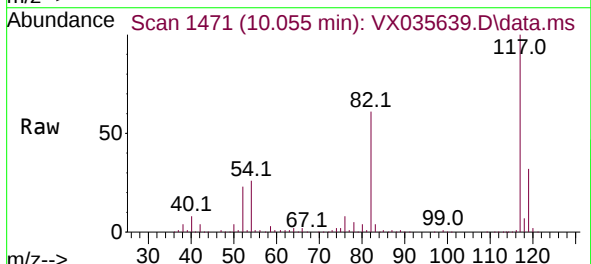

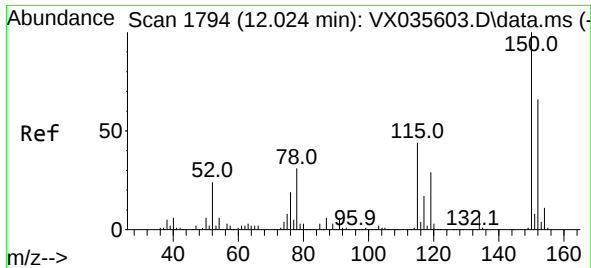

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.024 min Scan# 11

Delta R.T. 0.000 min

Lab File: VX035639.D


Acq: 12 May 2023 15:41

Instrument :

MSVOA_X

ClientSampleId :

STORAGE-BLANK-SAMPLE-MANAG

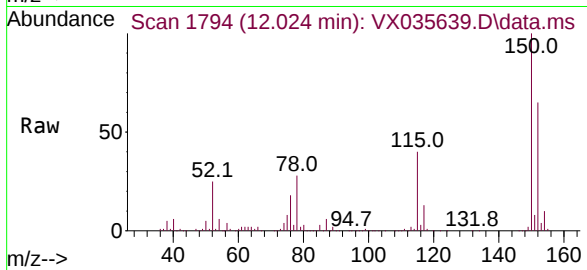

Tgt Ion:152 Resp: 150490

Ion Ratio Lower Upper

152 100

115 66.1 45.0 135.0

150 156.6 0.0 352.4

