

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051223\
 Data File : VX035627.D
 Acq On : 12 May 2023 10:34
 Operator : JC/MD
 Sample : VX0512MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0512MBL01

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051123W.M
 Title : SW846 8260

Signal : TIC: VX035627.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.379	691	704	720	rBV	137086	409161	32.71%	5.725%
2	5.544	720	731	745	rVV	237416	679627	54.33%	9.509%
3	5.952	787	798	814	rBV	169159	444349	35.52%	6.217%
4	6.757	919	930	944	rBV	395435	937599	74.95%	13.118%
5	8.647	1233	1240	1248	rBV	806174	1251004	100.00%	17.503%
6	10.055	1464	1471	1485	rBV	793047	1124906	89.92%	15.739%
7	11.079	1633	1639	1653	rBV	717296	882857	70.57%	12.352%
8	11.451	1696	1700	1706	rVB2	10717	14903	1.19%	0.209%
9	12.018	1788	1793	1803	rVB	840043	1051518	84.05%	14.712%
10	12.329	1840	1844	1849	rVB2	13783	17663	1.41%	0.247%
11	13.286	1996	2001	2006	rVB	11512	13780	1.10%	0.193%
12	13.585	2046	2050	2055	rVB	10931	14168	1.13%	0.198%
13	13.719	2069	2072	2077	rVB3	11904	15609	1.25%	0.218%
14	13.774	2077	2081	2085	rBV	11304	13415	1.07%	0.188%
15	13.963	2107	2112	2117	rBV3	12847	18218	1.46%	0.255%
16	15.182	2303	2312	2321	rBV9	6913	24924	1.99%	0.349%
17	15.542	2365	2371	2382	rBV	82464	129271	10.33%	1.809%
18	16.468	2517	2523	2531	rBV	56639	104475	8.35%	1.462%




Sum of corrected areas: 7147447

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051223\
Data File : VX035627.D
Acq On : 12 May 2023 10:34
Operator : JC/MD
Sample : VX0512MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0512MBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

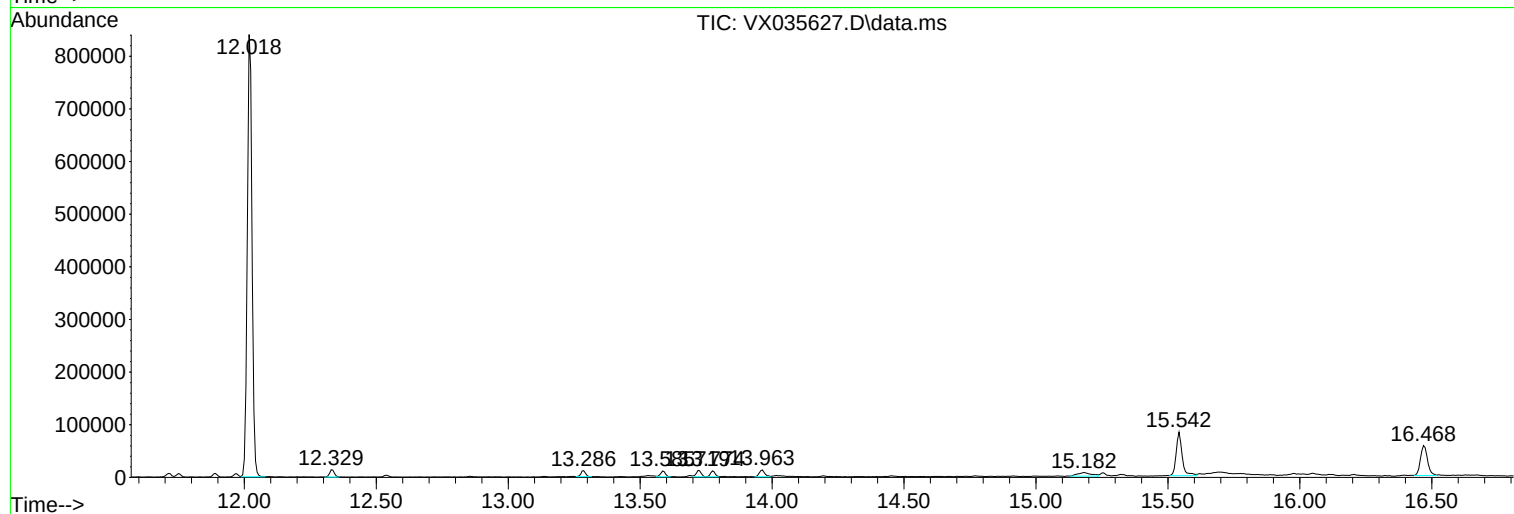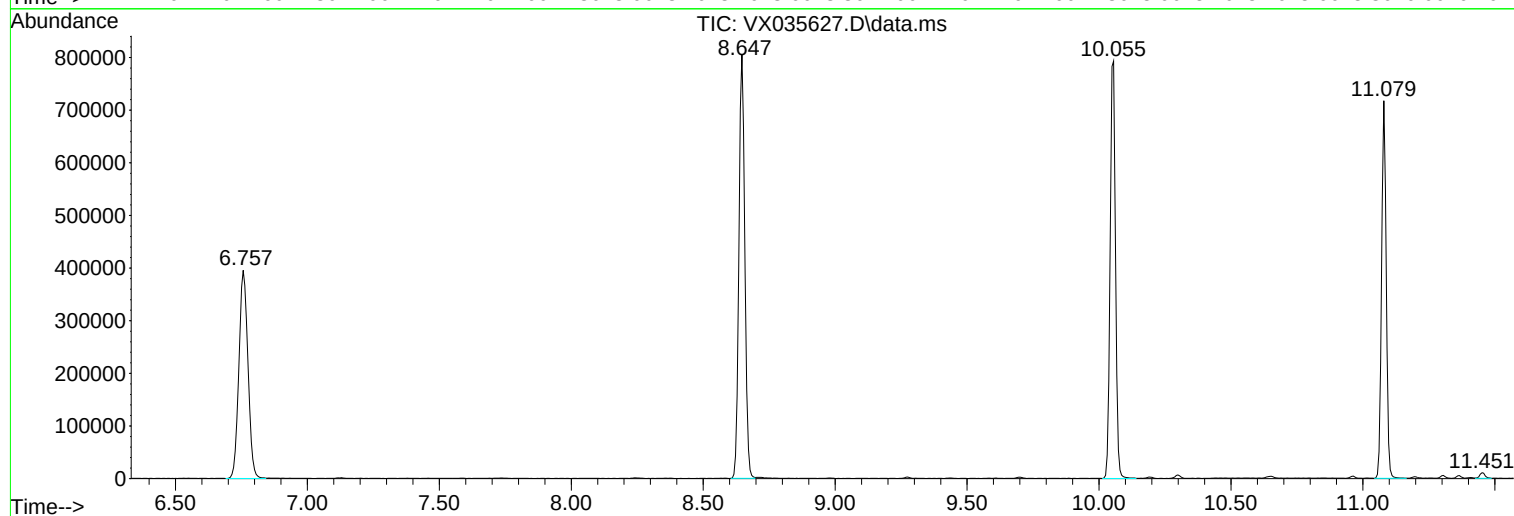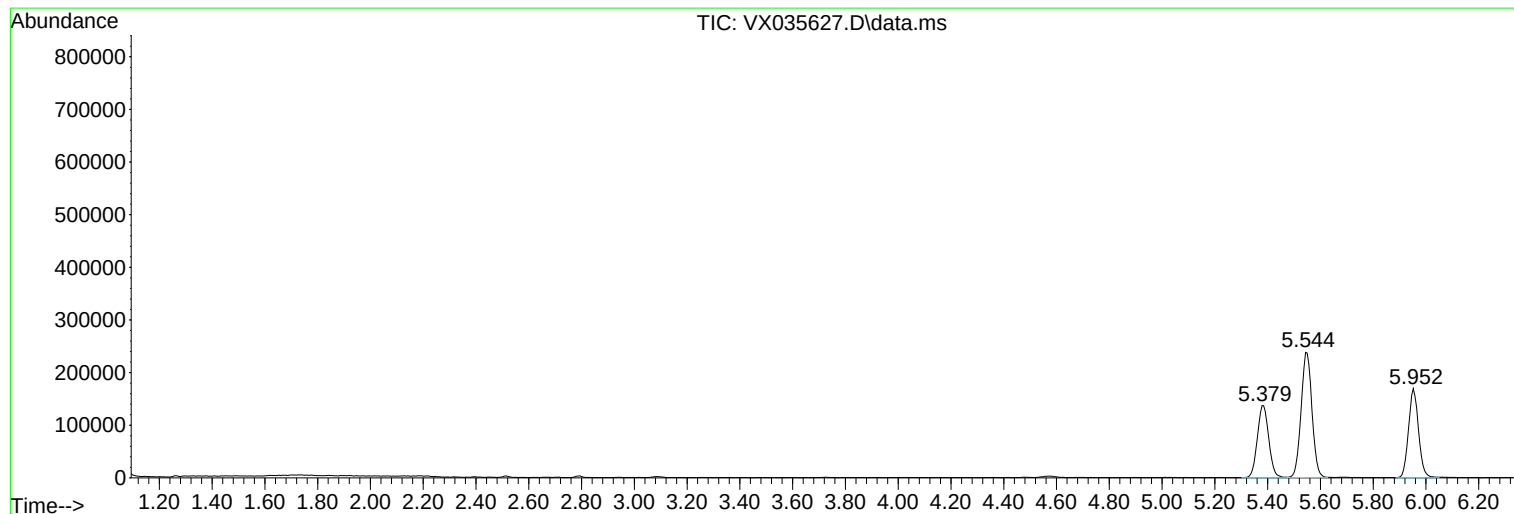

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051223\
Data File : VX035627.D
Acq On : 12 May 2023 10:34
Operator : JC/MD
Sample : VX0512MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0512MBL01










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Dodecane, 1-chloro- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
15.542	6.15 ug/l	129271	1,4-Dichlorobenzene-d4	12.024

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Dodecane, 1-chloro-	204	C12H25Cl	000112-52-7	91
2			n-Dodecylpyridinium chloride	283	C17H30ClN	000104-74-5	91
3			1-Chloroundecane	190	C11H23Cl	002473-03-2	90
4			Tetradecane, 1-chloro-	232	C14H29Cl	002425-54-9	58
5			Silane, trichlorodocosyl-	442	C22H45Cl3Si	007325-84-0	46

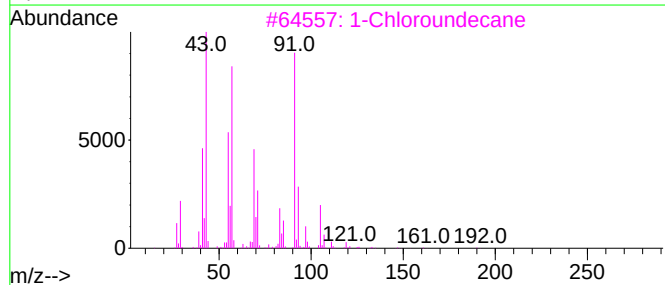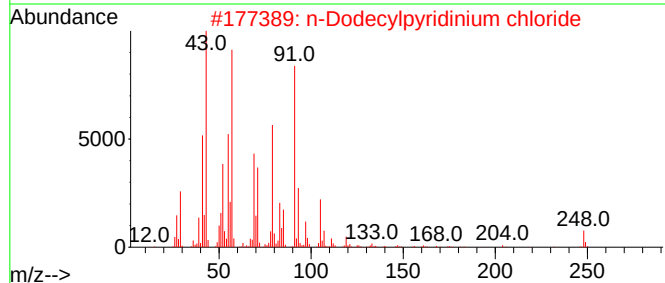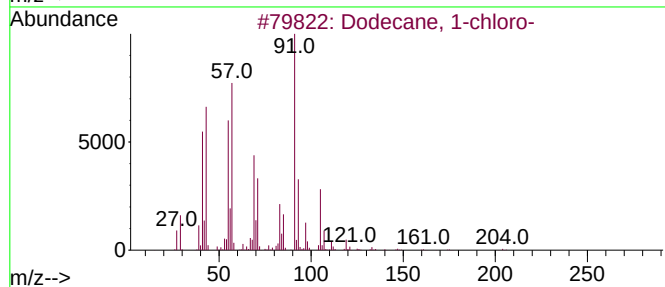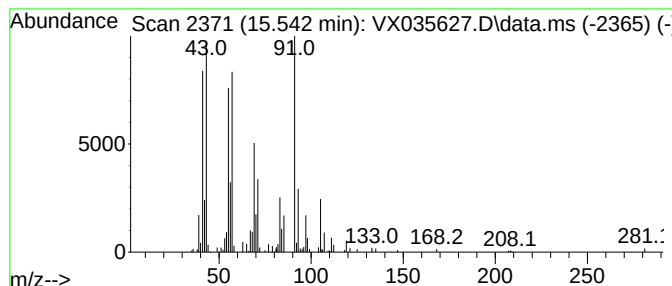

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051223\
Data File : VX035627.D
Acq On : 12 May 2023 10:34
Operator : JC/MD
Sample : VX0512MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0512MBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Dodecane, 1-chl...	15.542	6.2	ug/l	129271	4	12.024	1051520	50.0