

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051223\
Data File : VX035628.D
Acq On : 12 May 2023 10:57
Operator : JC/MD
Sample : VX0512WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0512WBL01

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051123W.M

Title : SW846 8260

Signal : TIC: VX035628.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.385	694	705	719	rBV	130922	381072	33.03%	5.944%
2	5.550	719	732	746	rVB	225011	636325	55.16%	9.925%
3	5.952	787	798	810	rBV	153784	418318	36.26%	6.525%
4	6.757	921	930	944	rBV	362506	867290	75.18%	13.528%
5	8.647	1233	1240	1249	rBV	735804	1153666	100.00%	17.994%
6	10.055	1465	1471	1485	rBV	741649	1029070	89.20%	16.051%
7	11.079	1634	1639	1651	rVB	636558	792665	68.71%	12.364%
8	12.018	1788	1793	1804	rBV	736189	924111	80.10%	14.414%
9	15.542	2362	2371	2381	rBV	73318	115001	9.97%	1.794%
10	16.469	2516	2523	2532	rBV2	49390	93773	8.13%	1.463%




Sum of corrected areas: 6411291

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051223\
Data File : VX035628.D
Acq On : 12 May 2023 10:57
Operator : JC/MD
Sample : VX0512WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0512WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

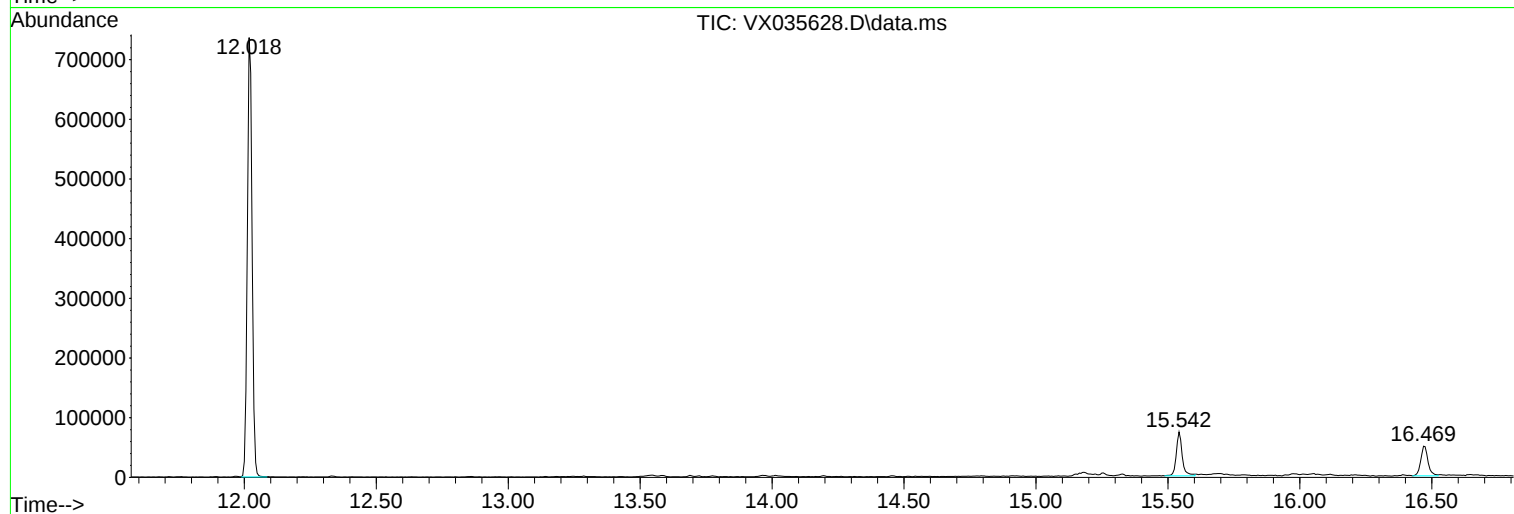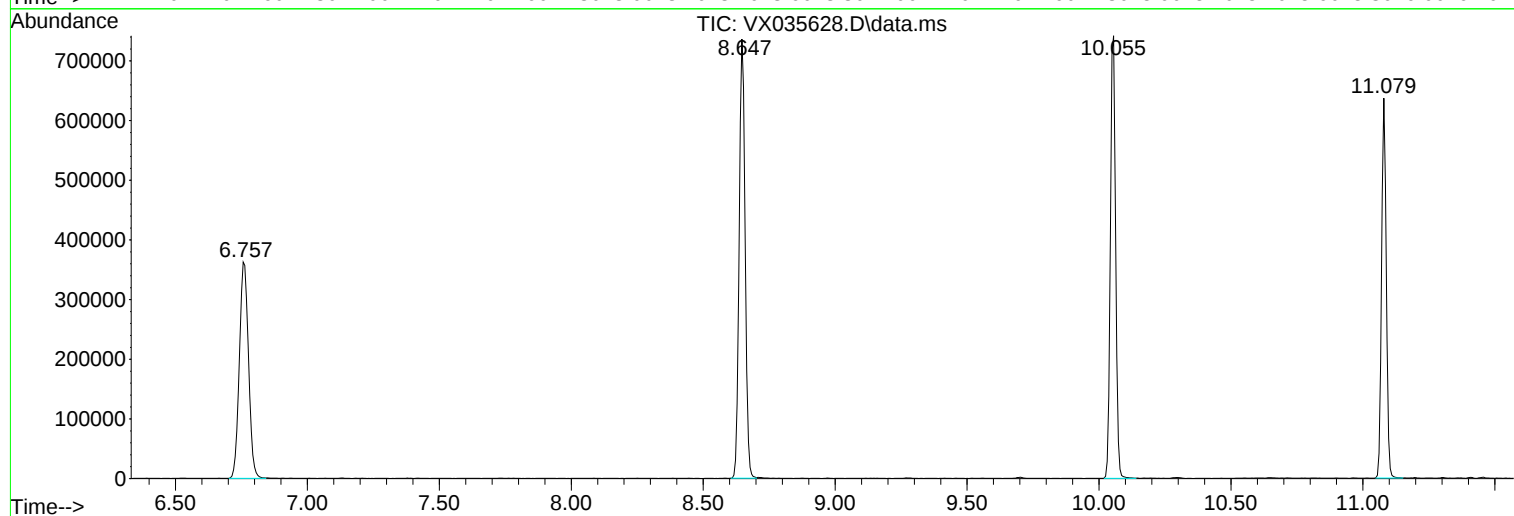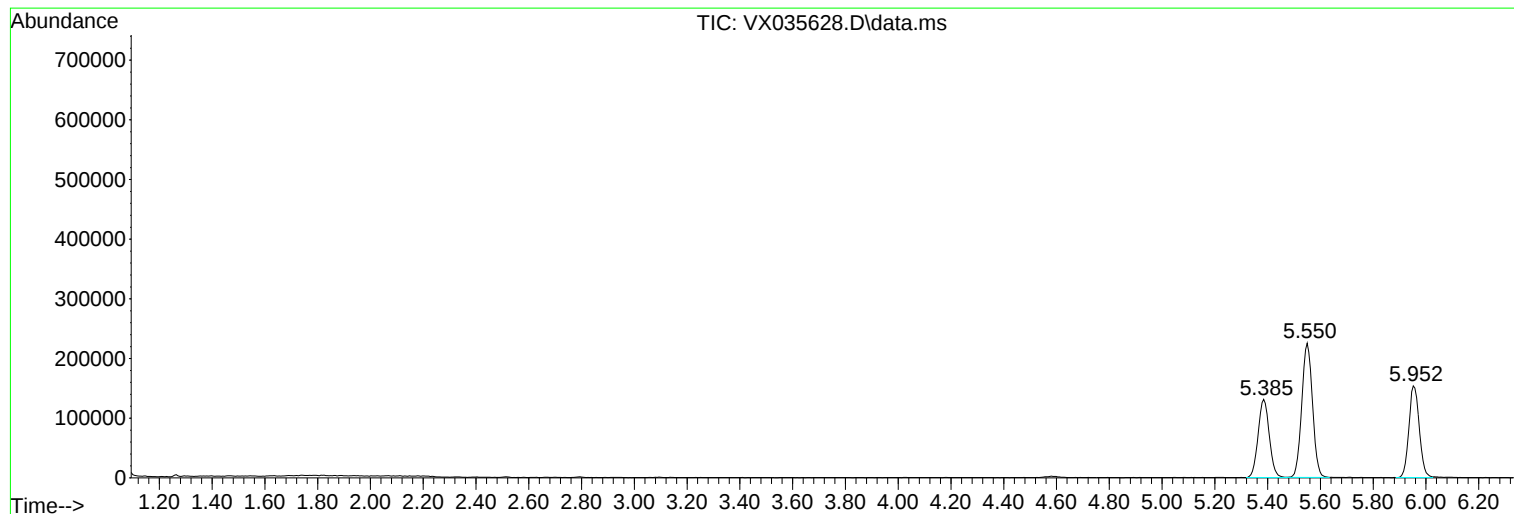

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051223\
Data File : VX035628.D
Acq On : 12 May 2023 10:57
Operator : JC/MD
Sample : VX0512WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0512WBL01










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Dodecane, 1-chloro- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
15.542	6.22 ug/l	115001	1,4-Dichlorobenzene-d4	12.024

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Dodecane, 1-chloro-	204	C12H25Cl	000112-52-7	90
2			1-Chloroundecane	190	C11H23Cl	002473-03-2	86
3			Tetradecane, 1-chloro-	232	C14H29Cl	002425-54-9	80
4			Chloroacetic acid, 4-tetradecyl ...	290	C16H31ClO2	1000280-08-6	35
5			Silane, trichlorodocosyl-	442	C22H45Cl3Si	007325-84-0	30

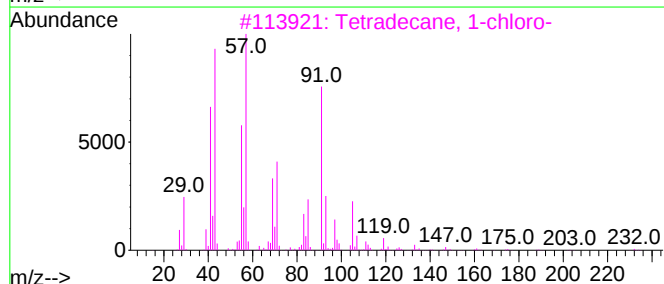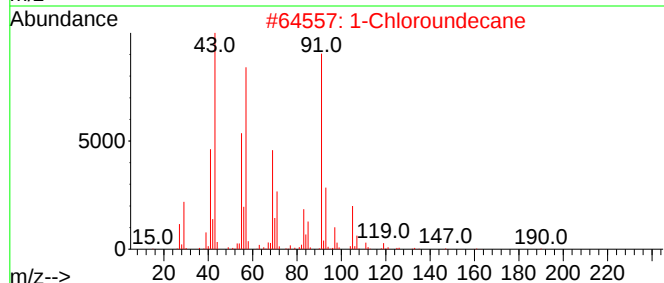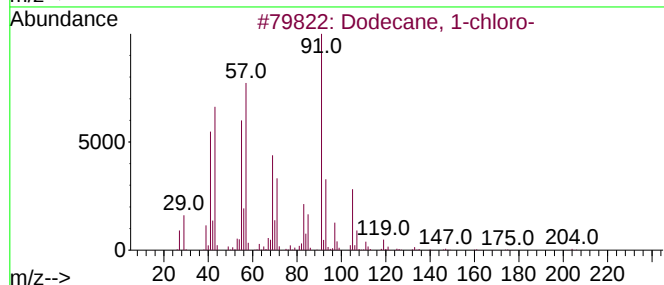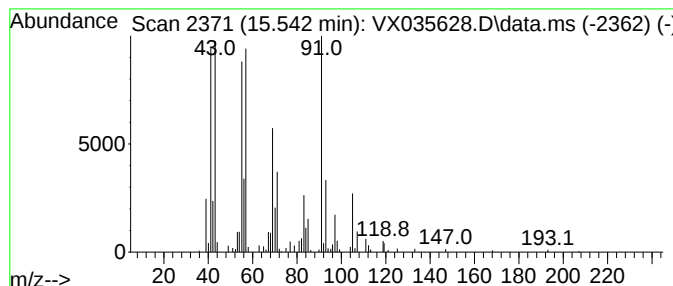

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051223\
Data File : VX035628.D
Acq On : 12 May 2023 10:57
Operator : JC/MD
Sample : VX0512WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0512WBL01










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Trichloroacetic acid, hexad... Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
16.468	5.07 ug/l	93773	1,4-Dichlorobenzene-d4	12.024

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Trichloroacetic acid, hexadecyl ...	386	C18H33Cl3O2	074339-54-1	74
2			Vinyl lauryl ether	212	C14H28O	000765-14-0	72
3			Dodecane, 1-chloro-	204	C12H25Cl	000112-52-7	72
4			Tetradecane, 1-chloro-	232	C14H29Cl	002425-54-9	64
5			Silane, trichlorodocosyl-	442	C22H45Cl3Si	007325-84-0	64

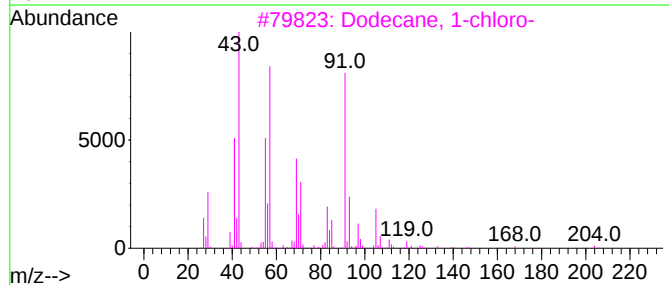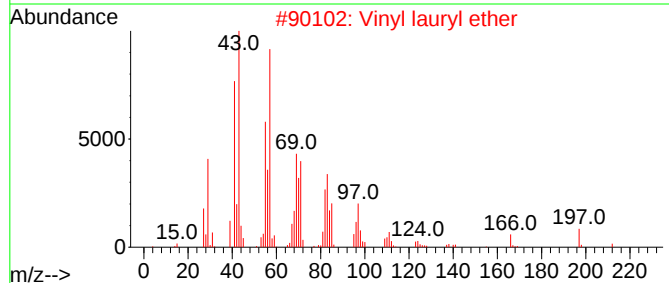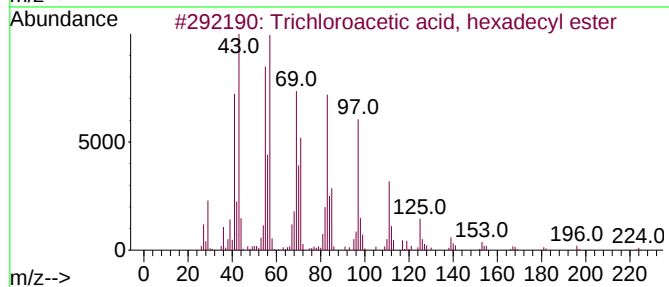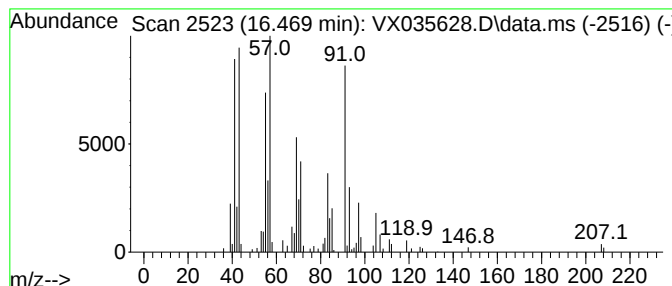

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051223\
Data File : VX035628.D
Acq On : 12 May 2023 10:57
Operator : JC/MD
Sample : VX0512WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0512WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Dodecane, 1-chl...	15.542	6.2	ug/l	115001	4	12.024	924111	50.0
Trichloroacetic...	16.468	5.1	ug/l	93773	4	12.024	924111	50.0