

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051223\
 Data File : VX035630.D
 Acq On : 12 May 2023 12:11
 Operator : JC/MD
 Sample : 02702-01 50X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 33998

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051123W.M
 Title : SW846 8260

Signal : TIC: VX035630.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.385	693	705	721	rBV2	127554	369935	32.82%	4.994%
2	5.550	721	732	748	rVB	220289	622579	55.24%	8.404%
3	5.958	787	799	818	rBV	147656	408983	36.29%	5.521%
4	6.763	920	931	947	rBV	352443	849226	75.34%	11.463%
5	8.647	1233	1240	1247	rBV	721202	1127129	100.00%	15.215%
6	8.720	1247	1252	1261	rVB	17113	30008	2.66%	0.405%
7	10.055	1465	1471	1483	rBV	718819	1003491	89.03%	13.546%
8	10.195	1489	1494	1500	rVB	19692	26446	2.35%	0.357%
9	10.299	1505	1511	1517	rBV	57492	78295	6.95%	1.057%
10	10.640	1562	1567	1575	rVB	51112	68201	6.05%	0.921%
11	11.079	1633	1639	1648	rBV	612515	778649	69.08%	10.511%
12	11.305	1670	1676	1681	rVV	13140	16095	1.43%	0.217%
13	11.378	1681	1688	1696	rVV	40740	74839	6.64%	1.010%
14	11.451	1696	1700	1709	rVB	28228	37740	3.35%	0.509%
15	11.610	1718	1726	1732	rBV	28338	35418	3.14%	0.478%
16	11.750	1745	1749	1758	rVB	77349	95193	8.45%	1.285%
17	12.018	1788	1793	1800	rVV	723048	937245	83.15%	12.652%
18	12.085	1800	1804	1813	rVB	42461	52135	4.63%	0.704%
19	12.244	1825	1830	1837	rBV2	41911	64213	5.70%	0.867%
20	12.329	1837	1844	1851	rVB5	17538	36004	3.19%	0.486%
21	12.530	1871	1877	1879	rBV	10629	14944	1.33%	0.202%
22	12.609	1887	1890	1893	rVV	13161	15595	1.38%	0.211%
23	12.701	1900	1905	1913	rBV2	16062	25057	2.22%	0.338%
24	12.920	1934	1941	1944	rVV2	9468	11993	1.06%	0.162%
25	12.963	1944	1948	1954	rVB	14910	18266	1.62%	0.247%
26	13.164	1977	1981	1986	rVB	19838	25131	2.23%	0.339%
27	13.292	1992	2002	2007	rBV2	58853	86326	7.66%	1.165%
28	13.420	2018	2023	2032	rVB	52835	66099	5.86%	0.892%
29	13.585	2046	2050	2056	rVB6	14387	19059	1.69%	0.257%
30	13.658	2056	2062	2069	rVB4	5863	12676	1.12%	0.171%
31	13.774	2077	2081	2088	rVB	19367	24779	2.20%	0.334%
32	13.853	2088	2094	2100	rVB3	10366	14392	1.28%	0.194%
33	13.926	2100	2106	2109	rBV2	10809	15539	1.38%	0.210%
34	13.963	2109	2112	2117	rVB4	10187	14935	1.33%	0.202%
35	14.225	2146	2155	2160	rBV	25384	42760	3.79%	0.577%
36	14.475	2190	2196	2206	rVB3	16406	25918	2.30%	0.350%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051223\
Data File : VX035630.D
Acq On : 12 May 2023 12:11
Operator : JC/MD
Sample : 02702-01 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
33998

Integration Parameters: RTEINT.P
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051123W.M
Title : SW846 8260

37	14.634	2215	2222	2226	rBV4	12107	22217	1.97%	0.300%
38	15.182	2304	2312	2321	rBV4	9263	28000	2.48%	0.378%
39	15.542	2363	2371	2380	rBV	73092	117735	10.45%	1.589%
40	16.469	2515	2523	2534	rBV	48065	94869	8.42%	1.281%


Sum of corrected areas: 7408114

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051223\
Data File : VX035630.D
Acq On : 12 May 2023 12:11
Operator : JC/MD
Sample : 02702-01 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
33998

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

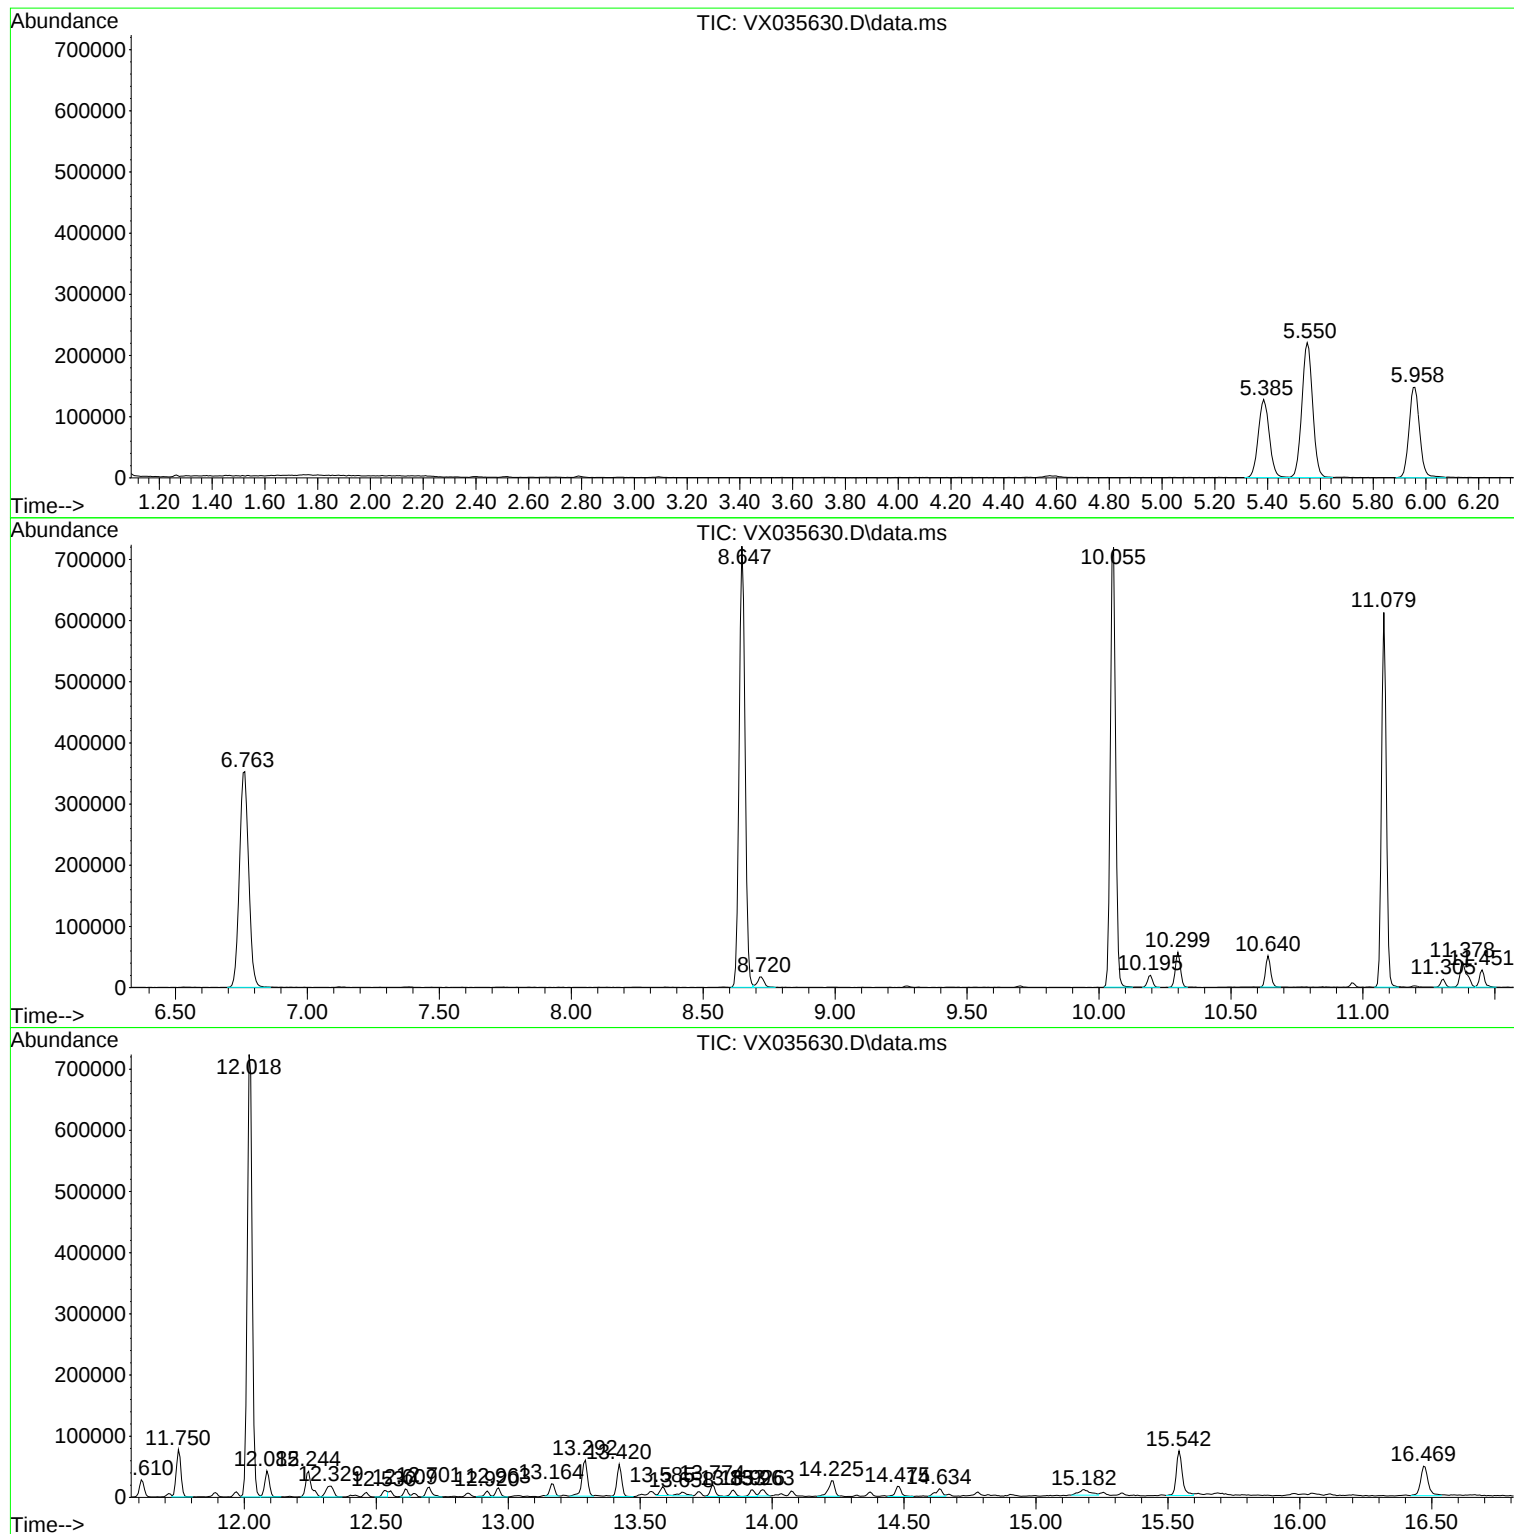

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051223\
Data File : VX035630.D
Acq On : 12 May 2023 12:11
Operator : JC/MD
Sample : 02702-01 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
33998










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Dodecane, 1-chloro- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
15.542	6.28 ug/l	117735	1,4-Dichlorobenzene-d4	12.024

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Dodecane, 1-chloro-	204	C12H25Cl	000112-52-7	90
2			Decane, 1-chloro-	176	C10H21Cl	001002-69-3	72
3			Octadecane, 1-(ethenyloxy)-	296	C20H40O	000930-02-9	52
4			1-Eicosanol	298	C20H42O	000629-96-9	52
5			Silane, trichlorodocosyl-	442	C22H45Cl3Si	007325-84-0	49

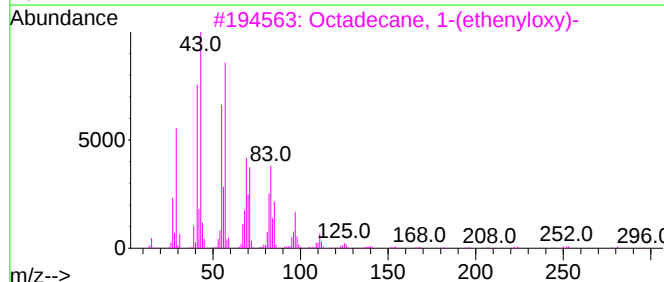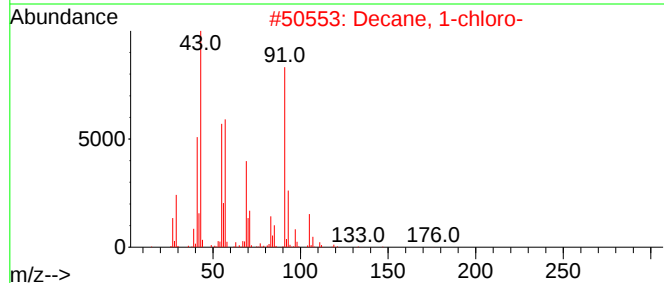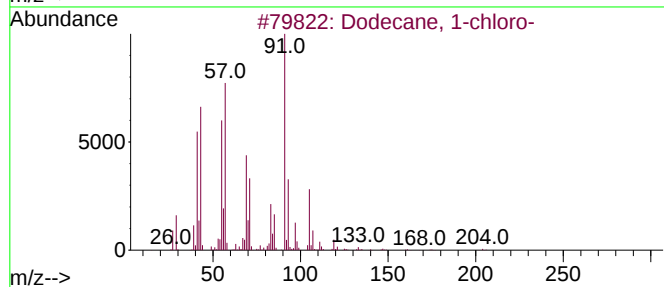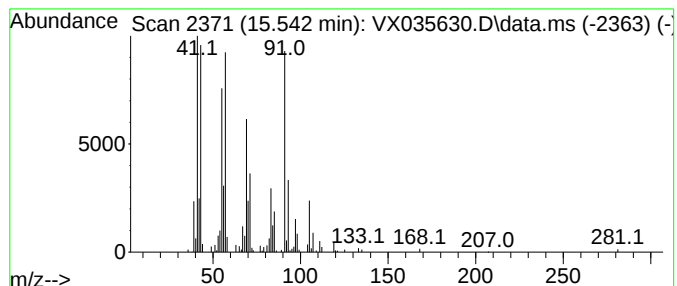

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051223\
Data File : VX035630.D
Acq On : 12 May 2023 12:11
Operator : JC/MD
Sample : 02702-01 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
33998










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Tetradecane, 1-chloro- Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
16.468	5.06 ug/l	94869	1,4-Dichlorobenzene-d4	12.024

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Dodecane, 1-chloro-	204	C12H25Cl	000112-52-7	80
2			Tetradecane, 1-chloro-	232	C14H29Cl	002425-54-9	64
3			Decane, 1-chloro-	176	C10H21Cl	001002-69-3	58
4			Decane, 1-(ethenyl)-	184	C12H24O	000765-05-9	46
5			1-Tridecene	182	C13H26	002437-56-1	46

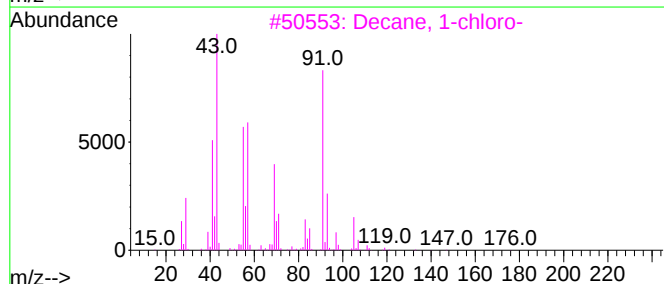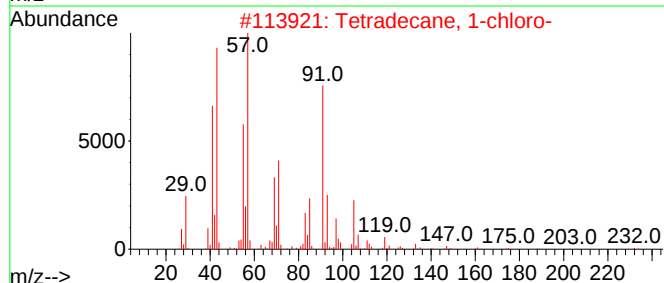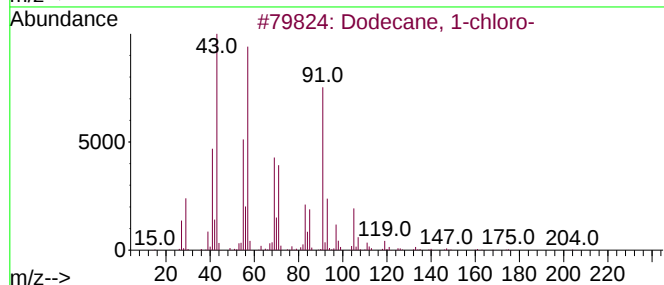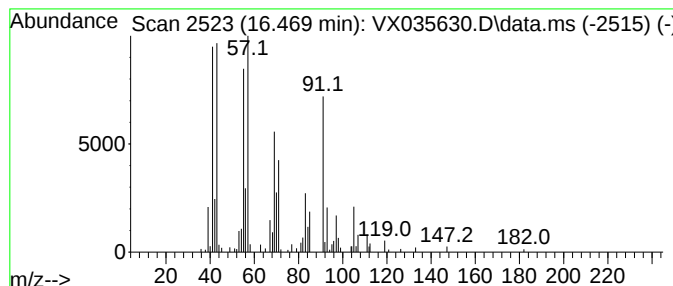

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051223\
Data File : VX035630.D
Acq On : 12 May 2023 12:11
Operator : JC/MD
Sample : 02702-01 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
33998

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Dodecane, 1-chl...	15.542	6.3	ug/l	117735	4	12.024	937245	50.0
Tetradecane, 1-...	16.468	5.1	ug/l	94869	4	12.024	937245	50.0