

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051223\
 Data File : VX035631.D
 Acq On : 12 May 2023 12:34
 Operator : JC/MD
 Sample : 02702-02 50X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 50033

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051123W.M
 Title : SW846 8260

Signal : TIC: VX035631.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.385	693	705	717	rBV	132855	380961	32.52%	5.378%
2	5.550	721	732	747	rVB2	222976	637734	54.44%	9.004%
3	5.952	788	798	808	rBV	160000	421643	35.99%	5.953%
4	6.038	808	812	825	rVB2	11614	30583	2.61%	0.432%
5	6.763	920	931	944	rBV	366611	880716	75.18%	12.434%
6	8.647	1232	1240	1247	rBV	746735	1171498	100.00%	16.539%
7	8.720	1247	1252	1259	rVB	54504	88384	7.54%	1.248%
8	10.055	1464	1471	1484	rBV	776948	1044484	89.16%	14.746%
9	10.305	1505	1512	1517	rBV	10741	16114	1.38%	0.227%
10	10.640	1562	1567	1573	rBV	64990	80723	6.89%	1.140%
11	11.079	1634	1639	1651	rVB	670477	827010	70.59%	11.676%
12	11.378	1682	1688	1690	rBV2	12281	17116	1.46%	0.242%
13	11.451	1696	1700	1707	rVB2	18391	22099	1.89%	0.312%
14	11.610	1722	1726	1731	rBV	19574	24563	2.10%	0.347%
15	12.018	1788	1793	1800	rBV	780216	982849	83.90%	13.876%
16	12.085	1800	1804	1808	rVB	27543	35854	3.06%	0.506%
17	12.244	1823	1830	1833	rBV	21286	30571	2.61%	0.432%
18	12.317	1837	1842	1849	rVB3	10230	18853	1.61%	0.266%
19	12.701	1899	1905	1913	rBV3	8875	14202	1.21%	0.201%
20	13.292	1997	2002	2006	rVB2	32566	44791	3.82%	0.632%
21	13.420	2018	2023	2031	rVB2	26488	34143	2.91%	0.482%
22	14.231	2144	2156	2160	rBV3	12765	25541	2.18%	0.361%
23	14.481	2188	2197	2203	rBV2	9836	15173	1.30%	0.214%
24	15.182	2303	2312	2321	rBV9	7063	25645	2.19%	0.362%
25	15.542	2365	2371	2379	rBV2	73914	114628	9.78%	1.618%
26	16.469	2515	2523	2536	rBV2	50808	97294	8.31%	1.374%




Sum of corrected areas: 7083172

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051223\
Data File : VX035631.D
Acq On : 12 May 2023 12:34
Operator : JC/MD
Sample : 02702-02 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
50033

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

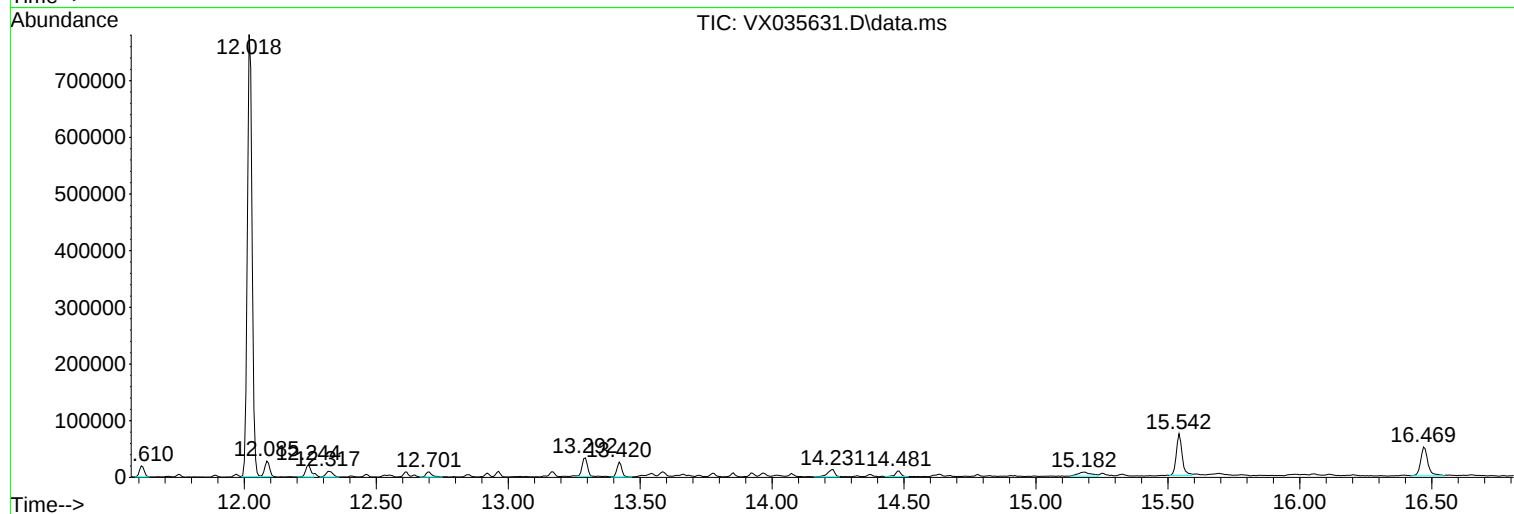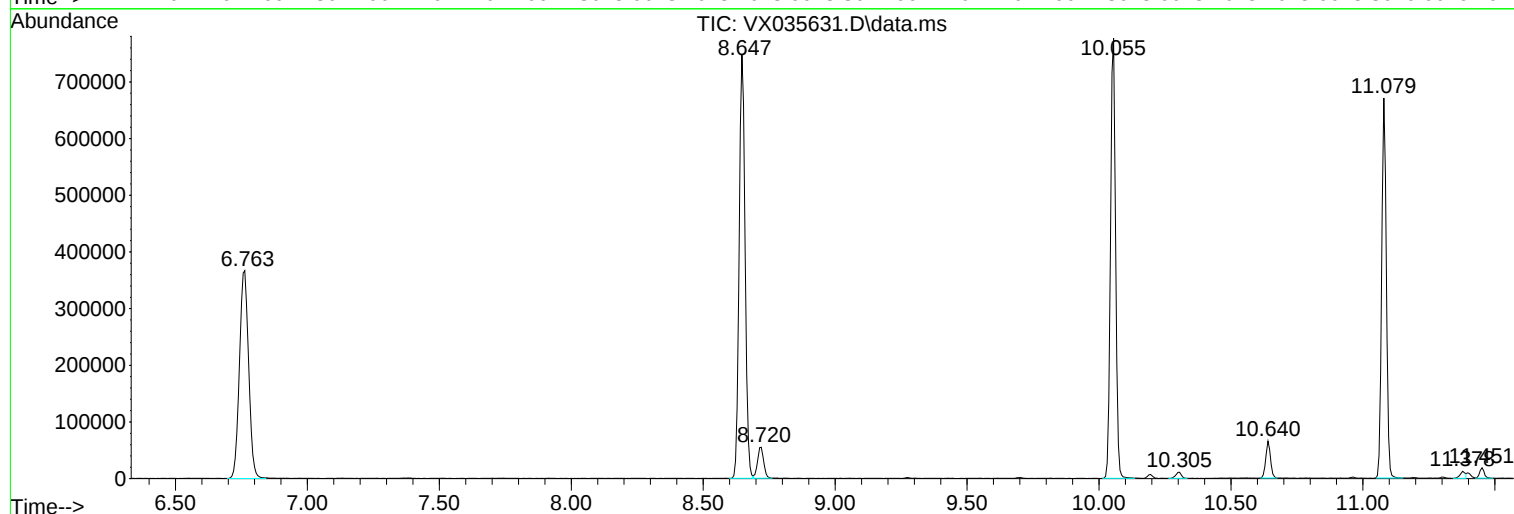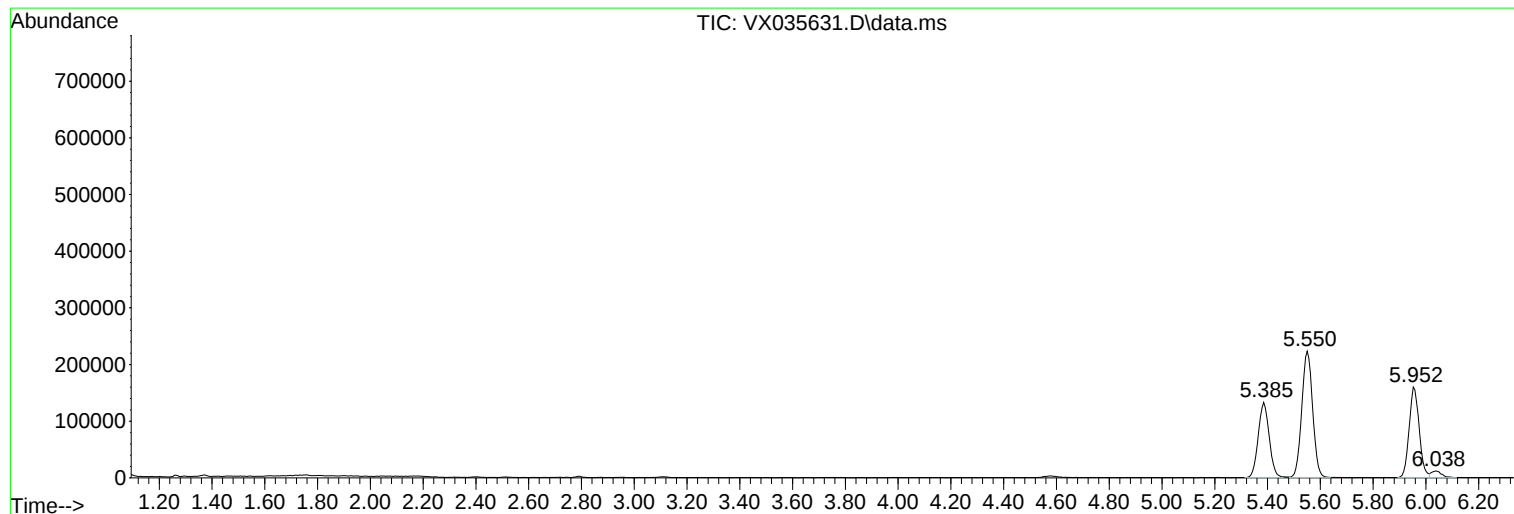

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051223\
Data File : VX035631.D
Acq On : 12 May 2023 12:34
Operator : JC/MD
Sample : 02702-02 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
50033










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Dodecane, 1-chloro- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
15.542	5.83 ug/l	114628	1,4-Dichlorobenzene-d4	12.018

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Dodecane, 1-chloro-	204	C12H25Cl	000112-52-7	91
2			1-Chloroundecane	190	C11H23Cl	002473-03-2	83
3			Decane, 1-chloro-	176	C10H21Cl	001002-69-3	80
4			1-(Ethenesulfonyl)dodecane	260	C14H28O2S	030719-66-5	58
5			1-Dodecene	168	C12H24	000112-41-4	50

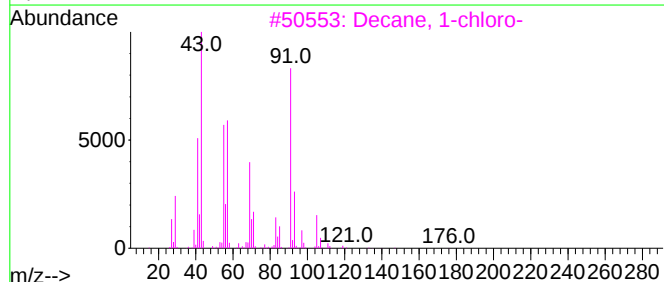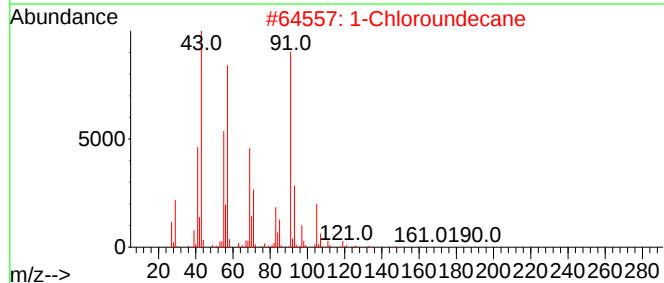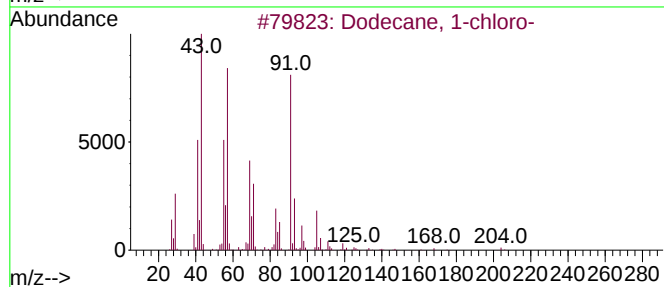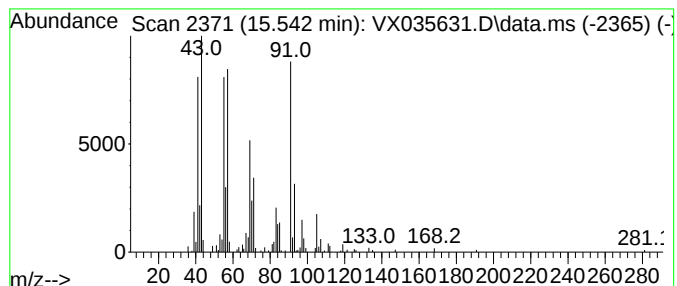

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051223\
Data File : VX035631.D
Acq On : 12 May 2023 12:34
Operator : JC/MD
Sample : 02702-02 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
50033

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
-----	-----	-----	-----	-----	-----	-----	-----	-----
Dodecane, 1-chl...	15.542	5.8	ug/l	114628	4	12.018	982849	50.0