

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051223\
 Data File : VX035633.D
 Acq On : 12 May 2023 13:21
 Operator : JC/MD
 Sample : 02755-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 A5560

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051123W.M

Title : SW846 8260

Signal : TIC: VX035633.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.385	692	705	719	rBV2	127424	369677	32.83%	5.584%
2	5.550	719	732	746	rVB	220917	616027	54.70%	9.305%
3	5.952	788	798	816	rBV	152466	408757	36.30%	6.175%
4	6.763	919	931	945	rBV	345001	841759	74.75%	12.715%
5	8.647	1233	1240	1247	rBV	727228	1126106	100.00%	17.011%
6	8.720	1247	1252	1262	rVB	197282	314297	27.91%	4.748%
7	10.055	1465	1471	1482	rBV	719859	992679	88.15%	14.995%
8	10.152	1482	1487	1492	rVV	53405	69461	6.17%	1.049%
9	11.079	1634	1639	1648	rBV	626767	767080	68.12%	11.587%
10	12.018	1788	1793	1804	rBV	698726	897345	79.69%	13.555%
11	15.176	2303	2311	2317	rBV8	5728	18076	1.61%	0.273%
12	15.542	2365	2371	2381	rBV	69550	107351	9.53%	1.622%
13	16.468	2516	2523	2532	rBV	49485	91444	8.12%	1.381%




Sum of corrected areas: 6620059

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051223\
Data File : VX035633.D
Acq On : 12 May 2023 13:21
Operator : JC/MD
Sample : 02755-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
A5560

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

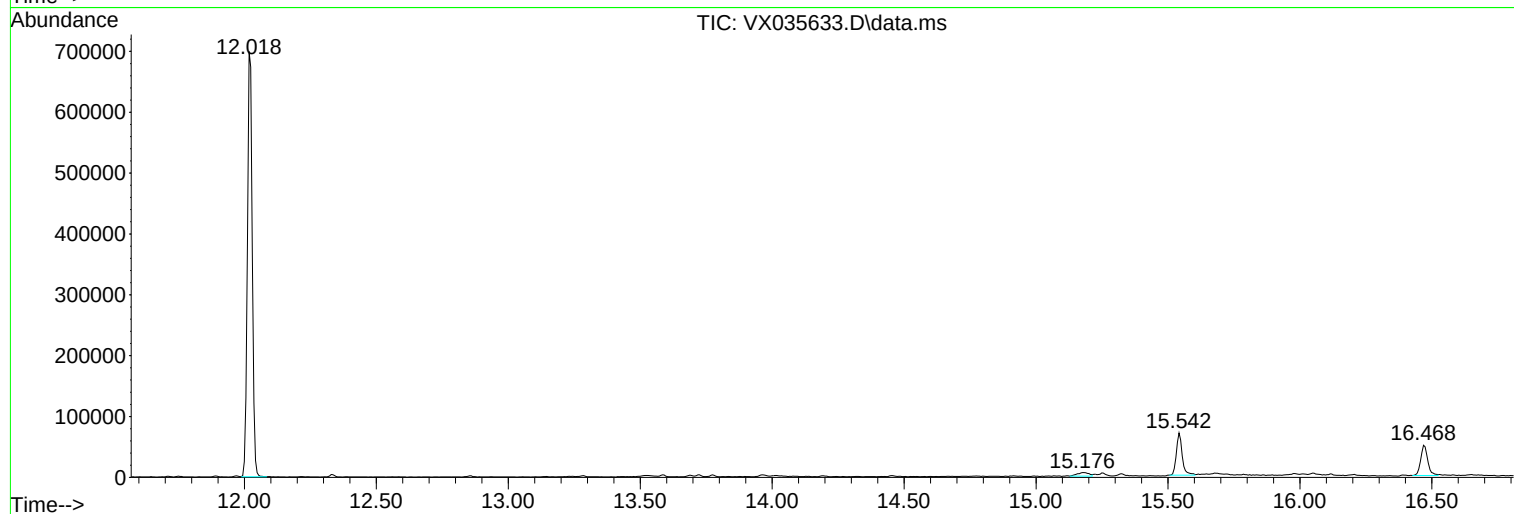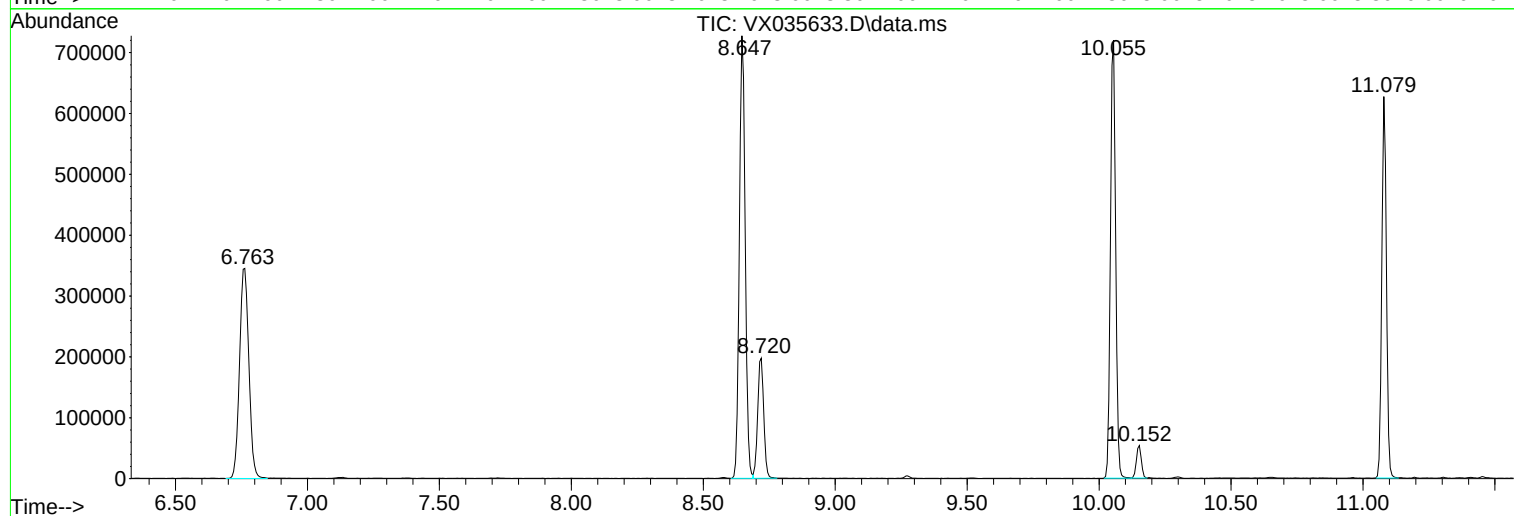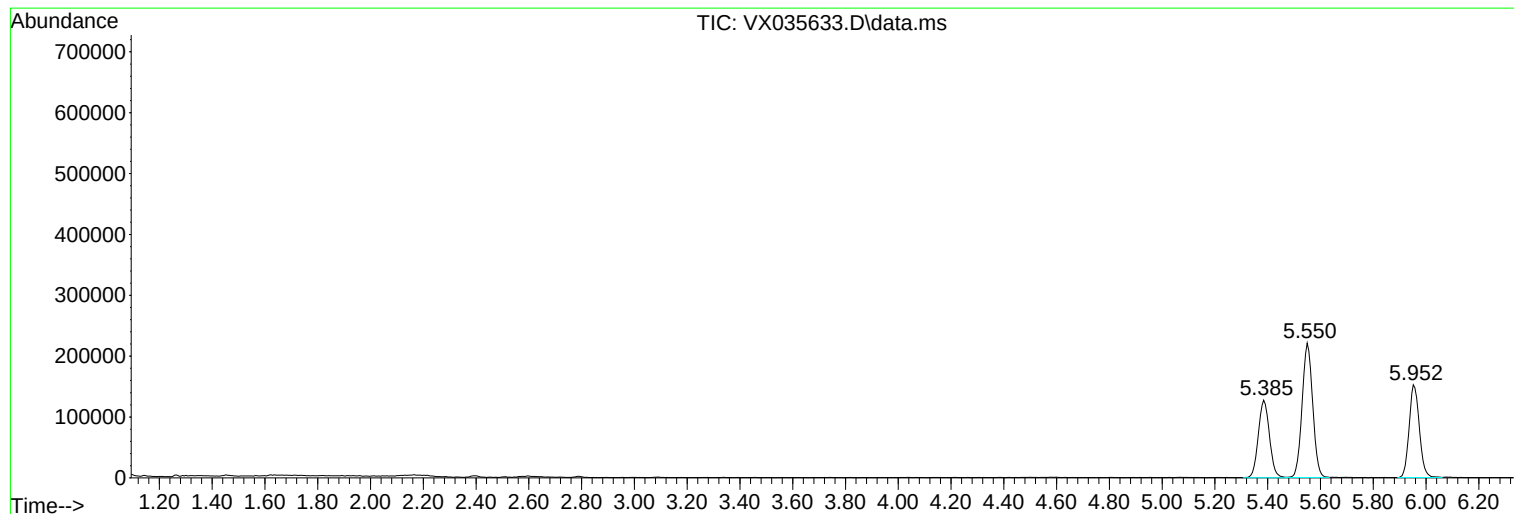

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051223\
Data File : VX035633.D
Acq On : 12 May 2023 13:21
Operator : JC/MD
Sample : 02755-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
A5560










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Dodecane, 1-chloro- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
15.542	5.98 ug/l	107351	1,4-Dichlorobenzene-d4	12.024

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Dodecane, 1-chloro-	204	C12H25Cl	000112-52-7	91
2			1-Chloroundecane	190	C11H23Cl	002473-03-2	90
3			Decane, 1-chloro-	176	C10H21Cl	001002-69-3	72
4			Tetradecane, 1-chloro-	232	C14H29Cl	002425-54-9	72
5			4-Heptafluorobutyryloxyhexadecane	438	C20H33F7O2	1010282-97-2	43

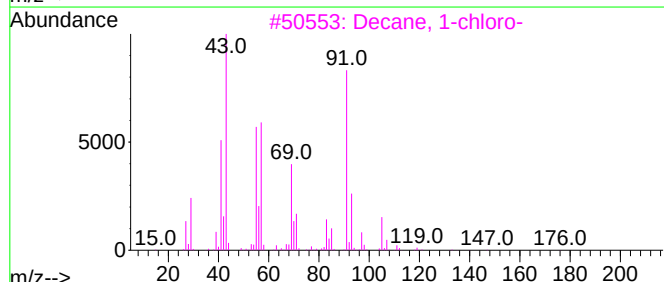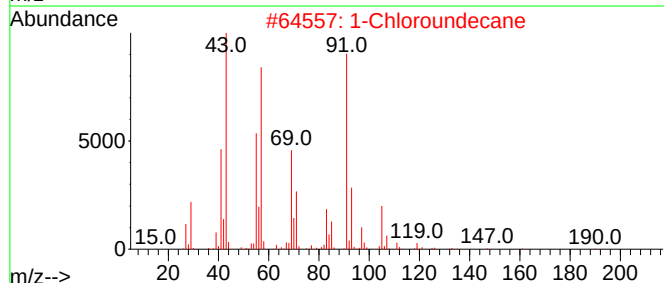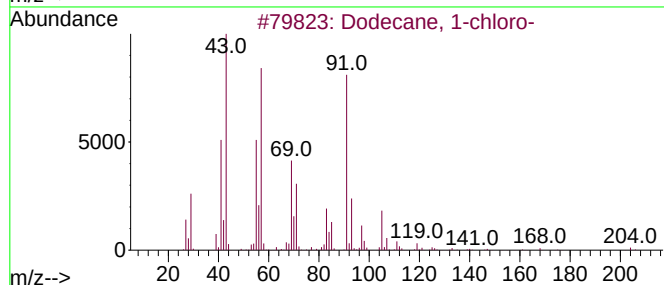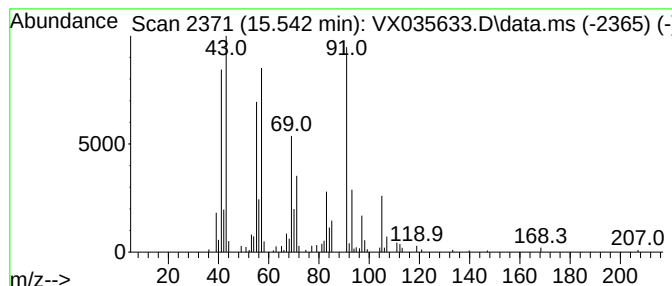

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051223\
Data File : VX035633.D
Acq On : 12 May 2023 13:21
Operator : JC/MD
Sample : 02755-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
A5560










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Tetradecane, 1-chloro- Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
16.468	5.10 ug/l	91444	1,4-Dichlorobenzene-d4	12.024

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Dodecane, 1-chloro-	204	C12H25Cl	000112-52-7	80
2			Tetradecane, 1-chloro-	232	C14H29Cl	002425-54-9	72
3			Octadecane, 1-(ethenyl)-	296	C20H40	000930-02-9	58
4			Trichloroacetic acid, hexadecyl ...	386	C18H33Cl3O2	074339-54-1	46
5			1-Chloroundecane	190	C11H23Cl	002473-03-2	38

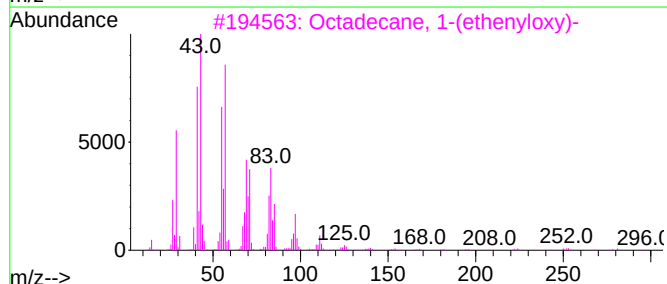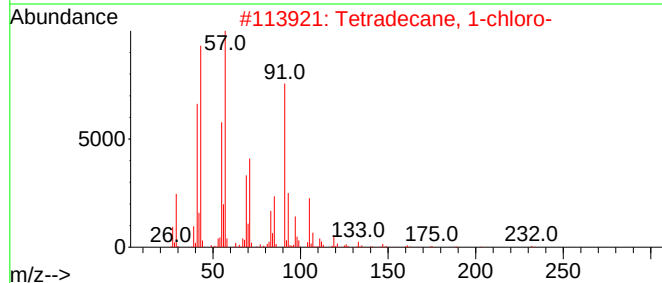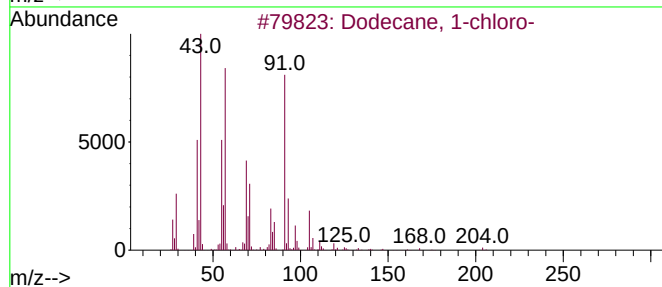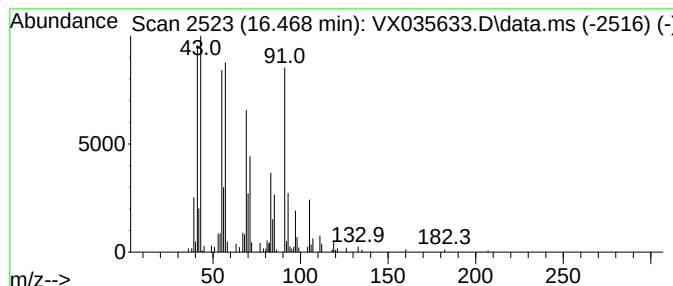

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051223\
Data File : VX035633.D
Acq On : 12 May 2023 13:21
Operator : JC/MD
Sample : 02755-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
A5560

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Dodecane, 1-chl...	15.542	6.0	ug/l	107351	4	12.024	897345	50.0
Tetradecane, 1-...	16.468	5.1	ug/l	91444	4	12.024	897345	50.0