

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051223\
Data File : VX035637.D
Acq On : 12 May 2023 14:54
Operator : JC/MD
Sample : 02777-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-5

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051123W.M

Title : SW846 8260

Signal : TIC: VX035637.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.385	692	705	721	rBV2	124215	361848	32.57%	5.813%
2	5.550	721	732	748	rVB	208536	599978	54.01%	9.639%
3	5.958	785	799	813	rBV	153760	403957	36.36%	6.490%
4	6.763	920	931	942	rBV	344398	832836	74.97%	13.380%
5	8.647	1233	1240	1249	rBV	710305	1110872	100.00%	17.847%
6	10.055	1465	1471	1484	rBV	718280	990096	89.13%	15.907%
7	11.079	1634	1639	1648	rBV	617802	776574	69.91%	12.476%
8	12.018	1788	1793	1801	rBV	714437	918480	82.68%	14.756%
9	15.182	2302	2312	2321	rBV9	7023	25496	2.30%	0.410%
10	15.542	2365	2371	2380	rBV2	70063	107854	9.71%	1.733%
11	16.469	2516	2523	2538	rBV2	48989	96458	8.68%	1.550%


Sum of corrected areas: 6224449

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051223\
Data File : VX035637.D
Acq On : 12 May 2023 14:54
Operator : JC/MD
Sample : 02777-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

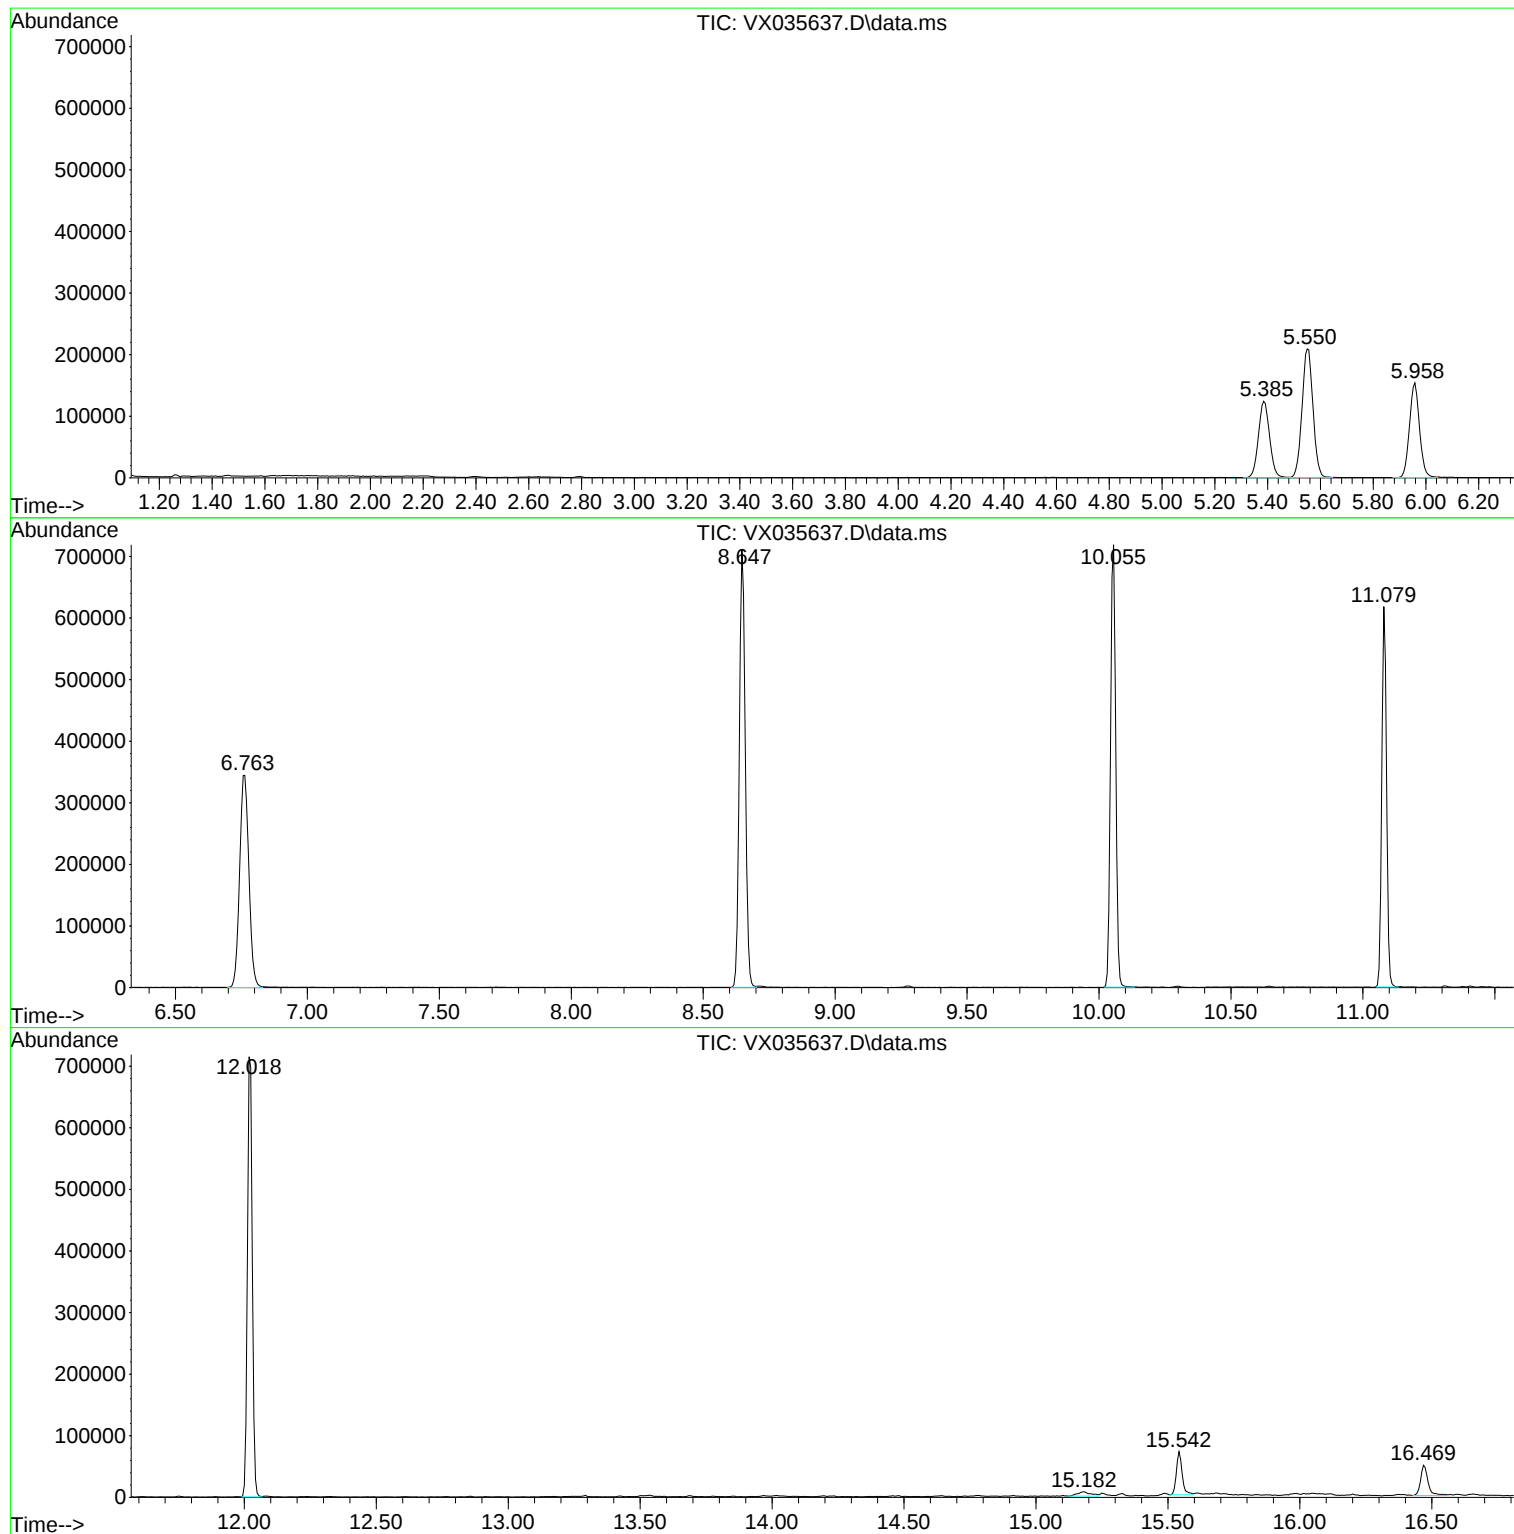

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051223\
Data File : VX035637.D
Acq On : 12 May 2023 14:54
Operator : JC/MD
Sample : 02777-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-5










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Dodecane, 1-chloro- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
15.542	5.87 ug/l	107854	1,4-Dichlorobenzene-d4	12.024

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Dodecane, 1-chloro-	204	C12H25Cl	000112-52-7	83
2			1-Chloroundecane	190	C11H23Cl	002473-03-2	80
3			1-Eicosanol	298	C20H42O	000629-96-9	47
4			Octane, 1-chloro-	148	C8H17Cl	000111-85-3	43
5			Nonane, 1-chloro-	162	C9H19Cl	002473-01-0	43

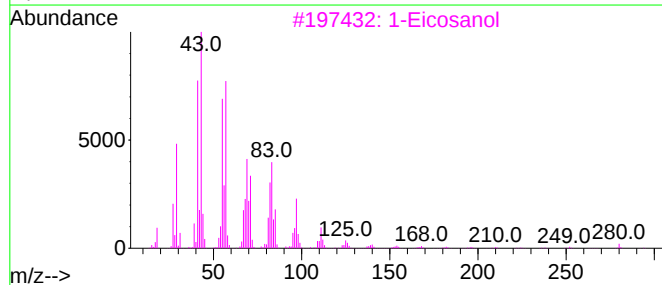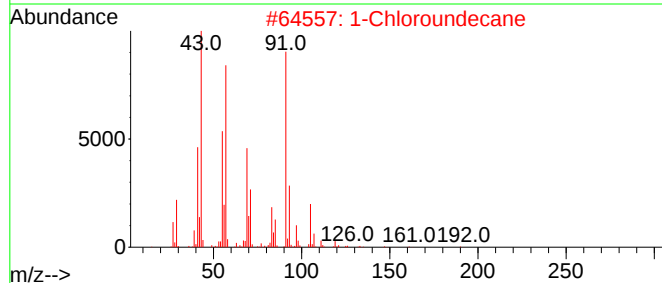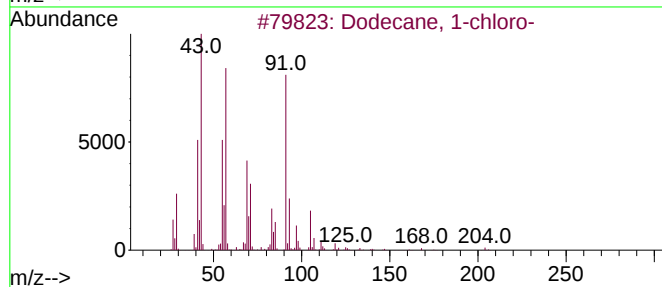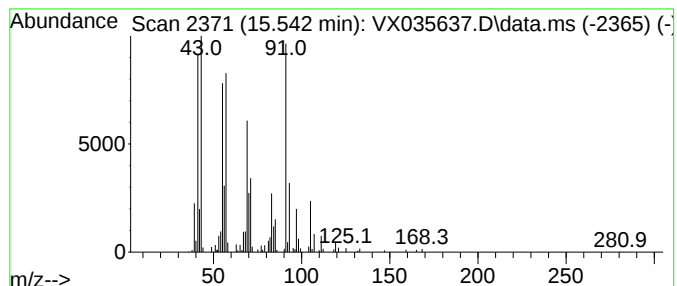

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051223\
Data File : VX035637.D
Acq On : 12 May 2023 14:54
Operator : JC/MD
Sample : 02777-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-5










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Tetradecane, 1-chloro- Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
16.469	5.25 ug/l	96458	1,4-Dichlorobenzene-d4	12.024

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Dodecane, 1-chloro-	204	C12H25Cl	000112-52-7	80
2			Tetradecane, 1-chloro-	232	C14H29Cl	002425-54-9	72
3			1-(2-Propen-1-yloxy)dodecane	226	C15H30O	006145-80-8	52
4			Decane, 1-(ethenyloxy)-	184	C12H24O	000765-05-9	49
5			Silane, trichlorodocosyl-	442	C22H45Cl3Si	007325-84-0	46

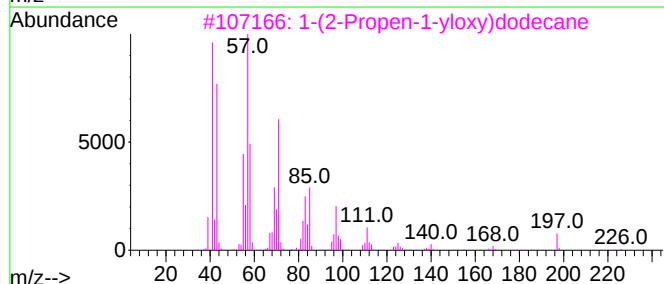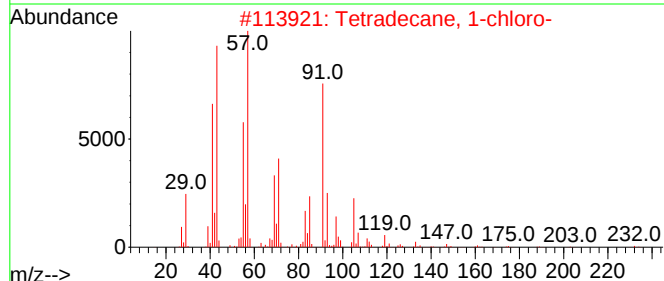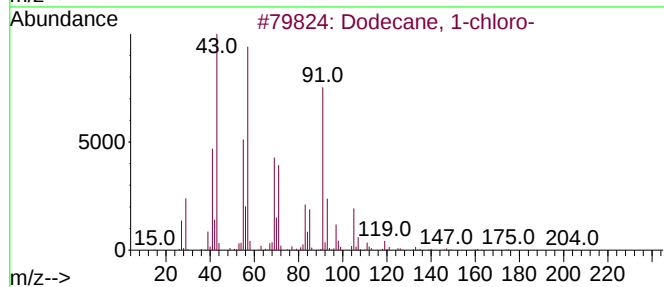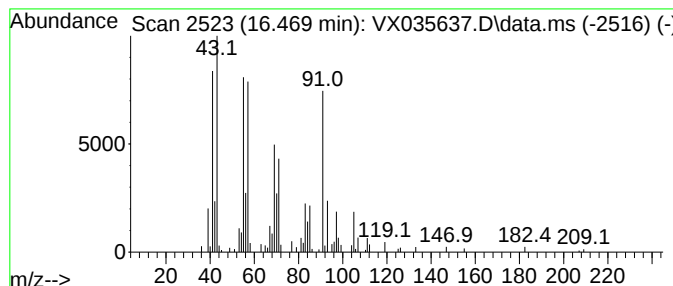

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051223\
Data File : VX035637.D
Acq On : 12 May 2023 14:54
Operator : JC/MD
Sample : 02777-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Dodecane, 1-chl...	15.542	5.9	ug/l	107854	4	12.024	918480	50.0
Tetradecane, 1-...	16.469	5.3	ug/l	96458	4	12.024	918480	50.0