

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051223\
Data File : VX035638.D
Acq On : 12 May 2023 15:18
Operator : JC/MD
Sample : 02777-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-4

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051123W.M

Title : SW846 8260

Signal : TIC: VX035638.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.385	692	705	719	rBV	123307	360788	32.84%	5.958%
2	5.550	721	732	746	rVB	213070	601710	54.78%	9.936%
3	5.958	788	799	812	rBV	147620	397078	36.15%	6.557%
4	6.763	920	931	946	rBV	350713	832034	75.74%	13.739%
5	8.647	1233	1240	1249	rBV	704088	1098480	100.00%	18.139%
6	10.055	1465	1471	1481	rBV	716541	968537	88.17%	15.993%
7	11.079	1634	1639	1649	rBV	590021	740372	67.40%	12.226%
8	12.018	1788	1793	1808	rVB	659915	848134	77.21%	14.005%
9	15.176	2301	2311	2316	rBV9	6762	19330	1.76%	0.319%
10	15.542	2365	2371	2380	rBV	67437	105744	9.63%	1.746%
11	16.468	2517	2523	2534	rBV2	46903	83622	7.61%	1.381%




Sum of corrected areas: 6055829

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051223\
Data File : VX035638.D
Acq On : 12 May 2023 15:18
Operator : JC/MD
Sample : 02777-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

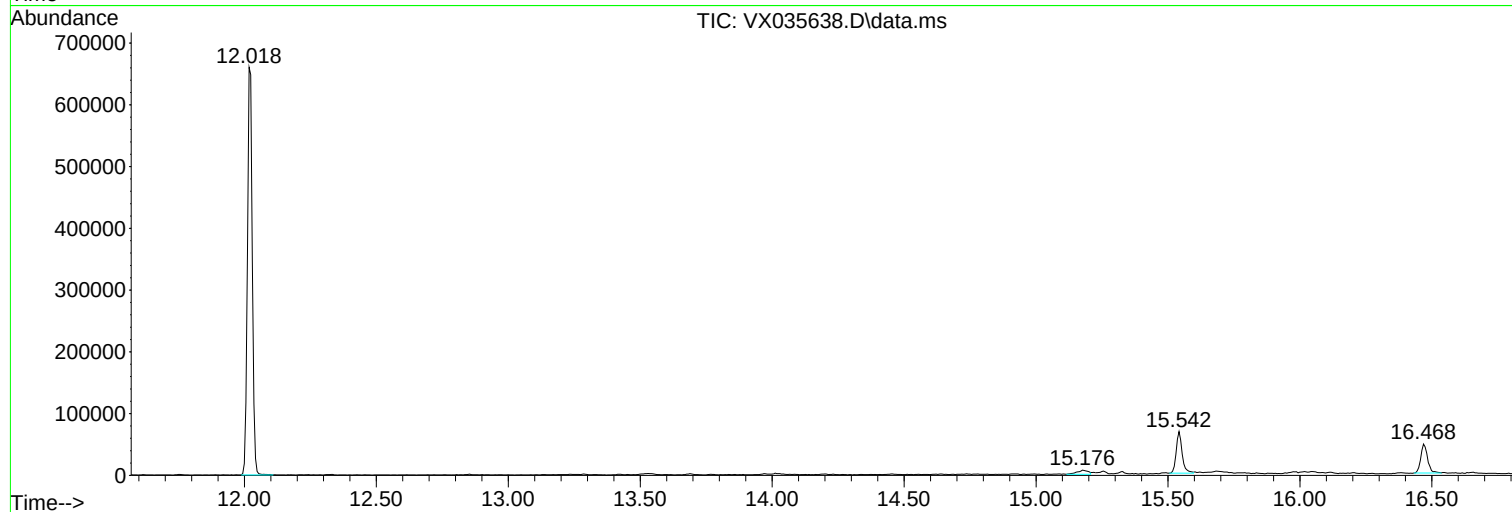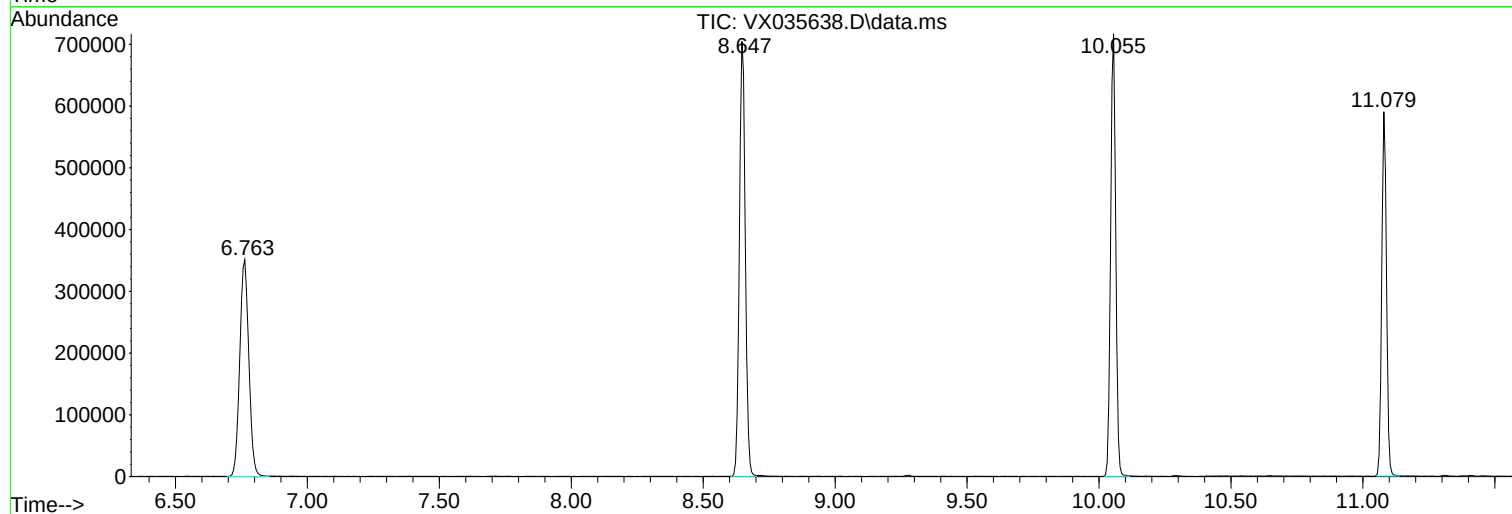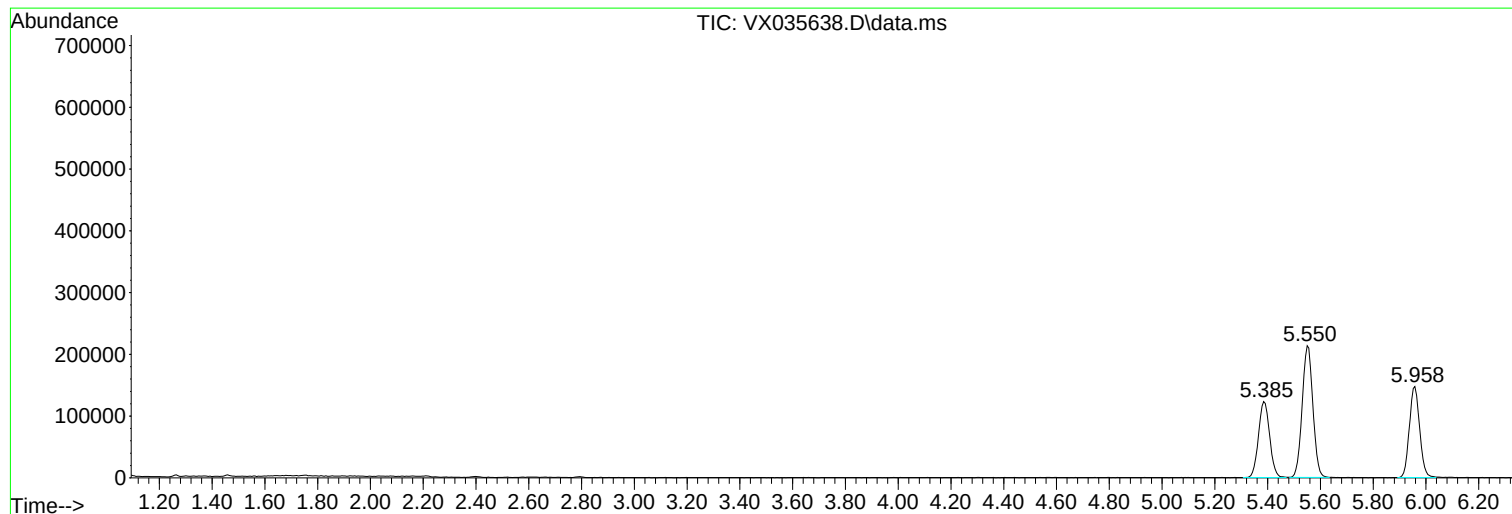

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051223\
Data File : VX035638.D
Acq On : 12 May 2023 15:18
Operator : JC/MD
Sample : 02777-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-4










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Dodecane, 1-chloro- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
15.542	6.23 ug/l	105744	1,4-Dichlorobenzene-d4	12.024

Hit#	of 5	Tentative ID	MW	MolForm	CAS#	Qual
1		Dodecane, 1-chloro-	204	C12H25Cl	000112-52-7	91
2		1-Chloroundecane	190	C11H23Cl	002473-03-2	90
3		Decane, 1-chloro-	176	C10H21Cl	001002-69-3	64
4		Silane, trichlorodocosyl-	442	C22H45Cl3Si	007325-84-0	45
5		Cyclododecane	168	C12H24	000294-62-2	38

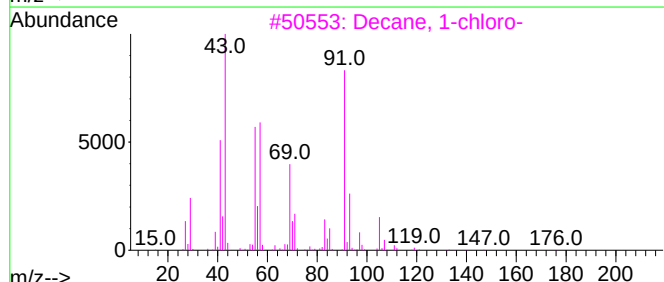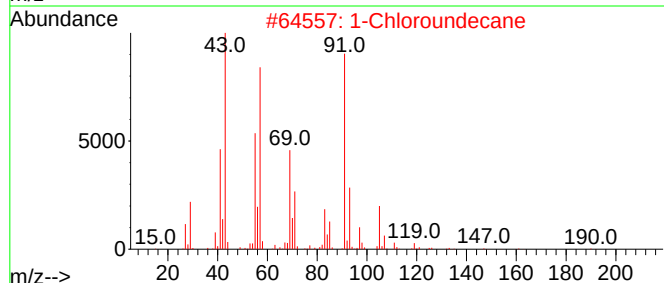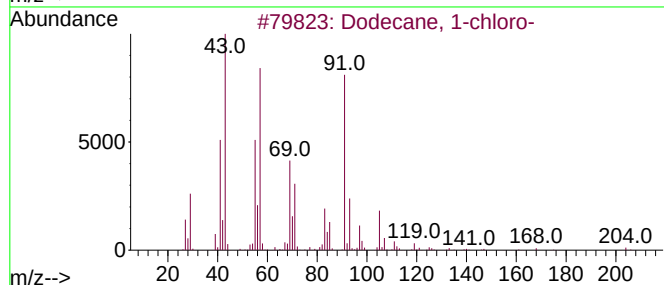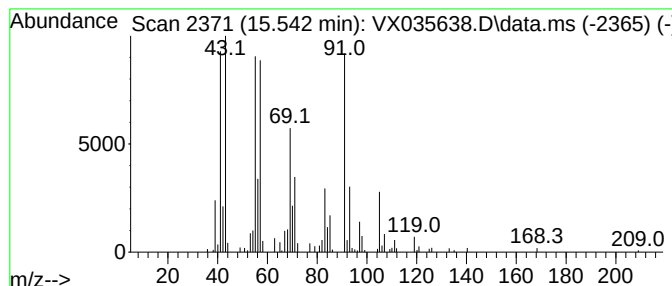

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051223\
Data File : VX035638.D
Acq On : 12 May 2023 15:18
Operator : JC/MD
Sample : 02777-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Decane, 1-chl...	15.542	6.2	ug/l	105744	4	12.024	848134	50.0