

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051223\
Data File : VX035639.D
Acq On : 12 May 2023 15:41
Operator : JC/MD
Sample : 02777-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SAMPLE-MANAG

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051123W.M

Title : SW846 8260

Signal : TIC: VX035639.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.385	692	705	720	rBV	134739	392598	32.47%	5.812%
2	5.550	720	732	748	rVB	231148	656587	54.31%	9.720%
3	5.958	788	799	815	rBV	158440	430776	35.63%	6.377%
4	6.763	920	931	945	rBV	377676	905328	74.88%	13.402%
5	8.647	1233	1240	1249	rBV	789519	1209069	100.00%	17.898%
6	10.055	1465	1471	1485	rBV	807550	1090438	90.19%	16.142%
7	11.079	1634	1639	1650	rBV	686809	849336	70.25%	12.573%
8	12.018	1788	1793	1801	rBV	786553	1006056	83.21%	14.893%
9	15.182	2303	2312	2317	rBV10	7781	20528	1.70%	0.304%
10	15.542	2364	2371	2380	rBV	69065	105472	8.72%	1.561%
11	16.475	2517	2524	2537	rBV2	44984	89079	7.37%	1.319%




Sum of corrected areas: 6755267

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051223\
Data File : VX035639.D
Acq On : 12 May 2023 15:41
Operator : JC/MD
Sample : 02777-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SAMPLE-MANAG

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

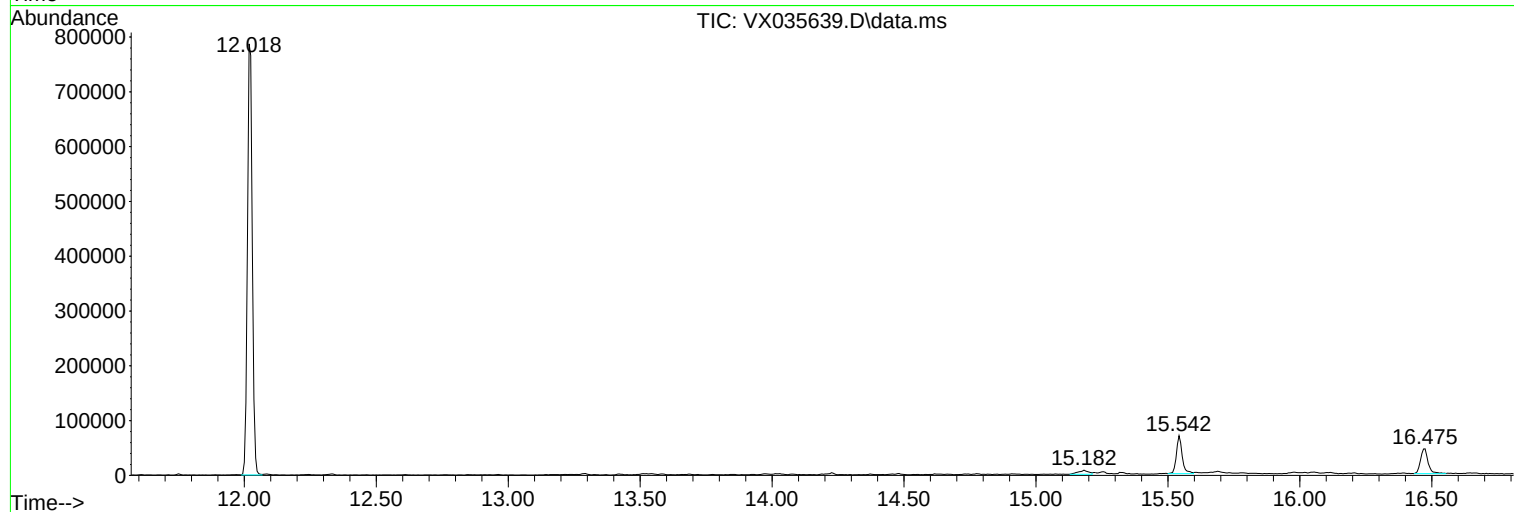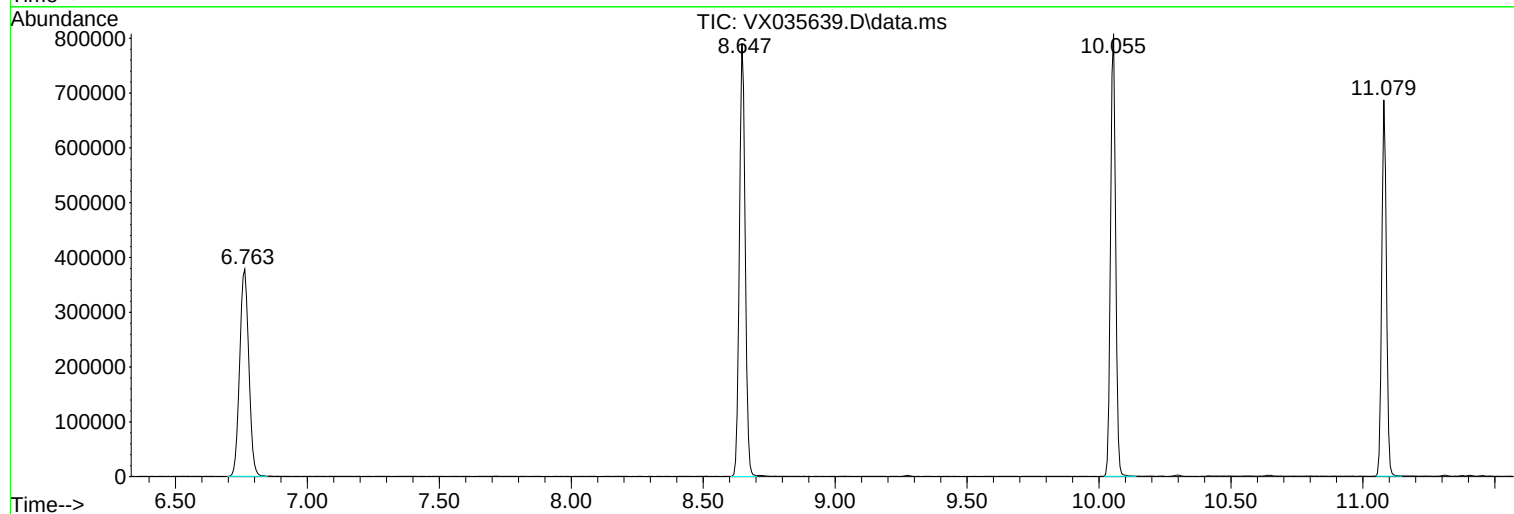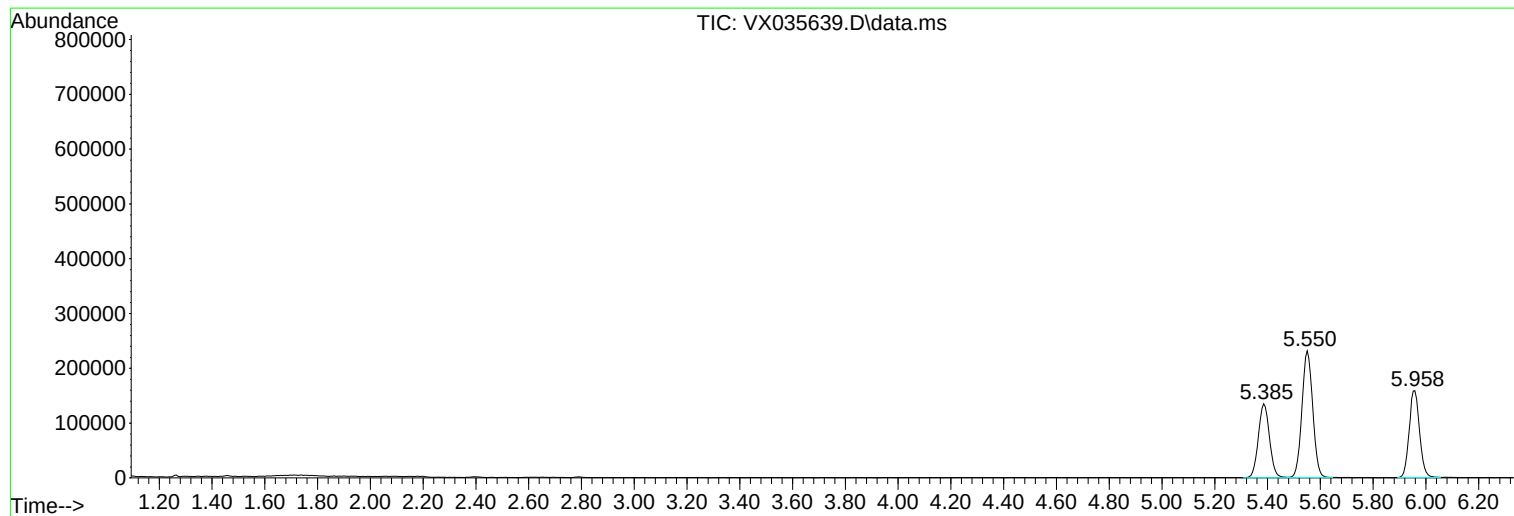

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051223\
Data File : VX035639.D
Acq On : 12 May 2023 15:41
Operator : JC/MD
Sample : 02777-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SAMPLE-MANAG










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Dodecane, 1-chloro- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
15.542	5.24 ug/l	105472	1,4-Dichlorobenzene-d4	12.024

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Dodecane, 1-chloro-	204	C12H25Cl	000112-52-7	90
2			1-Chloroundecane	190	C11H23Cl	002473-03-2	90
3			Oxalic acid, allyl hexadecyl ester	354	C21H38O4	1000309-24-4	46
4			Oxalic acid, allyl dodecyl ester	298	C17H30O4	1000309-24-0	46
5			Silane, trichlorodocosyl-	442	C22H45Cl3Si	007325-84-0	46

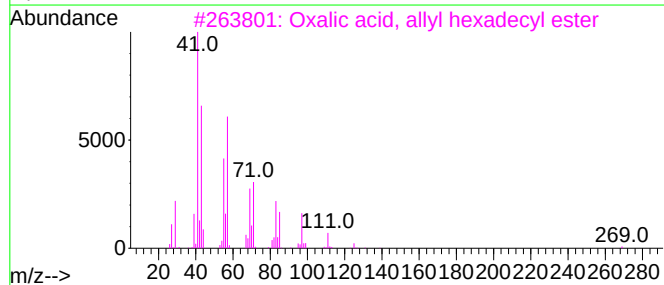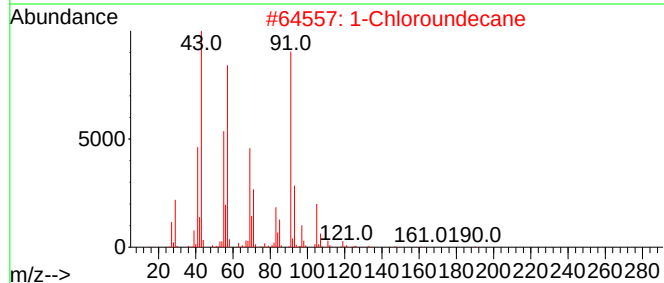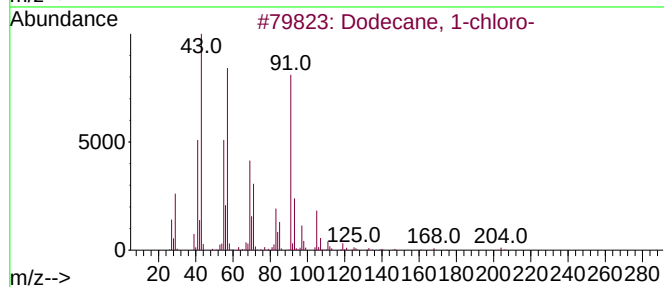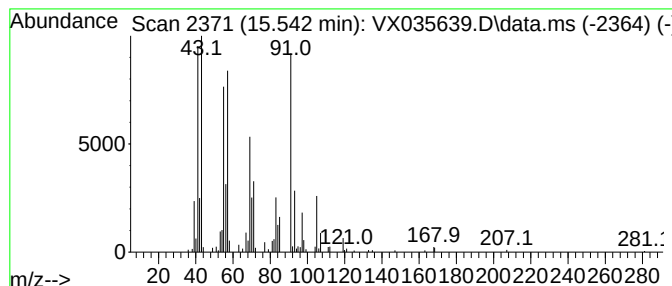

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051223\
Data File : VX035639.D
Acq On : 12 May 2023 15:41
Operator : JC/MD
Sample : 02777-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SAMPLE-MANAG

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Dodecane, 1-chl...	15.542	5.2	ug/l	105472	4	12.024	1006060	50.0