

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051225\
 Data File : VX046147.D
 Acq On : 12 May 2025 18:39
 Operator : JC/MD
 Sample : Q2004-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 R0202

Quant Time: May 13 03:22:40 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X050525W.M
 Quant Title : SW846 8260
 QLast Update : Tue May 06 07:12:22 2025
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.544	168	70343	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	140056	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.049	117	129585	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	54287	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	71472	54.500	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	109.000%
35) Dibromofluoromethane	5.385	113	52448	52.003	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	104.000%
50) Toluene-d8	8.647	98	177698	50.906	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	101.820%
62) 4-Bromofluorobenzene	11.079	95	64667	48.295	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	=	96.600%
Target Compounds						
					Qvalue	
16) Acetone	2.380	43	19702	37.469	ug/l	97
18) Methyl Acetate	2.709	43	1920	1.574	ug/l	93
20) Methylene Chloride	2.782	84	3356	3.331	ug/l	95
43) Isopropyl Acetate	6.355	43	3558	1.393	ug/l #	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051225\
Data File : VX046147.D
Acq On : 12 May 2025 18:39
Operator : JC/MD
Sample : Q2004-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
R0202


Quant Time: May 13 03:22:40 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X050525W.M
Quant Title : SW846 8260
QLast Update : Tue May 06 07:12:22 2025
Response via : Initial Calibration

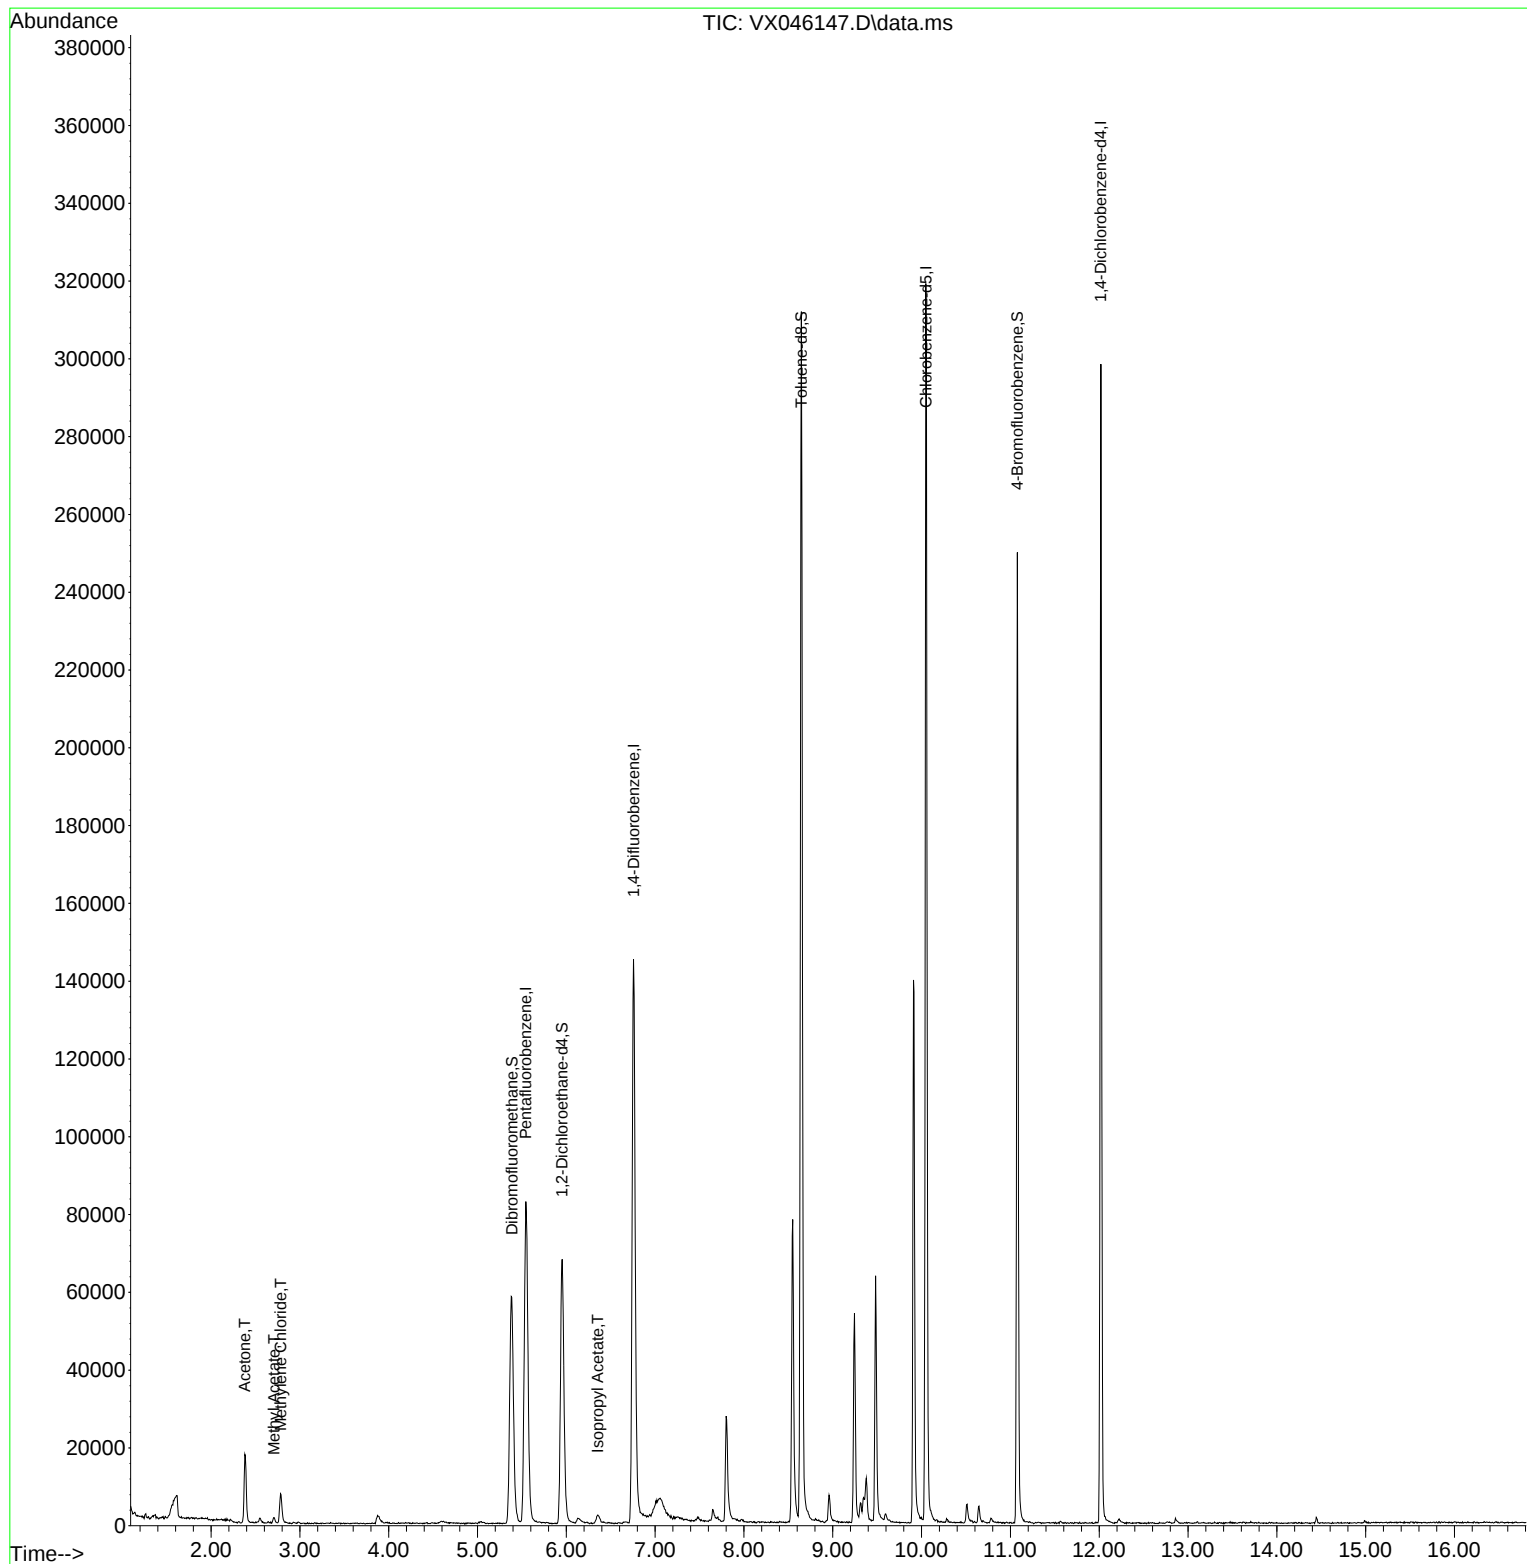



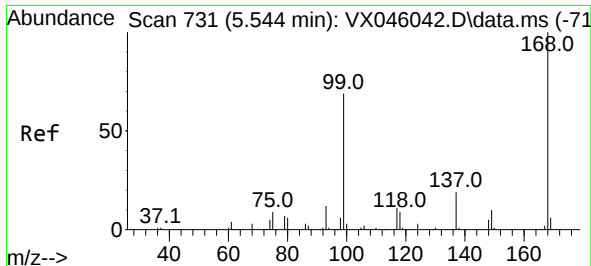


#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.544 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX046147.D
Acq: 12 May 2025 18:39

Instrument :
MSVOA_X
ClientSampleId :
R0202







Tgt Ion:168 Resp: 70343
Ion Ratio Lower Upper
168 100
99 74.3 54.9 82.3

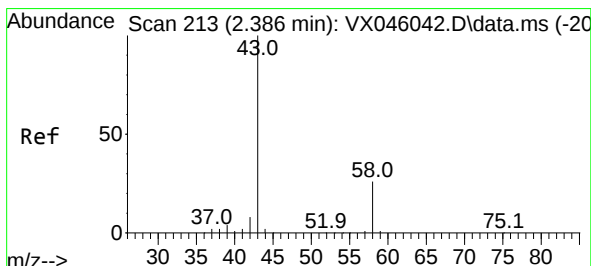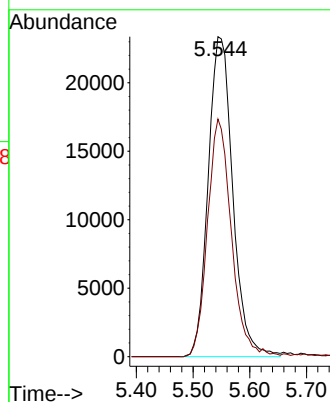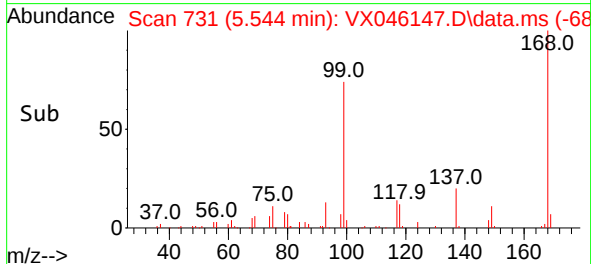

#16
Acetone
Concen: 37.469 ug/l
RT: 2.380 min Scan# 212
Delta R.T. -0.006 min
Lab File: VX046147.D
Acq: 12 May 2025 18:39

Tgt Ion: 43 Resp: 19702
Ion Ratio Lower Upper
43 100
58 24.8 21.2 31.8


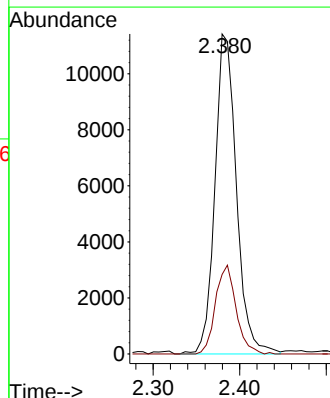

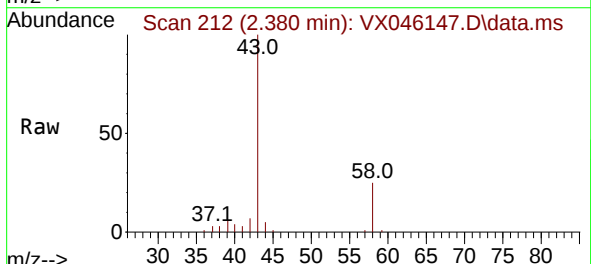




#18
Methyl Acetate
Concen: 1.574 ug/l
RT: 2.709 min Scan# 20
Delta R.T. 0.006 min
Lab File: VX046147.D
Acq: 12 May 2025 18:39




Instrument :
MSVOA_X
ClientSampleId :
R0202


Tgt Ion: 43 Resp: 1920
Ion Ratio Lower Upper
43 100
74 17.7 16.7 25.1

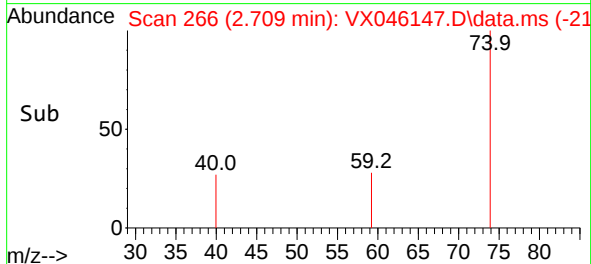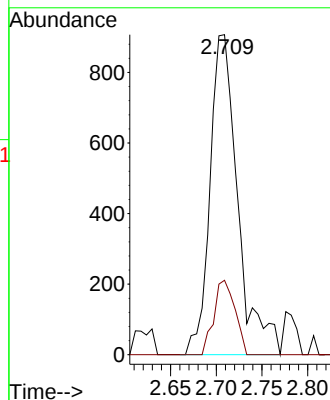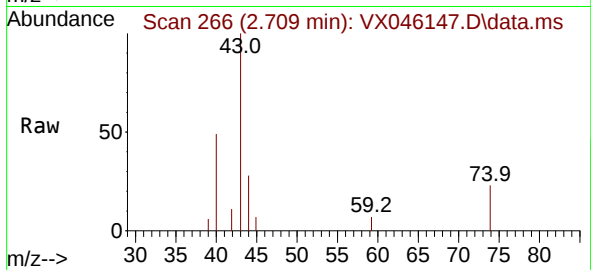

#20
Methylene Chloride
Concen: 3.331 ug/l
RT: 2.782 min Scan# 278
Delta R.T. 0.000 min
Lab File: VX046147.D
Acq: 12 May 2025 18:39

Tgt Ion: 84 Resp: 3356
Ion Ratio Lower Upper
84 100
49 132.9 113.9 170.9
51 38.9 33.5 50.3
86 66.5 53.8 80.8

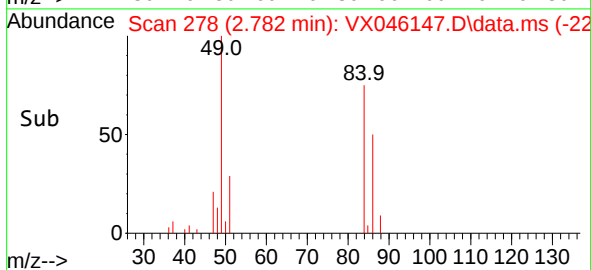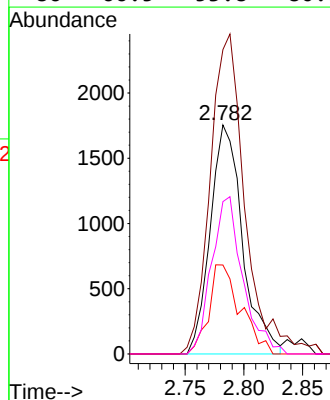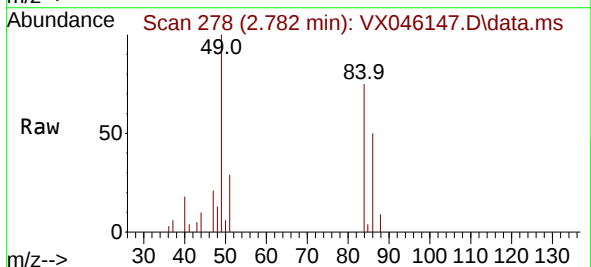

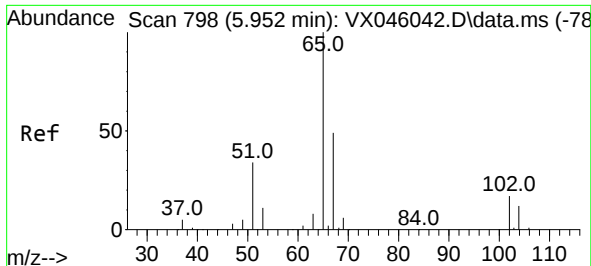

#33

1,2-Dichloroethane-d4

Concen: 54.500 ug/l

RT: 5.952 min Scan# 798

Delta R.T. 0.000 min

Lab File: VX046147.D

Acq: 12 May 2025 18:39

Instrument :

MSVOA_X

ClientSampleId :





R0202

Tgt Ion: 65 Resp: 71472

Ion Ratio Lower Upper

65 100

67 48.9 0.0 99.0

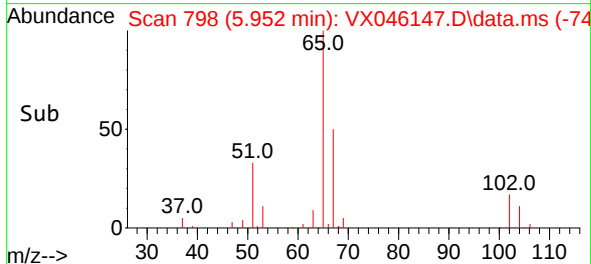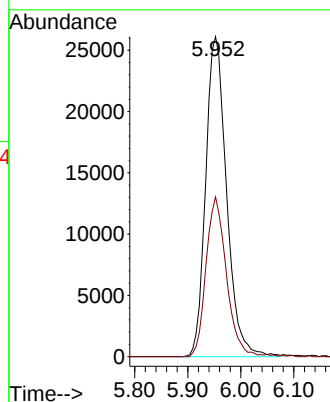

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.757 min Scan# 930

Delta R.T. 0.000 min

Lab File: VX046147.D

Acq: 12 May 2025 18:39




Tgt Ion: 114 Resp: 140056


Ion Ratio Lower Upper

114 100

63 23.2 0.0 49.2

88 16.9 0.0 33.6


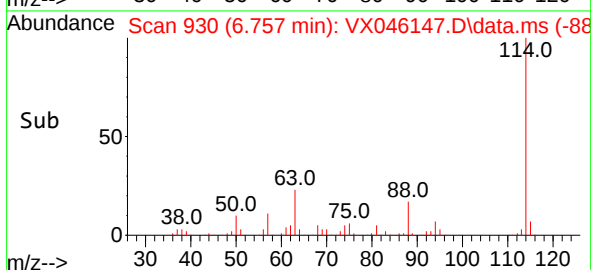
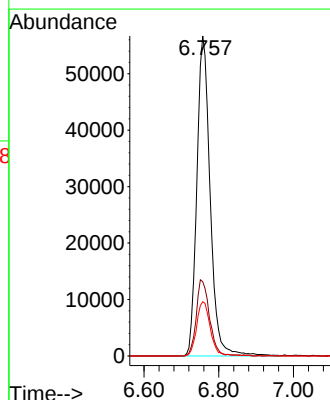
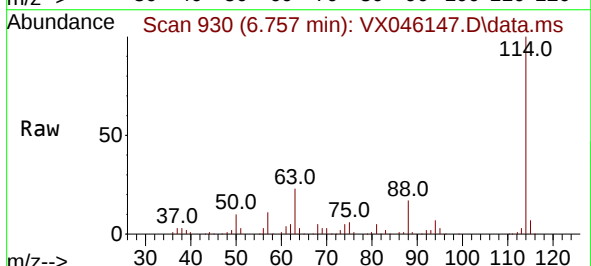


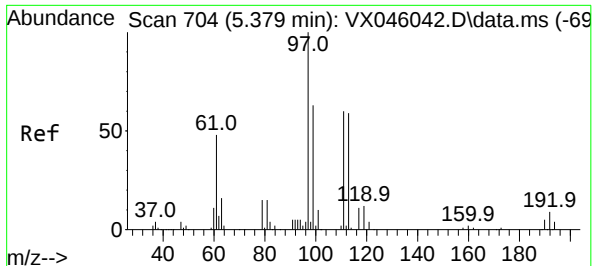

#35
 Dibromofluoromethane
 Concen: 52.003 ug/l
 RT: 5.385 min Scan# 704
 Delta R.T. 0.006 min
 Lab File: VX046147.D
 Acq: 12 May 2025 18:39




Instrument :
 MSVOA_X
 ClientSampleId :
 R0202


Tgt Ion:113 Resp: 52448
 Ion Ratio Lower Upper
 113 100
 111 101.0 83.1 124.7
 192 16.4 13.3 19.9

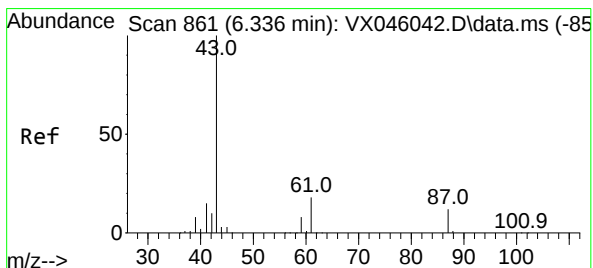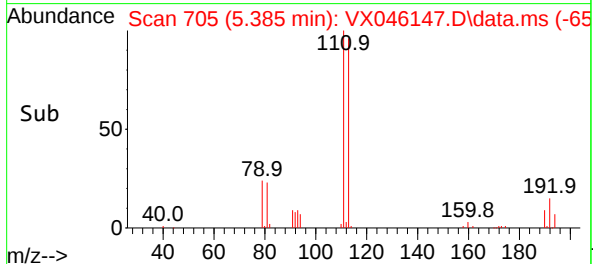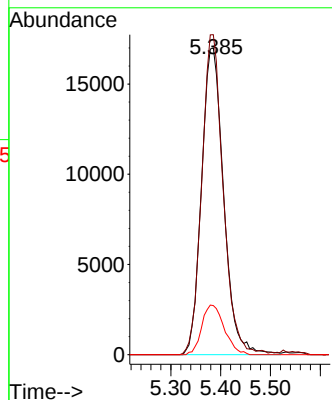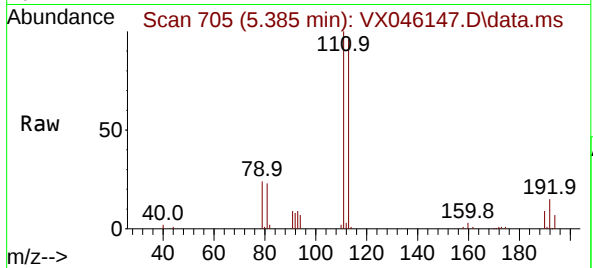

#43
 Isopropyl Acetate
 Concen: 1.393 ug/l
 RT: 6.355 min Scan# 864
 Delta R.T. 0.018 min
 Lab File: VX046147.D
 Acq: 12 May 2025 18:39

Tgt Ion: 43 Resp: 3558
 Ion Ratio Lower Upper
 43 100
 61 14.4 14.3 21.5
 87 7.7 9.5 14.3#


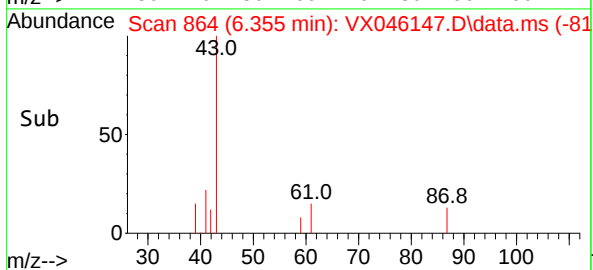
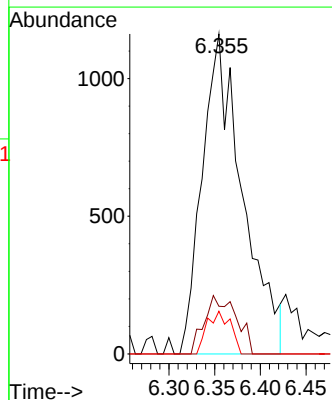
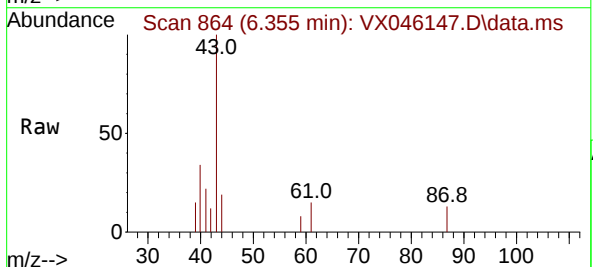




#50
Toluene-d8
Concen: 50.906 ug/l
RT: 8.647 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX046147.D
Acq: 12 May 2025 18:39




Instrument :
MSVOA_X
ClientSampleId :
R0202


Tgt Ion: 98 Resp: 177698
Ion Ratio Lower Upper
98 100
100 65.6 53.5 80.3

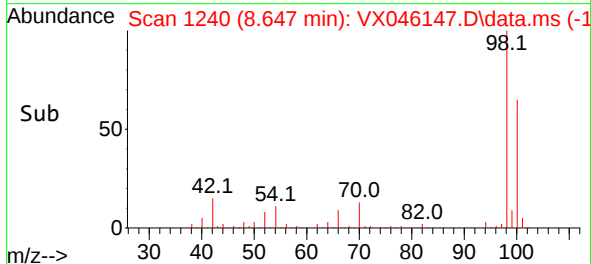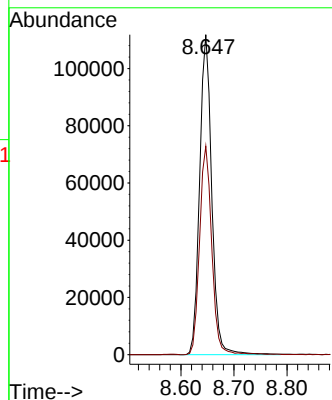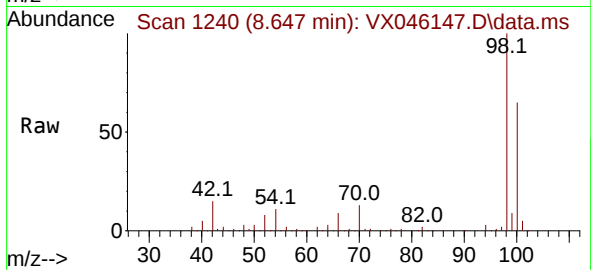

#62
4-Bromofluorobenzene
Concen: 48.295 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX046147.D
Acq: 12 May 2025 18:39

Tgt Ion: 95 Resp: 64667
Ion Ratio Lower Upper
95 100
174 67.6 0.0 135.8
176 64.1 0.0 131.4


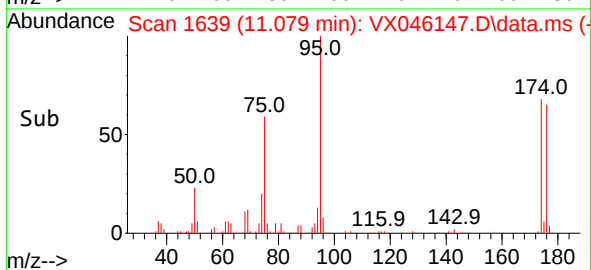
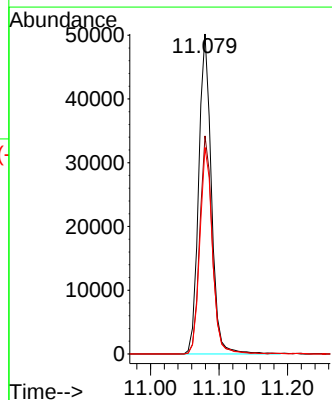
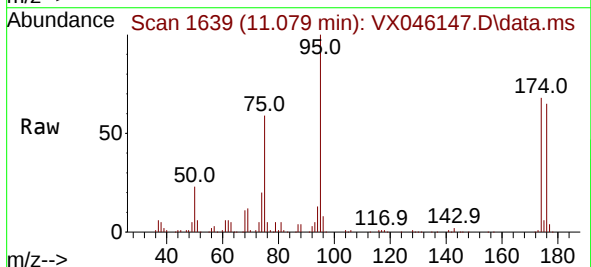




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.049 min Scan# 1470
Delta R.T. 0.000 min
Lab File: VX046147.D
Acq: 12 May 2025 18:39

Instrument :
MSVOA_X
ClientSampleId :
R0202

Tgt Ion:117 Resp: 129585
Ion Ratio Lower Upper
117 100
82 62.6 50.6 76.0
119 31.6 25.8 38.6

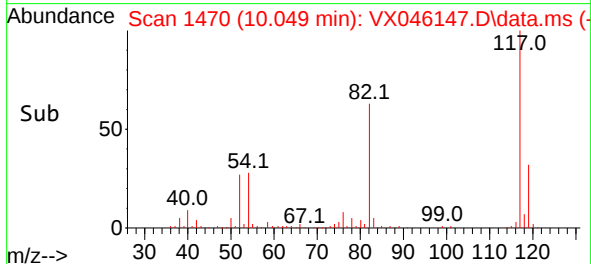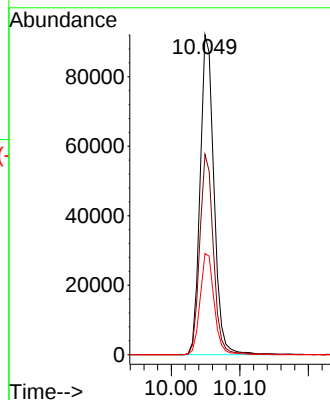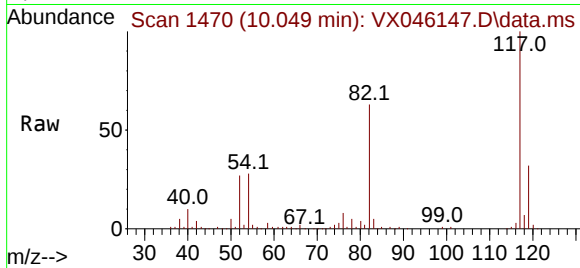

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.018 min Scan# 1793
Delta R.T. 0.000 min
Lab File: VX046147.D
Acq: 12 May 2025 18:39

Tgt Ion:152 Resp: 54287
Ion Ratio Lower Upper
152 100
115 64.0 46.9 140.7
150 153.8 0.0 351.0

