

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX051320\
 Data File : VX016183.D
 Acq On : 13 May 2020 16:36
 Operator : JC/SP
 Sample : L2626-13
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 Z4-TB7-200512

Quant Time: May 14 07:05:26 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X050420W.M
 Quant Title : SW846 8260
 QLast Update : Wed May 06 06:43:32 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.64	168	271100	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.83	114	451357	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.10	117	439692	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.06	152	220756	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.04	65	166670	46.72	ug/l	0.00
Spiked Amount	50.000		Recovery	=	93.44%	
35) Dibromofluoromethane	5.47	113	132312	46.27	ug/l	0.00
Spiked Amount	50.000		Recovery	=	92.54%	
50) Toluene-d8	8.70	98	549475	49.87	ug/l	0.00
Spiked Amount	50.000		Recovery	=	99.74%	
62) 4-Bromofluorobenzene	11.12	95	216575	51.68	ug/l	0.00
Spiked Amount	50.000		Recovery	=	103.36%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX051320\
Data File : VX016183.D
Acq On : 13 May 2020 16:36
Operator : JC/SP
Sample : L2626-13
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
Z4-TB7-200512

Quant Time: May 14 07:05:26 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X050420W.M
Quant Title : SW846 8260
QLast Update : Wed May 06 06:43:32 2020
Response via : Initial Calibration

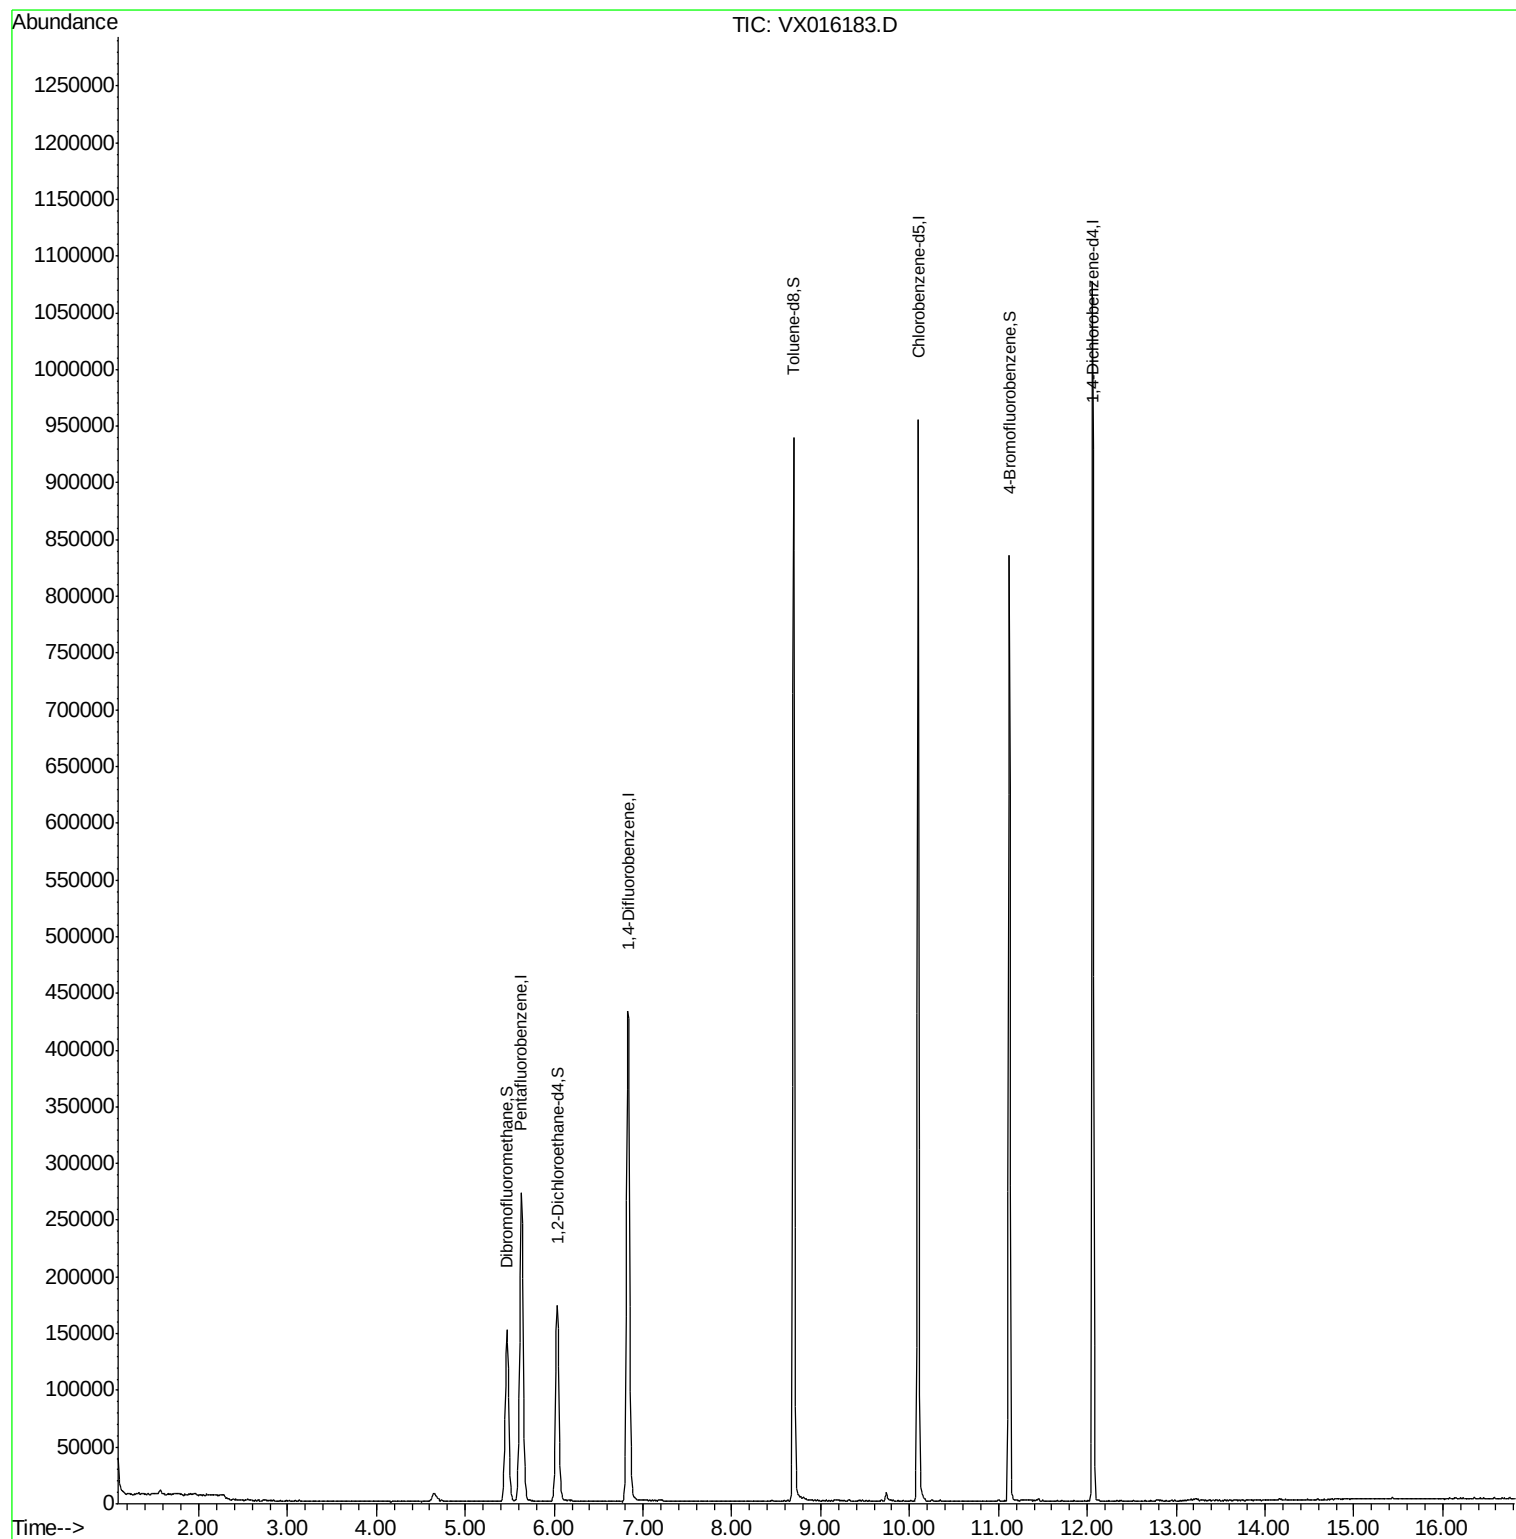

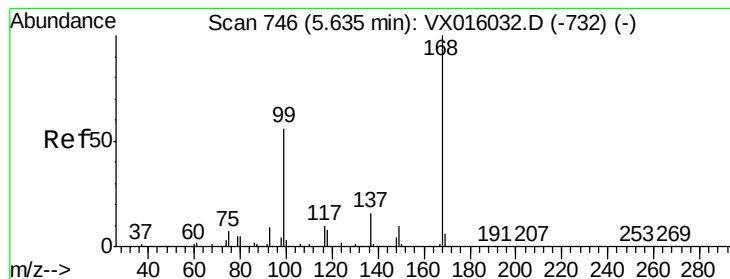

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.64 min Scan# 746

Delta R.T. -0.00 min

Lab File: VX016183.D

Acq: 13 May 2020 16:36

Instrument :

MSVOA_X

ClientSampleId :


Z4-TB7-200512

Tot Ion:168 Resp: 271100

Ion Ratio Lower Upper

168 100

99 54.9 45.0 67.4

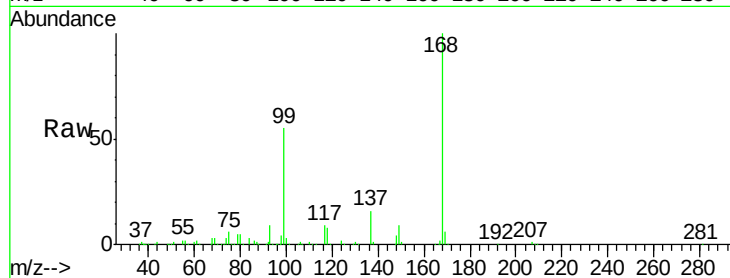

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.64

100000

80000



60000

40000

20000

0

Time-->

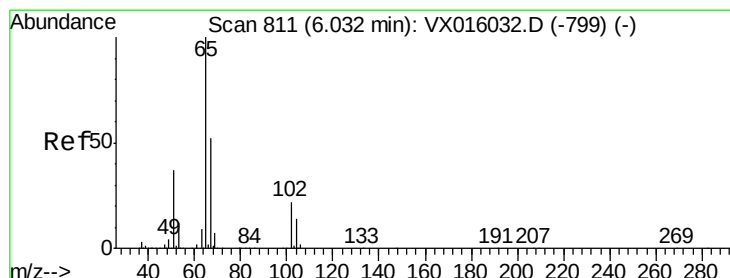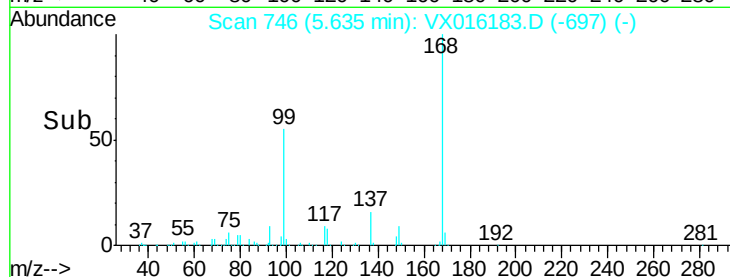

#33

1,2-Dichloroethane-d4

Concen: 46.720 ug/l

RT: 6.04 min Scan# 812

Delta R.T. 0.01 min

Lab File: VX016183.D


Acq: 13 May 2020 16:36

Tgt Ion: 65 Resp: 166670

Ion Ratio Lower Upper

65 100

67 52.3 0.0 104.8

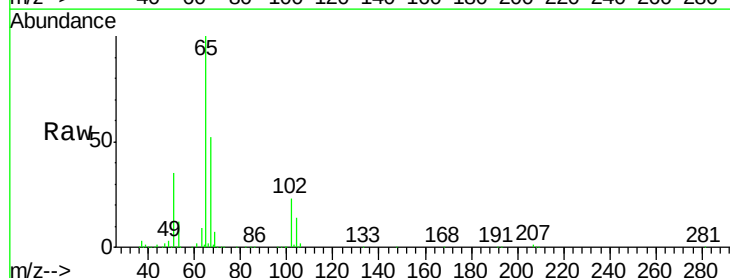

Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

6.04


60000


40000

20000

0

Time-->

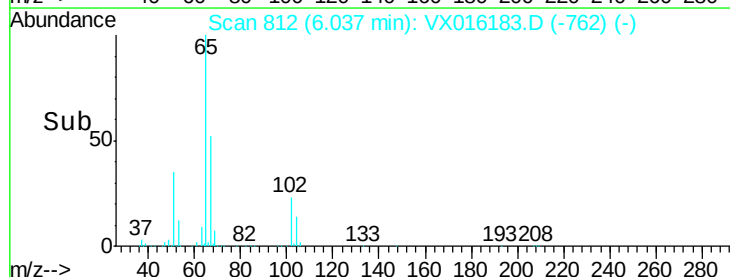

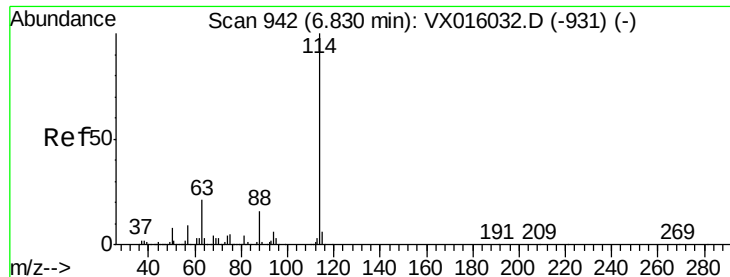

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.83 min Scan# 942

Delta R.T. -0.00 min

Lab File: VX016183.D

Acq: 13 May 2020 16:36

Instrument :

MSVOA_X

ClientSampleId :

Z4-TB7-200512


Tot Ion:114 Resp: 451357

Ion Ratio Lower Upper

114 100

63 20.2 0.0 42.8




88 15.5 0.0 31.4

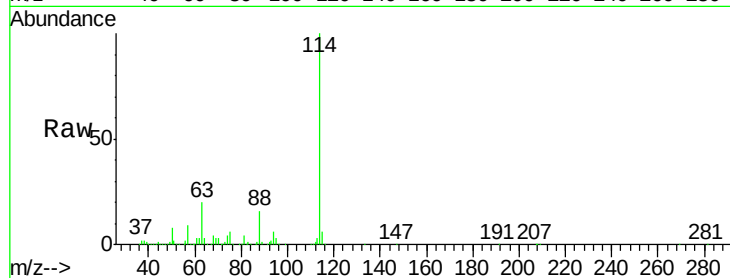

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

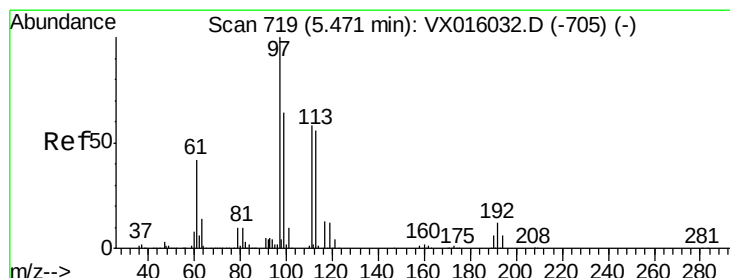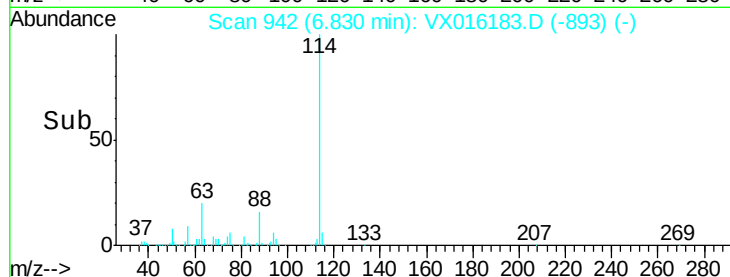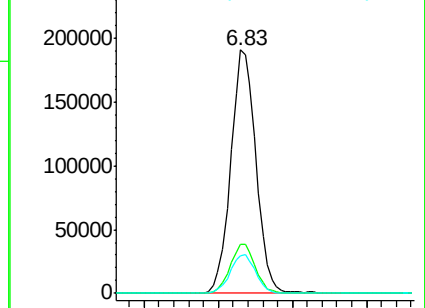

#35

Dibromofluoromethane

Concen: 46.270 ug/l

RT: 5.47 min Scan# 719

Delta R.T. -0.00 min

Lab File: VX016183.D

Acq: 13 May 2020 16:36


Tgt Ion:113 Resp: 132312

Ion Ratio Lower Upper

113 100

111 102.7 81.6 122.4



192 21.7 17.0 25.4

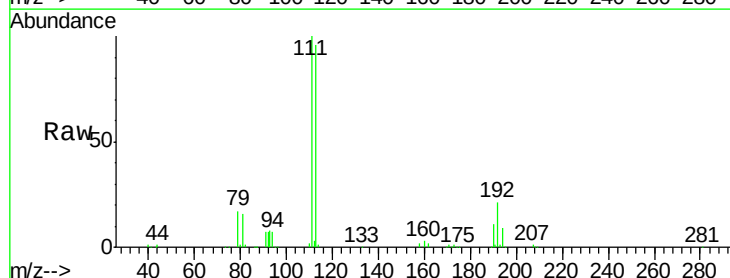


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V



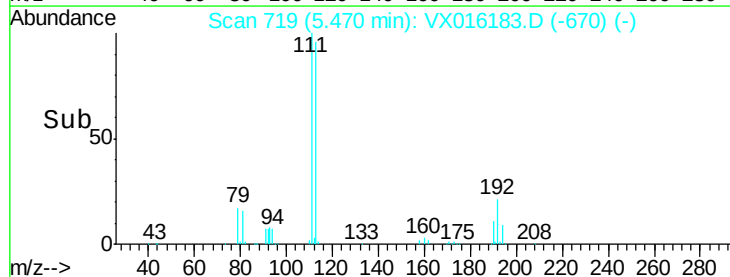
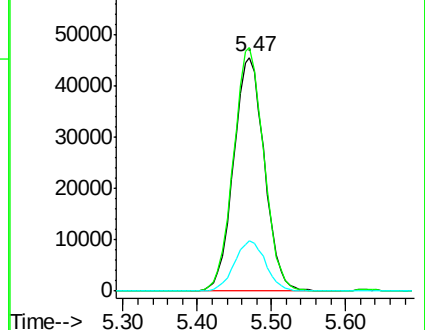


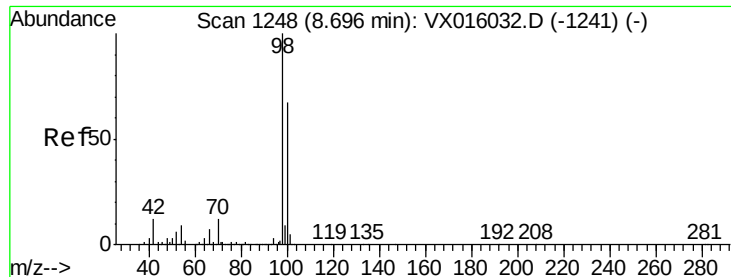

#50
Toluene-d8
Concen: 49.871 ug/l
RT: 8.70 min Scan# 1248
Delta R.T. -0.00 min
Lab File: VX016183.D
Acq: 13 May 2020 16:36




Instrument :
MSVOA_X
ClientSampleId :
Z4-TB7-200512


Tot Ion: 98 Resp: 549475
Ion Ratio Lower Upper
98 100
100 67.2 53.7 80.5

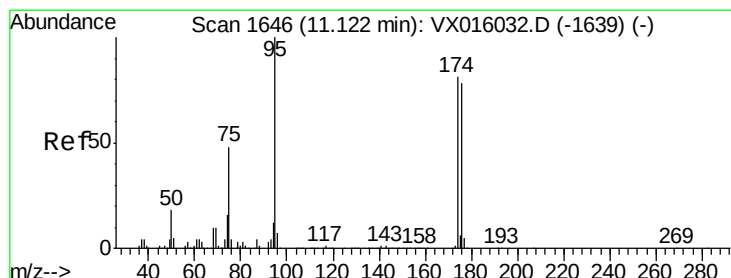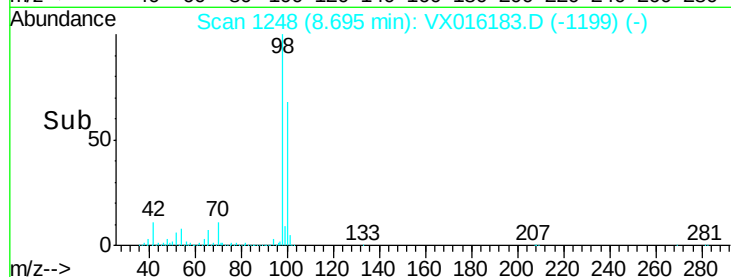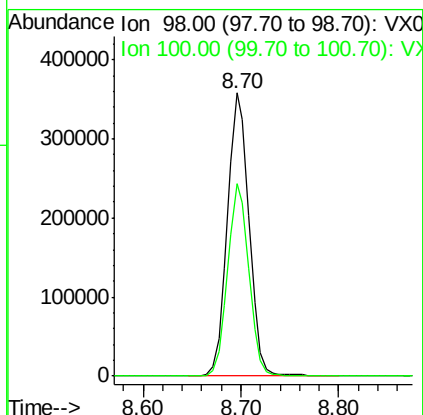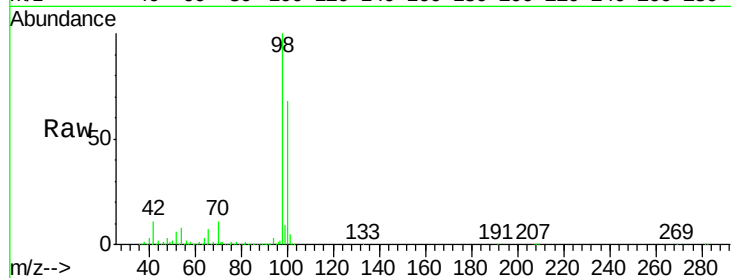

#62
4-Bromofluorobenzene
Concen: 51.680 ug/l
RT: 11.12 min Scan# 1646
Delta R.T. -0.00 min
Lab File: VX016183.D
Acq: 13 May 2020 16:36

Tgt Ion: 95 Resp: 216575
Ion Ratio Lower Upper
95 100
174 81.8 0.0 159.4
176 78.5 0.0 157.6


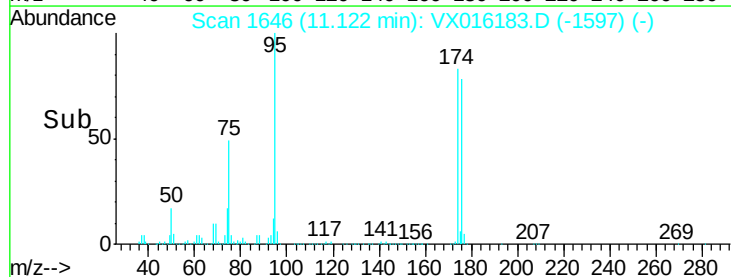
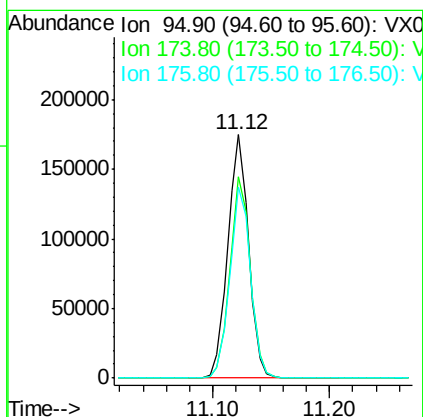
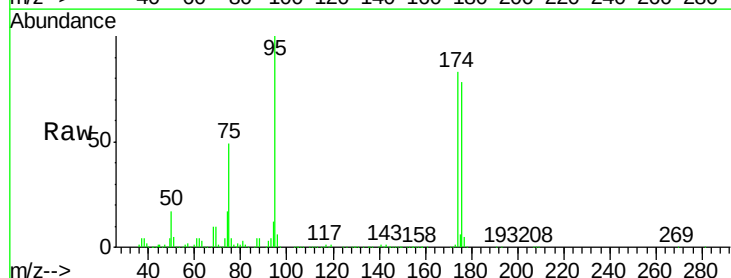


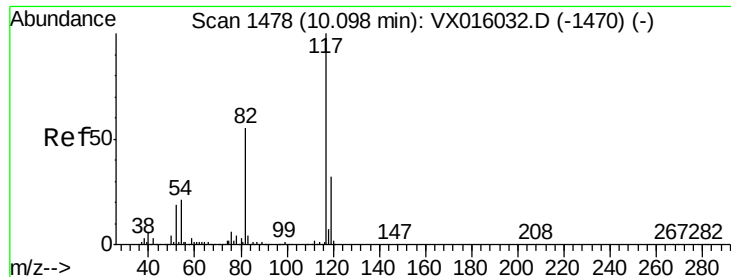

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.10 min Scan# 1478
Delta R.T. -0.00 min
Lab File: VX016183.D
Acq: 13 May 2020 16:36

Instrument :
MSVOA_X
ClientSampleId :
Z4-TB7-200512

Tot Ion:117 Resp: 439692
Ion Ratio Lower Upper
117 100
82 54.2 44.4 66.6
119 32.8 25.5 38.3

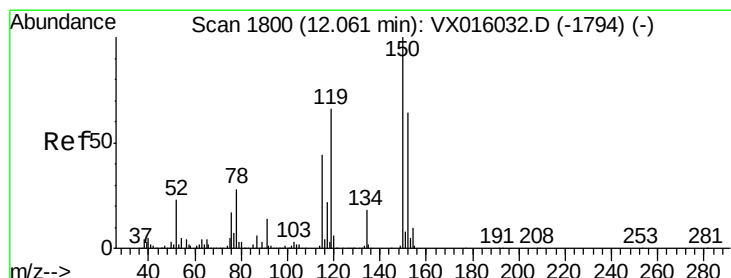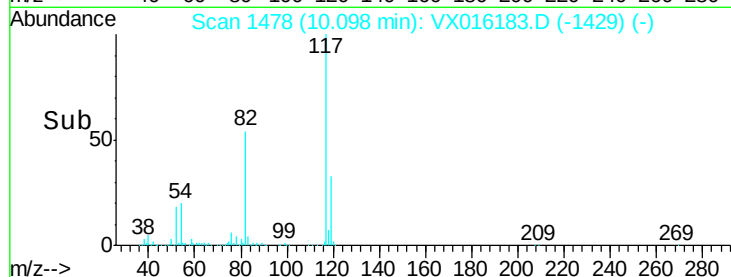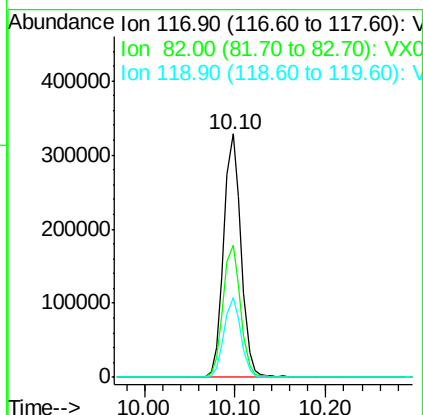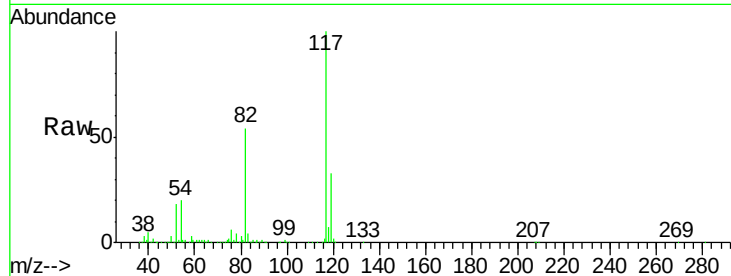

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.06 min Scan# 1800
Delta R.T. -0.00 min
Lab File: VX016183.D
Acq: 13 May 2020 16:36

Tgt Ion:152 Resp: 220756
Ion Ratio Lower Upper
152 100
115 58.2 41.3 124.1
150 157.3 0.0 352.2

