

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX051320\
 Data File : VX016206.D
 Acq On : 14 May 2020 02:24
 Operator : JC/SP
 Sample : L2500-05
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 OK-02-051220

Quant Time: May 14 07:45:23 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X050420W.M
 Quant Title : SW846 8260
 QLast Update : Wed May 06 06:43:32 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.63	168	275809	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.84	114	458803	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.10	117	457925	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.06	152	238493	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.04	65	168126	46.32	ug/l	0.00
Spiked Amount 50.000			Recovery	=	92.64%	
35) Dibromofluoromethane	5.47	113	135489	46.61	ug/l	0.00
Spiked Amount 50.000			Recovery	=	93.22%	
50) Toluene-d8	8.70	98	574545	51.30	ug/l	0.00
Spiked Amount 50.000			Recovery	=	102.60%	
62) 4-Bromofluorobenzene	11.12	95	231639	54.38	ug/l	0.00
Spiked Amount 50.000			Recovery	=	108.76%	
Target Compounds						
16) Acetone	2.42	43	14588	9.008	ug/l	99
20) Methylene Chloride	2.84	84	4714	1.412	ug/l	88
43) Isopropyl Acetate	6.42	43	77493	9.279	ug/l	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX051320\
Data File : VX016206.D
Acq On : 14 May 2020 02:24
Operator : JC/SP
Sample : L2500-05
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
OK-02-051220

Quant Time: May 14 07:45:23 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X050420W.M
Quant Title : SW846 8260
QLast Update : Wed May 06 06:43:32 2020
Response via : Initial Calibration

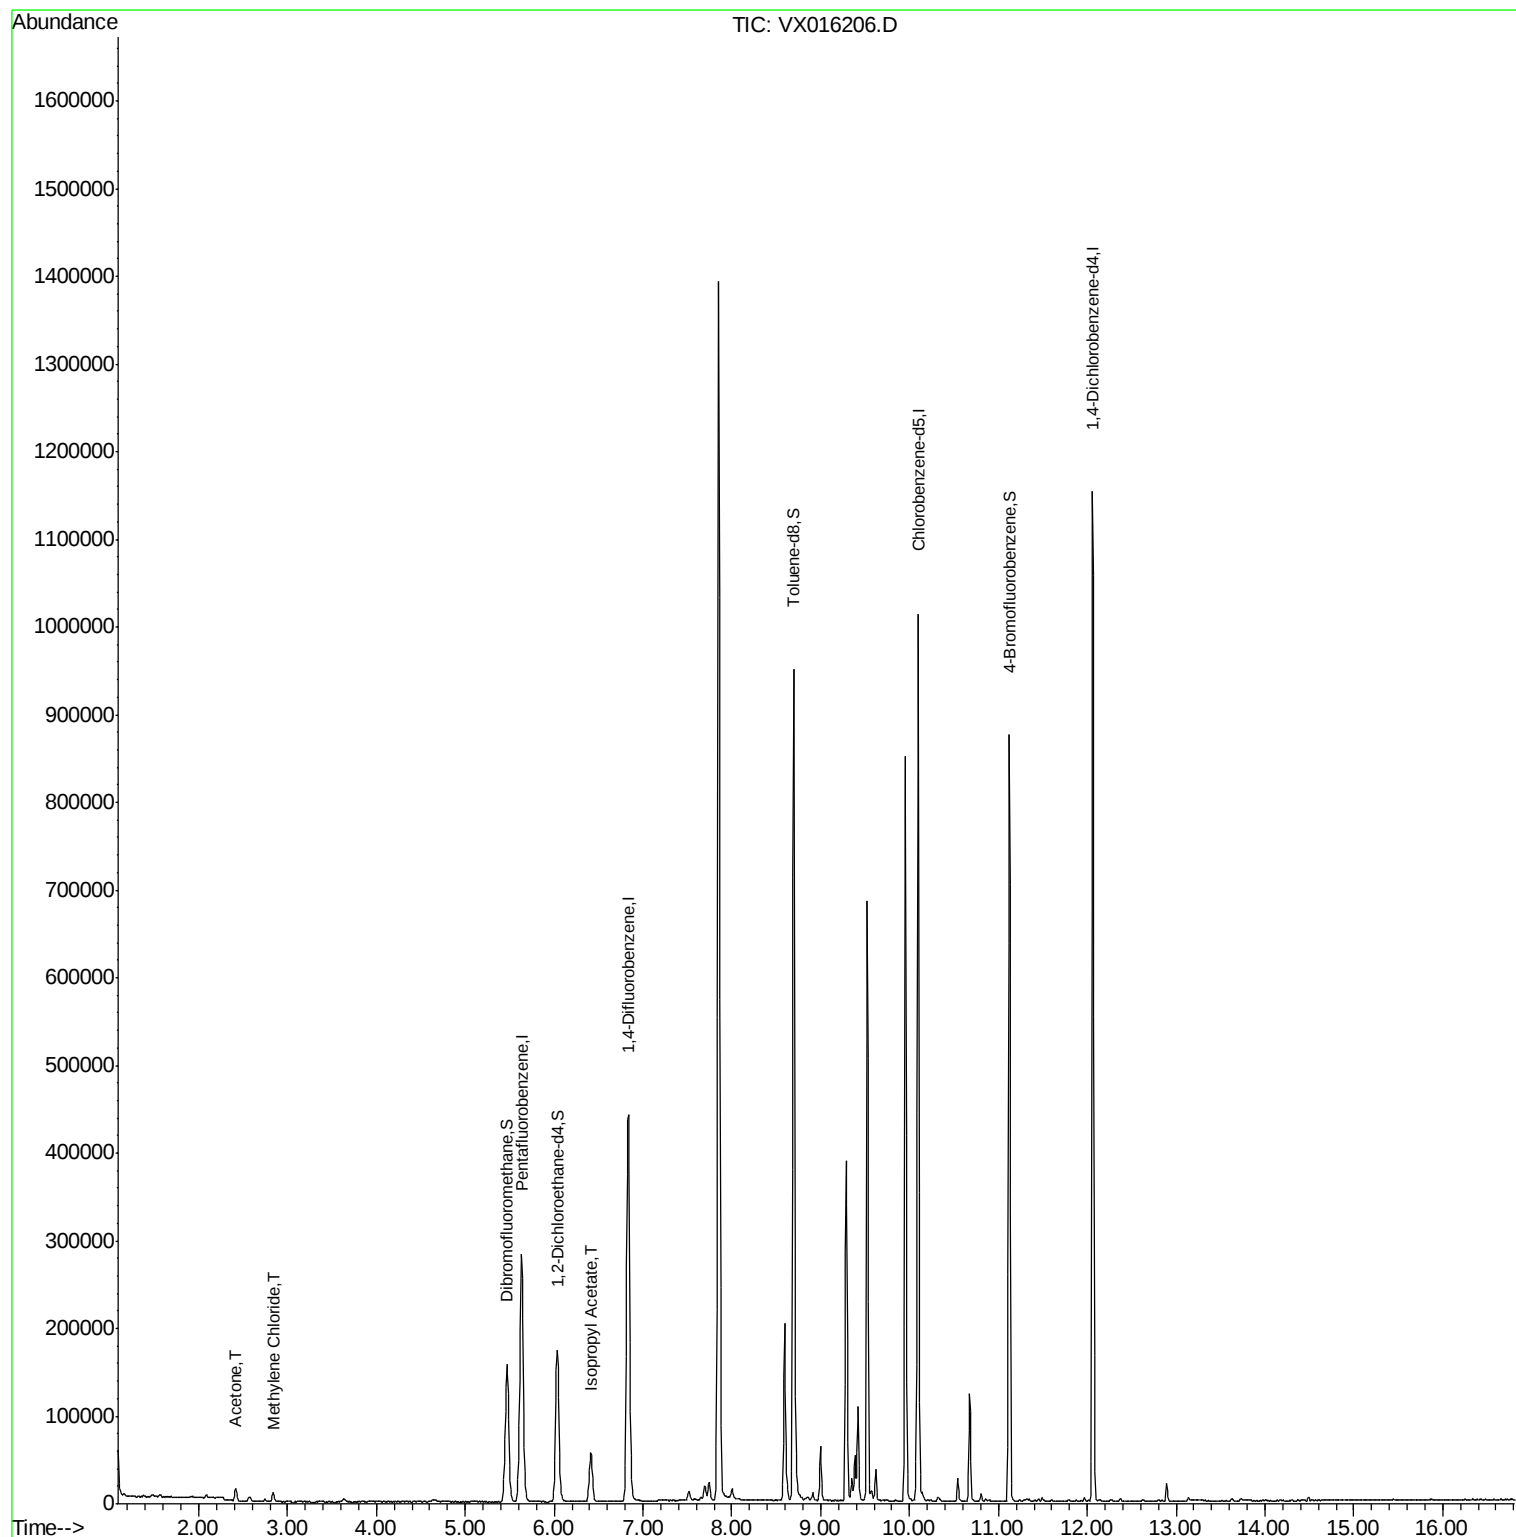



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.63 min Scan# 746

Delta R.T. -0.00 min

Lab File: VX016206.D

Acq: 14 May 2020 02:24

Instrument :

MSVOA_X

ClientSampleId :


OK-02-051220

Tot Ion:168 Resp: 275809

Ion Ratio Lower Upper

168 100

99 56.6 45.0 67.4

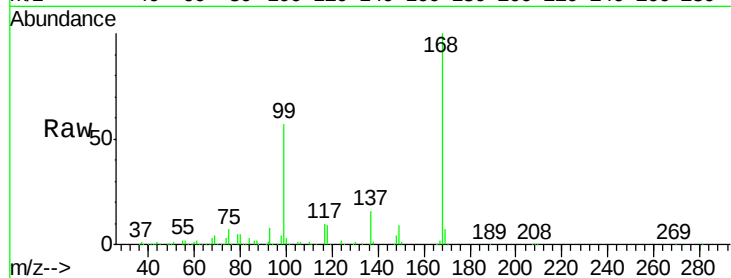

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.63

100000

80000



60000

40000

20000

0

Time-->

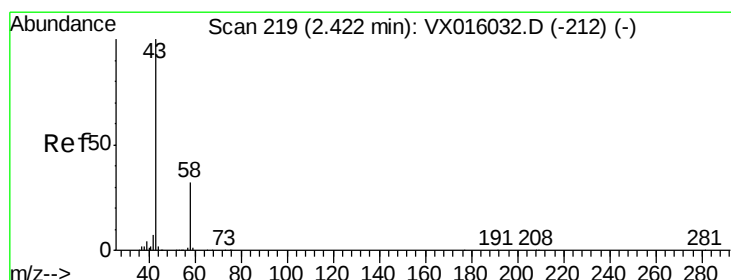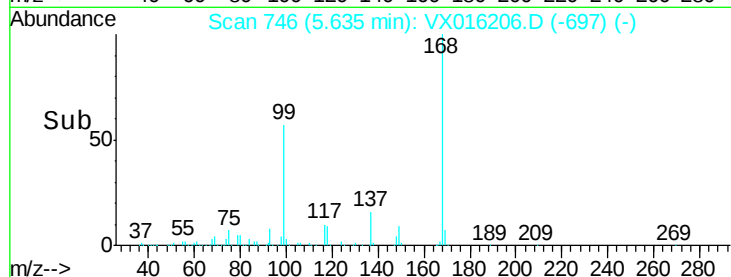

#16

Acetone

Concen: 9.008 ug/l

RT: 2.42 min Scan# 218

Delta R.T. -0.01 min

Lab File: VX016206.D


Acq: 14 May 2020 02:24

Tgt Ion: 43 Resp: 14588

Ion Ratio Lower Upper

43 100

58 32.5 25.4 38.0

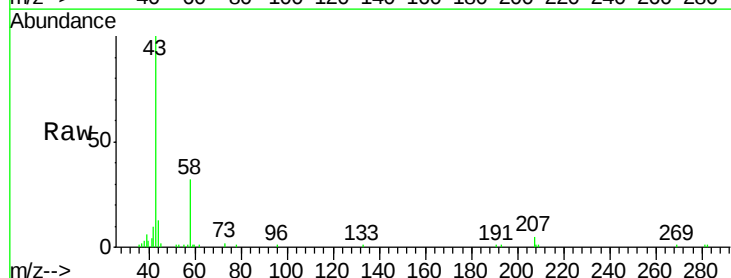

Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0

2.42

10000

8000


6000


4000

2000

0

Time-->




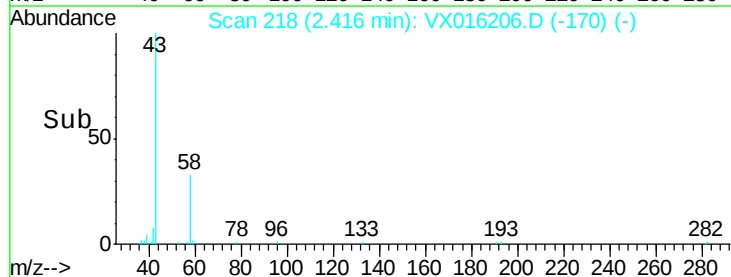


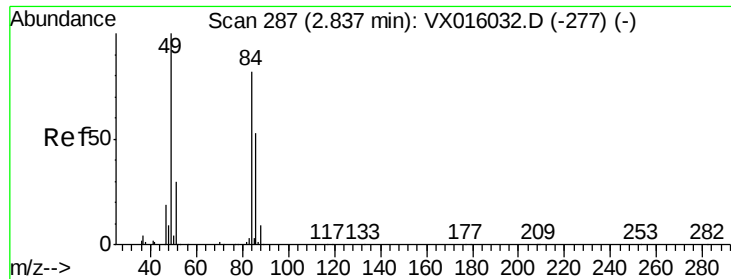

#20
Methvlene Chloride
Concen: 1.412 ug/l
RT: 2.84 min Scan# 287
Delta R.T. -0.00 min
Lab File: VX016206.D
Acq: 14 May 2020 02:24




Instrument :
MSVOA_X
ClientSampleId :
OK-02-051220


Tot Ion:	84	Resp:	4714
Ion	Ratio	Lower	Upper
84	100		
49	105.2	97.3	145.9
51	40.5	29.3	43.9
86	55.4	51.3	76.9

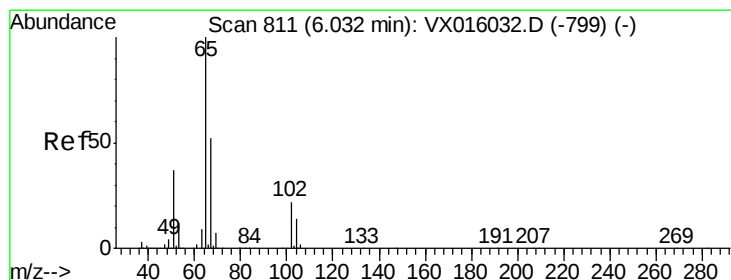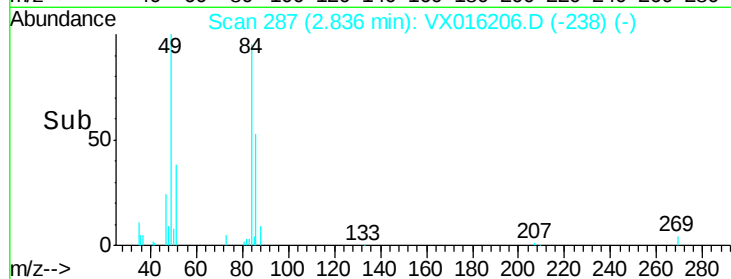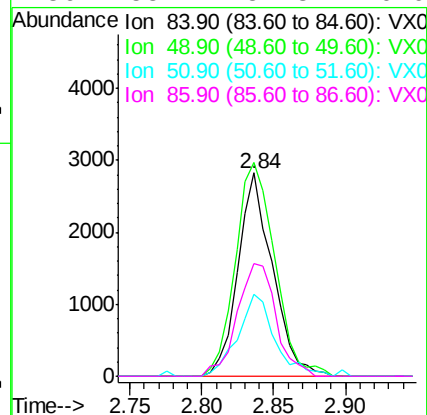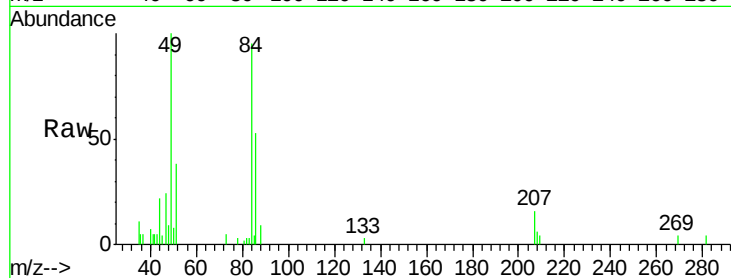

#33
1,2-Dichloroethane-d4
Concen: 46.324 ug/l
RT: 6.04 min Scan# 812
Delta R.T. 0.01 min
Lab File: VX016206.D
Acq: 14 May 2020 02:24

Tgt Ion:	65	Resp:	168126
Ion	Ratio	Lower	Upper
65	100		
67	52.3	0.0	104.8

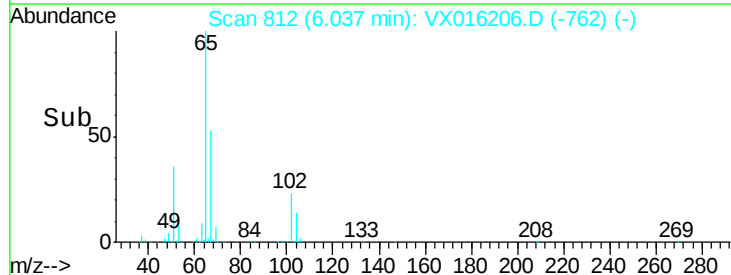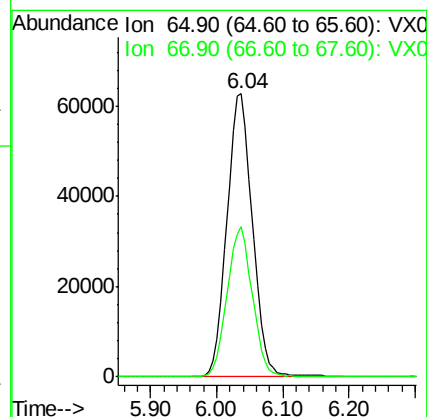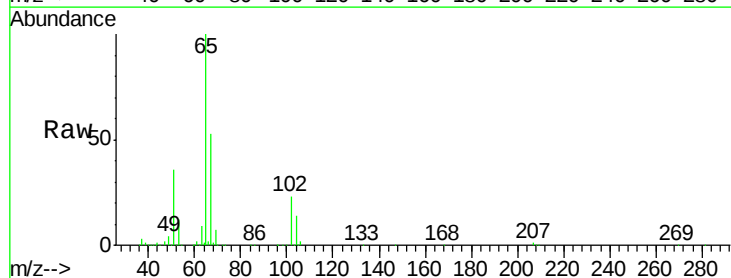

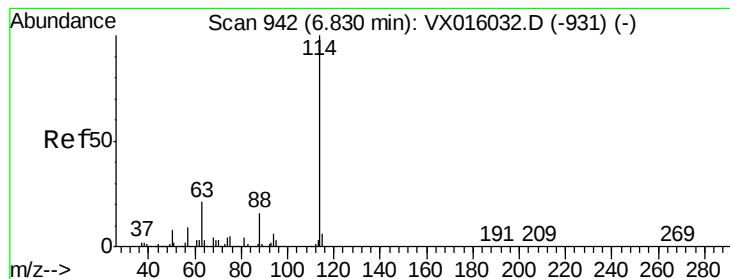

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.84 min Scan# 943

Delta R.T. 0.01 min

Lab File: VX016206.D

Acq: 14 May 2020 02:24

Instrument :

MSVOA_X

ClientSampleId :

OK-02-051220


Tot Ion:114 Resp: 458803

Ion Ratio Lower Upper

114 100

63 21.4 0.0 42.8




88 16.1 0.0 31.4

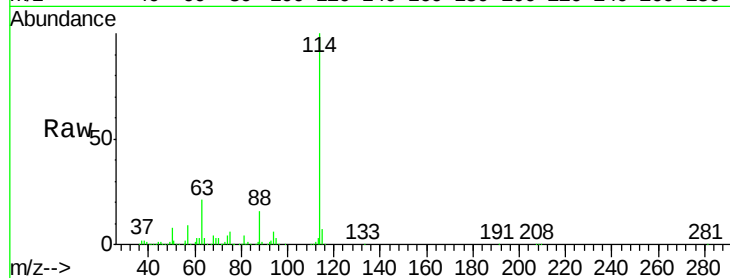

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

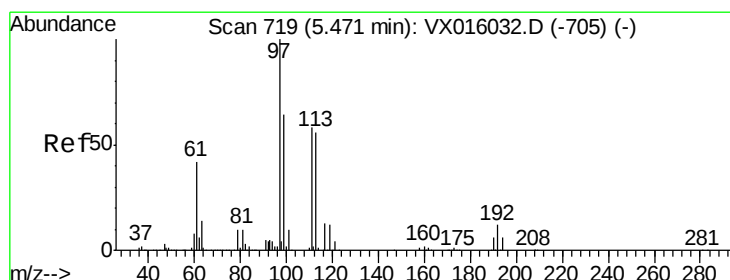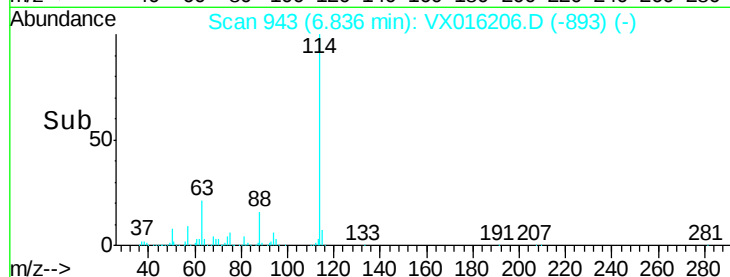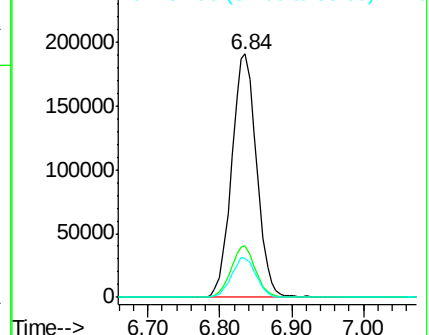

#35

Dibromofluoromethane

Concen: 46.612 ug/l

RT: 5.47 min Scan# 719

Delta R.T. -0.00 min

Lab File: VX016206.D

Acq: 14 May 2020 02:24


Tgt Ion:113 Resp: 135489

Ion Ratio Lower Upper

113 100

111 103.4 81.6 122.4



192 21.8 17.0 25.4

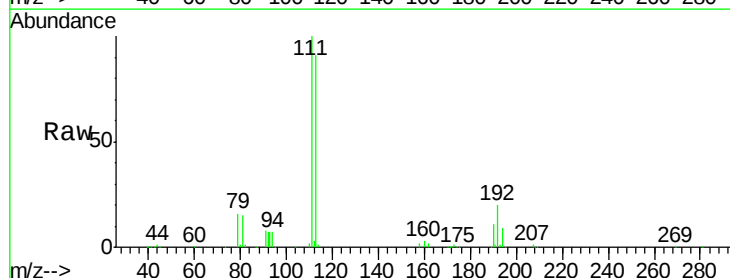


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

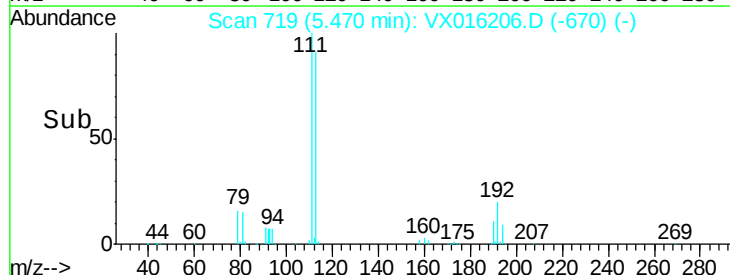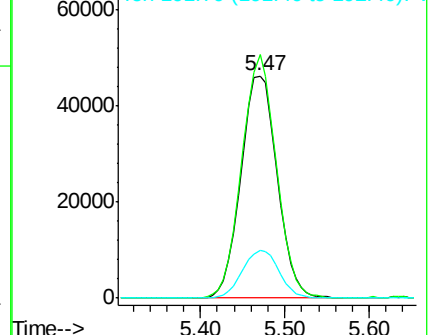

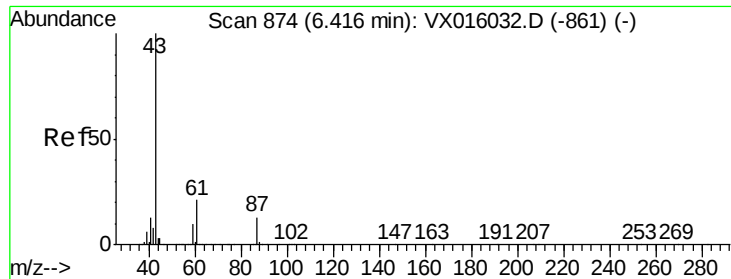

#43

Isopropyl Acetate

Concen: 9.279 ug/l

RT: 6.42 min Scan# 874

Delta R.T. -0.00 min

Lab File: VX016206.D

Acq: 14 May 2020 02:24

Instrument :

MSVOA_X

ClientSampleId :

OK-02-051220


Tot Ion: 43 Resp: 77493

Ion Ratio Lower Upper

43 100

61 21.8 17.0 25.4




87 14.5 11.0 16.6

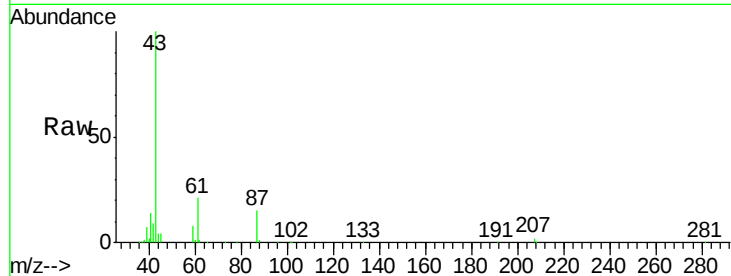

Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 61.00 (60.70 to 61.70): VX0

Ion 87.00 (86.70 to 87.70): VX0

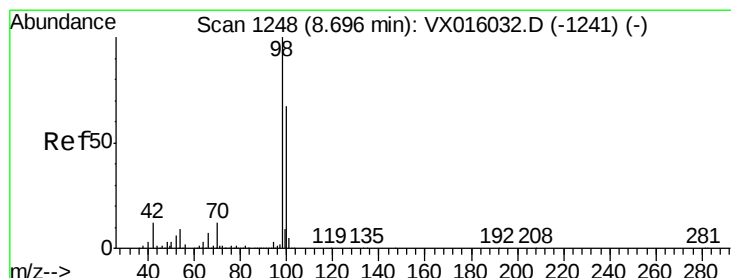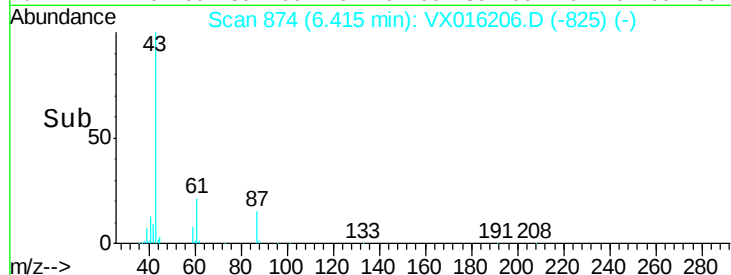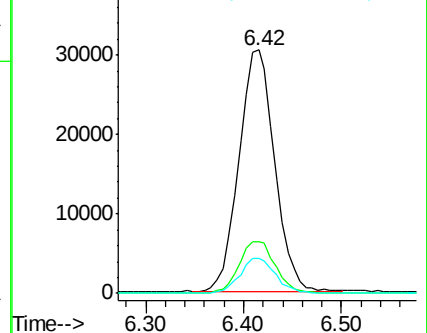

#50

Toluene-d8

Concen: 51.300 ug/l

RT: 8.70 min Scan# 1248

Delta R.T. -0.00 min

Lab File: VX016206.D


Acq: 14 May 2020 02:24

Tgt Ion: 98 Resp: 574545

Ion Ratio Lower Upper



98 100


100 67.6 53.7 80.5

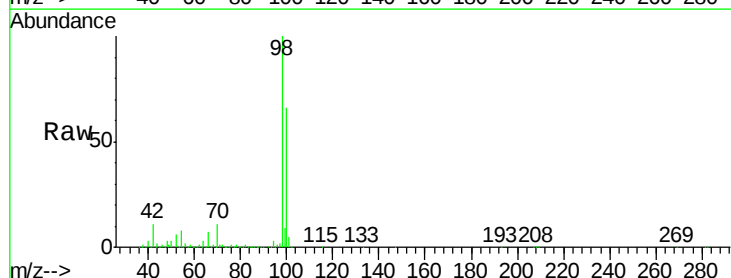

Abundance Ion 98.00 (97.70 to 98.70): VX0

Ion 100.00 (99.70 to 100.70): VX0

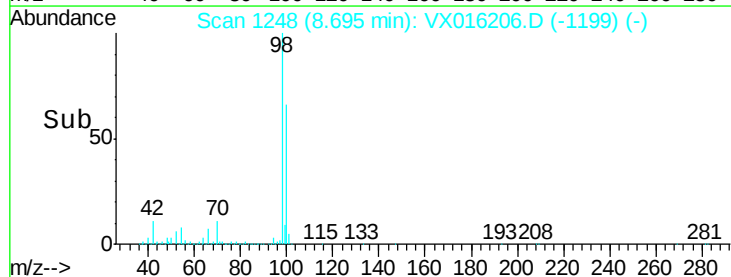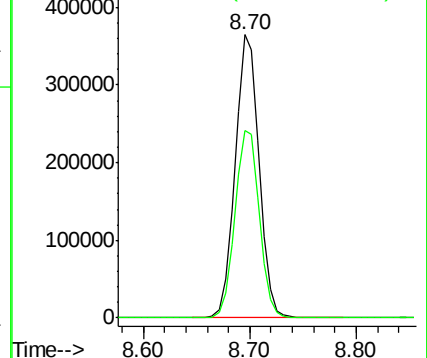

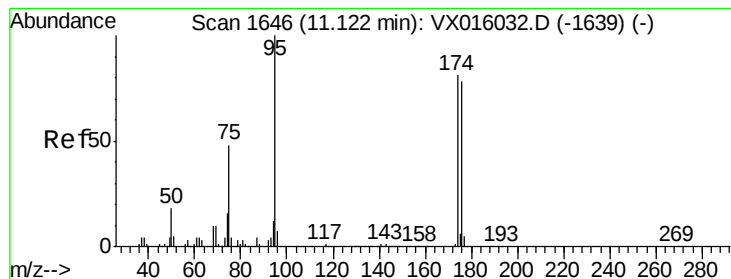

#62

4-Bromofluorobenzene

Concen: 54.377 ug/l

RT: 11.12 min Scan# 1646

Delta R.T. -0.00 min

Lab File: VX016206.D

Acq: 14 May 2020 02:24

Instrument :

MSVOA_X

ClientSampleId :

OK-02-051220


Tot Ion: 95 Resp: 231639

Ion Ratio Lower Upper

95 100

174 80.7 0.0 159.4




176 77.9 0.0 157.6

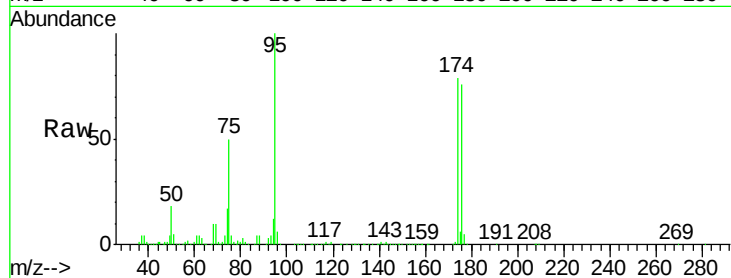

Abundance Ion 94.90 (94.60 to 95.60): VX016206.D (-1597) (-)

Ion 173.80 (173.50 to 174.50): VX016206.D (-1597) (-)

Ion 175.80 (175.50 to 176.50): VX016206.D (-1597) (-)

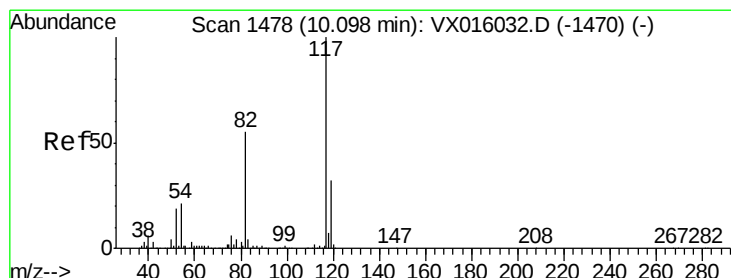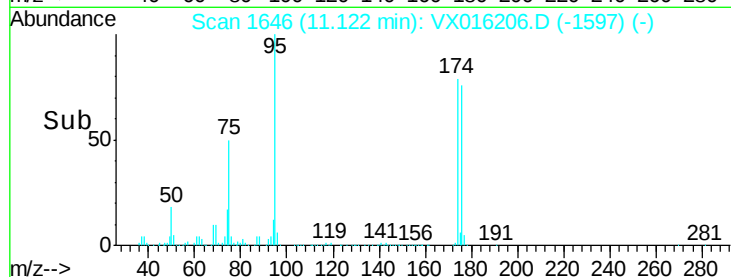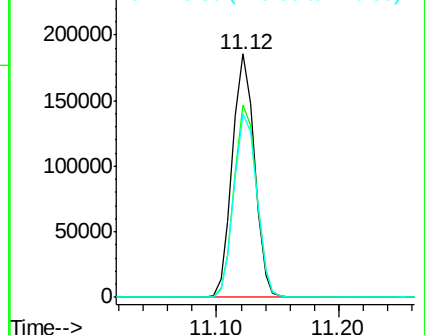

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.10 min Scan# 1478

Delta R.T. -0.00 min

Lab File: VX016206.D

Acq: 14 May 2020 02:24


Tgt Ion: 117 Resp: 457925

Ion Ratio Lower Upper

117 100

82 53.9 44.4 66.6



119 32.0 25.5 38.3

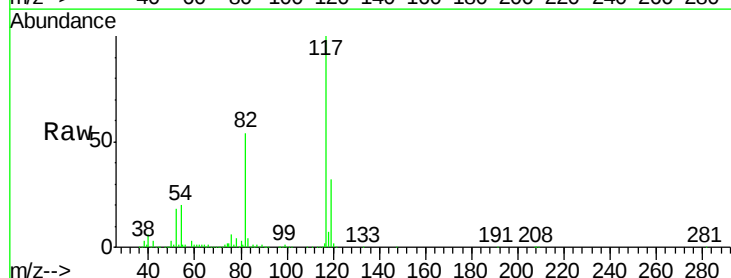


Abundance Ion 116.90 (116.60 to 117.60): VX016206.D (-1429) (-)

Ion 82.00 (81.70 to 82.70): VX016206.D (-1429) (-)

Ion 118.90 (118.60 to 119.60): VX016206.D (-1429) (-)

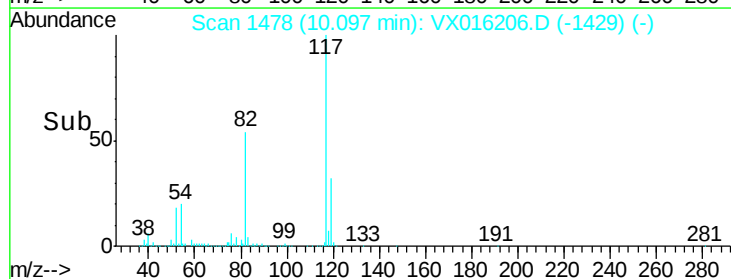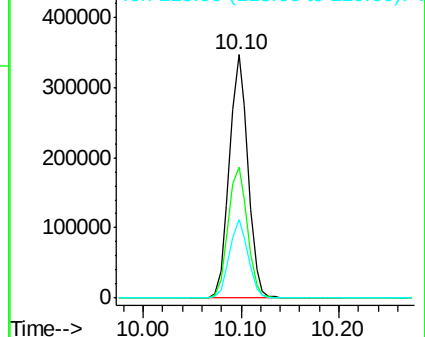

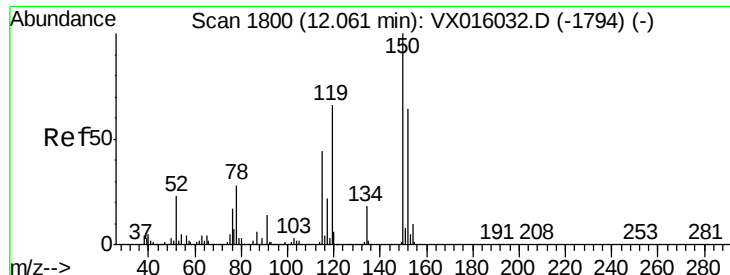

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.06 min Scan# 1800

Delta R.T. -0.00 min

Lab File: VX016206.D

Acq: 14 May 2020 02:24

Instrument :

MSVOA_X

ClientSampleId :

OK-02-051220


Tot Ion:152 Resp: 238493

Ion Ratio Lower Upper

152 100

115 58.4 41.3 124.1

150 157.8 0.0 352.2

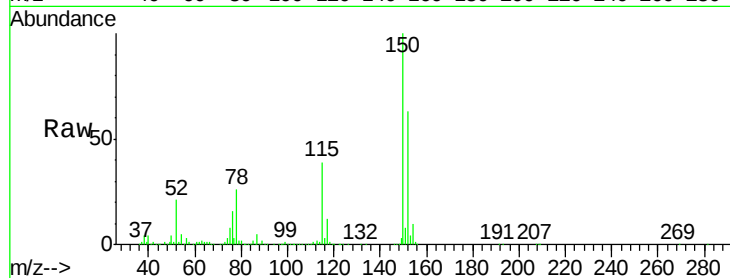

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

