
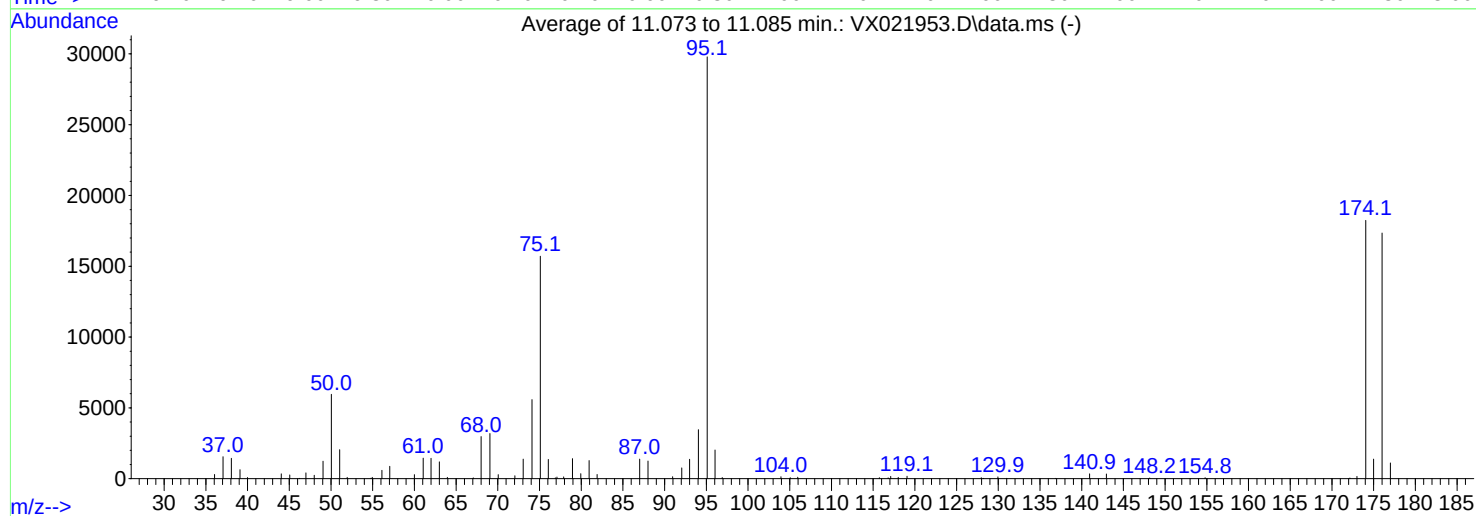


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051321\
 Data File : VX021953.D
 Acq On : 13 May 2021 08:52
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X051321W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Thu May 13 06:11:35 2021

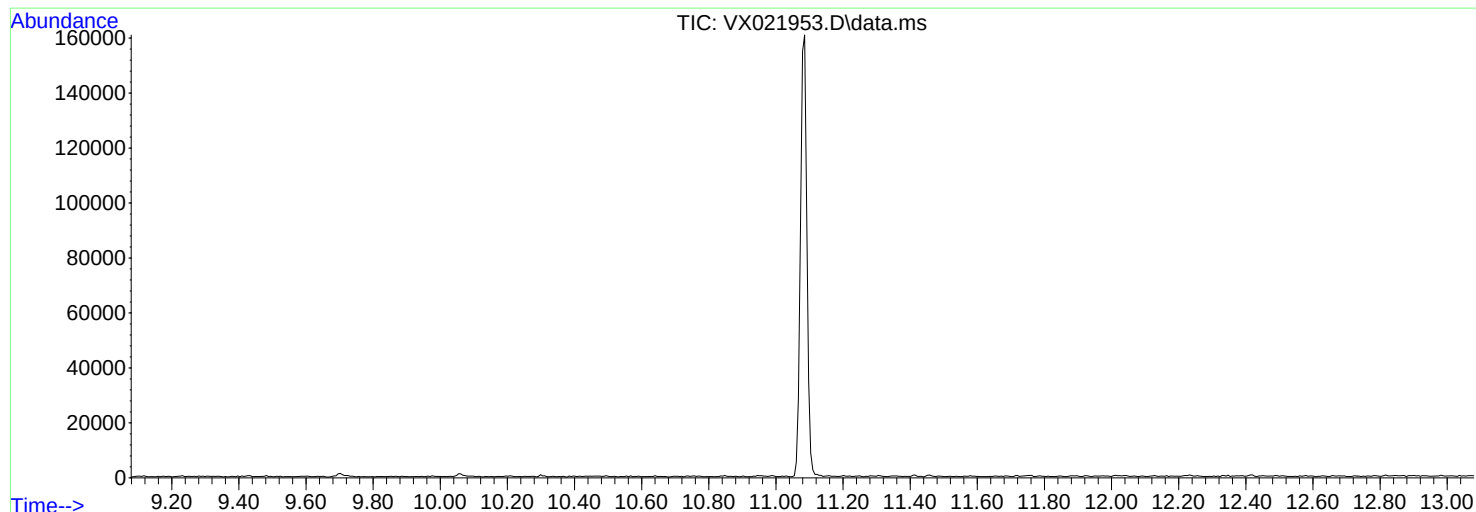

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.0	5951	PASS
75	95	30	60	52.7	15704	PASS
95	95	100	100	100.0	29789	PASS
96	95	5	9	6.8	2021	PASS
173	174	0.00	2	0.9	162	PASS
174	95	50	100	61.2	18239	PASS
175	174	5	9	7.6	1380	PASS
176	174	95	101	95.1	17345	PASS
177	176	5	9	6.4	1105	PASS