

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051322\
 Data File : VX028668.D
 Acq On : 13 May 2022 11:22
 Operator : JC/MD
 Sample : VX0513MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0513MBL01

Quant Time: May 16 02:17:45 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051222W.M
 Quant Title : SW846 8260
 QLast Update : Thu May 12 14:58:53 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	235140	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	417330	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	369546	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	152319	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	162500	50.415	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	=	100.840%
35) Dibromofluoromethane	5.385	113	131781	48.196	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	=	96.400%
50) Toluene-d8	8.647	98	496202	48.134	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	=	96.260%
62) 4-Bromofluorobenzene	11.079	95	166233	43.173	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	=	86.340%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051322\
Data File : VX028668.D
Acq On : 13 May 2022 11:22
Operator : JC/MD
Sample : VX0513MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0513MBL01

Quant Time: May 16 02:17:45 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051222W.M
Quant Title : SW846 8260
QLast Update : Thu May 12 14:58:53 2022
Response via : Initial Calibration




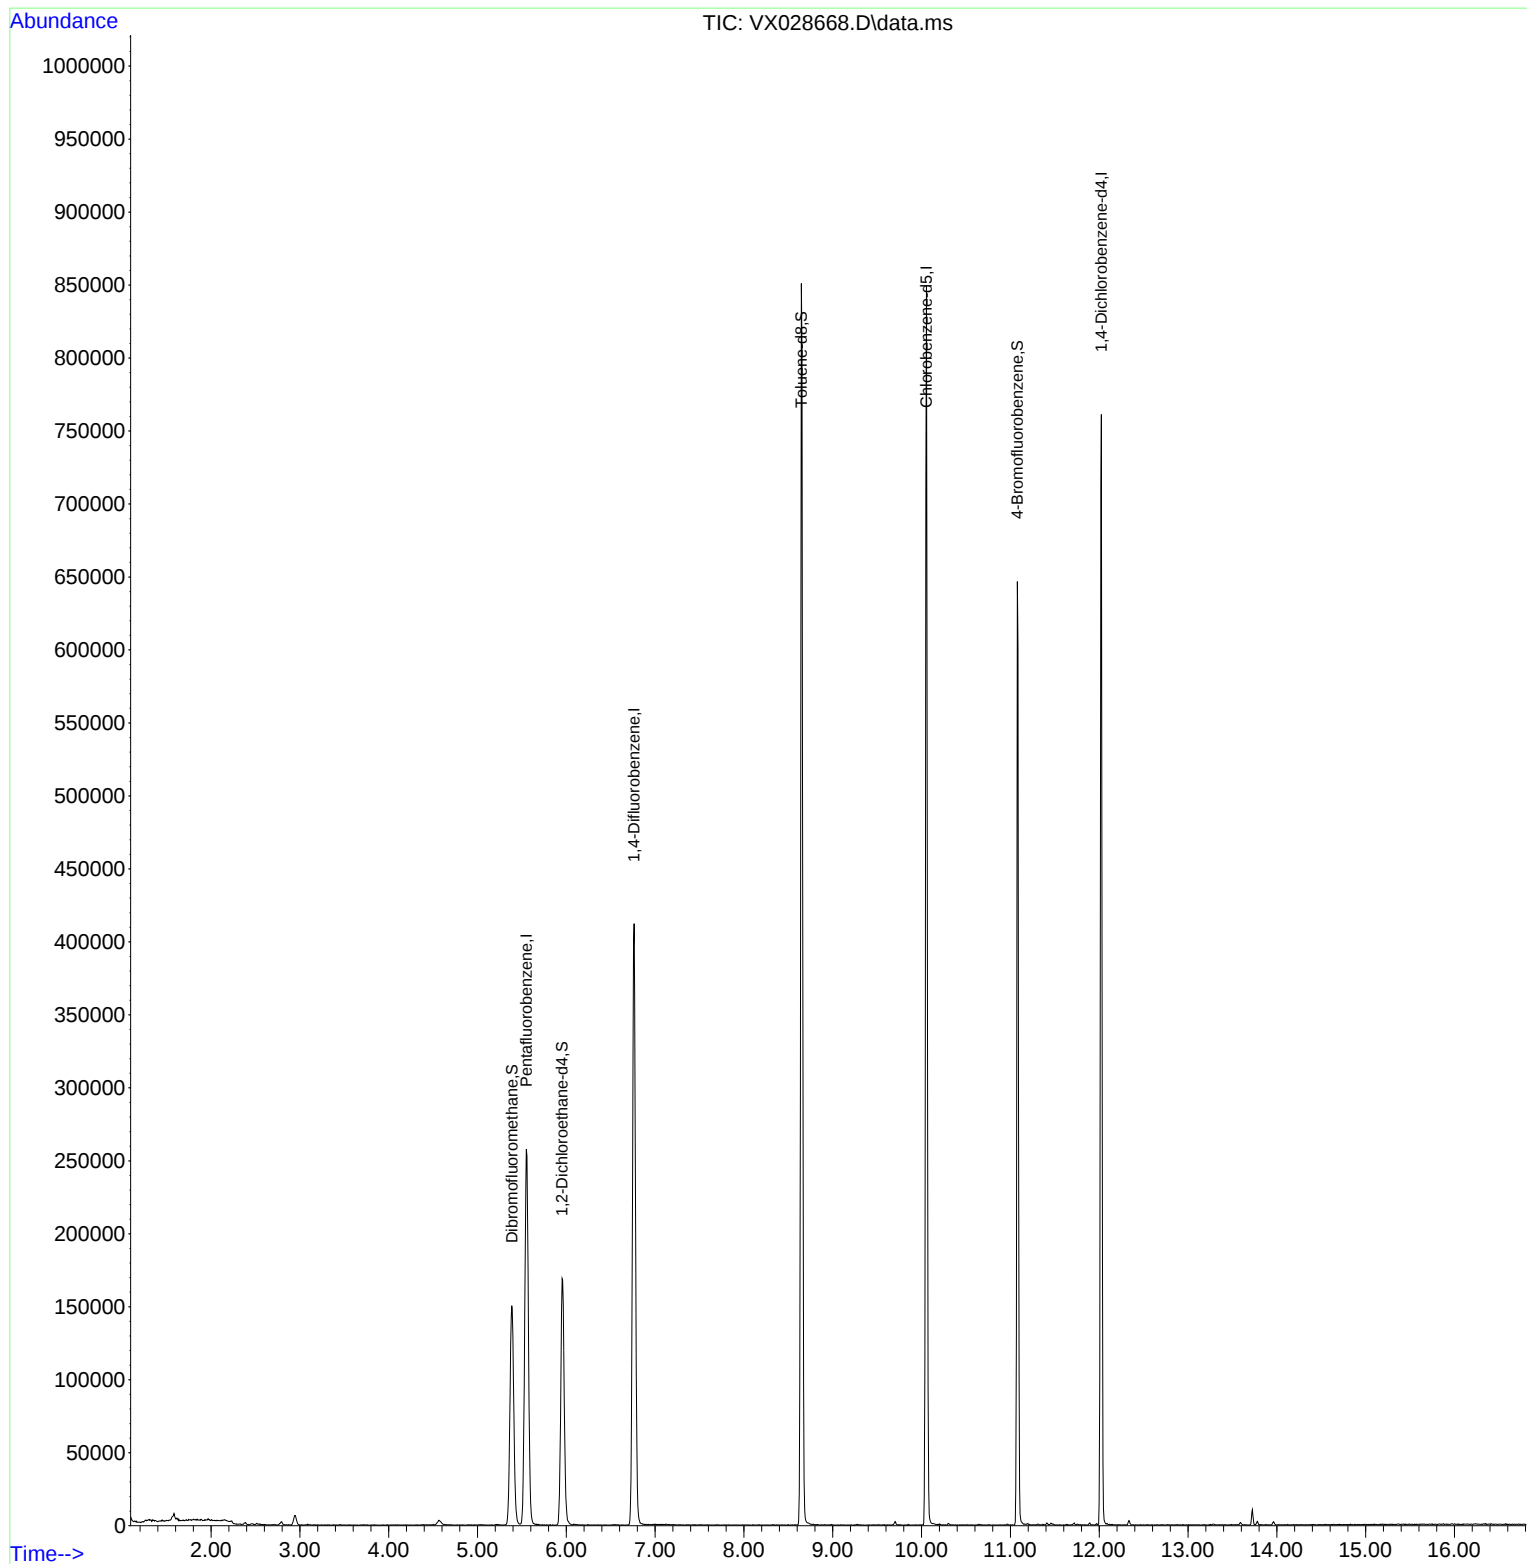


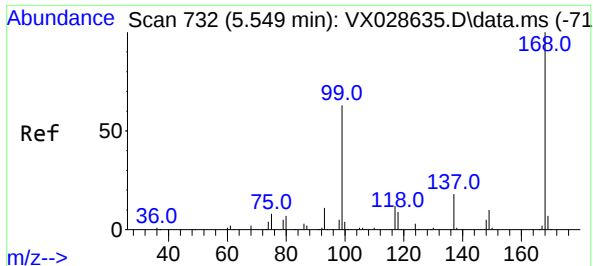

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. 0.001 min
Lab File: VX028668.D
Acq: 13 May 2022 11:22




Instrument :
MSVOA_X
ClientSampleId :
VX0513MBL01


Tgt Ion:168 Resp: 235140
Ion Ratio Lower Upper
168 100
99 61.4 41.7 62.5

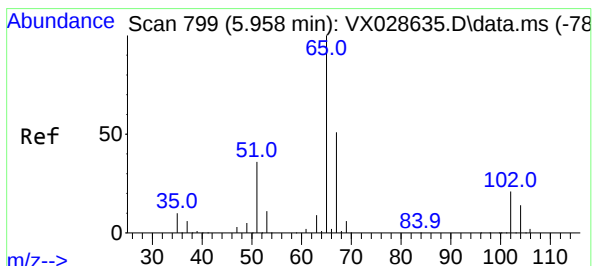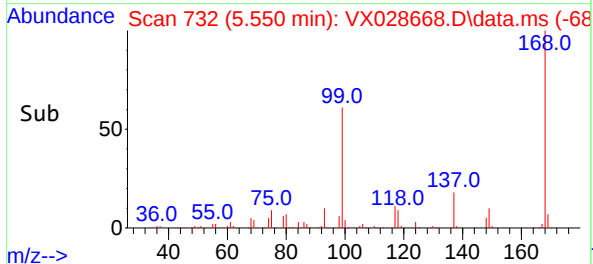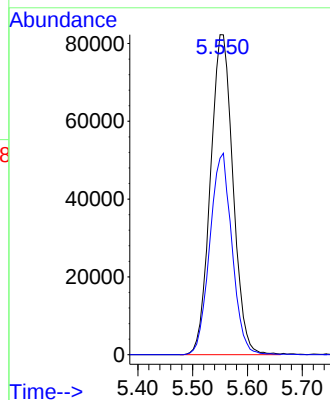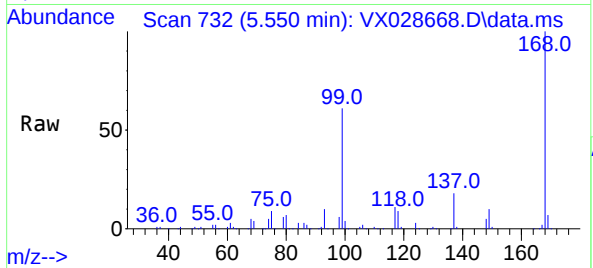

#33
1,2-Dichloroethane-d4
Concen: 50.415 ug/l
RT: 5.952 min Scan# 798
Delta R.T. -0.006 min
Lab File: VX028668.D
Acq: 13 May 2022 11:22

Tgt Ion: 65 Resp: 162500
Ion Ratio Lower Upper
65 100
67 50.6 0.0 107.4


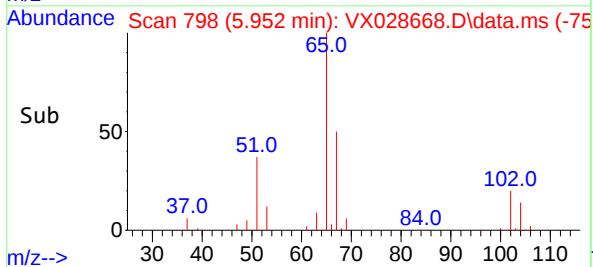
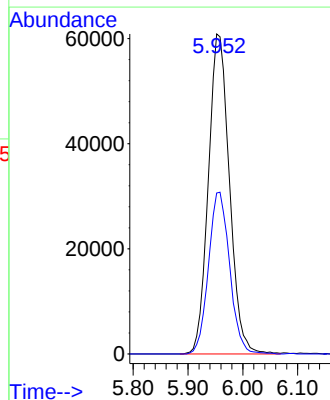
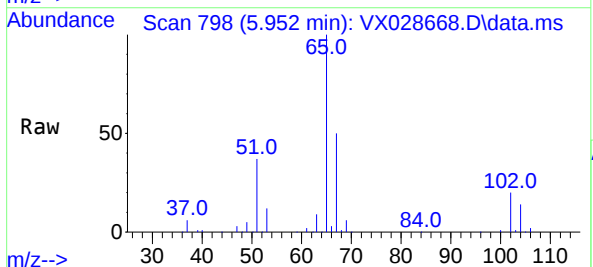


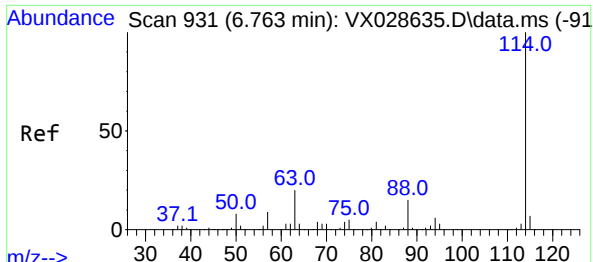

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 911
Delta R.T. 0.000 min
Lab File: VX028668.D
Acq: 13 May 2022 11:22




Instrument :
MSVOA_X
ClientSampleId :
VX0513MBL01


Tgt Ion:114 Resp: 417330
Ion Ratio Lower Upper
114 100
63 20.1 0.0 36.8
88 16.0 0.0 32.4

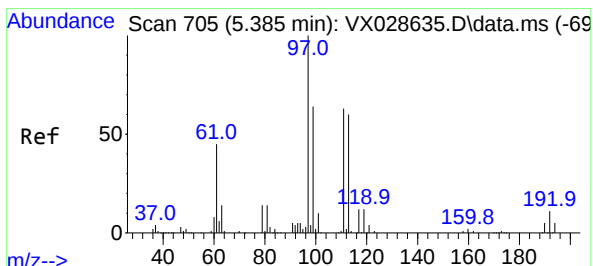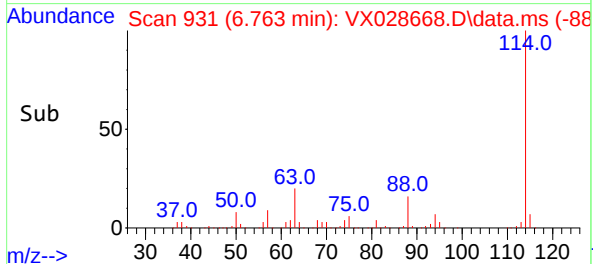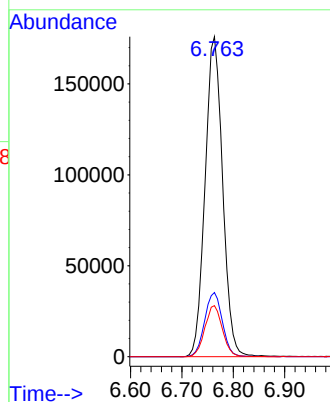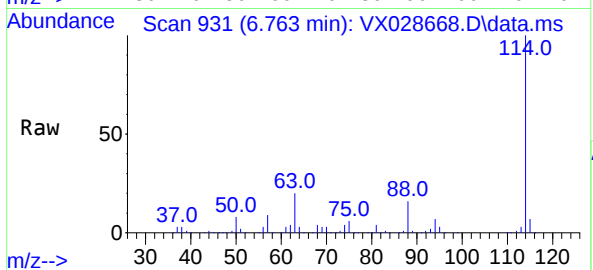

#35
Dibromofluoromethane
Concen: 48.196 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.000 min
Lab File: VX028668.D
Acq: 13 May 2022 11:22

Tgt Ion:113 Resp: 131781
Ion Ratio Lower Upper
113 100
111 102.9 82.8 124.2
192 18.0 16.9 25.3

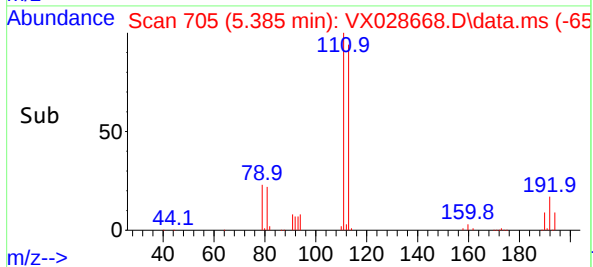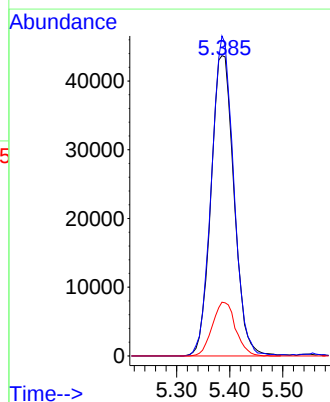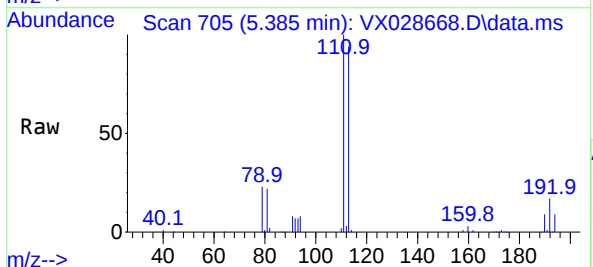

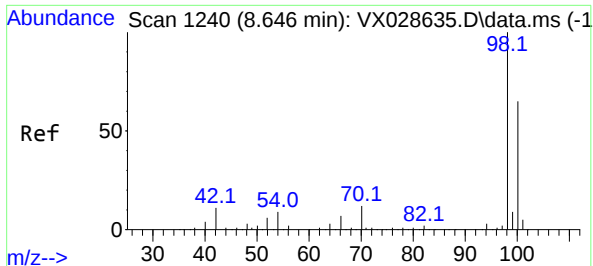

#50

Toluene-d8

Concen: 48.134 ug/l

RT: 8.647 min Scan# 11

Delta R.T. 0.001 min

Lab File: VX028668.D

Acq: 13 May 2022 11:22

Instrument :

MSVOA_X

ClientSampleId :





VX0513MBL01

Tgt Ion: 98 Resp: 496202

Ion Ratio Lower Upper

98 100

100 65.4 52.6 78.8

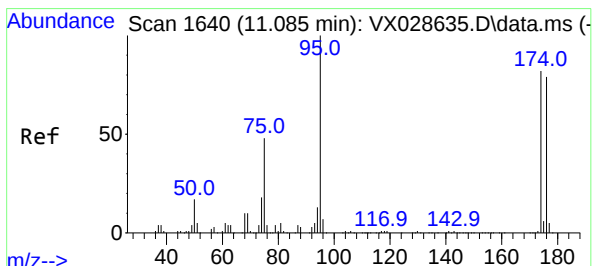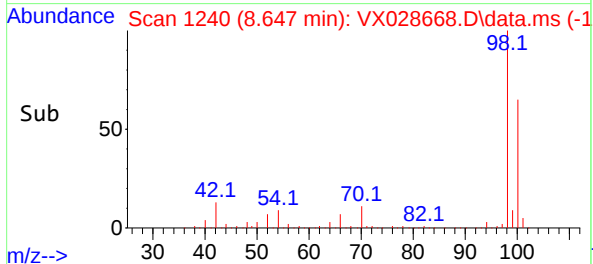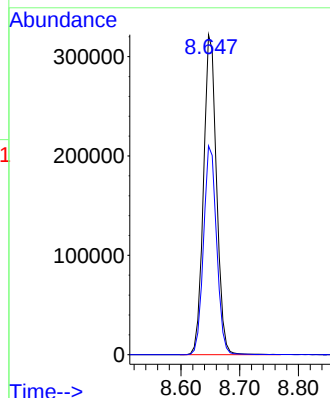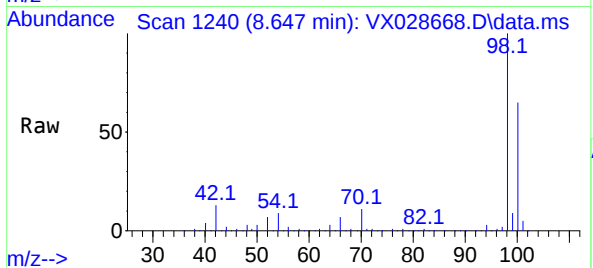

#62

4-Bromofluorobenzene

Concen: 43.173 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. -0.006 min

Lab File: VX028668.D

Acq: 13 May 2022 11:22




Tgt Ion: 95 Resp: 166233


Ion Ratio Lower Upper

95 100

174 75.4 0.0 163.0

176 71.8 0.0 155.0


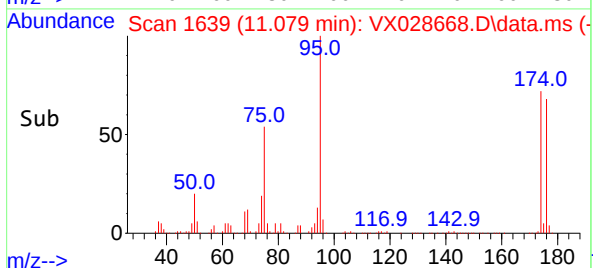
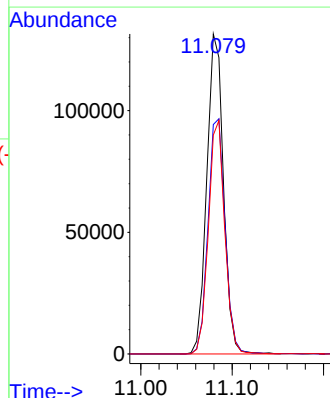
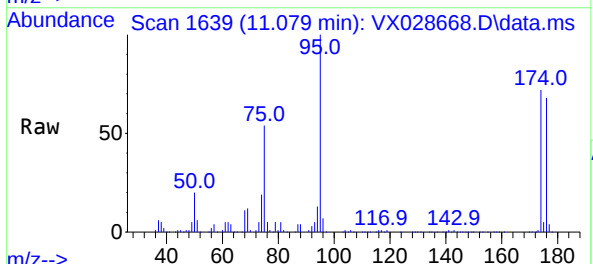


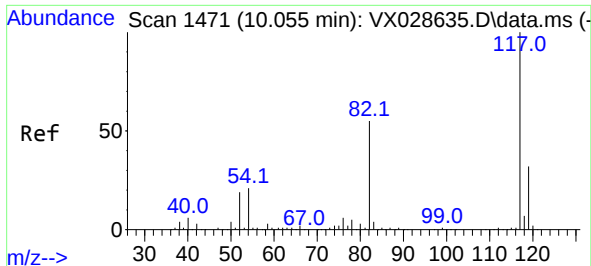

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX028668.D
Acq: 13 May 2022 11:22

Instrument :
MSVOA_X
ClientSampleId :
VX0513MBL01

Tgt Ion:117 Resp: 369546
Ion Ratio Lower Upper
117 100
82 55.2 41.8 62.8
119 31.8 24.8 37.2

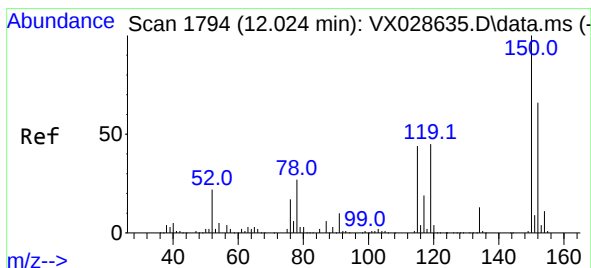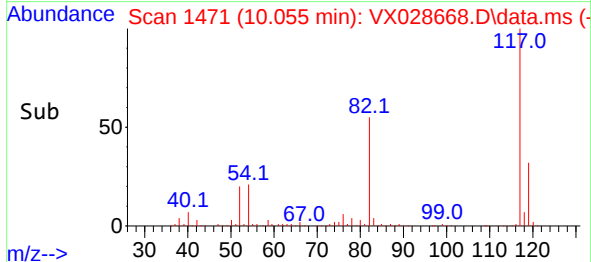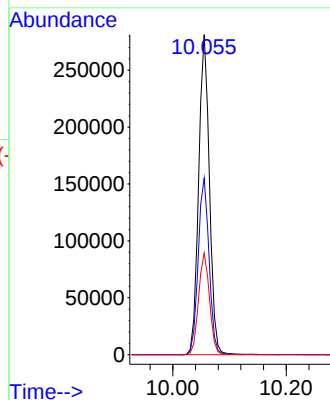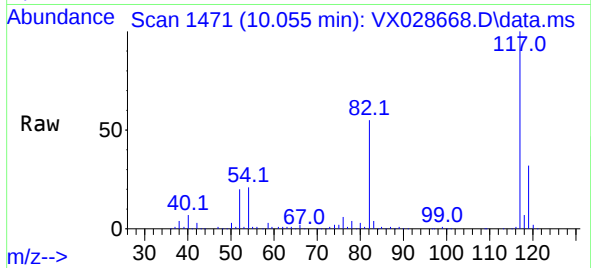

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX028668.D
Acq: 13 May 2022 11:22

Tgt Ion:152 Resp: 152319
Ion Ratio Lower Upper
152 100
115 62.0 37.5 112.7
150 157.3 0.0 338.2

