

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051322\
 Data File : VX028689.D
 Acq On : 13 May 2022 19:37
 Operator : JC/MD
 Sample : N2861-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 STORAGE-BLANK-SAMPLE-MANAG

Quant Time: May 16 02:24:46 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051222W.M
 Quant Title : SW846 8260
 QLast Update : Thu May 12 14:58:53 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	223572	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.769	114	414793	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	395496	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	174138	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	166637	54.374	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	=	108.740%
35) Dibromofluoromethane	5.391	113	137719	50.676	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	=	101.360%
50) Toluene-d8	8.653	98	507063	49.488	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	=	98.980%
62) 4-Bromofluorobenzene	11.079	95	183634	47.984	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	=	95.960%


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051322\
Data File : VX028689.D
Acq On : 13 May 2022 19:37
Operator : JC/MD
Sample : N2861-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SAMPLE-MANAG

Quant Time: May 16 02:24:46 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051222W.M
Quant Title : SW846 8260
QLast Update : Thu May 12 14:58:53 2022
Response via : Initial Calibration




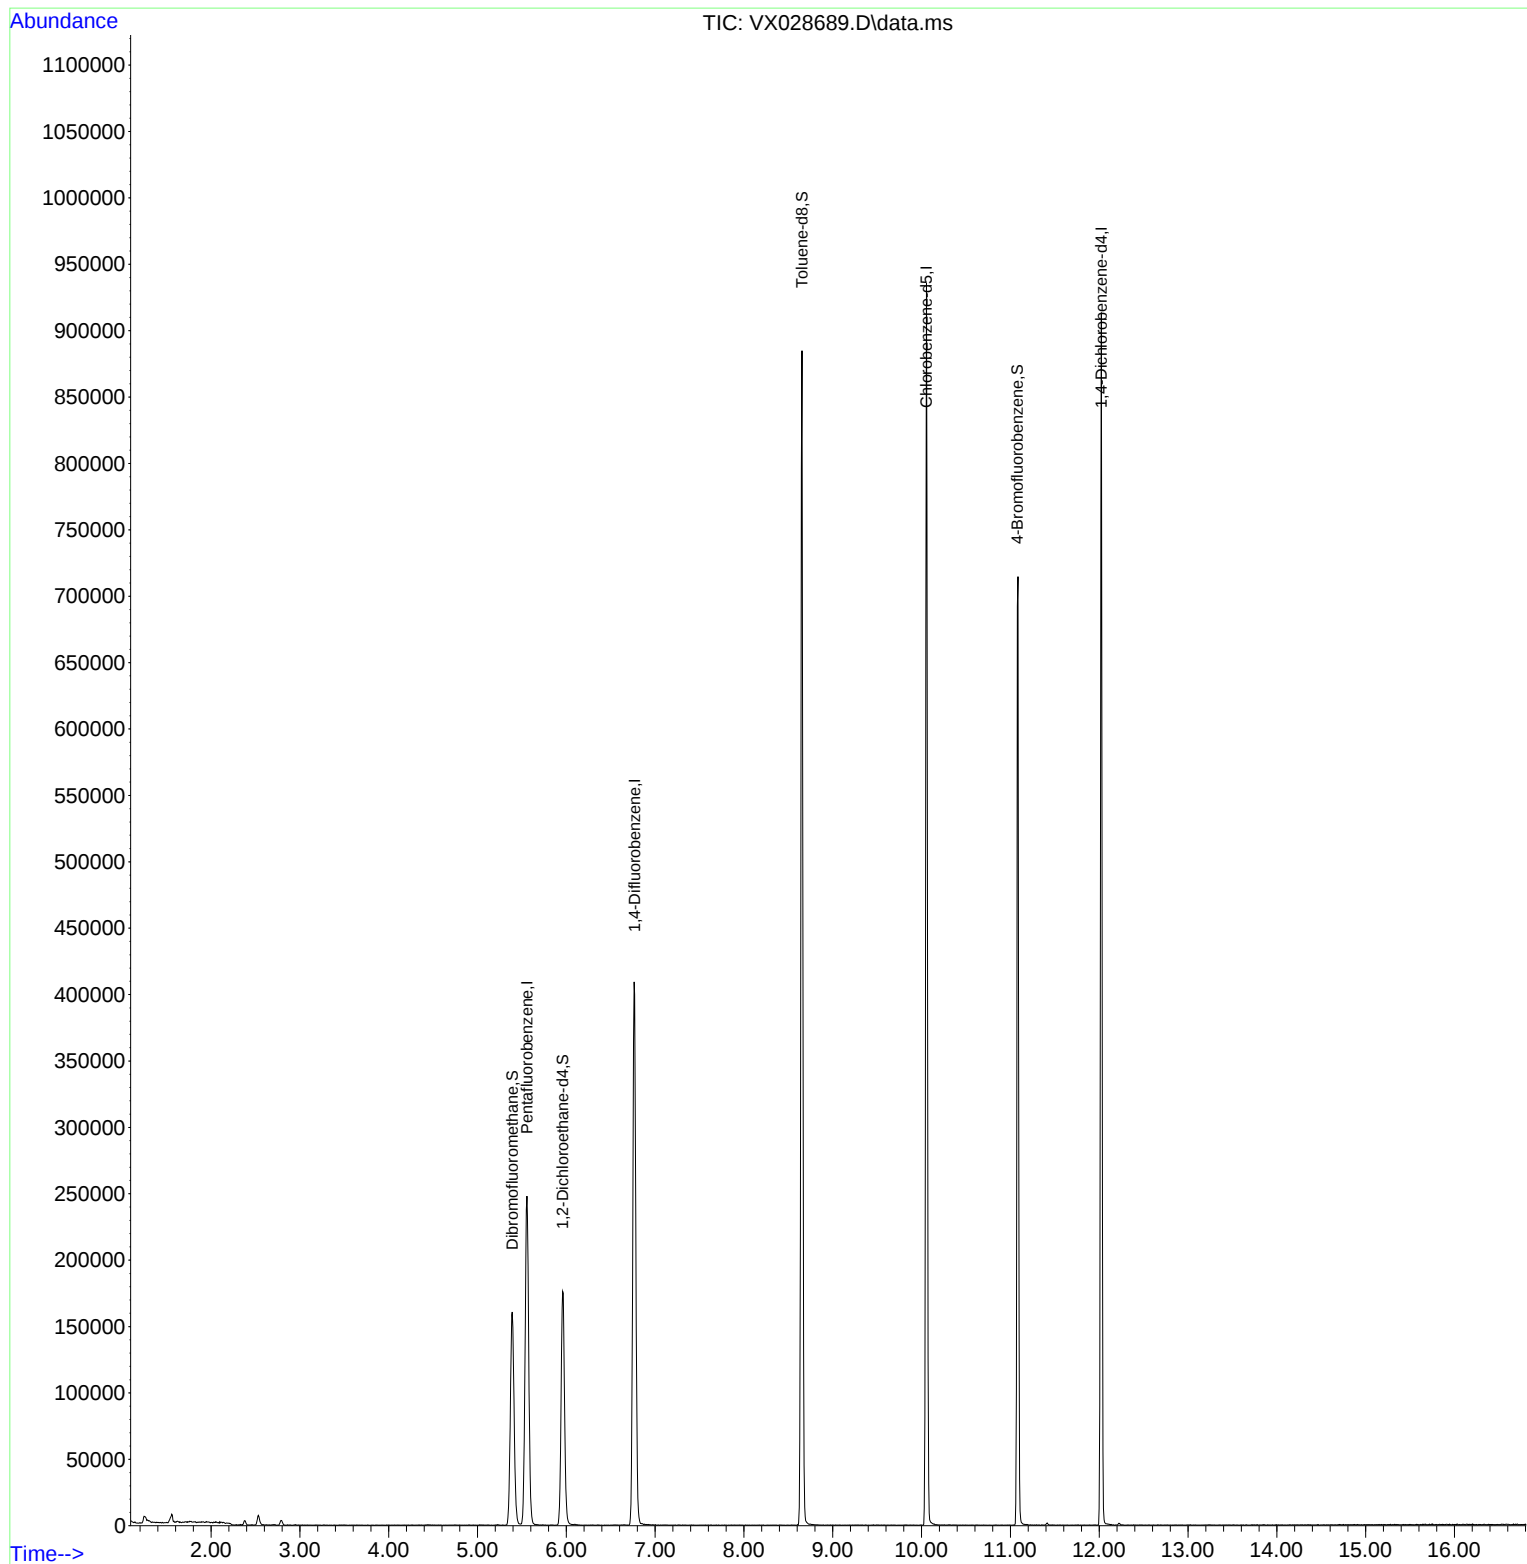




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. 0.007 min
Lab File: VX028689.D
Acq: 13 May 2022 19:37




Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SAMPLE-MANAG


Tgt Ion:168 Resp: 223572
Ion Ratio Lower Upper
168 100
99 60.8 41.7 62.5

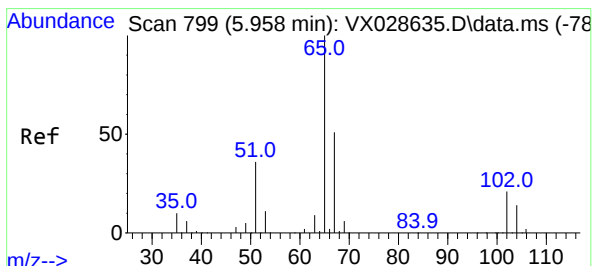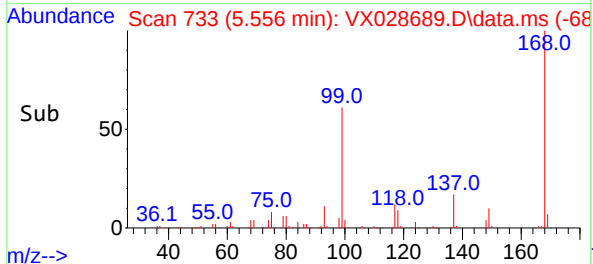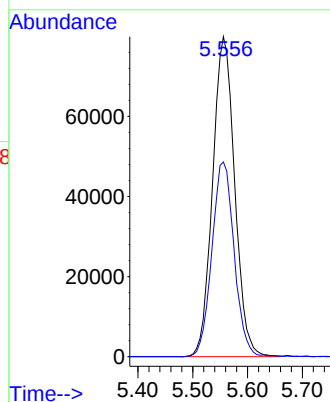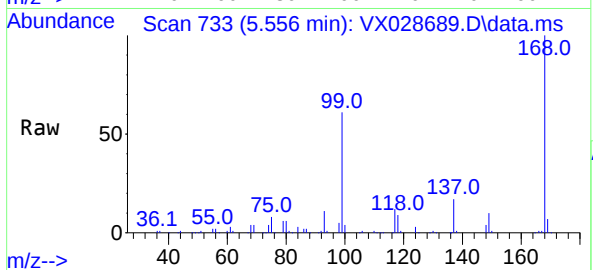

#33
1,2-Dichloroethane-d4
Concen: 54.374 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.000 min
Lab File: VX028689.D
Acq: 13 May 2022 19:37

Tgt Ion: 65 Resp: 166637
Ion Ratio Lower Upper
65 100
67 51.7 0.0 107.4

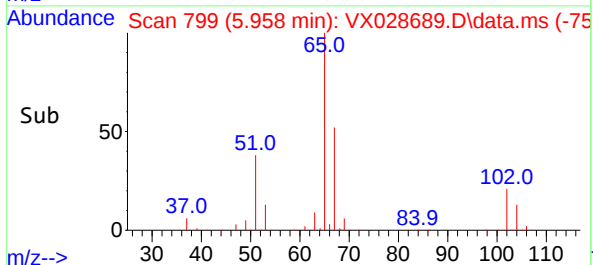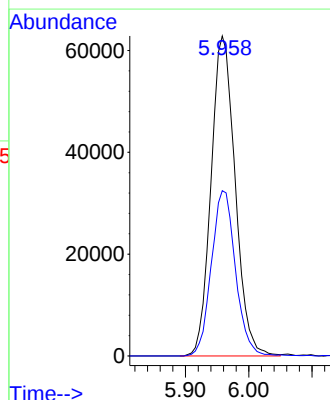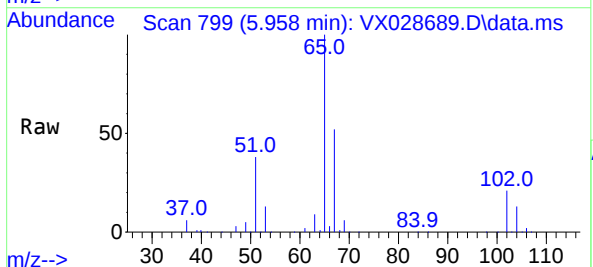

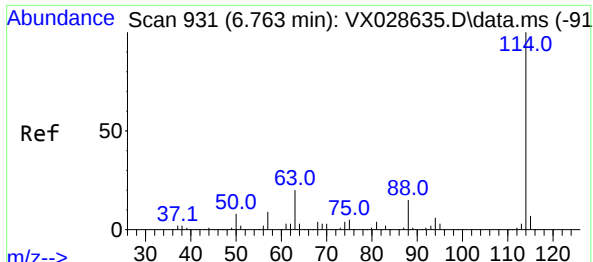

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.769 min Scan# 91

Delta R.T. 0.006 min

Lab File: VX028689.D

Acq: 13 May 2022 19:37

Instrument :

MSVOA_X

ClientSampleId :

STORAGE-BLANK-SAMPLE-MANAG





Tgt Ion:114 Resp: 414793

Ion Ratio Lower Upper

114 100

63 18.9 0.0 36.8

88 15.1 0.0 32.4

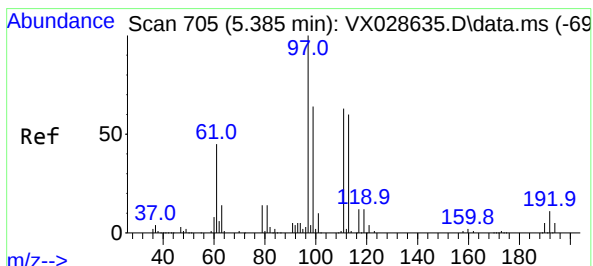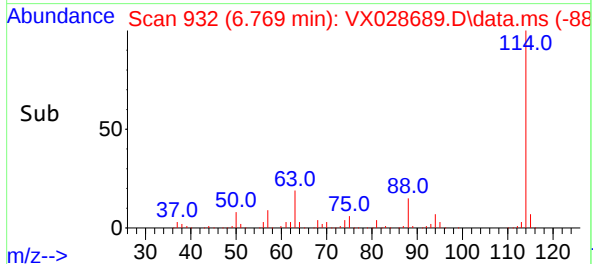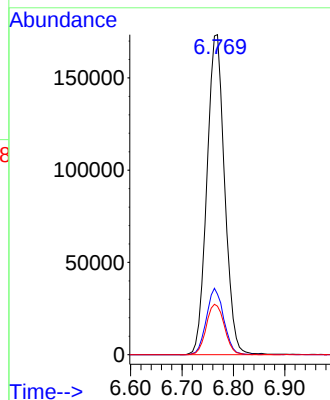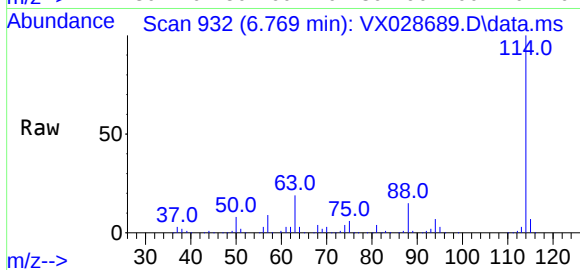

#35

Dibromofluoromethane

Concen: 50.676 ug/l

RT: 5.391 min Scan# 706

Delta R.T. 0.006 min

Lab File: VX028689.D

Acq: 13 May 2022 19:37




Tgt Ion:113 Resp: 137719


Ion Ratio Lower Upper

113 100

111 103.0 82.8 124.2

192 17.8 16.9 25.3


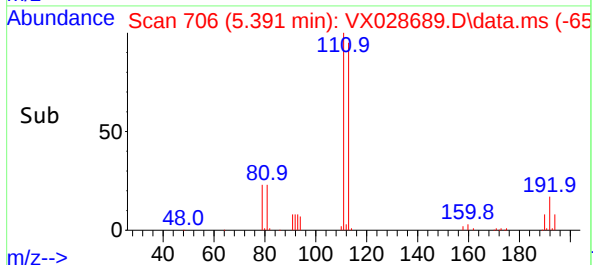
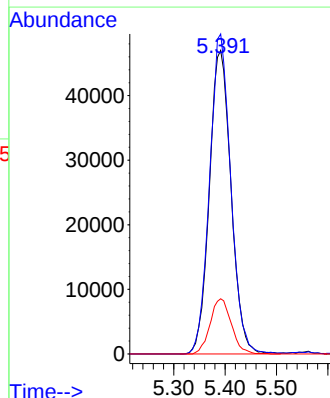
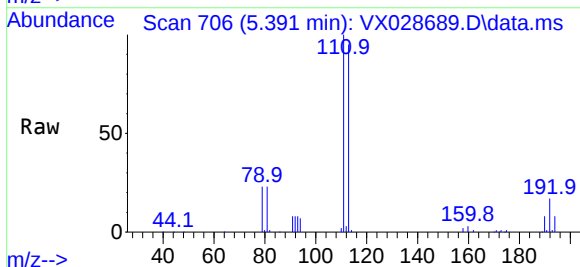


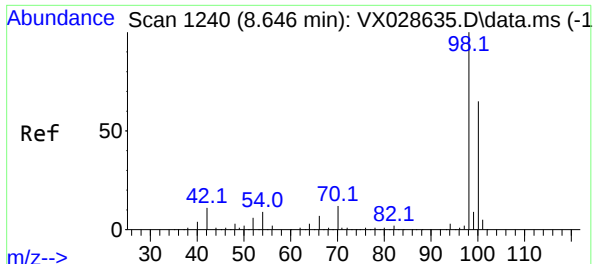

#50
Toluene-d8
Concen: 49.488 ug/l
RT: 8.653 min Scan# 11
Delta R.T. 0.007 min
Lab File: VX028689.D
Acq: 13 May 2022 19:37




Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SAMPLE-MANAG


Tgt Ion: 98 Resp: 507063
Ion Ratio Lower Upper
98 100
100 65.6 52.6 78.8

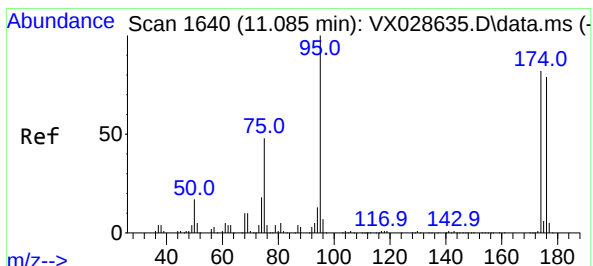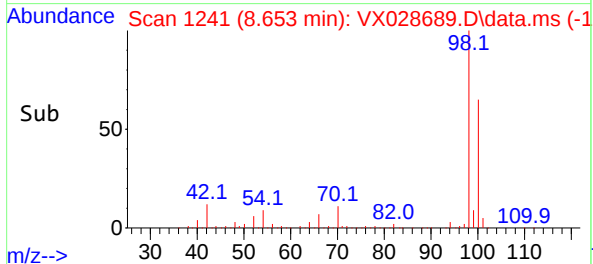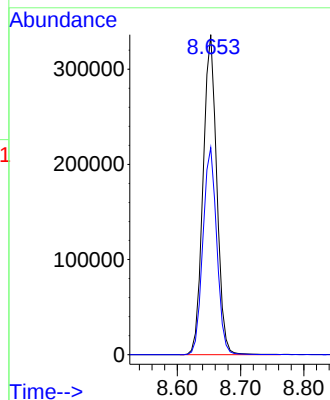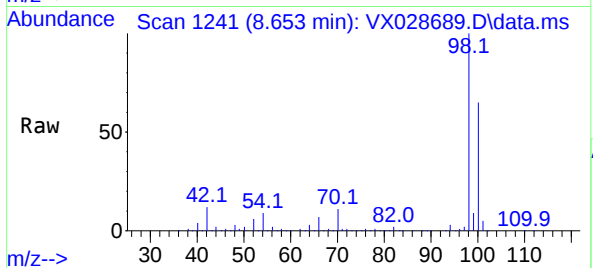

#62
4-Bromofluorobenzene
Concen: 47.984 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.006 min
Lab File: VX028689.D
Acq: 13 May 2022 19:37

Tgt Ion: 95 Resp: 183634
Ion Ratio Lower Upper
95 100
174 76.1 0.0 163.0
176 73.5 0.0 155.0


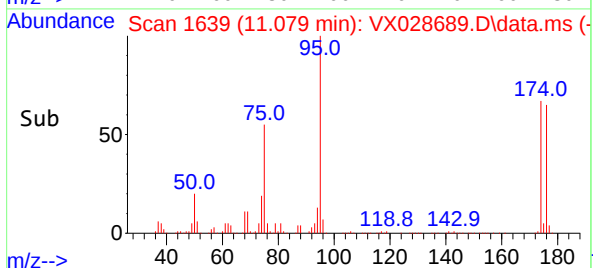
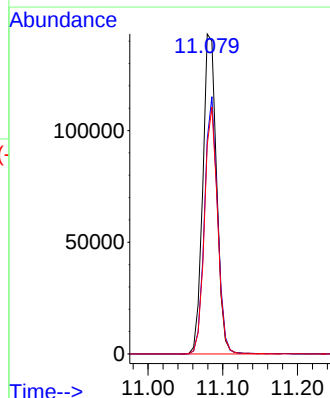
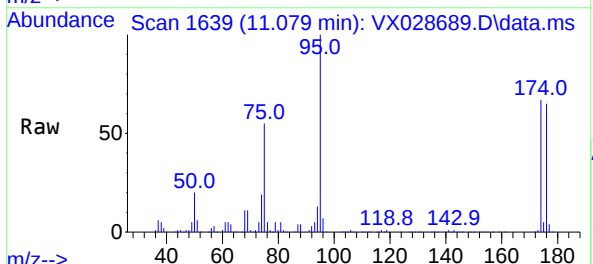


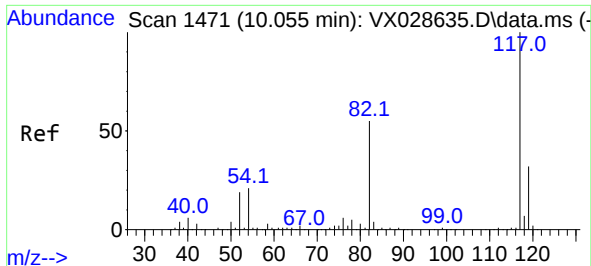

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX028689.D
Acq: 13 May 2022 19:37

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SAMPLE-MANAG

Tgt Ion:117 Resp: 395496
Ion Ratio Lower Upper
117 100
82 58.2 41.8 62.8
119 32.7 24.8 37.2

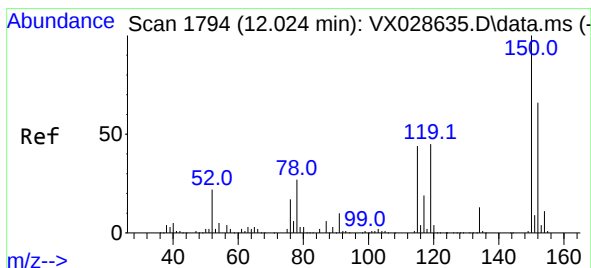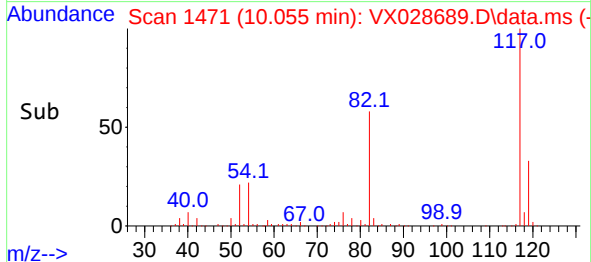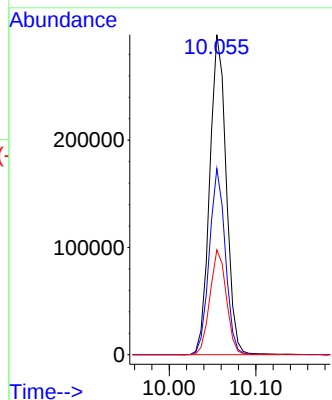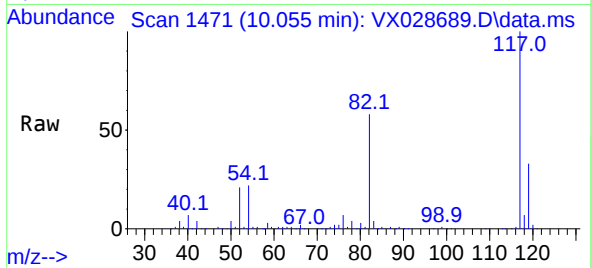

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX028689.D
Acq: 13 May 2022 19:37

Tgt Ion:152 Resp: 174138
Ion Ratio Lower Upper
152 100
115 62.0 37.5 112.7
150 158.3 0.0 338.2

